




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010175.D
 Acq On : 02 May 2022 16:25
 Operator : CG/JU
 Sample : N2562-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW474

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:36:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

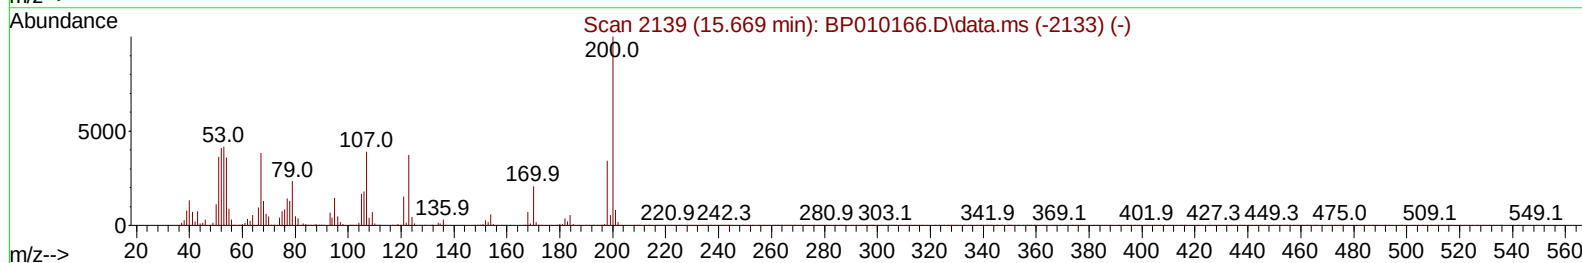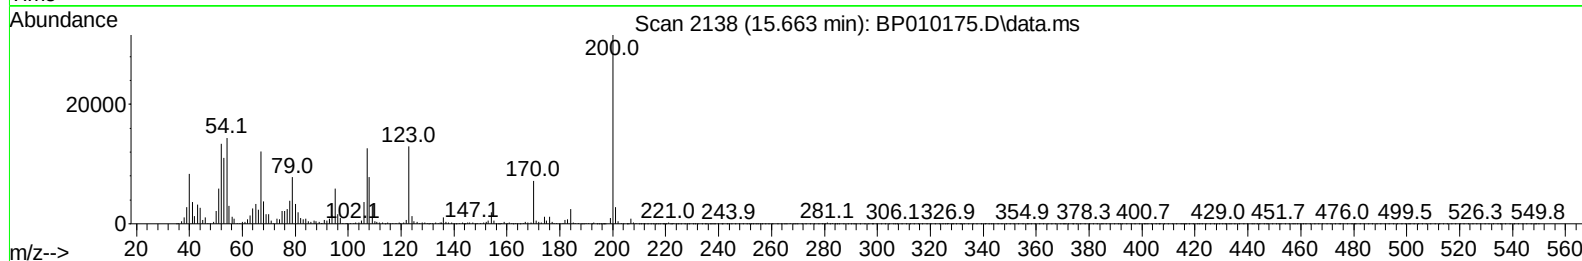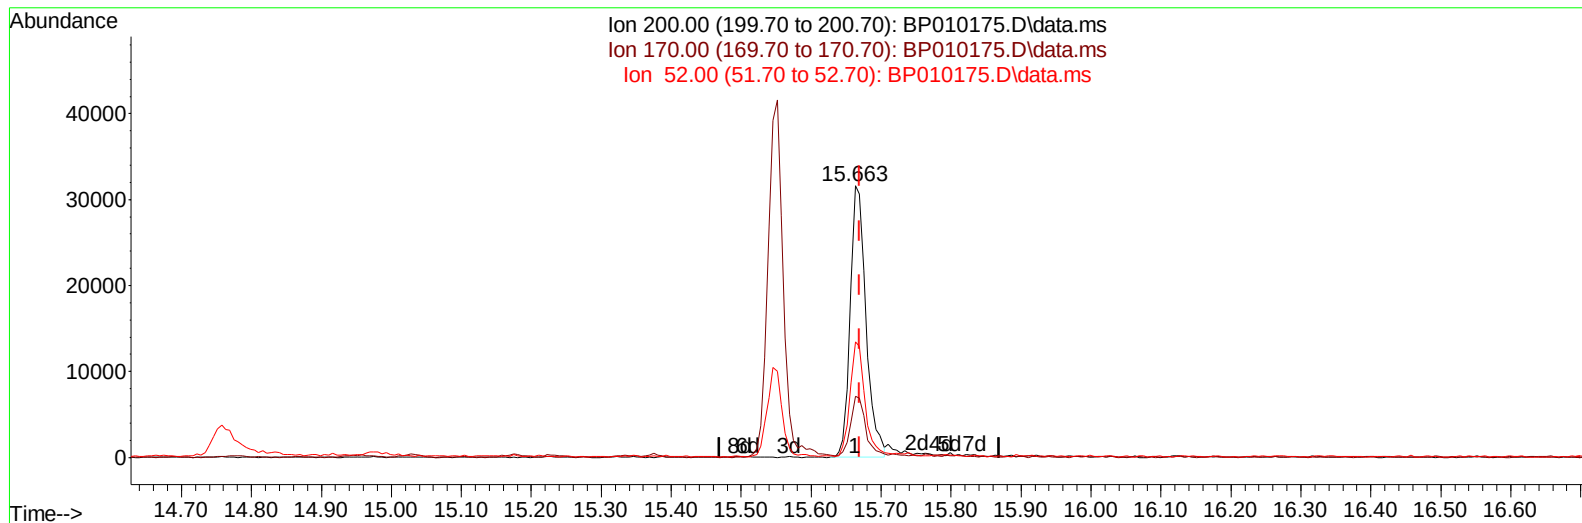

TIC: BP010175.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.663min (-0.006) 7.48 ng/ul

response 49149

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	22.62
52.00	21.20	42.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010175.D
Acq On : 02 May 2022 16:25
Operator : CG/JU
Sample : N2562-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW474

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:36:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

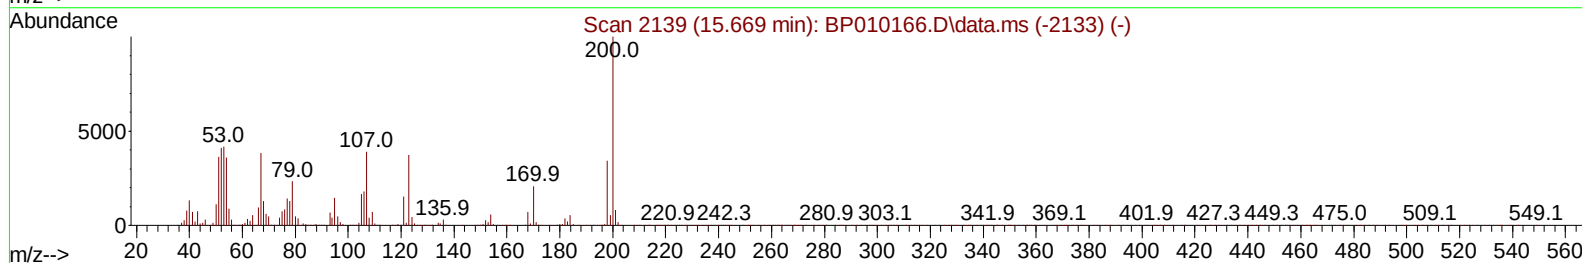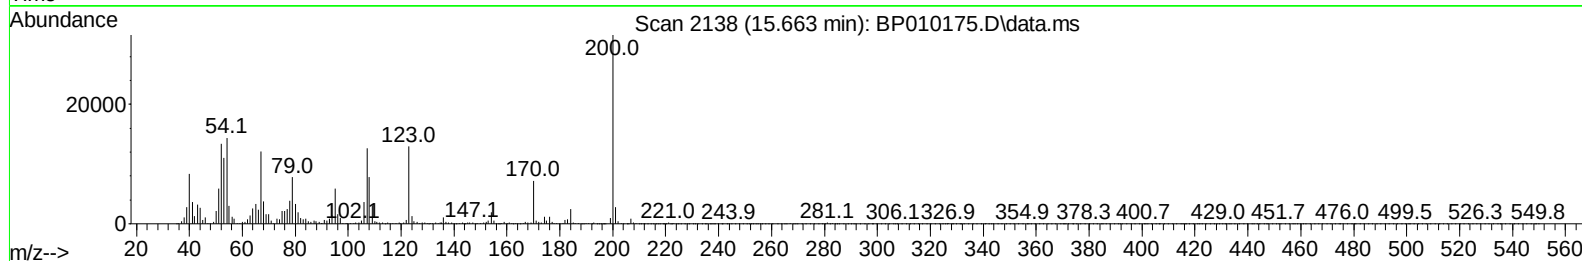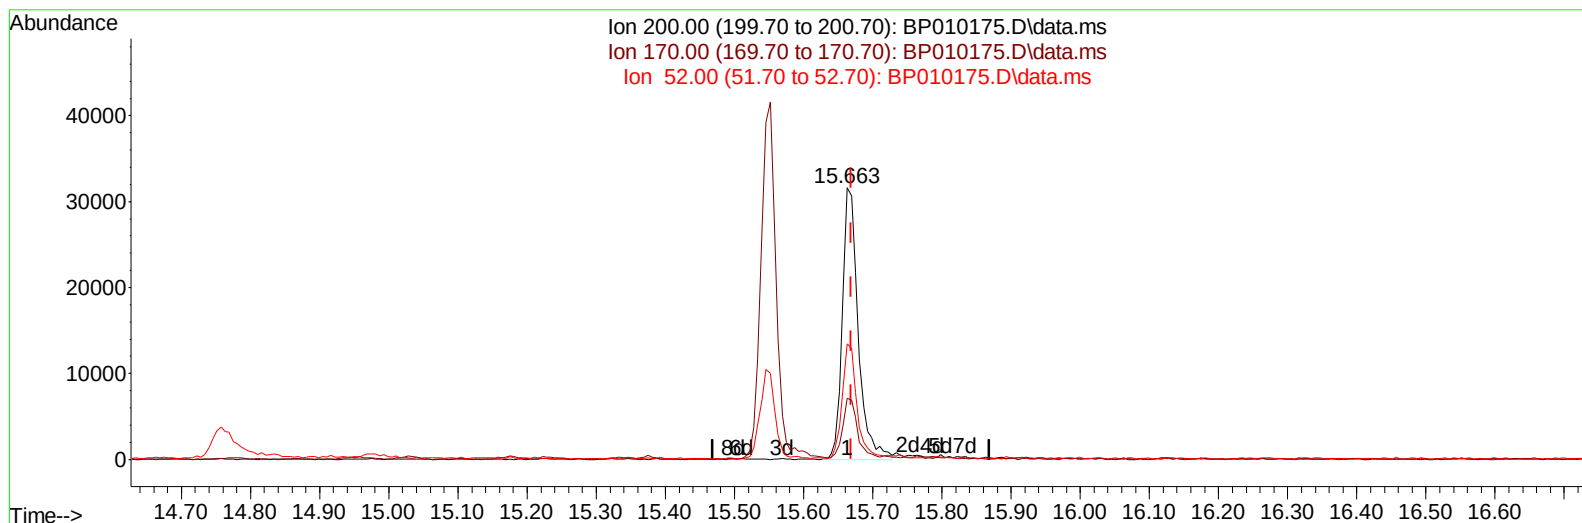

TIC: BP010175.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.663min (-0.006) 7.71 ng/ul m

response 50626

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.00	22.62
52.00	21.20	42.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010175.D
 Acq On : 02 May 2022 16:25
 Operator : CG/JU
 Sample : N2562-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW474

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:36:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	180908	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	788214	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	528762	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	1039074	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.392	240	727974	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	636193	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	10636	2.564	ng/uL	0.00
4) Pyridine-d5	3.787	84	56583	4.848	ng/ul	0.01
7) Phenol-d5	7.087	99	212710	12.927	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	148558	15.046	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	173861	14.267	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	184383	13.524	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	92613	14.773	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	100432	14.669	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	171837	12.892	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131	238620	12.486	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	635619	15.453	ng/ul	0.00
49) Acenaphthylene-d8	14.246	160	685674	13.774	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	61556	8.129	ng/ul	0.00
60) Fluorene-d10	15.551	176	538945	15.232	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	50626m	7.705	ng/ul	0.00
73) Anthracene-d10	17.404	188	830734	16.526	ng/ul	0.00
81) Pyrene-d10	19.639	212	900349	21.747	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	590601	17.708	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010175.D
Acq On : 02 May 2022 16:25
Operator : CG/JU
Sample : N2562-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW474

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:36:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

