




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010180.D
 Acq On : 02 May 2022 19:13
 Operator : CG/JU
 Sample : N2562-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

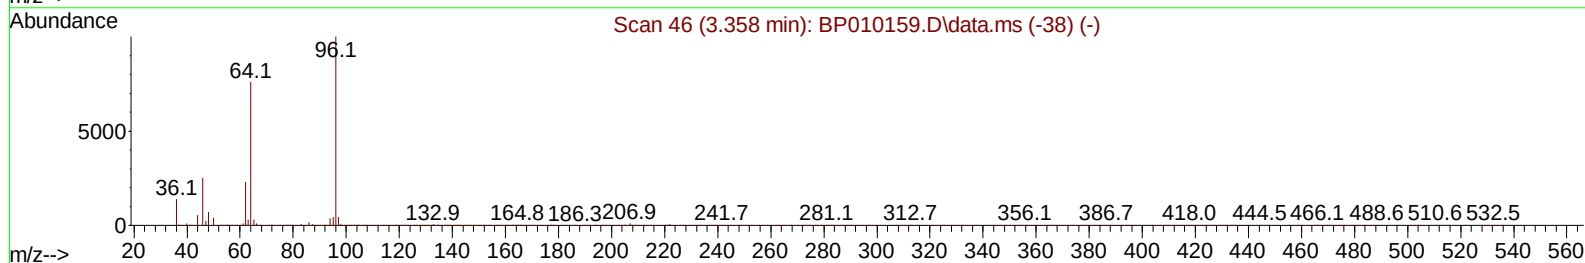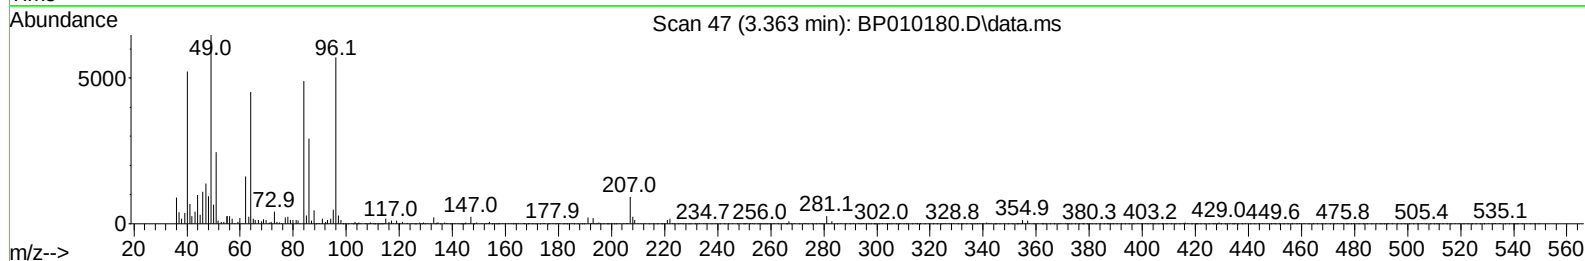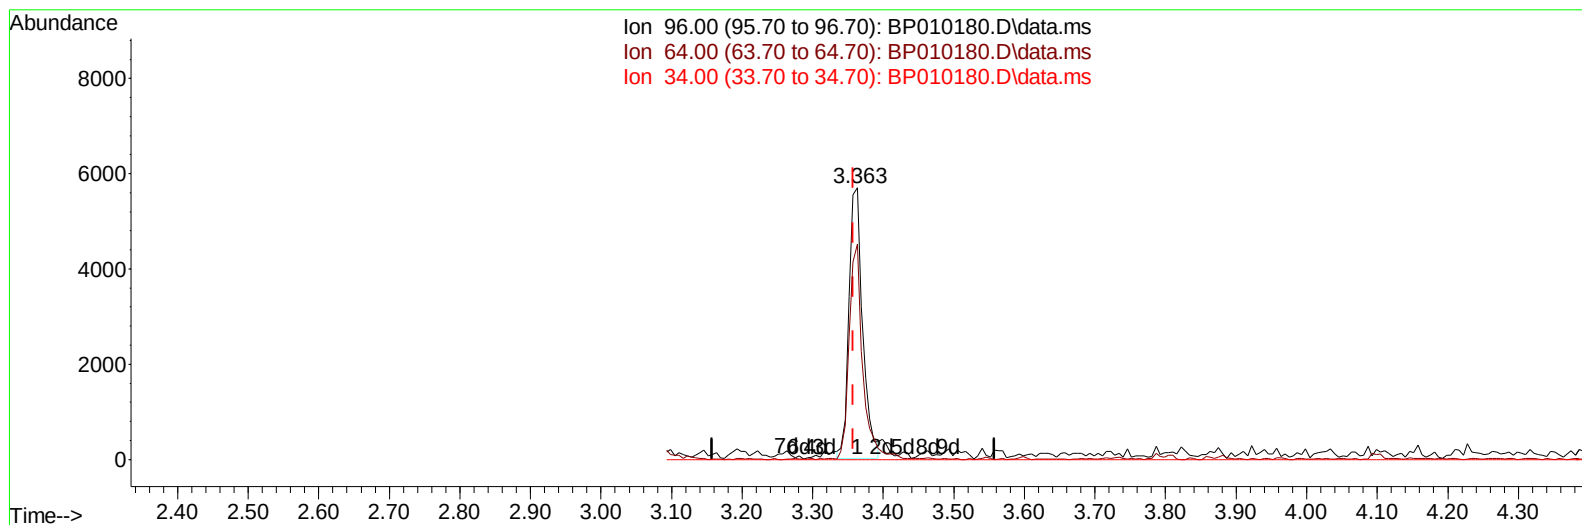

TIC: BP010180.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.363min (+ 0.005) 2.16 ng/uL

response 7783

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.37#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

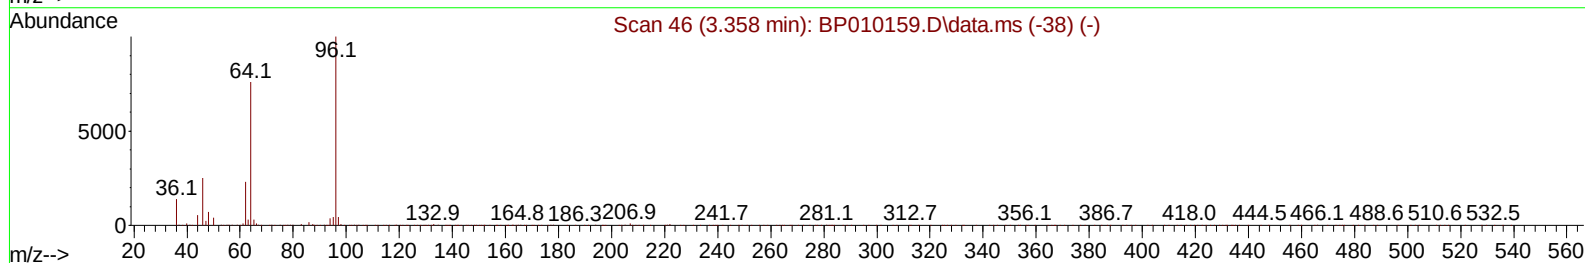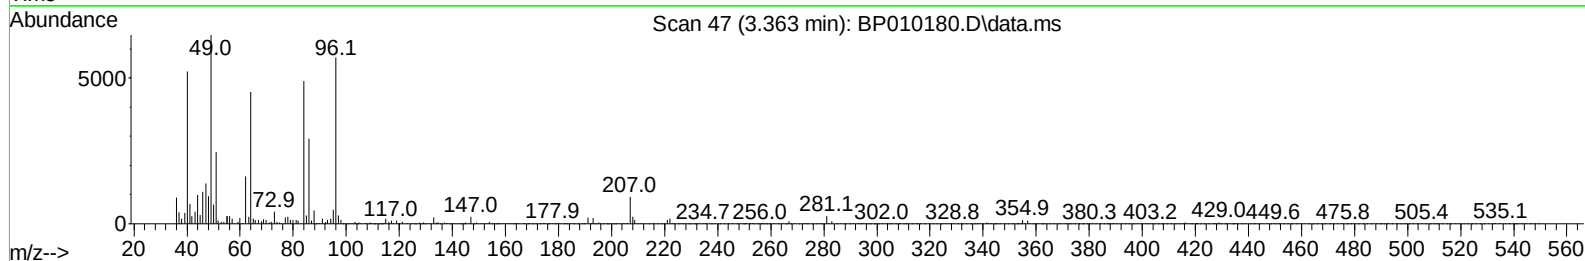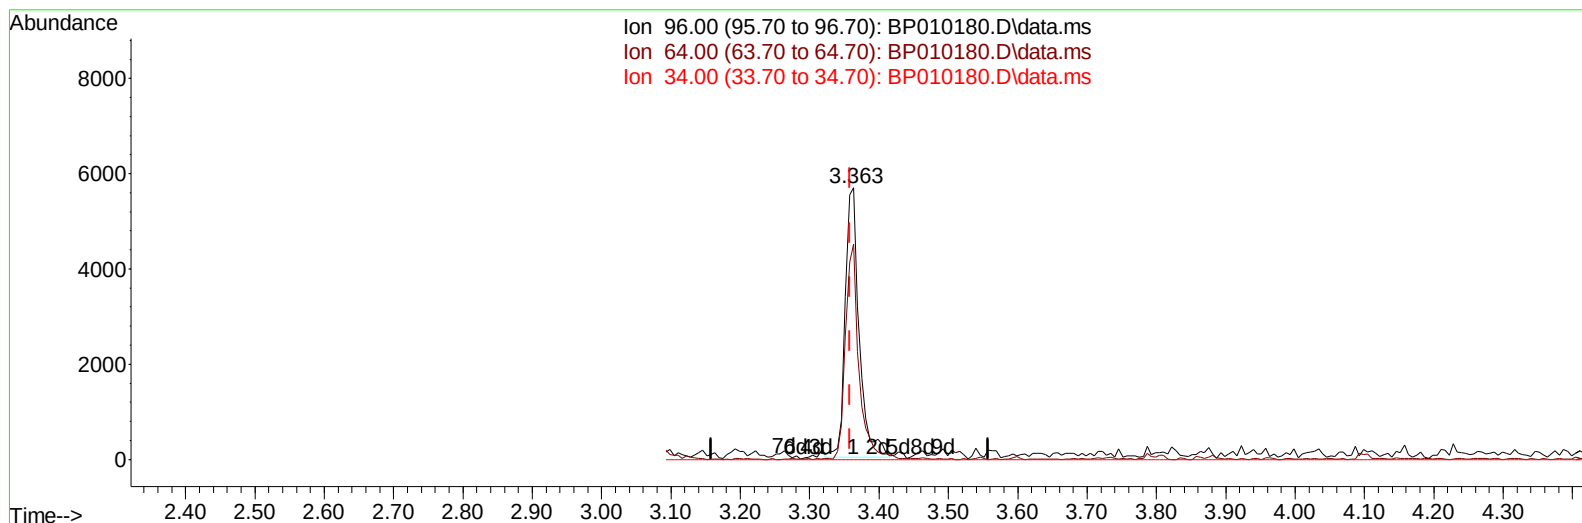

TIC: BP010180.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.363min (+ 0.005) 2.23 ng/uL m

response 8039

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.37#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010180.D
 Acq On : 02 May 2022 19:13
 Operator : CG/JU
 Sample : N2562-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

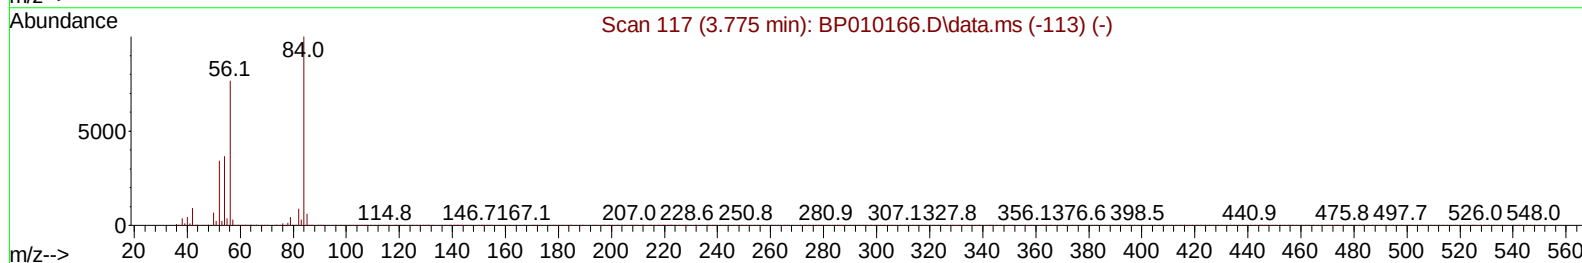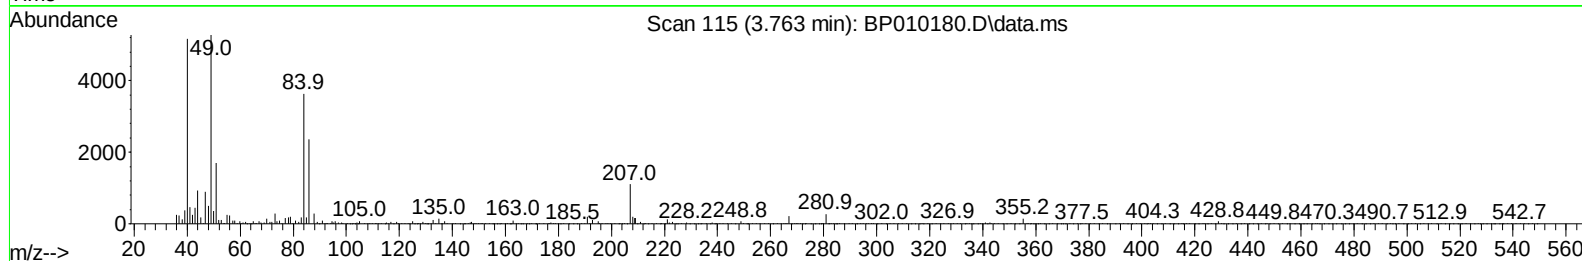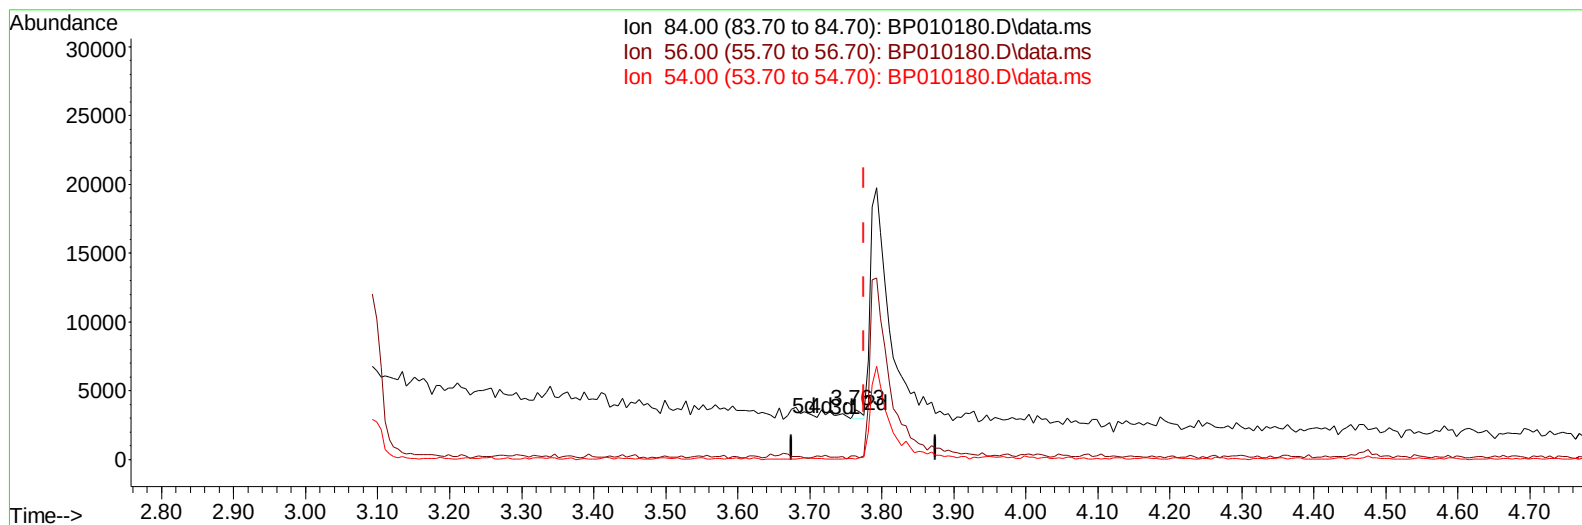

TIC: BP010180.D\data.ms

(4) Pyridine-d5 (S)

3.763min (-0.012) 0.05 ng/u1

response 515

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	6.65#
54.00	24.80	1.13#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

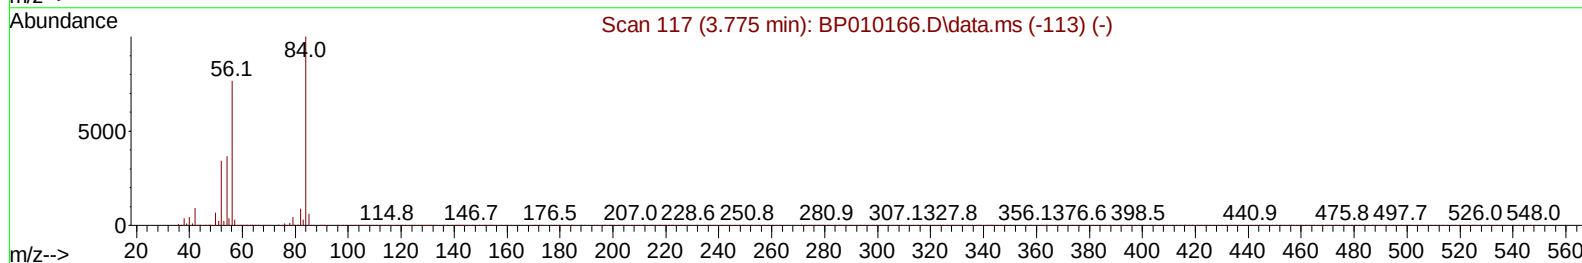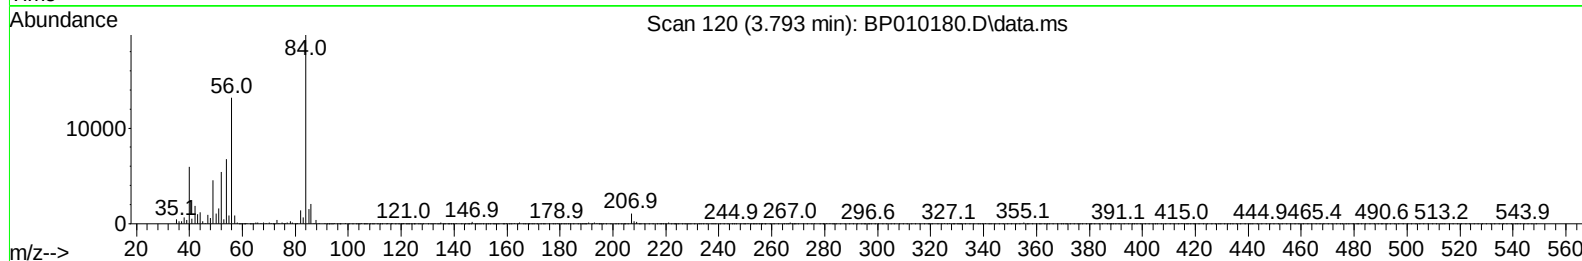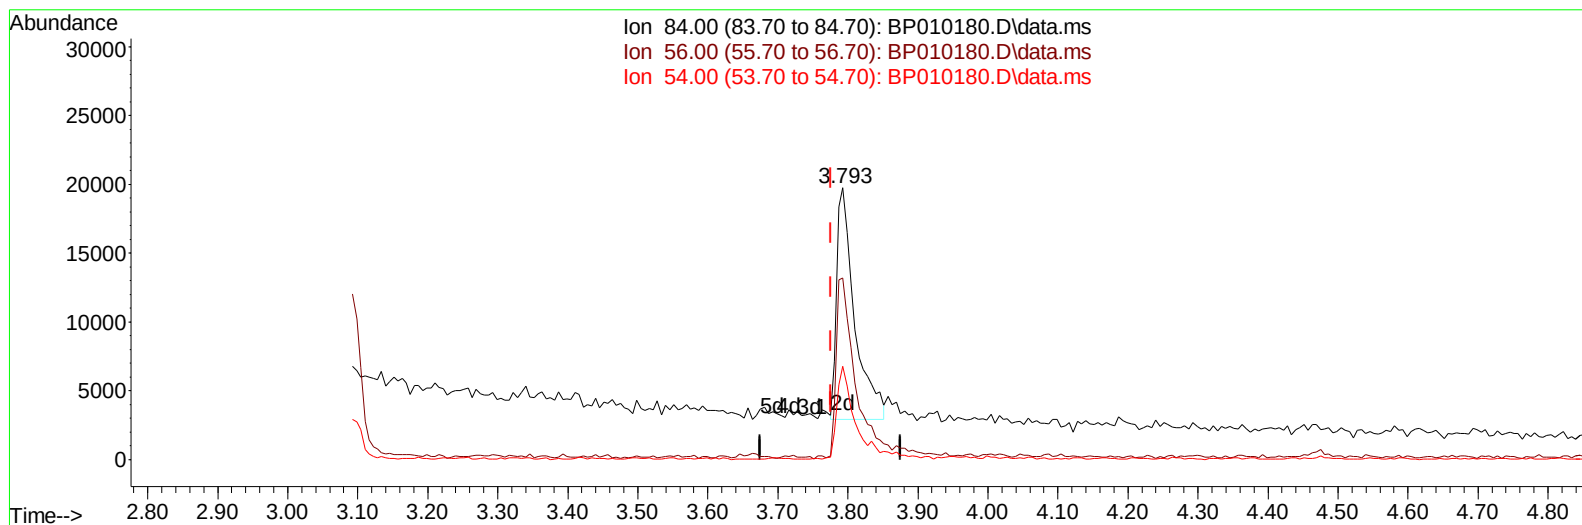

TIC: BP010180.D\data.ms

(4) Pyridine-d5 (S)

3.793min (+ 0.017) 2.96 ng/ul m

response 30028

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	66.88#
54.00	24.80	34.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

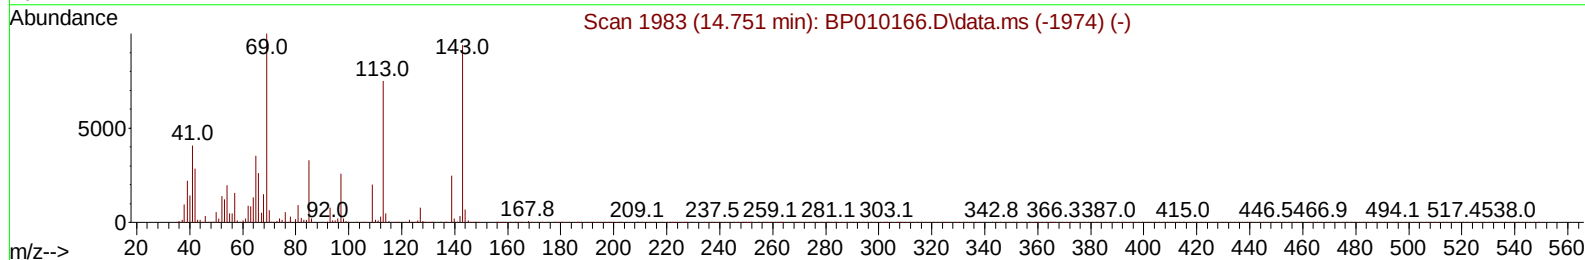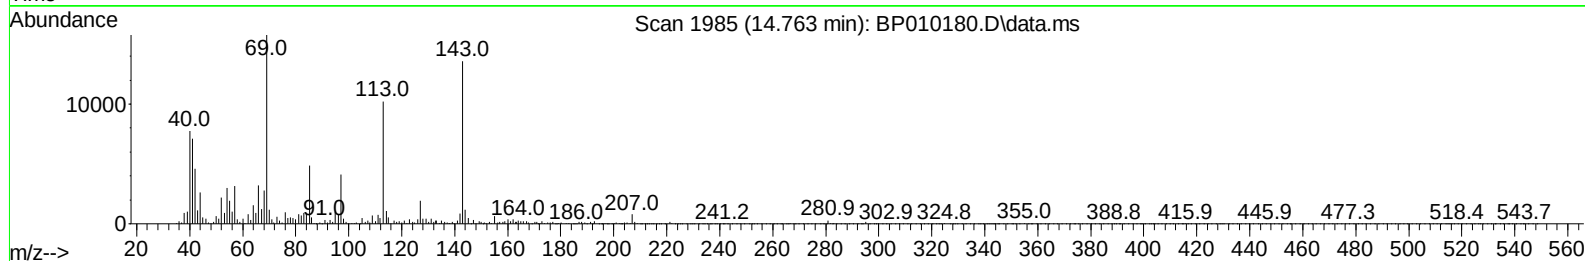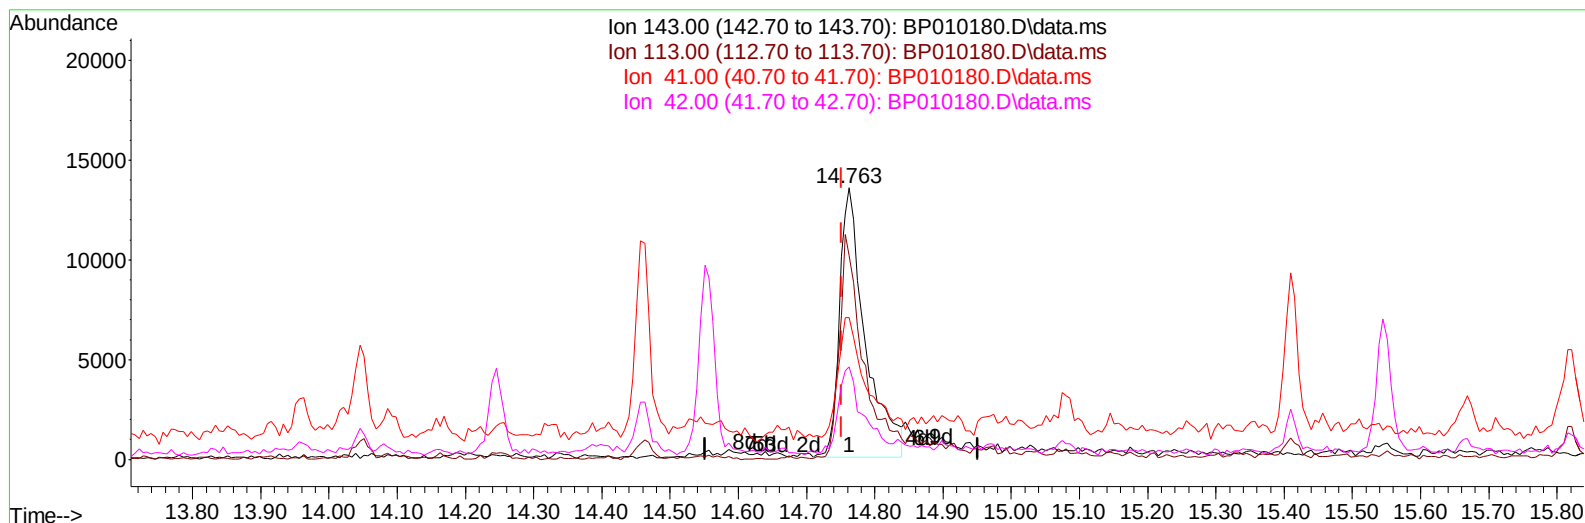

TIC: BP010180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.011) 5.51 ng/ul

response 35156

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.18#
41.00	23.20	52.25#
42.00	18.00	33.98#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

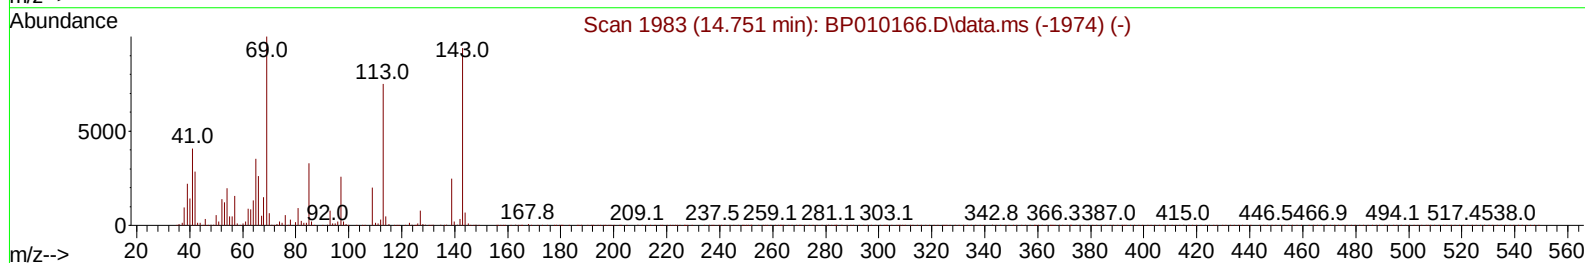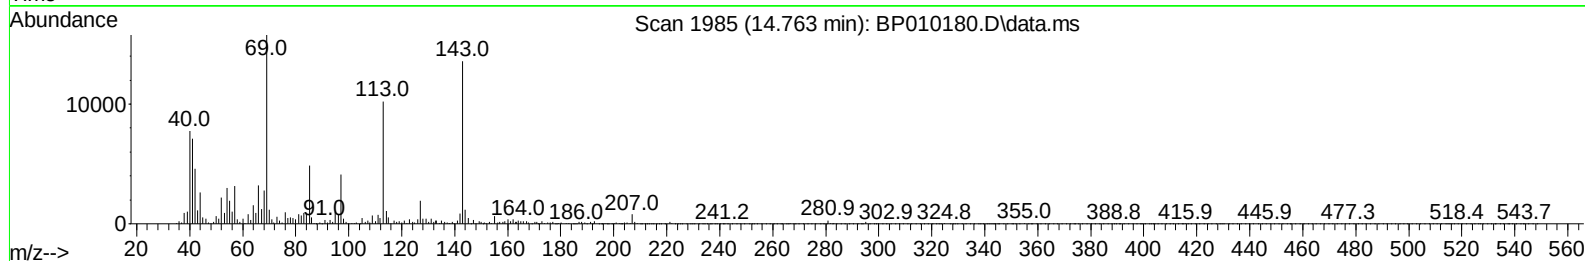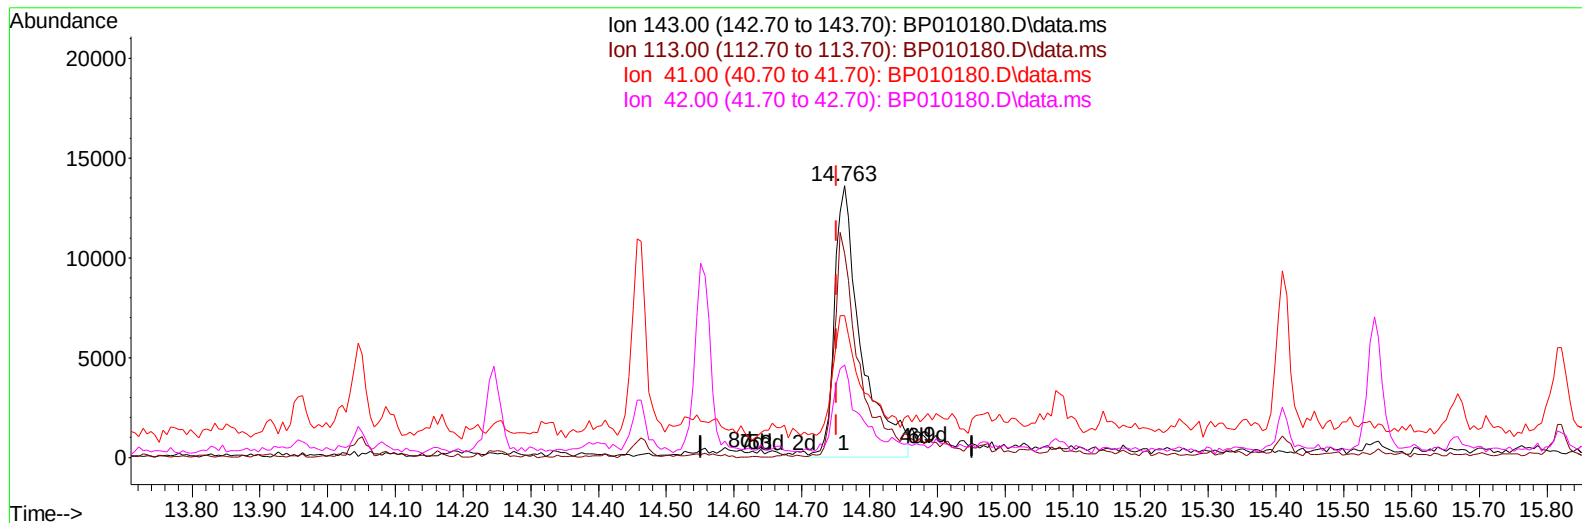

TIC: BP010180.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.011) 5.88 ng/ul m

response 37573

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	75.18#
41.00	23.20	52.25#
42.00	18.00	33.98#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010180.D
 Acq On : 02 May 2022 19:13
 Operator : CG/JU
 Sample : N2562-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW462

Manual IntegrationsAPPROVED

Quant Time: May 03 01:37:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	157335	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	683905	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	445902	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	831669	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	614149	20.000	ng/ul	# 0.00
88) Perylene-d12	23.833	264	576832	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	8039m	2.228	ng/uL	0.00
4) Pyridine-d5	3.793	84	30028m	2.958	ng/ul	0.02
7) Phenol-d5	7.087	99	149462	10.444	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.251	67	110359	12.851	ng/ul	0.00
11) 2-Chlorophenol-d4	7.457	132	126930	11.976	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	120051	10.125	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	66937	12.306	ng/ul	0.00
24) 2-Nitrophenol-d4	9.810	143	73030	12.293	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.351	165	118820	10.274	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131	157044	9.471	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	432549	12.470	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	498067	11.864	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	37573m	5.884	ng/ul	0.01
60) Fluorene-d10	15.545	176	370904	12.431	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	30289	5.760	ng/ul	0.00
73) Anthracene-d10	17.404	188	526771	13.092	ng/ul	0.00
81) Pyrene-d10	19.633	212	601521	17.222	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	444002	14.682	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:37:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

