




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010185.D
Acq On : 02 May 2022 22:35
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Manual IntegrationsAPPROVED

Quant Time: May 03 01:38:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

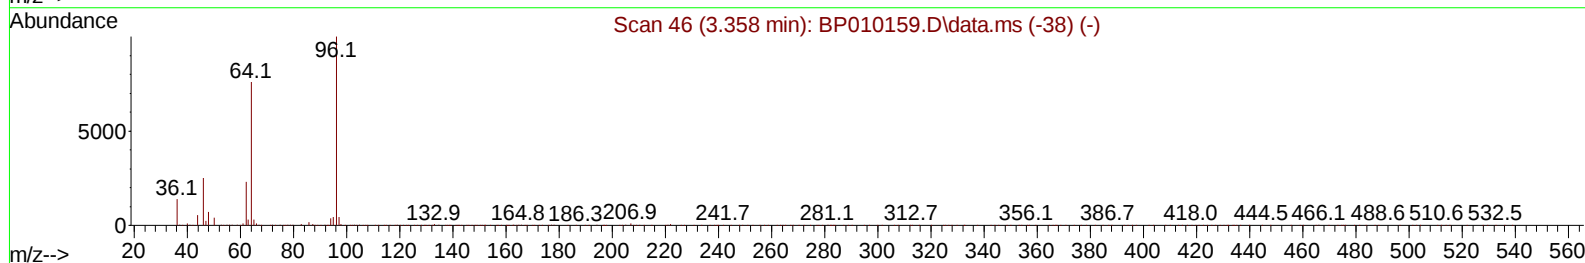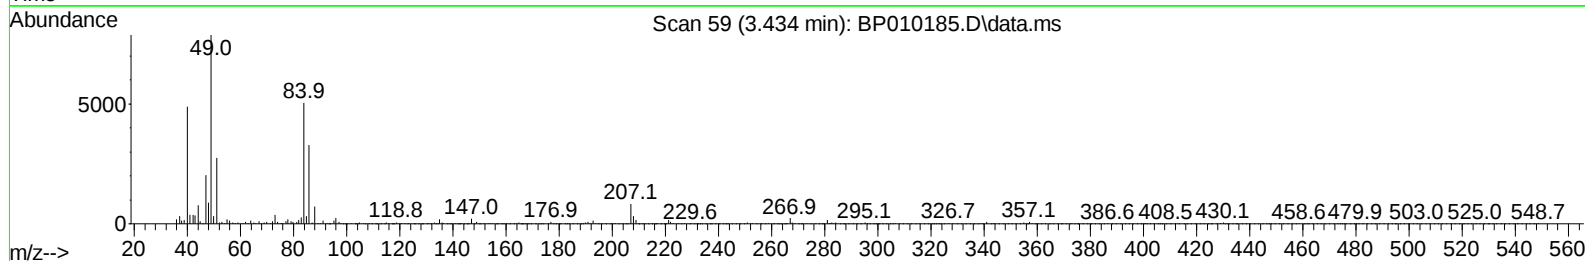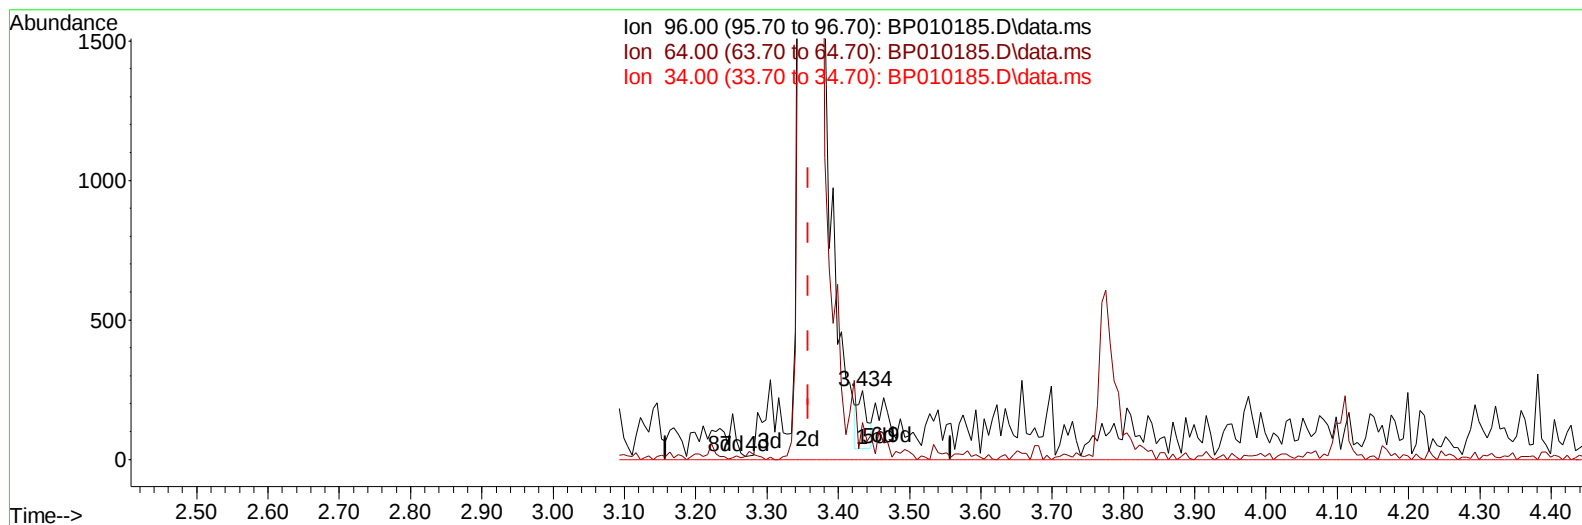

TIC: BP010185.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.434min (+ 0.076) 0.06 ng/uL

response 193

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	53.66
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010185.D
 Acq On : 02 May 2022 22:35
 Operator : CG/JU
 Sample : PB144528BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK528

Manual IntegrationsAPPROVED

Quant Time: May 03 01:38:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

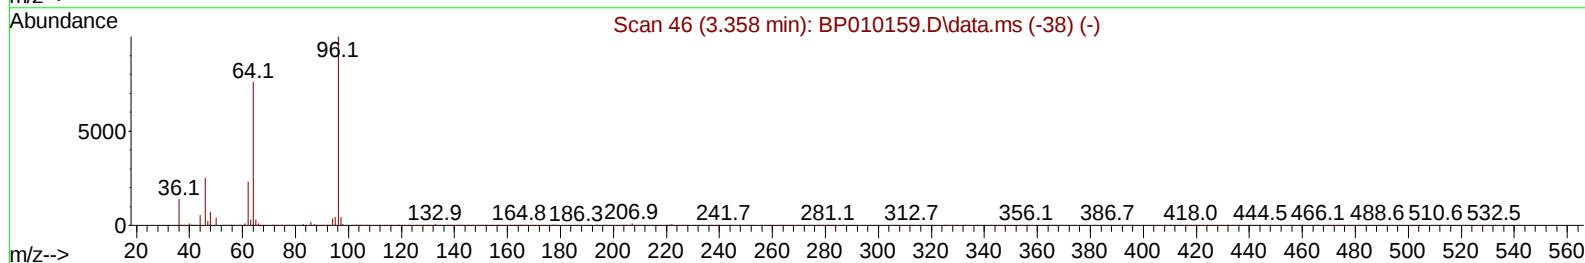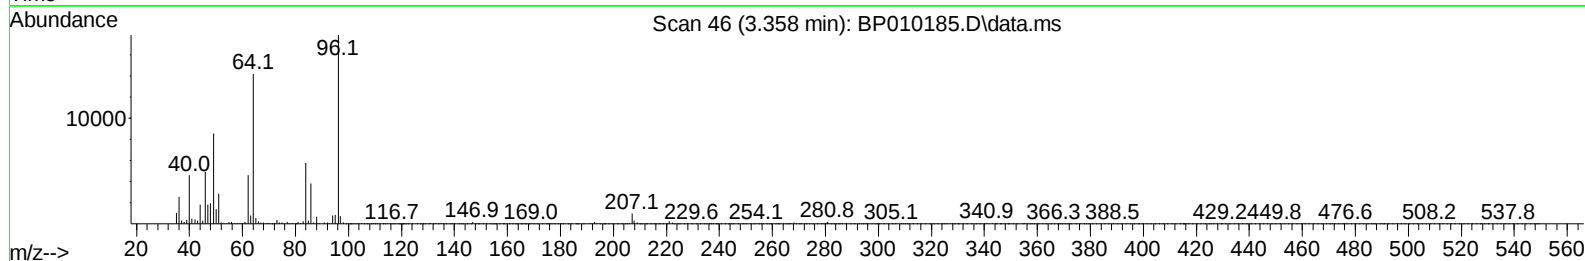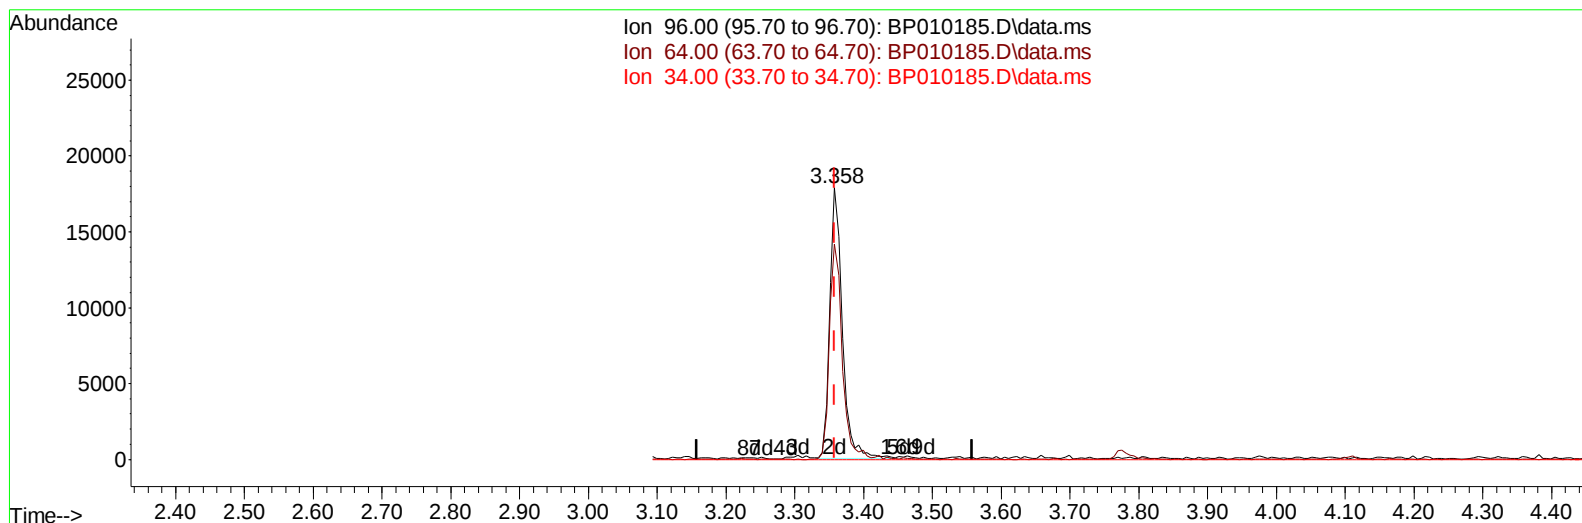

TIC: BP010185.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 6.74 ng/uL m

response 22819

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.38#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010185.D
Acq On : 02 May 2022 22:35
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:38:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

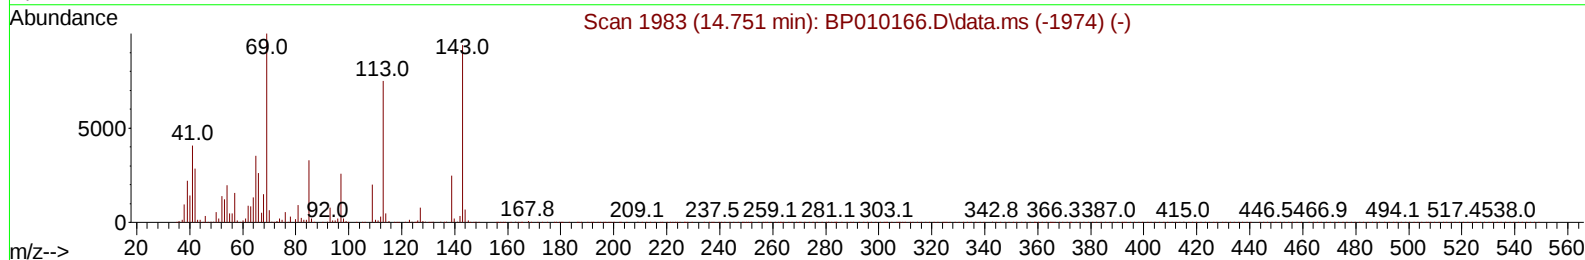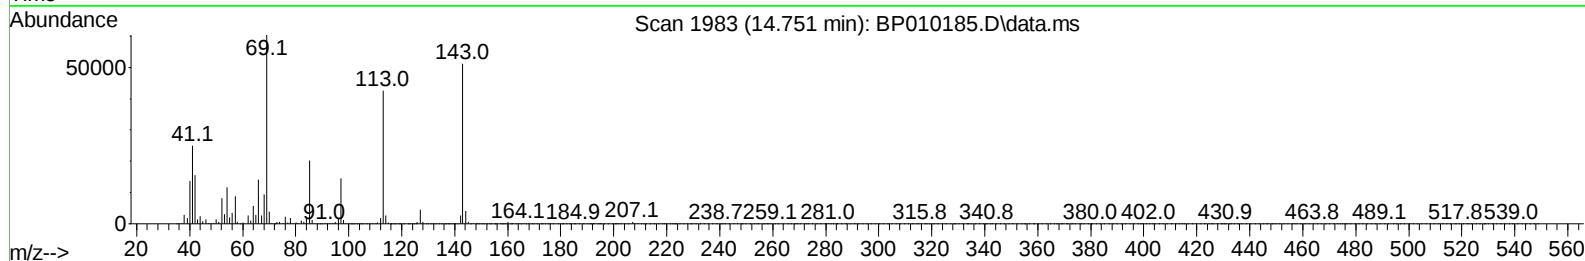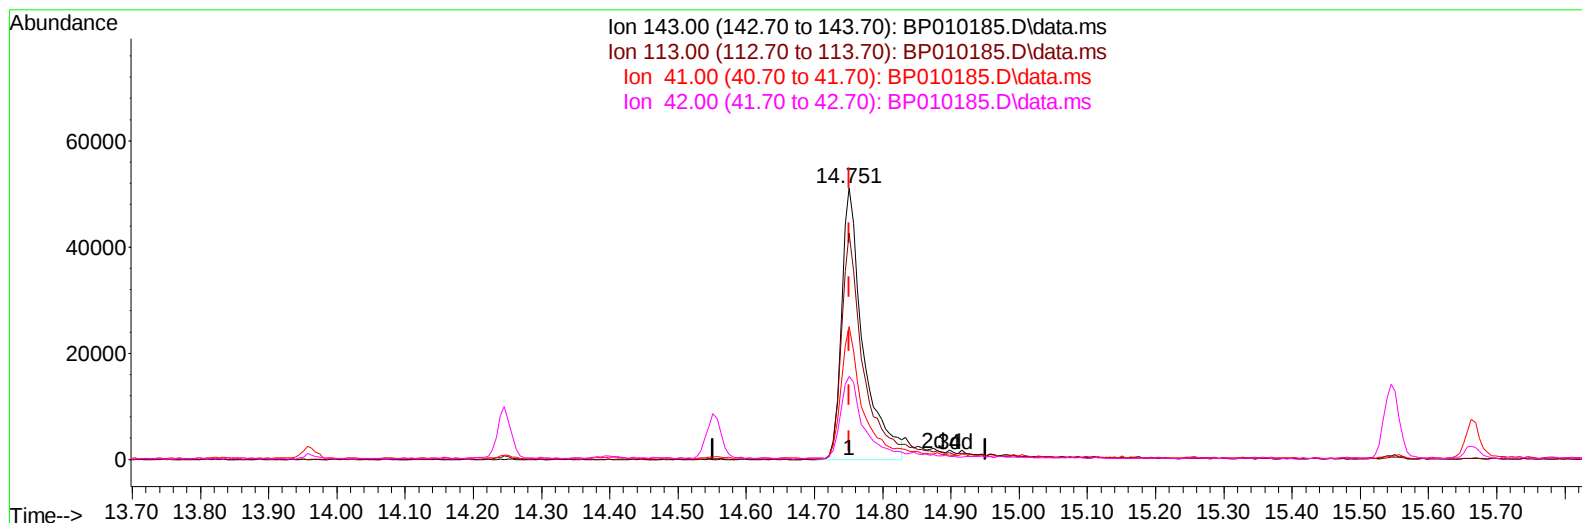

TIC: BP010185.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.000) 21.49 ng/u1

response 111668

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.40#
41.00	23.20	48.98#
42.00	18.00	30.54#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010185.D
Acq On : 02 May 2022 22:35
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:38:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

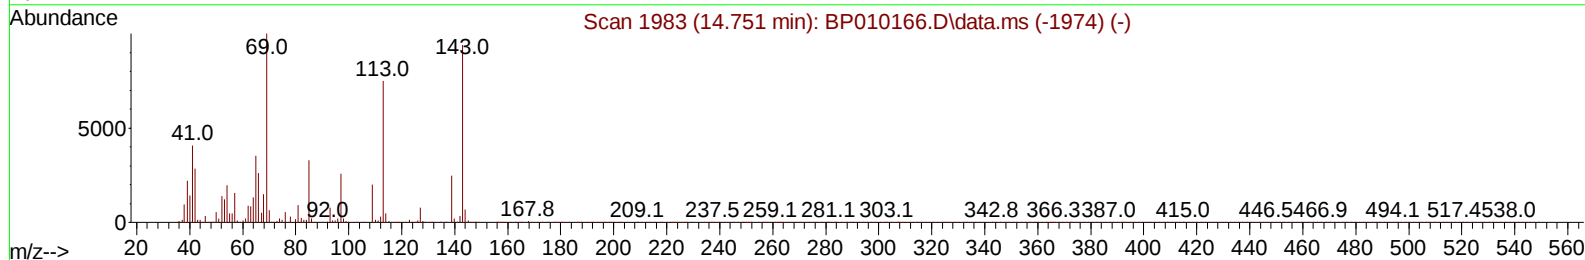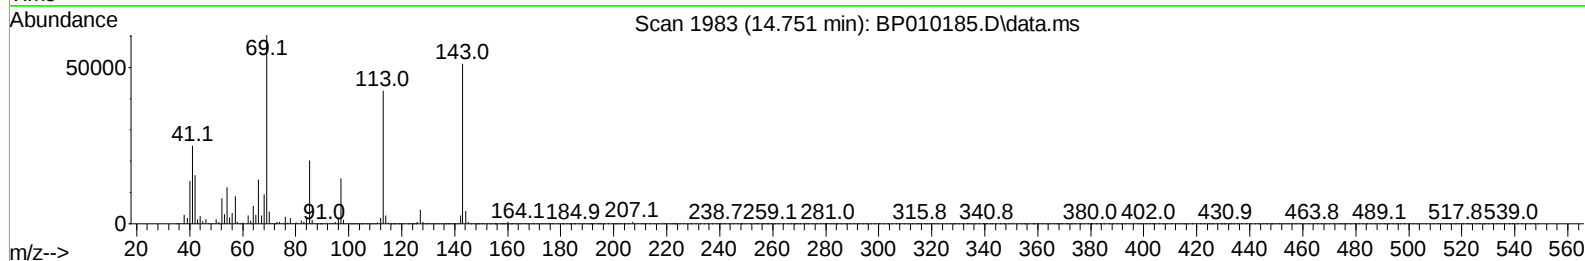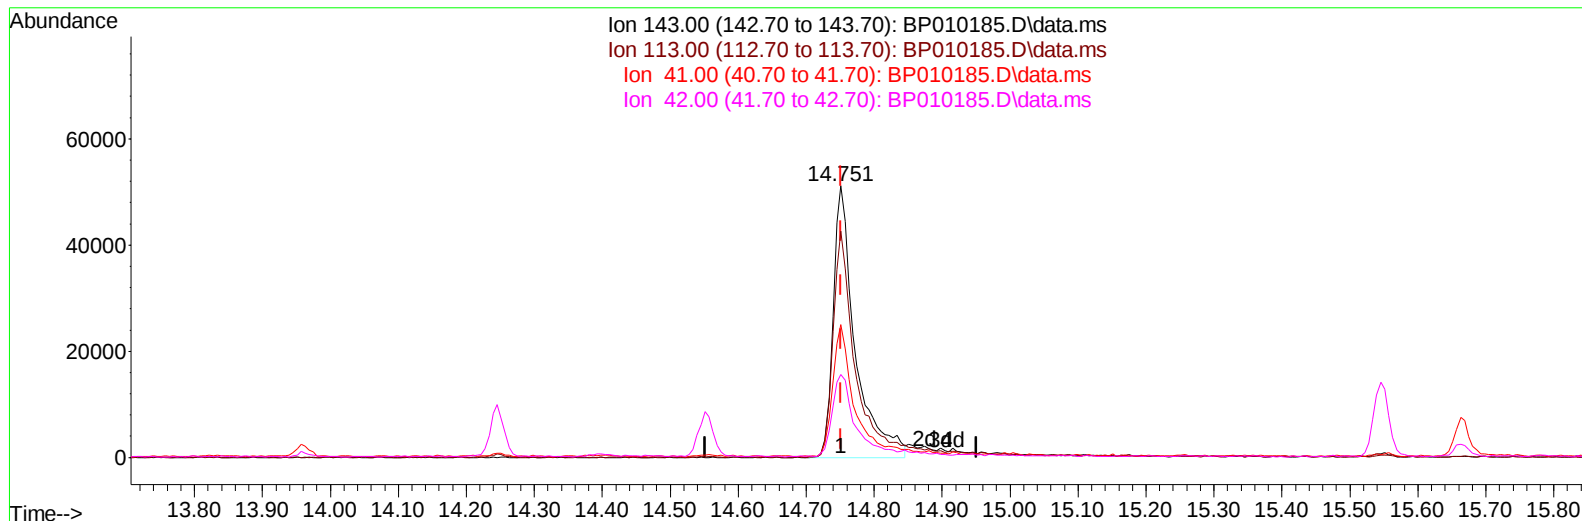

TIC: BP010185.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.000) 22.11 ng/ul m

response 114888

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.40#
41.00	23.20	48.98#
42.00	18.00	30.54#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010185.D
 Acq On : 02 May 2022 22:35
 Operator : CG/JU
 Sample : PB144528BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK528

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:38:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	147675	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	597680	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	362870	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	685547	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	626635	20.000	ng/ul	# 0.00
88) Perylene-d12	23.833	264	615599	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	22819m	6.738	ng/uL	0.00
4) Pyridine-d5	3.775	84	305375	32.054	ng/ul	0.00
7) Phenol-d5	7.087	99	379128	28.225	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	268181	33.273	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	315570	31.722	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	319013	28.665	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	162519	34.188	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	178559	34.394	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	290389	28.732	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	423851	29.248	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	936542	33.179	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1088798	31.871	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	114888m	22.109	ng/ul	0.00
60) Fluorene-d10	15.545	176	781013	32.165	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	116878	26.963	ng/ul	0.00
73) Anthracene-d10	17.404	188	1133698	34.182	ng/ul	0.00
81) Pyrene-d10	19.633	212	1302926	36.561	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	1172728	36.338	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010185.D
Acq On : 02 May 2022 22:35
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:38:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

