




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010187.D
 Acq On : 02 May 2022 23:43
 Operator : CG/JU
 Sample : N2615-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A6

Manual IntegrationsAPPROVED

Quant Time: May 03 01:39:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

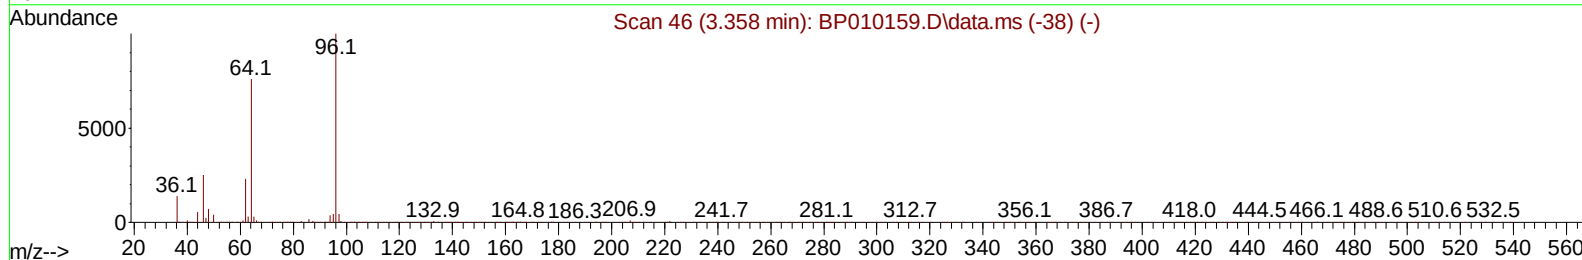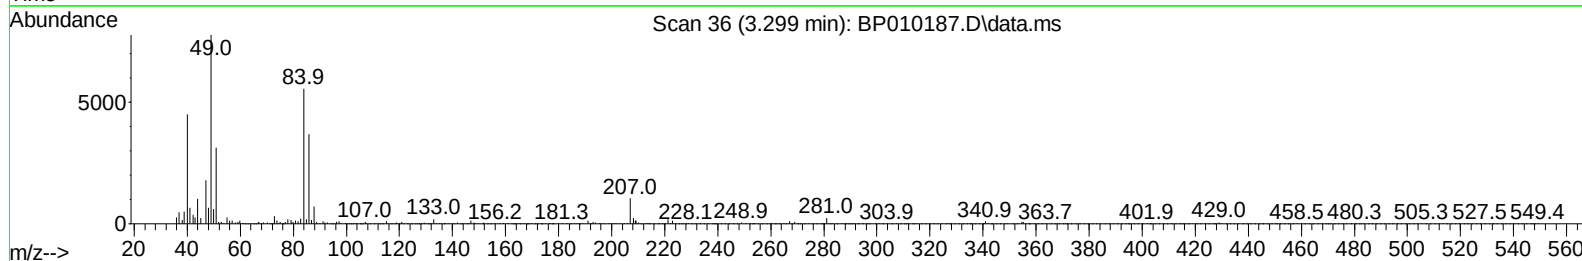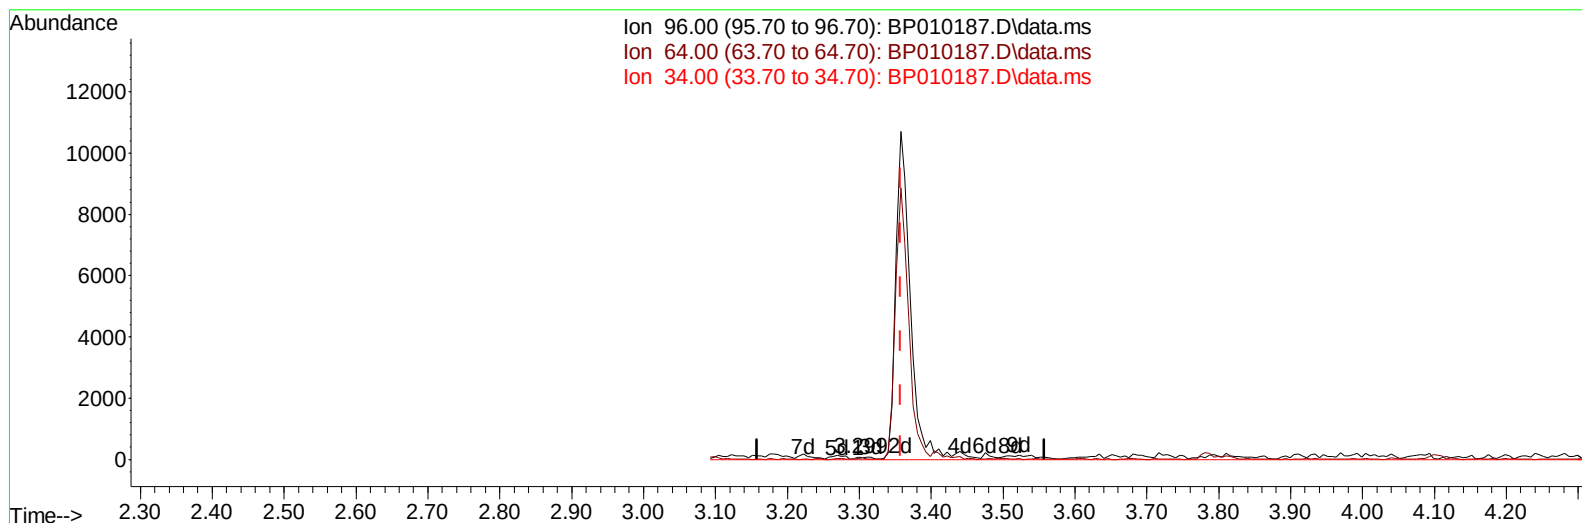

TIC: BP010187.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.299min (-0.059) 0.01 ng/uL

response 47

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	58.21
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010187.D
 Acq On : 02 May 2022 23:43
 Operator : CG/JU
 Sample : N2615-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A6

Manual IntegrationsAPPROVED

Quant Time: May 03 01:39:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

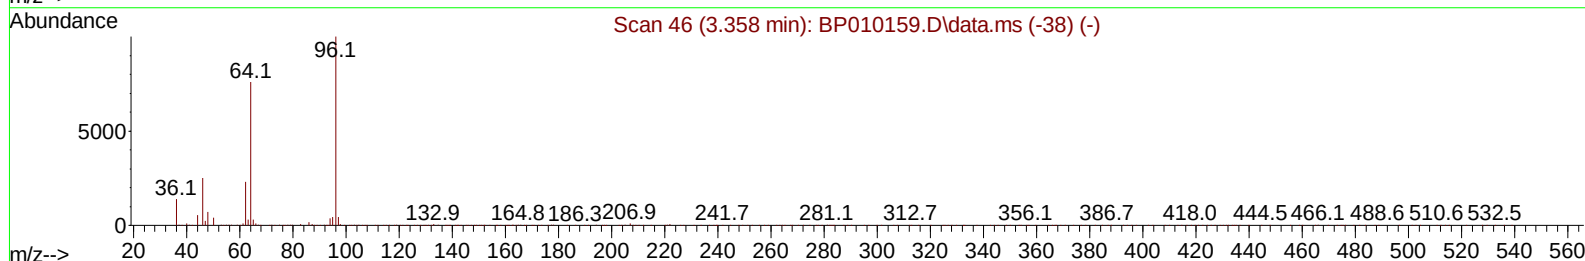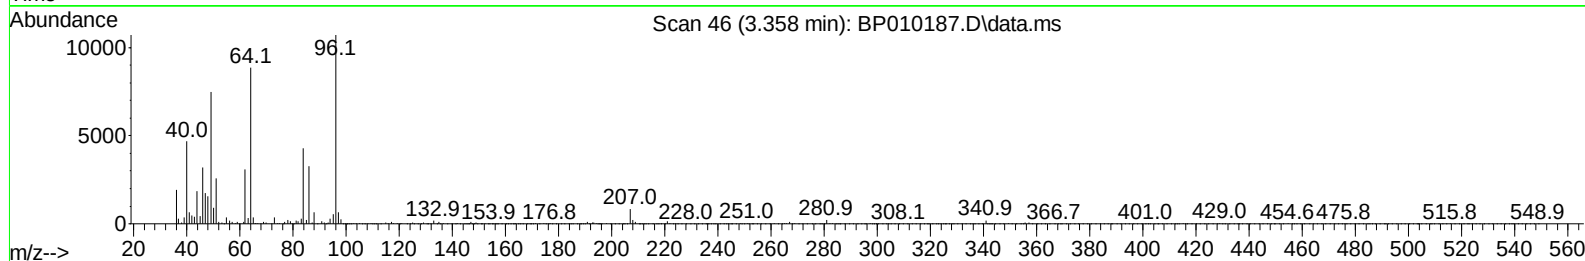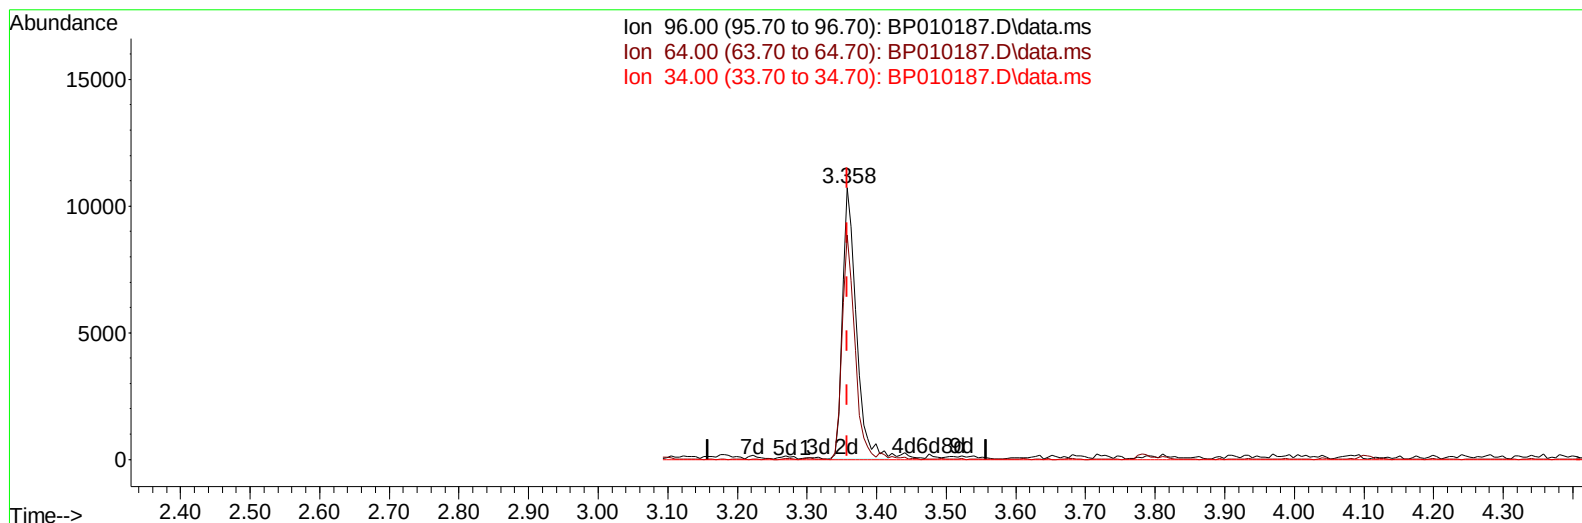

TIC: BP010187.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 3.90 ng/uL m

response 14804

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	82.70#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010187.D
Acq On : 02 May 2022 23:43
Operator : CG/JU
Sample : N2615-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:39:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

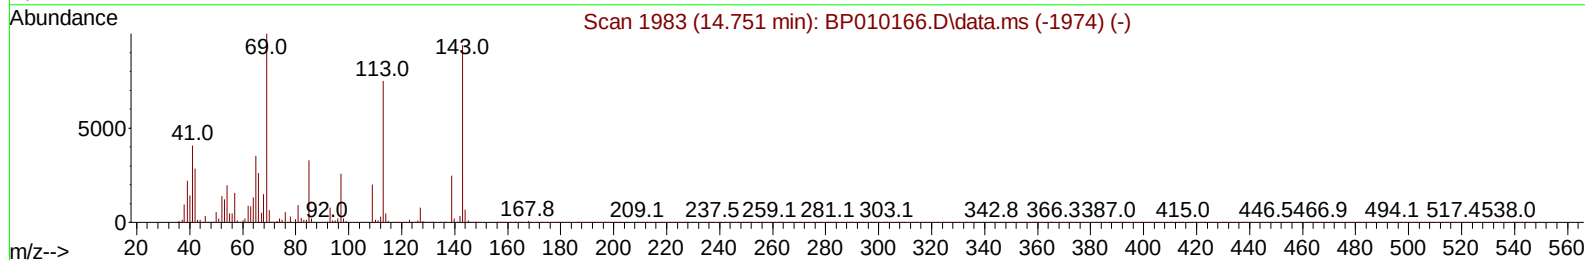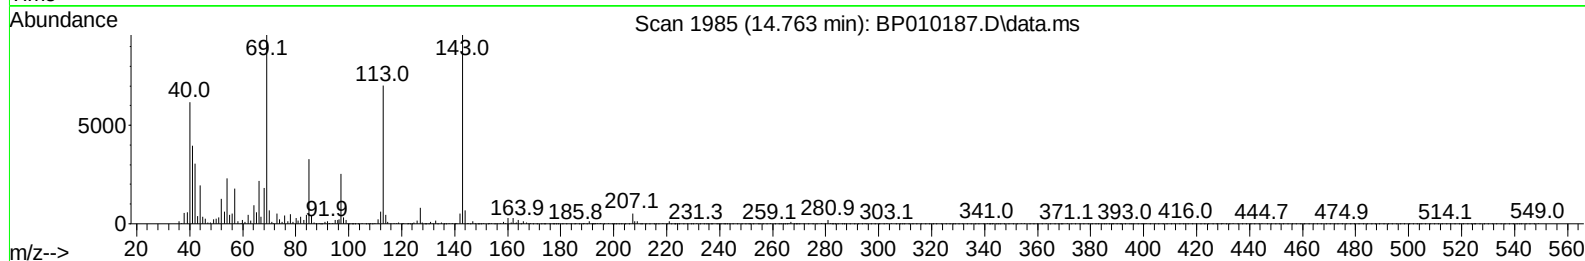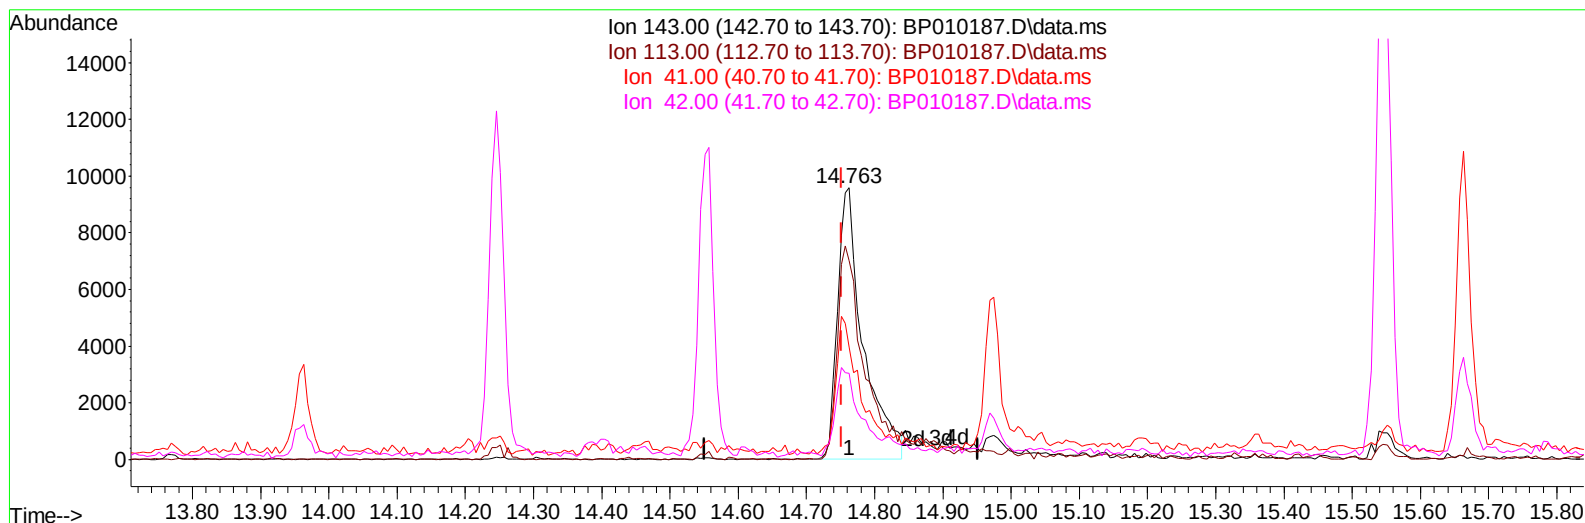

TIC: BP010187.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.012) 3.66 ng/ul

response 24914

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	73.13#
41.00	23.20	41.45#
42.00	18.00	31.82#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010187.D
Acq On : 02 May 2022 23:43
Operator : CG/JU
Sample : N2615-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:39:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

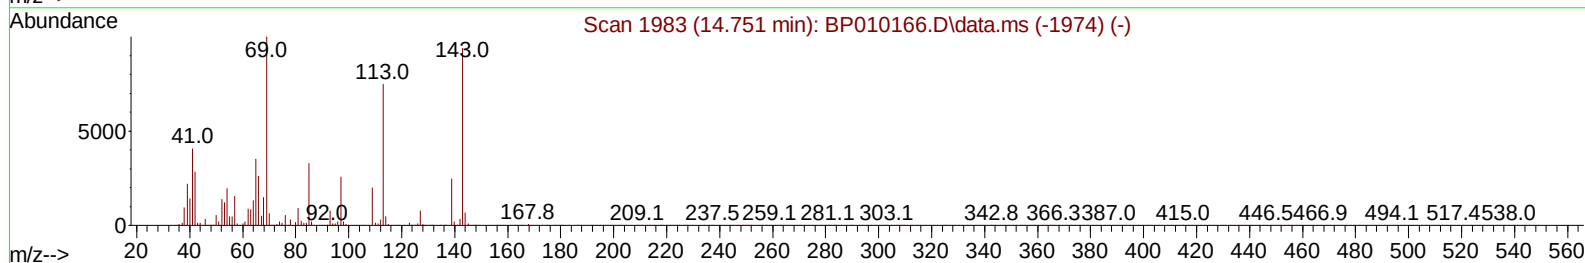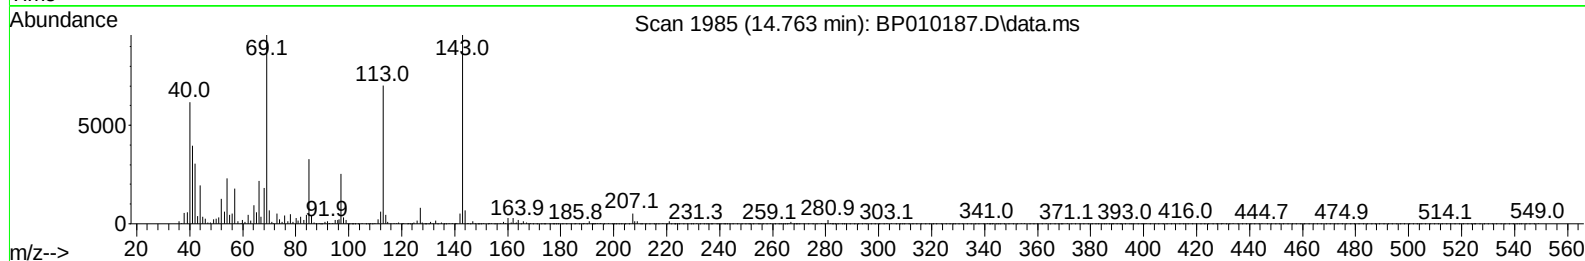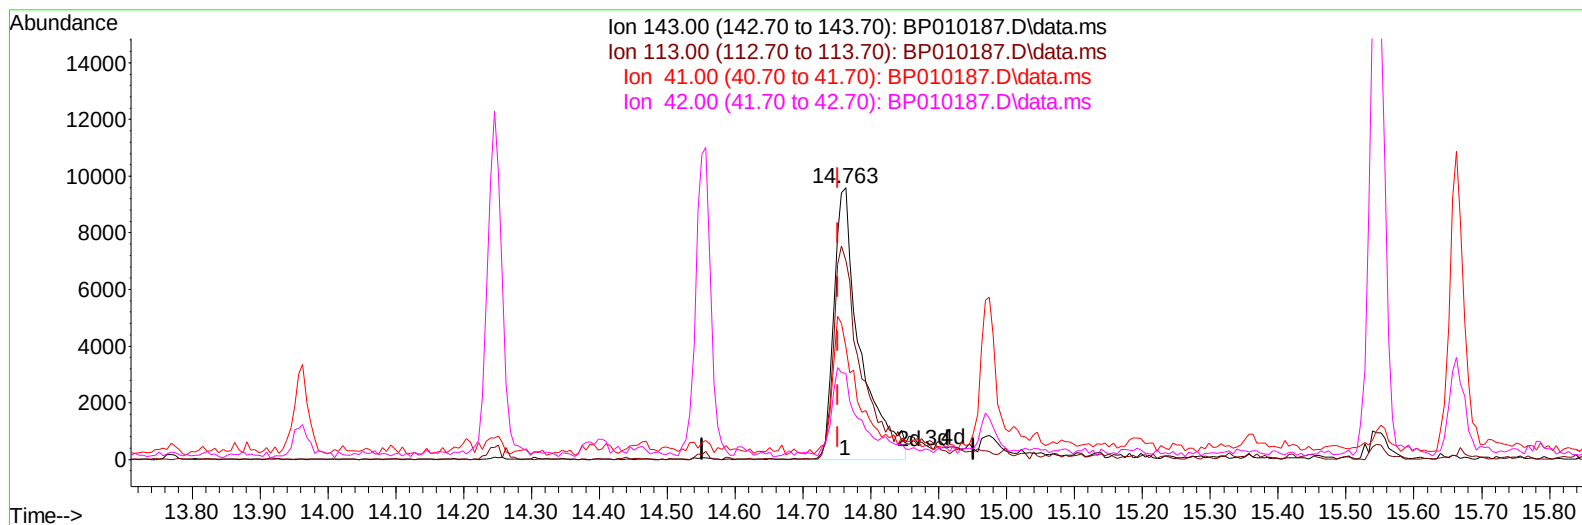

TIC: BP010187.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.012) 3.75 ng/ul m

response 25560

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	73.13#
41.00	23.20	41.45#
42.00	18.00	31.82#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010187.D
 Acq On : 02 May 2022 23:43
 Operator : CG/JU
 Sample : N2615-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A6

Manual IntegrationsAPPROVED

Quant Time: May 03 01:39:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	165355	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	714427	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	475341	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	899147	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	669066	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	601060	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	14804m	3.904	ng/uL	0.00
4) Pyridine-d5	3.781	84	77587	7.273	ng/ul	0.00
7) Phenol-d5	7.087	99	74012	4.921	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	275064	30.478	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	240294	21.573	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	158269	12.701	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	171851	30.244	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	181857	29.305	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	293876	24.326	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	384146	22.177	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	1191358	32.220	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1327318	29.660	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	25560m	3.755	ng/ul	0.01
60) Fluorene-d10	15.545	176	1005443	31.611	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	169737	29.855	ng/ul	0.00
73) Anthracene-d10	17.404	188	1597256	36.719	ng/ul	0.00
81) Pyrene-d10	19.633	212	1652529	43.430	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	1277364	40.537	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.393	88	4597	1.167	ng/ul#	40

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010187.D
Acq On : 02 May 2022 23:43
Operator : CG/JU
Sample : N2615-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:39:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

