




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010190.D
Acq On : 03 May 2022 01:23
Operator : CG/JU
Sample : N2615-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 02:53:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

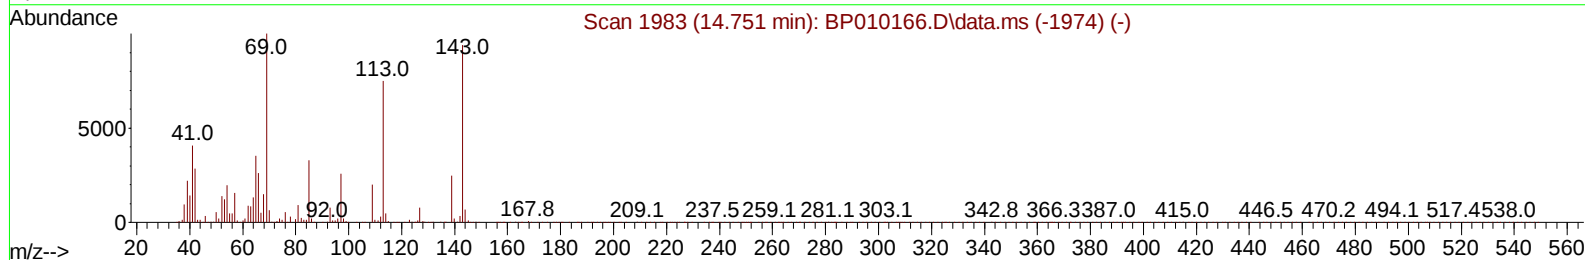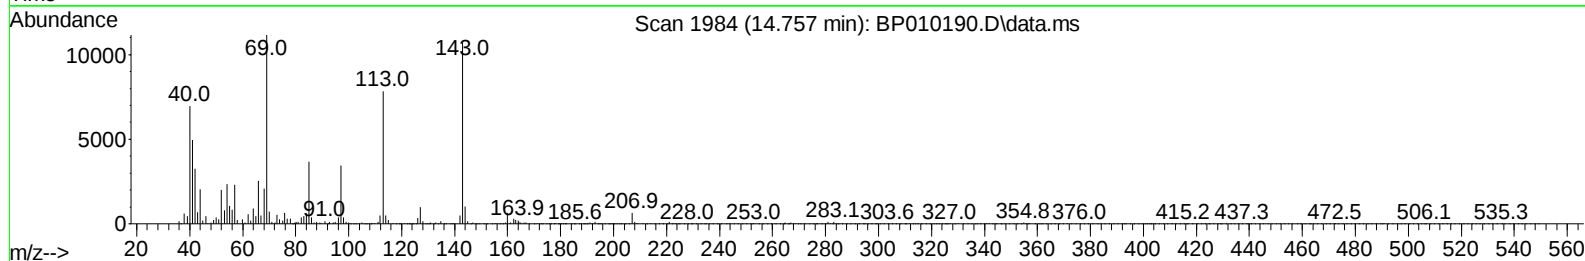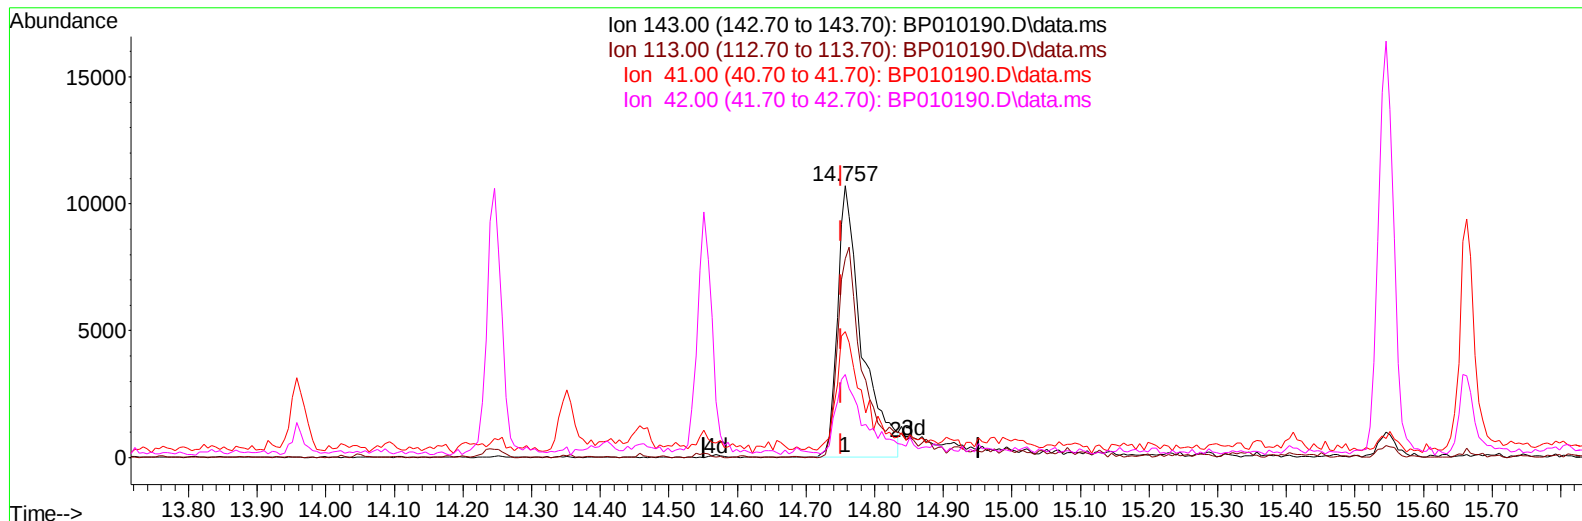

TIC: BP010190.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 4.59 ng/u1

response 26439

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	73.21#
41.00	23.20	46.28#
42.00	18.00	30.46#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010190.D
Acq On : 03 May 2022 01:23
Operator : CG/JU
Sample : N2615-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A8

Manual IntegrationsAPPROVED

Quant Time: May 03 02:53:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

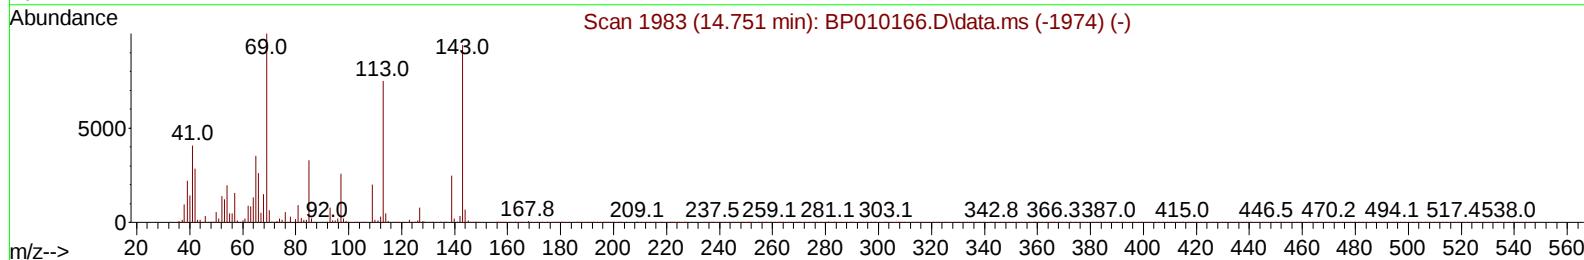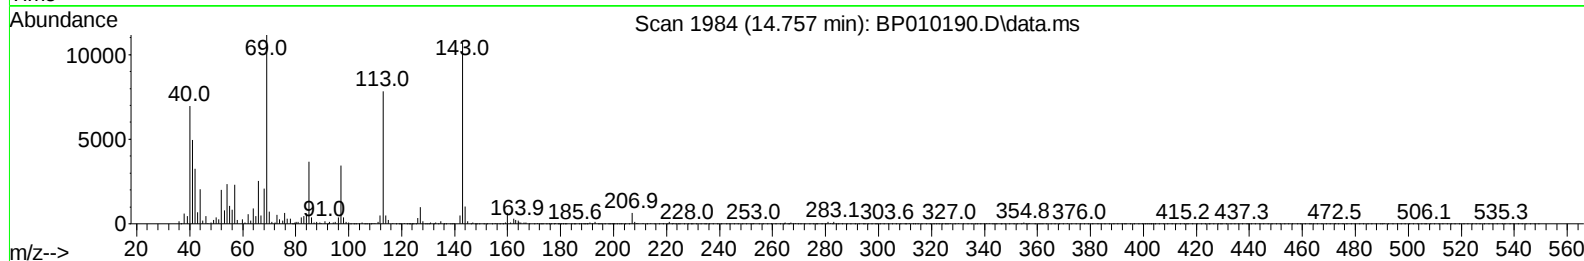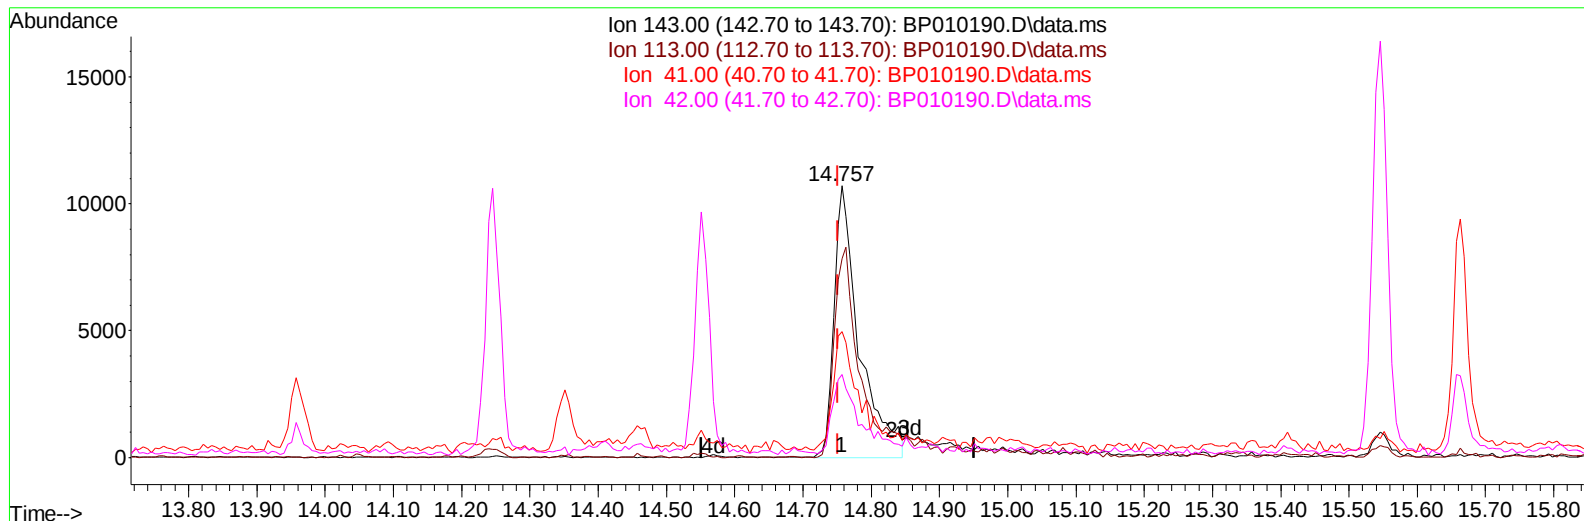

TIC: BP010190.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 4.73 ng/ul m

response 27245

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	73.21#
41.00	23.20	46.28#
42.00	18.00	30.46#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010190.D
 Acq On : 03 May 2022 01:23
 Operator : CG/JU
 Sample : N2615-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A8

Manual IntegrationsAPPROVED

Quant Time: May 03 02:53:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	157647	20.000	ng/ul	0.00
20) Naphthalene-d8	10.728	136	663504	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	402128	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	754572	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	649444	20.000	ng/ul	# 0.00
88) Perylene-d12	23.827	264	651457	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	16366	4.527	ng/uL	0.00
4) Pyridine-d5	3.781	84	95354	9.376	ng/ul	0.00
7) Phenol-d5	7.087	99	87188	6.080	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	278727	32.394	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	258321	24.325	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	175259	14.752	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	171637	32.525	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	180540	31.325	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	282337	25.164	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131	380817	23.672	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	1095390	35.018	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1179716	31.161	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	27245m	4.731	ng/ul	0.00
60) Fluorene-d10	15.545	176	891590	33.135	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	145119	30.415	ng/ul	0.00
73) Anthracene-d10	17.404	188	1375966	37.692	ng/ul	0.00
81) Pyrene-d10	19.633	212	1541181	41.728	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1340486	39.249	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010190.D
Acq On : 03 May 2022 01:23
Operator : CG/JU
Sample : N2615-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 02:53:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

