




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010194.D
 Acq On : 03 May 2022 03:38
 Operator : CG/JU
 Sample : N2615-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 03 05:26:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

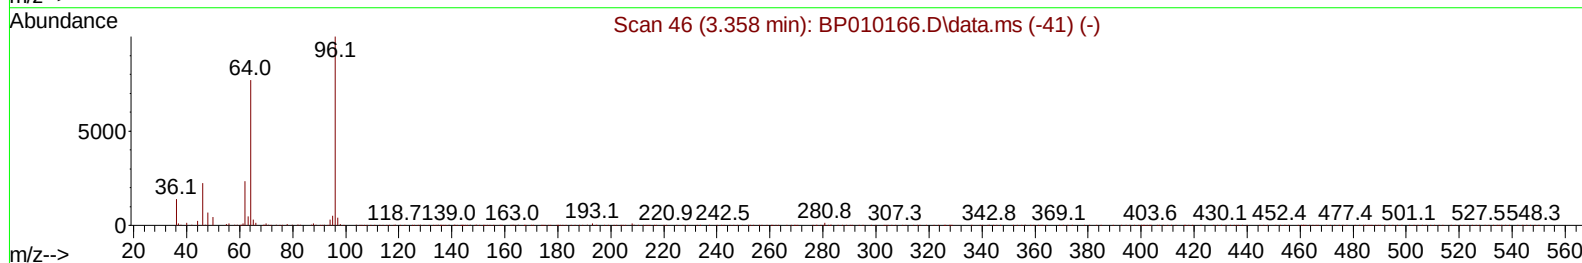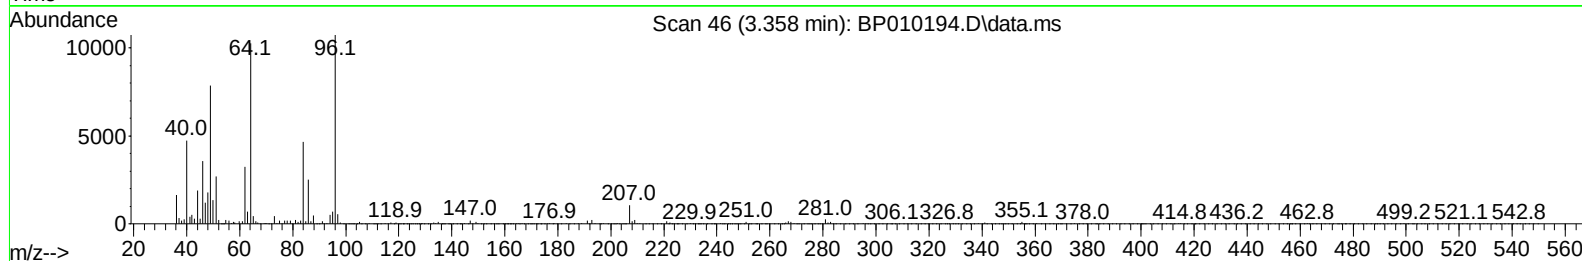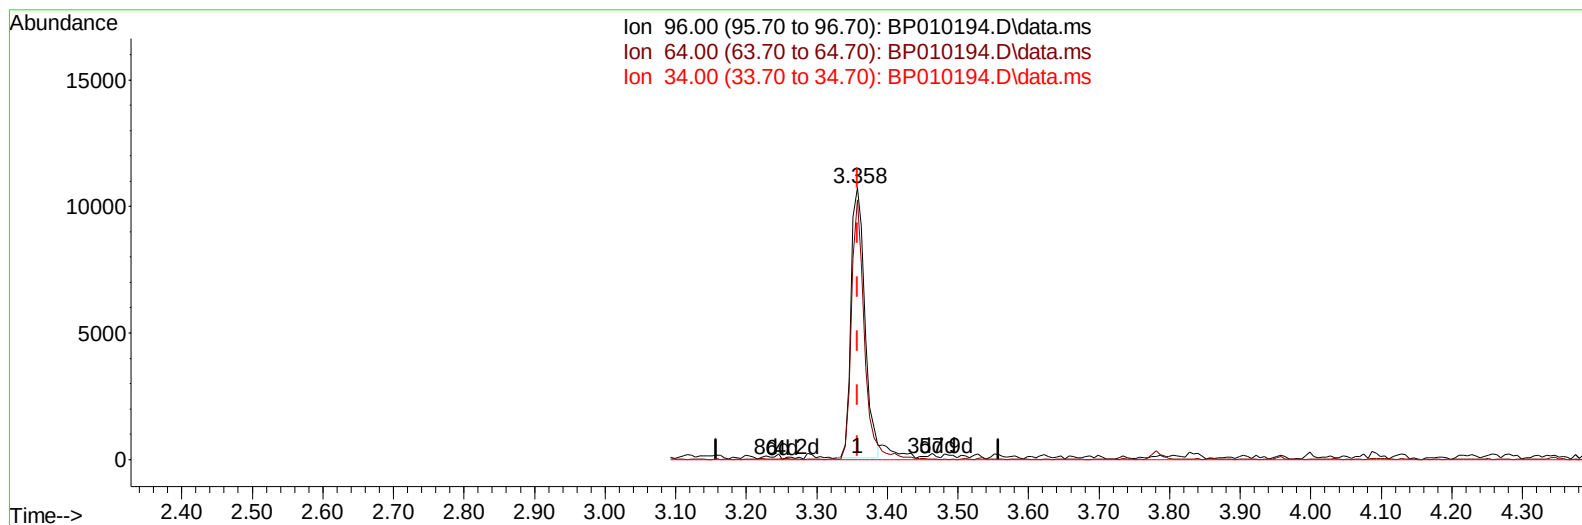

TIC: BP010194.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 7.91 ng/uL

response 14535

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	95.64#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010194.D
 Acq On : 03 May 2022 03:38
 Operator : CG/JU
 Sample : N2615-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 03 05:26:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

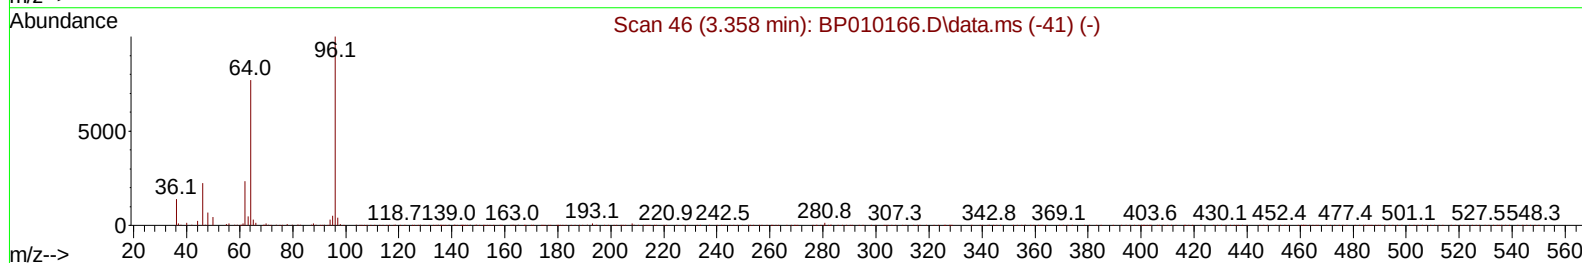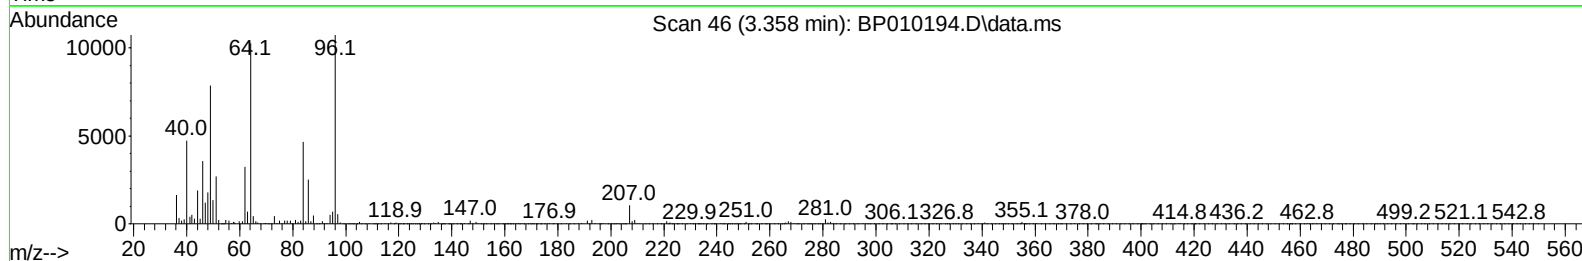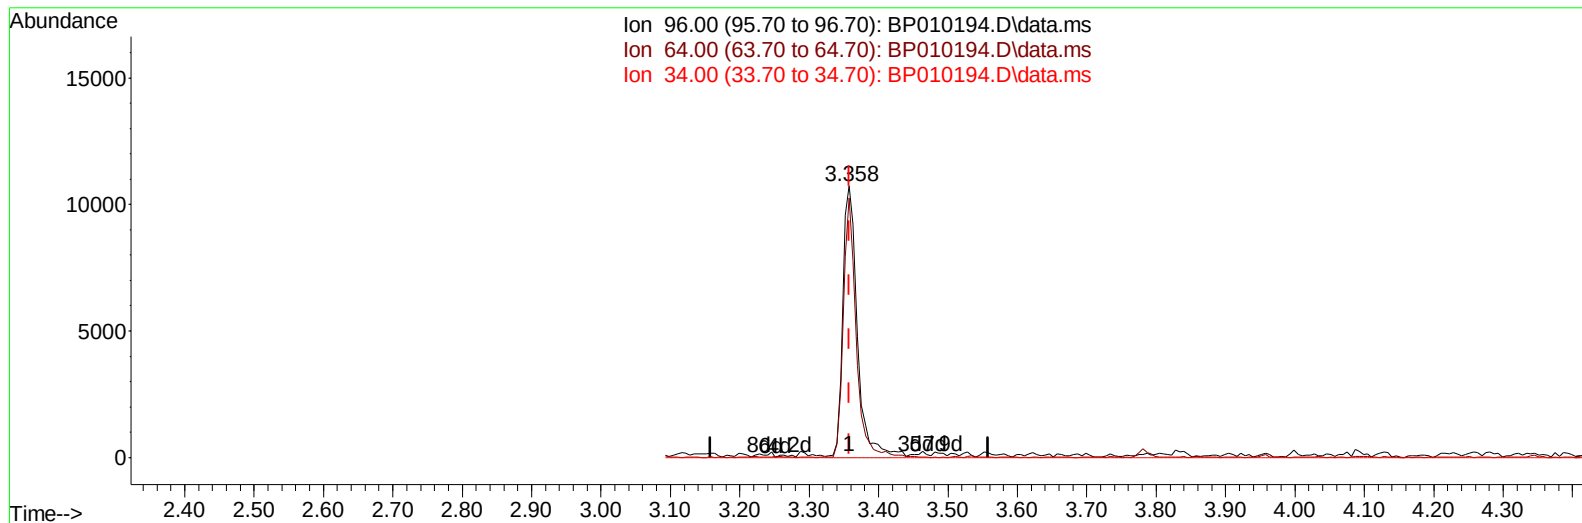

TIC: BP010194.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 8.44 ng/uL m

response 15500

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	95.64#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010194.D
Acq On : 03 May 2022 03:38
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 05:26:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

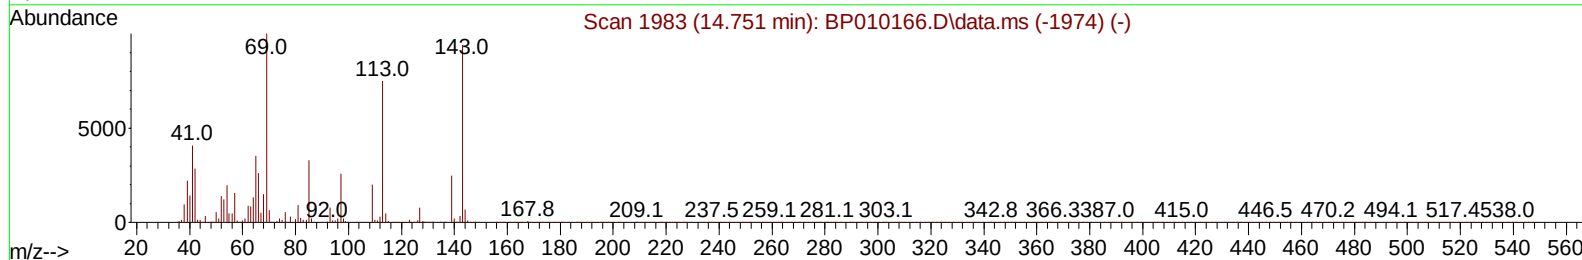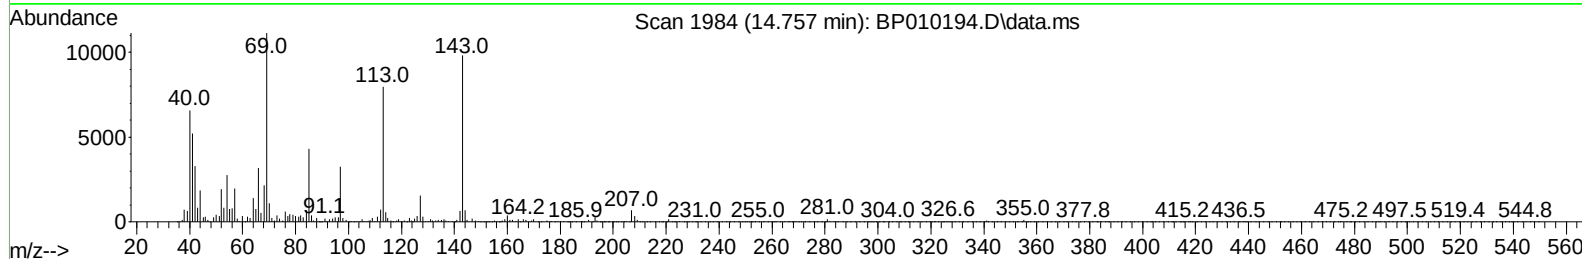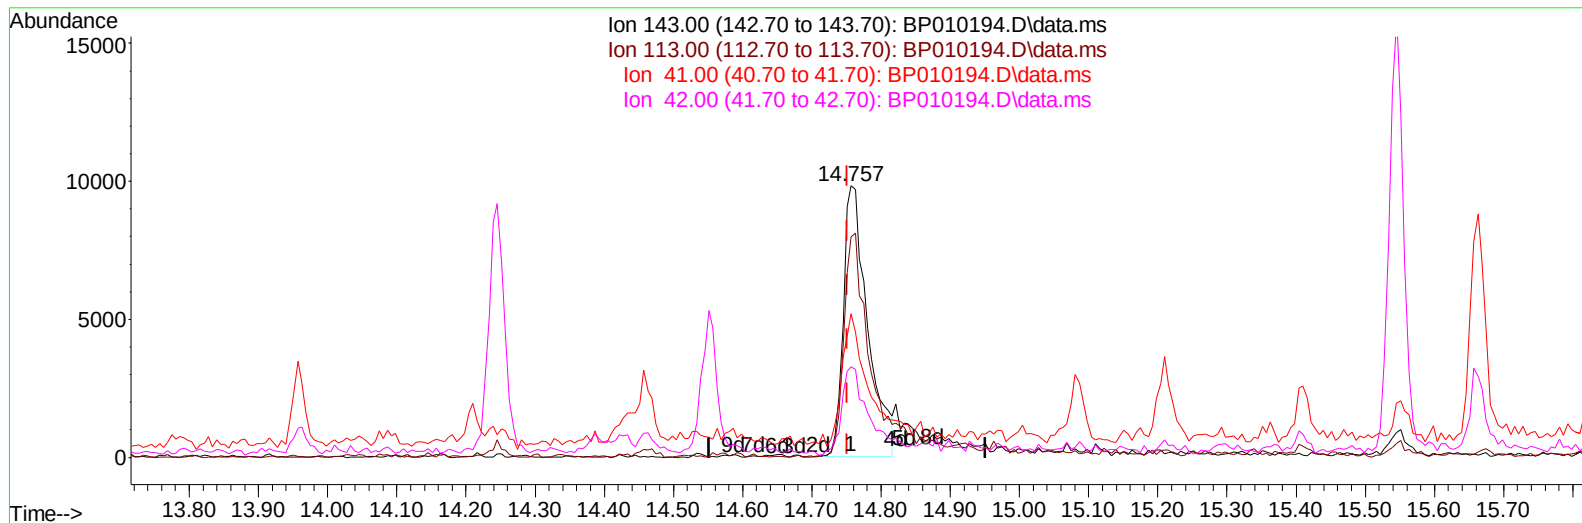

TIC: BP010194.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 7.90 ng/ul

response 23904

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.14#
41.00	23.20	53.02#
42.00	18.00	33.47#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010194.D
Acq On : 03 May 2022 03:38
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 05:26:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

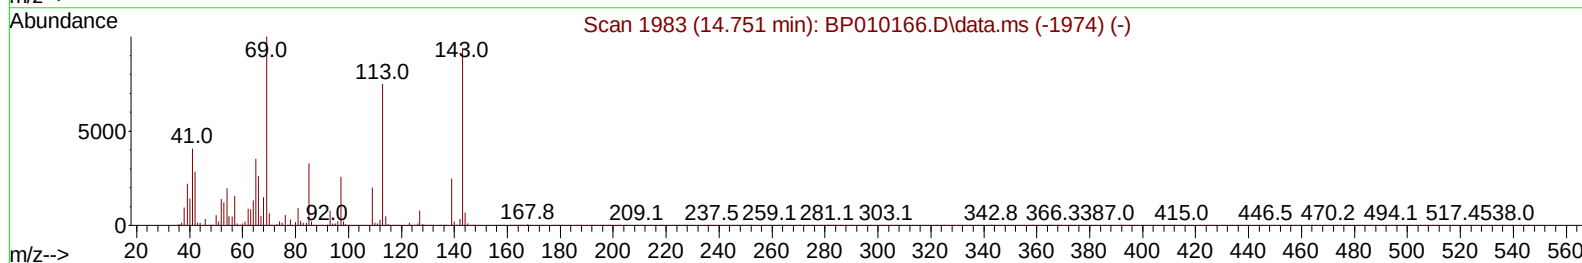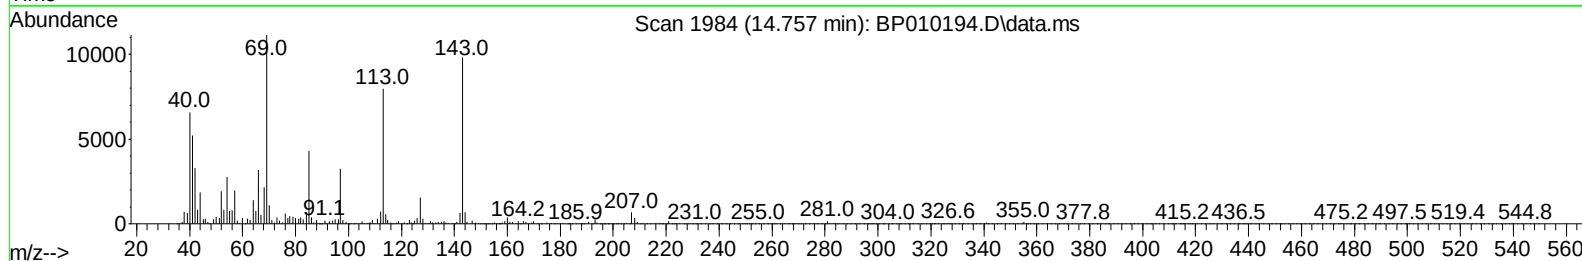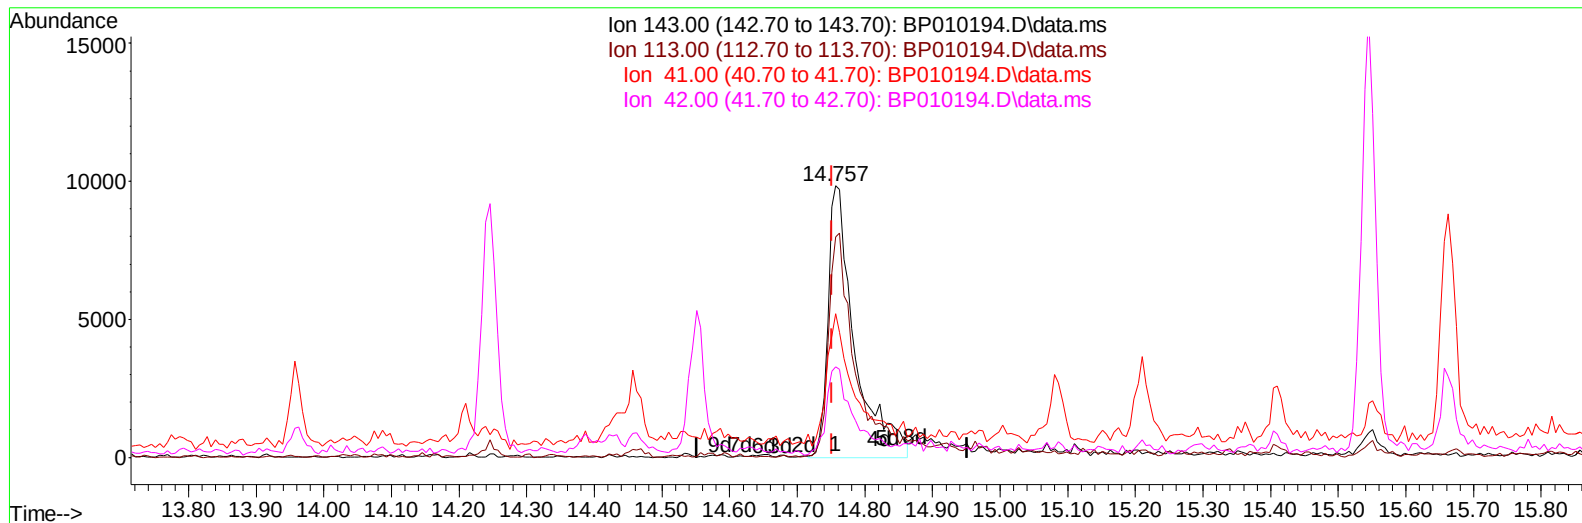

TIC: BP010194.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 8.97 ng/ul m

response 27167

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.14#
41.00	23.20	53.02#
42.00	18.00	33.47#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010194.D
 Acq On : 03 May 2022 03:38
 Operator : CG/JU
 Sample : N2615-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 05:26:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	80085	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	326820	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.551	164	211416	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	434145	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	402975	20.000	ng/ul	# 0.00
88) Perylene-d12	23.827	264	394206	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	15500m	8.440	ng/uL	0.00
4) Pyridine-d5	3.781	84	98533	19.071	ng/ul	0.00
7) Phenol-d5	7.081	99	75371	10.347	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	246555	56.407	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	229220	42.489	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	151423	25.089	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	148319	57.060	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	157613	55.520	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	254502	46.051	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	350393	44.218	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	975271	59.302	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1064651	53.490	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	27167m	8.973	ng/ul	0.00
60) Fluorene-d10	15.545	176	835867	59.085	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	136137	49.592	ng/ul	0.00
73) Anthracene-d10	17.404	188	1356529	64.586	ng/ul	0.00
81) Pyrene-d10	19.633	212	1628793	71.073	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	1463289	70.805	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010194.D
Acq On : 03 May 2022 03:38
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 03 05:26:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

