




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010197.D
Acq On : 03 May 2022 05:19
Operator : CG/JU
Sample : N2615-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 06:15:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

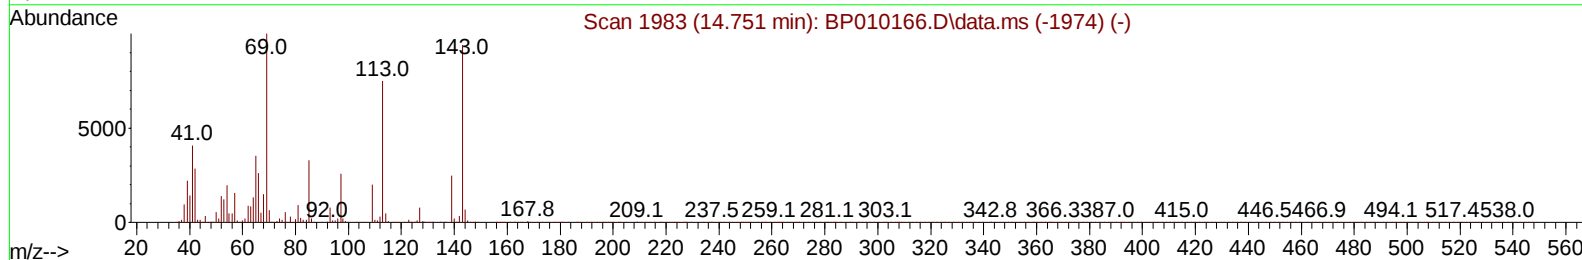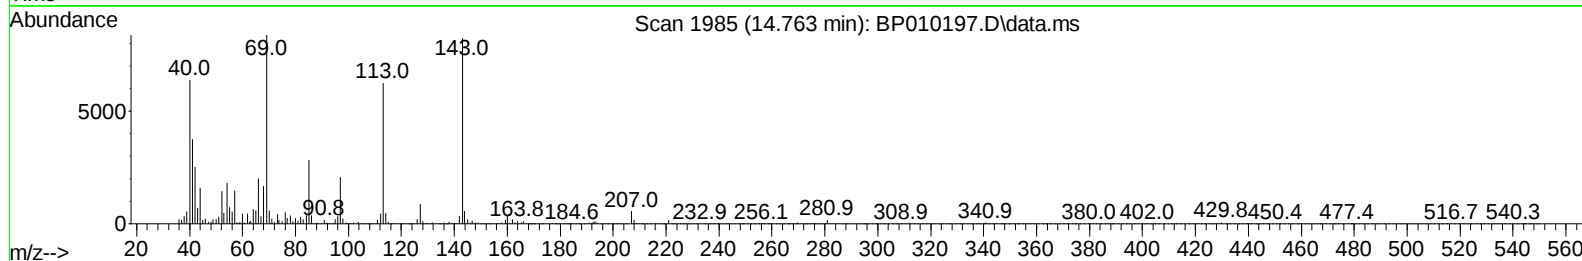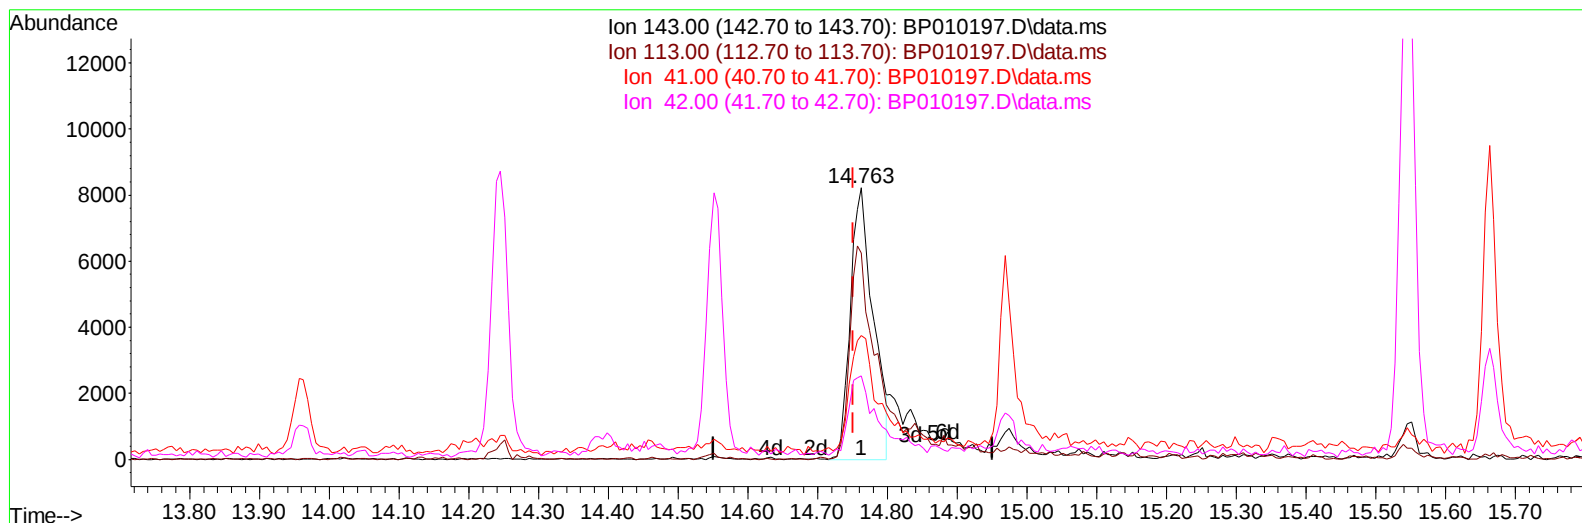

TIC: BP010197.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.011) 3.59 ng/u1

response 18623

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.11#
41.00	23.20	45.70#
42.00	18.00	30.82#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010197.D
Acq On : 03 May 2022 05:19
Operator : CG/JU
Sample : N2615-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B0

Manual IntegrationsAPPROVED

Quant Time: May 03 06:15:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

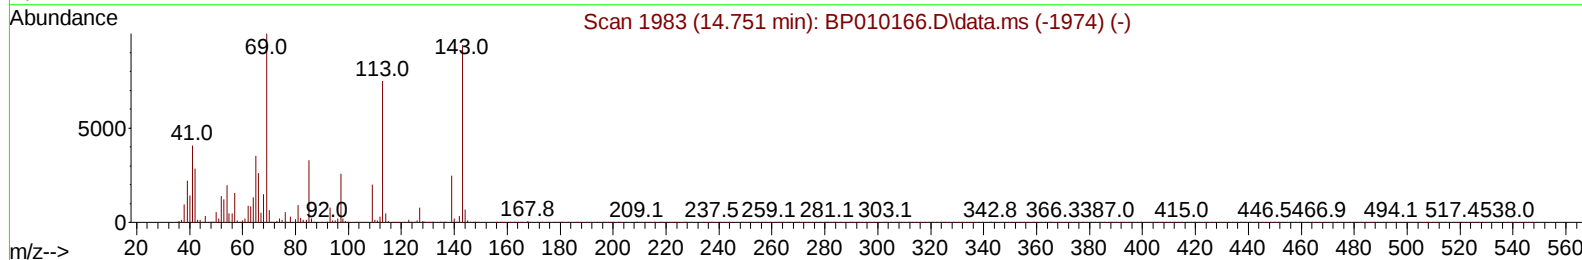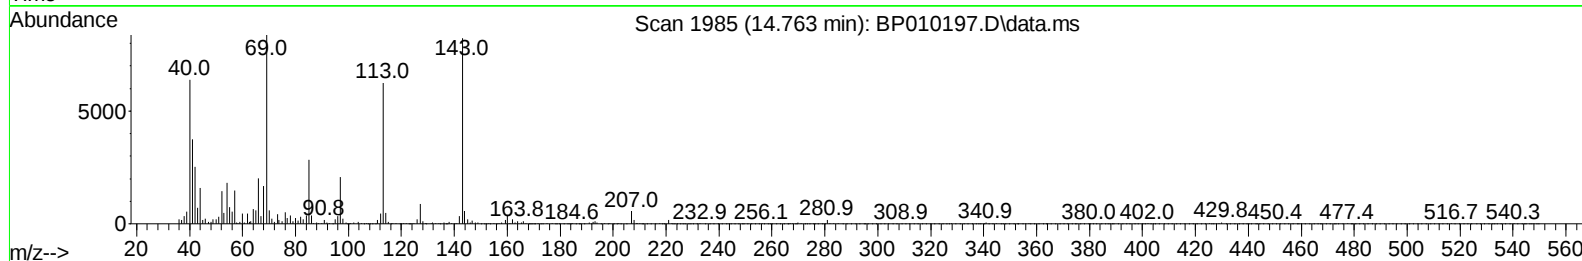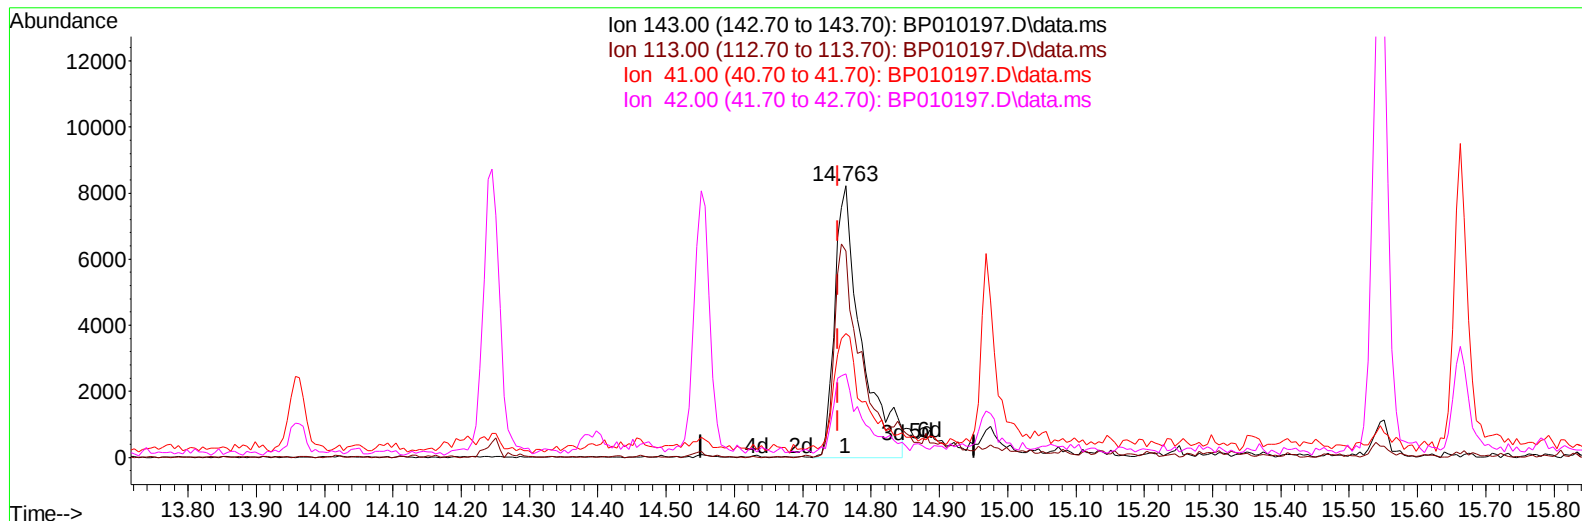

TIC: BP010197.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.011) 4.37 ng/ul m

response 22639

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.11#
41.00	23.20	45.70#
42.00	18.00	30.82#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010197.D
 Acq On : 03 May 2022 05:19
 Operator : CG/JU
 Sample : N2615-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 06:15:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	142791	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	589241	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.551	164	362016	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	735476	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	653633	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	641145	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	15350	4.688	ng/uL	0.00
4) Pyridine-d5	3.781	84	64101	6.959	ng/ul	0.00
7) Phenol-d5	7.087	99	76862	5.918	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	277587	35.618	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	245548	25.528	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	157295	14.617	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	164524	35.106	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	170994	33.408	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	268938	26.991	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	355612	24.891	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	1009550	35.849	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1161644	34.084	ng/ul	0.00
54) 4-Nitrophenol-d4	14.763	143	22639m	4.367	ng/ul	0.01
60) Fluorene-d10	15.545	176	864197	35.675	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	139437	29.983	ng/ul	0.00
73) Anthracene-d10	17.404	188	1403091	39.433	ng/ul	0.00
81) Pyrene-d10	19.633	212	1621618	43.624	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264	1380999	41.086	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010197.D
Acq On : 03 May 2022 05:19
Operator : CG/JU
Sample : N2615-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 06:15:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

