




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010203.D
 Acq On : 03 May 2022 10:53
 Operator : CG/JU
 Sample : N2615-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:08:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

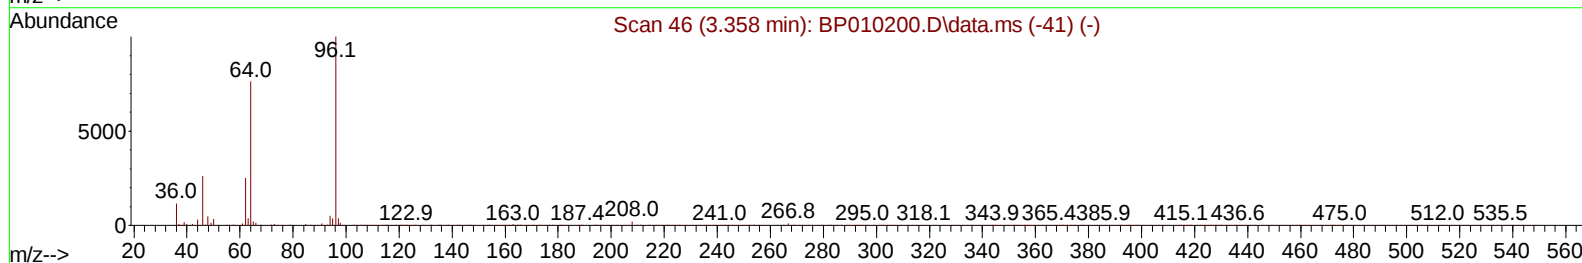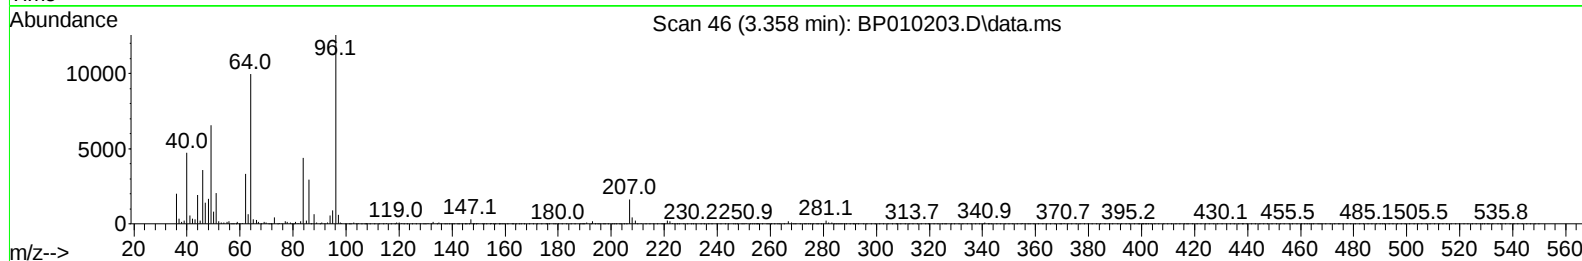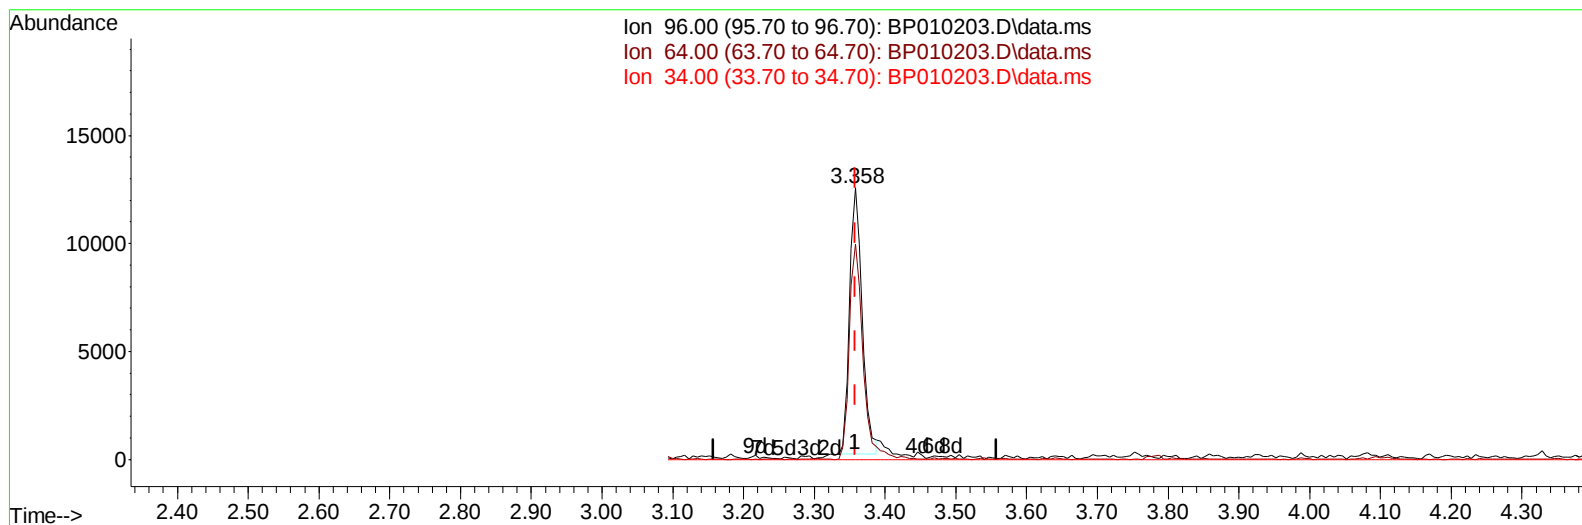

TIC: BP010203.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (+ 0.000) 4.41 ng/uL

response 15332

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.32#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010203.D
 Acq On : 03 May 2022 10:53
 Operator : CG/JU
 Sample : N2615-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:08:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

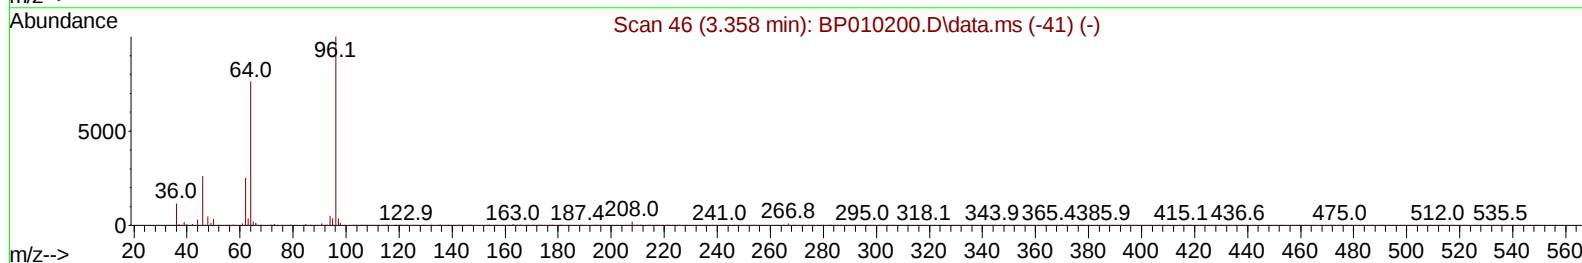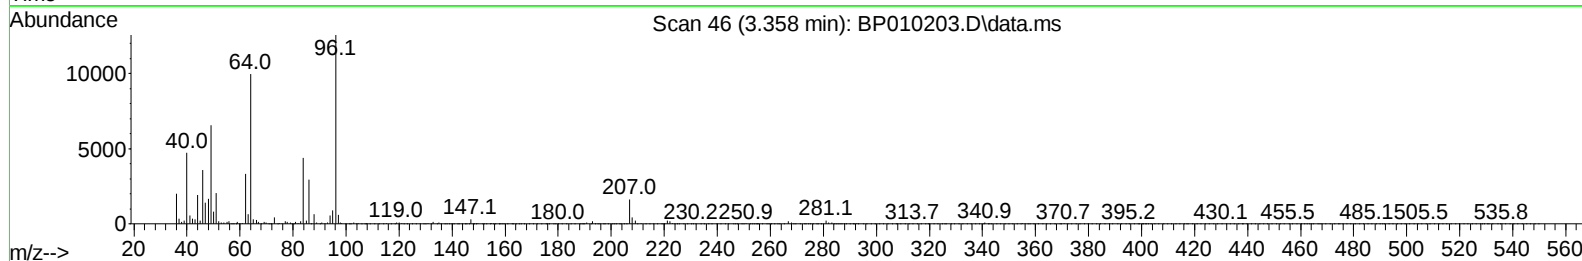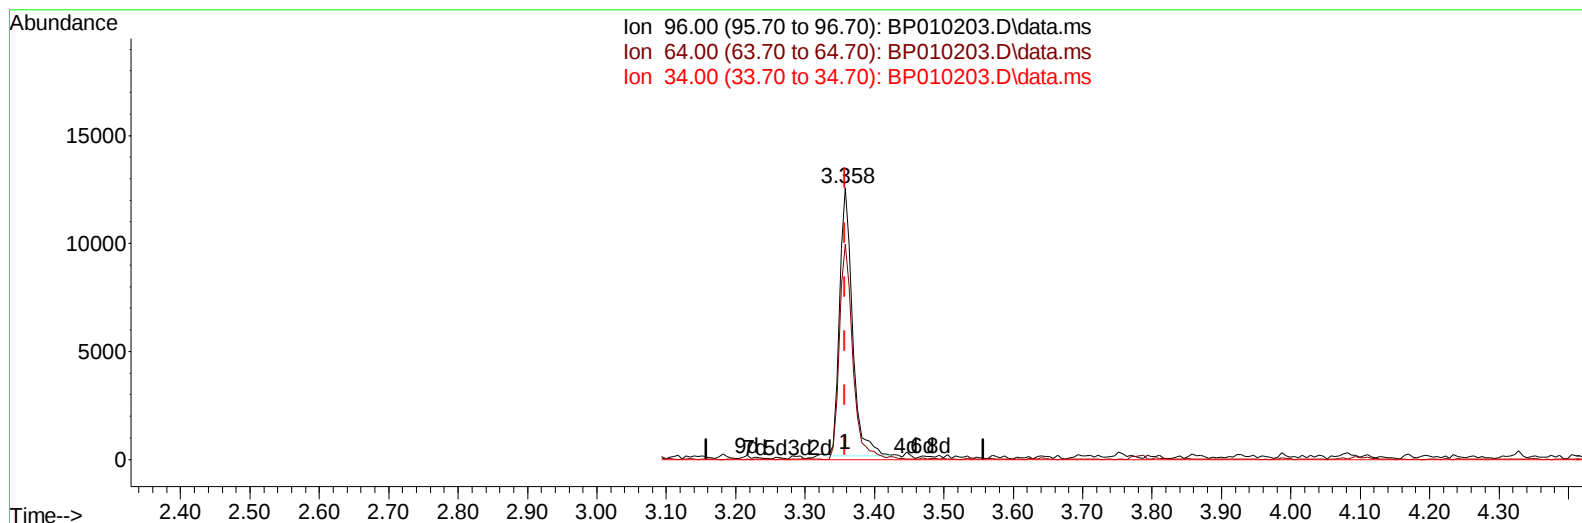

TIC: BP010203.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (+ 0.000) 4.66 ng/uL m

response 16218

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.32#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010203.D
Acq On : 03 May 2022 10:53
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:08:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

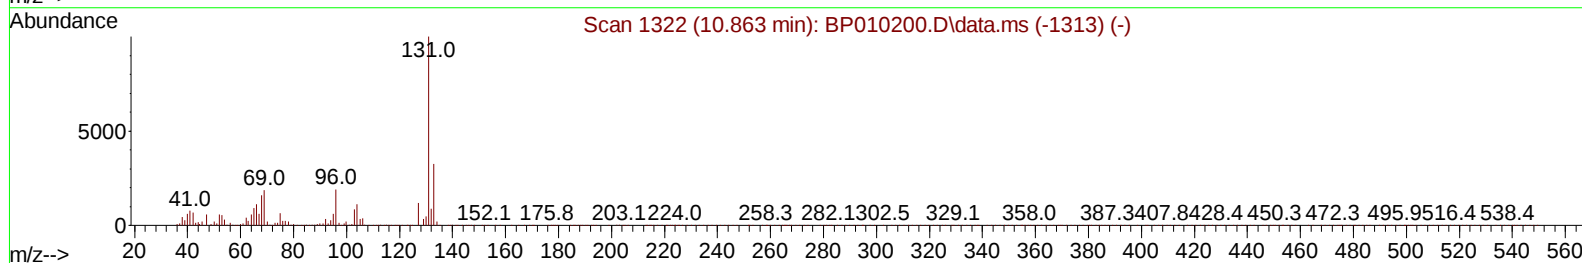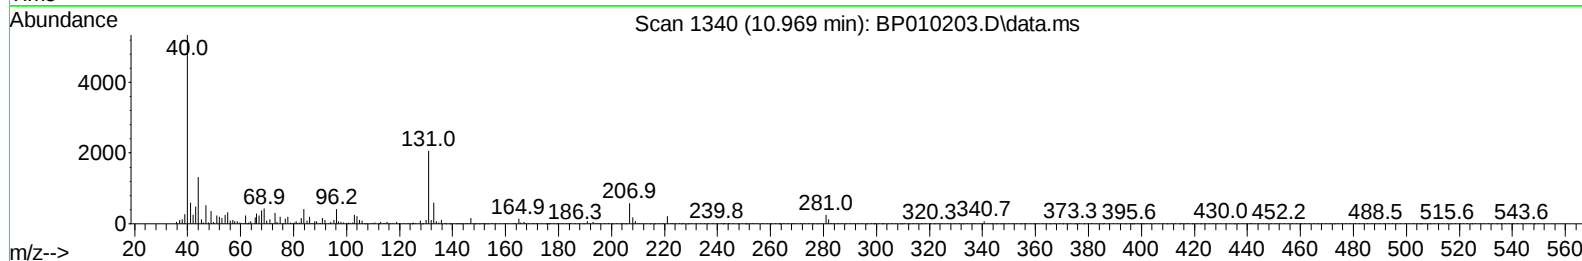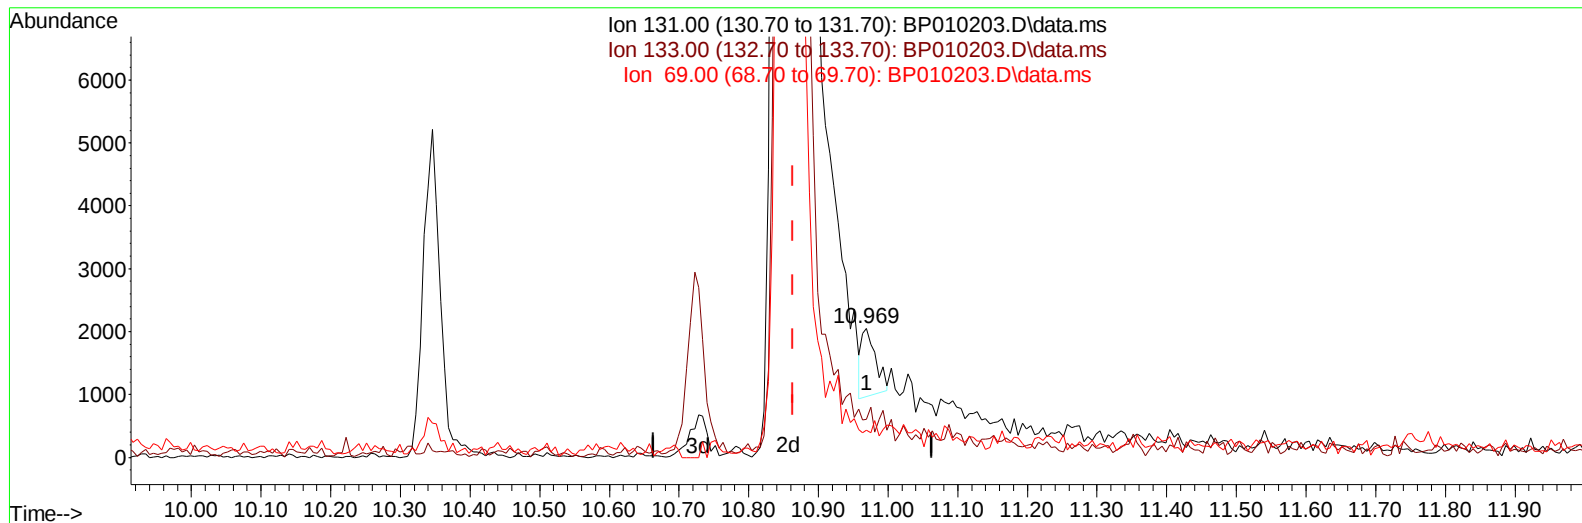

TIC: BP010203.D\data.ms

(31) 4-Chloroaniline-d4 (S)**10.969min (+ 0.106) 0.10 ng/u1****response 1539**

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	29.49
69.00	26.10	21.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010203.D
Acq On : 03 May 2022 10:53
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:08:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

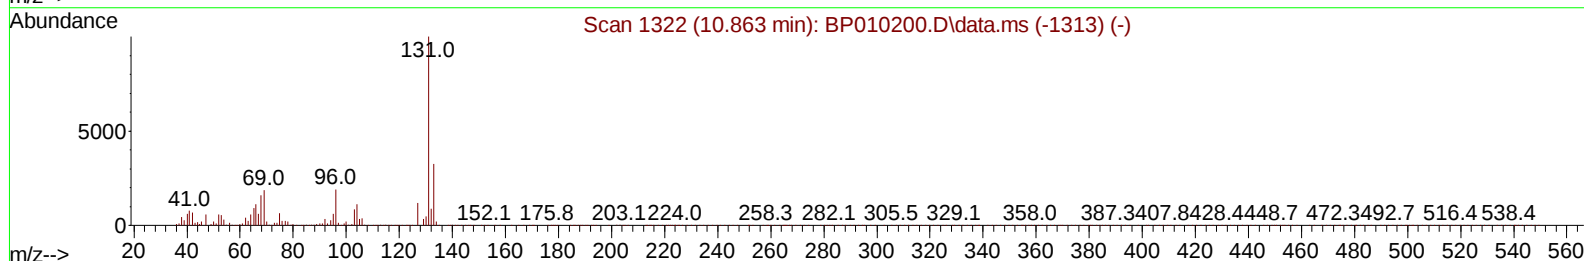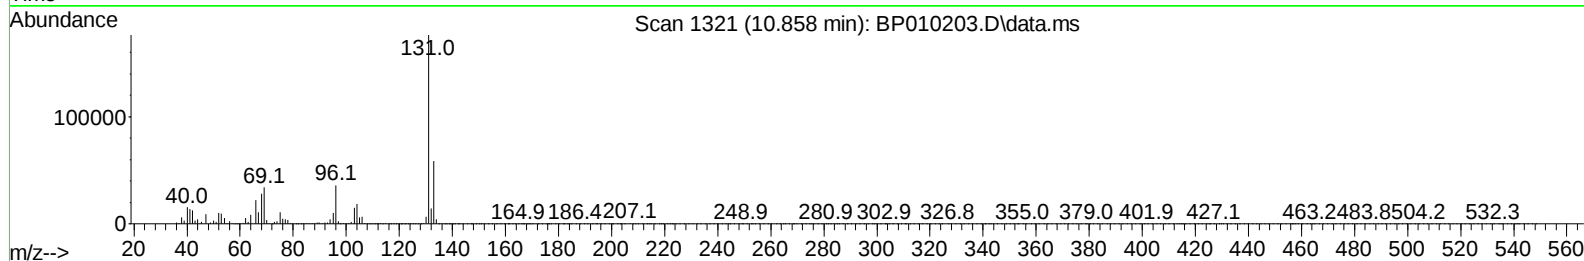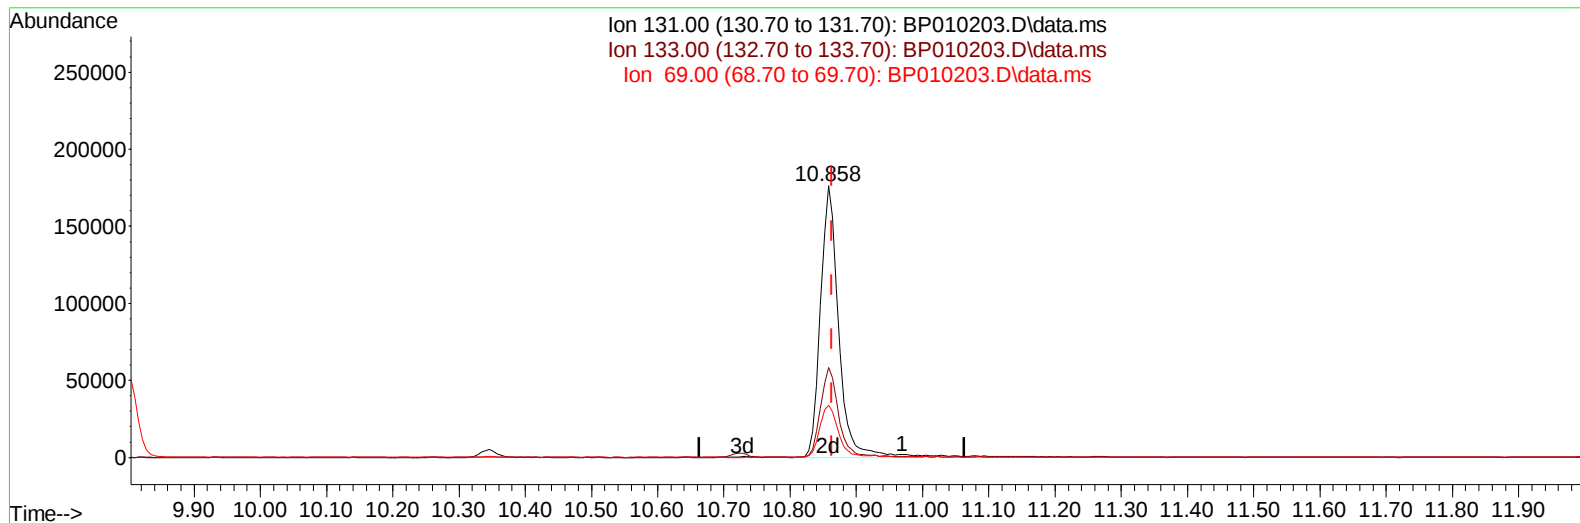

TIC: BP010203.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.858min (-0.006) 22.70 ng/ul m

response 335194

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	33.22
69.00	26.10	19.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010203.D
Acq On : 03 May 2022 10:53
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:08:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

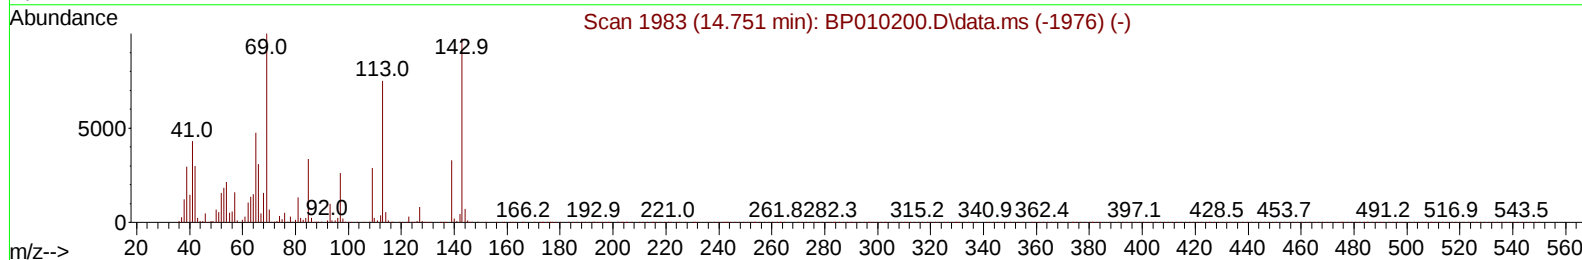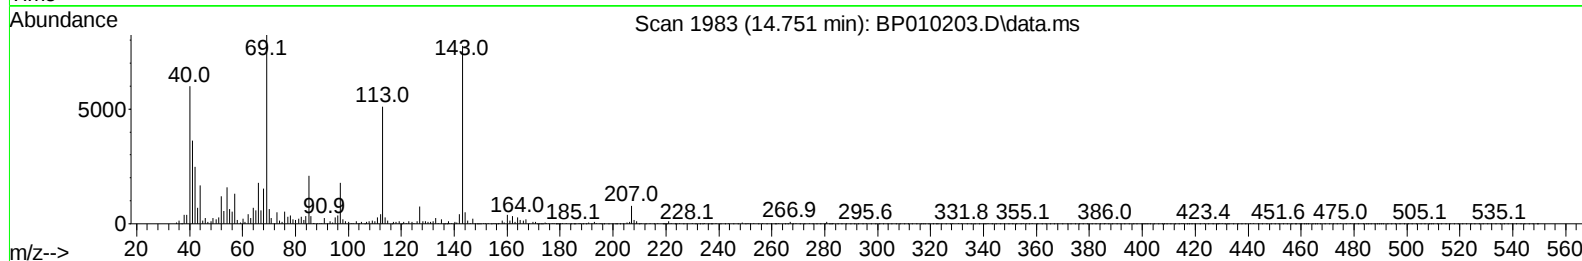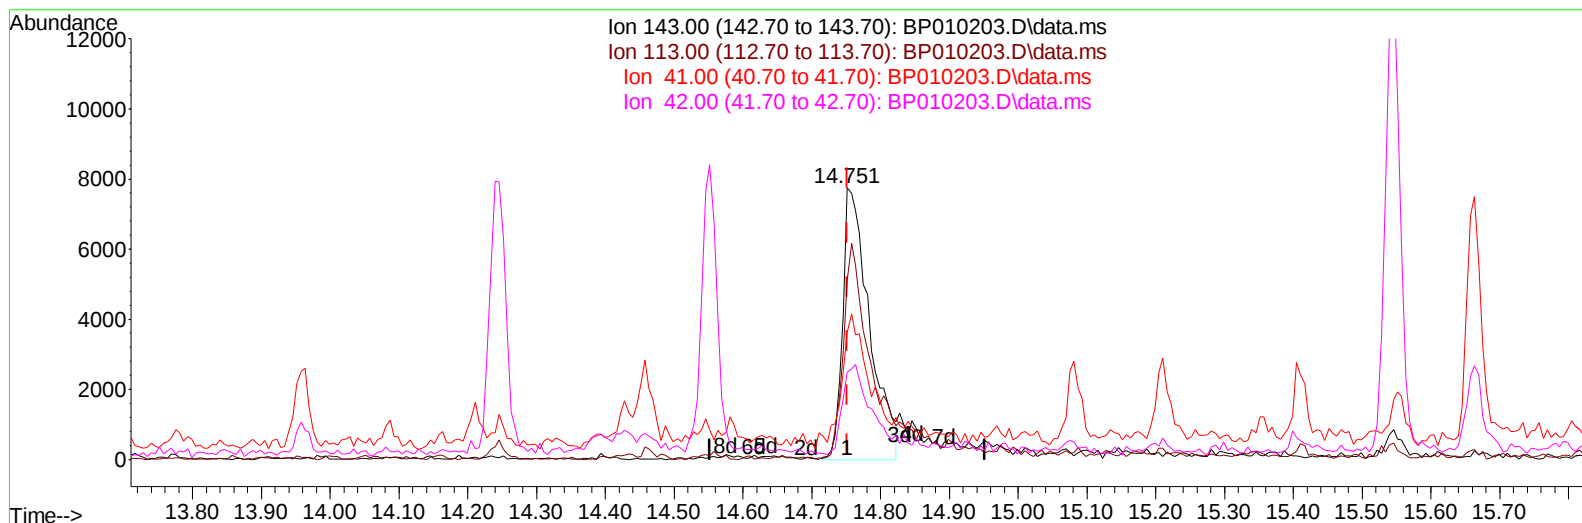

TIC: BP010203.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.000) 3.99 ng/u1

response 21047

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	65.88#
41.00	23.20	46.88#
42.00	18.00	32.12#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010203.D
Acq On : 03 May 2022 10:53
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:08:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

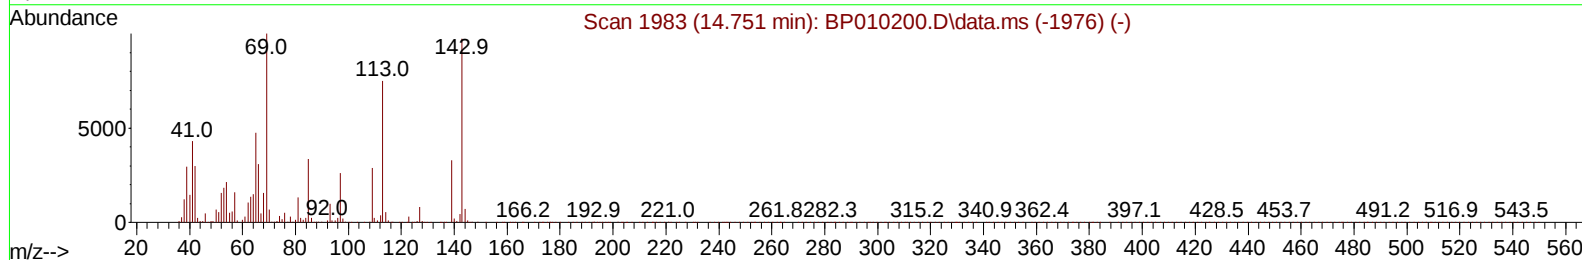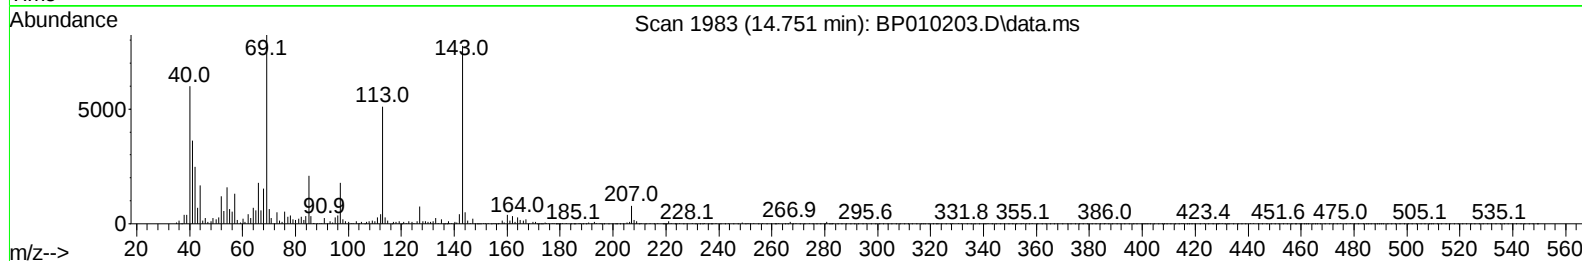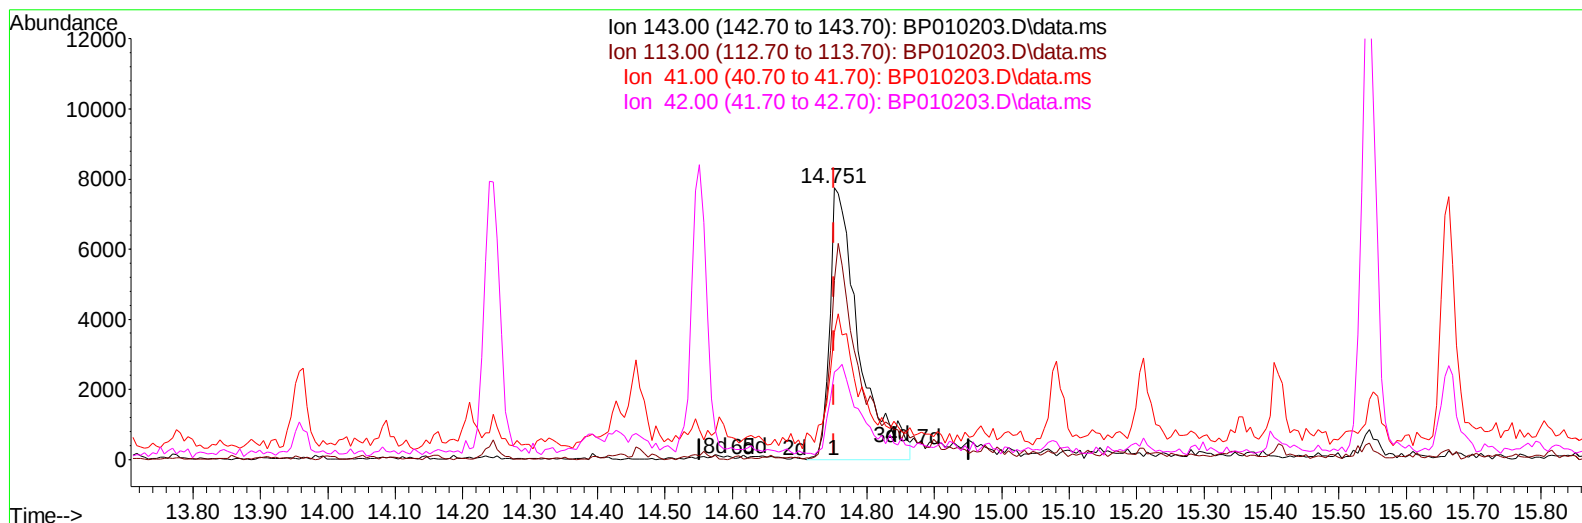

TIC: BP010203.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.000) 4.40 ng/ul m

response 23172

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	65.88#
41.00	23.20	46.88#
42.00	18.00	32.12#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010203.D
 Acq On : 03 May 2022 10:53
 Operator : CG/JU
 Sample : N2615-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:08:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	151691	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.722	136	608905	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	367974	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	741092	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	698262	20.000	ng/ul	# 0.00
88) Perylene-d12	23.827	264	695538	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	16218m	4.662	ng/uL	0.00
4) Pyridine-d5	3.781	84	98995	10.116	ng/ul	0.00
7) Phenol-d5	7.087	99	74705	5.414	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	246362	29.757	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	222411	21.766	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	146523	12.817	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	143390	29.608	ng/ul	0.00
24) 2-Nitrophenol-d4	9.805	143	150500	28.455	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	240837	23.390	ng/ul	0.00
31) 4-Chloroaniline-d4	10.858	131	335194m	22.704	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	876163	30.609	ng/ul	0.00
49) Acenaphthylene-d8	14.246	160	978399	28.242	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	23172m	4.397	ng/ul	0.00
60) Fluorene-d10	15.545	176	745900	30.293	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	119827	25.571	ng/ul	0.00
73) Anthracene-d10	17.404	188	1190623	33.208	ng/ul	0.00
81) Pyrene-d10	19.634	212	1434536	36.125	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.669	264	1312855	36.004	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010203.D
Acq On : 03 May 2022 10:53
Operator : CG/JU
Sample : N2615-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:08:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

