




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010205.D
 Acq On : 03 May 2022 12:00
 Operator : CG/JU
 Sample : N2623-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFJ4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:09:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

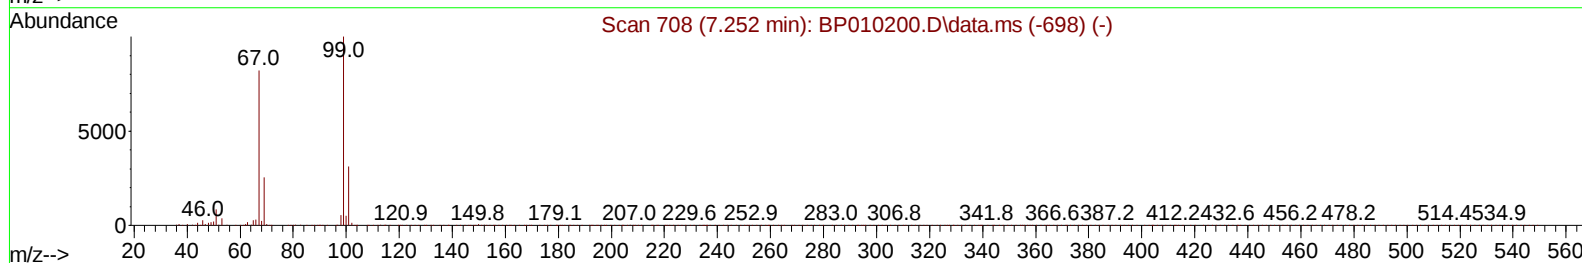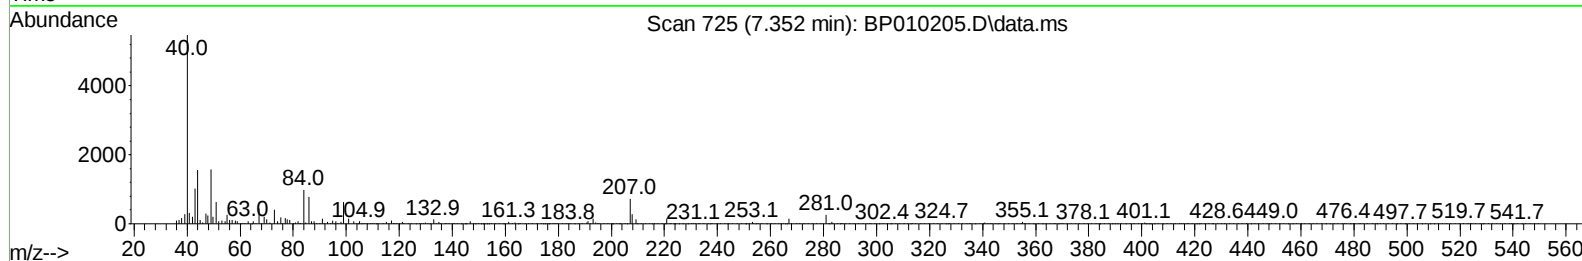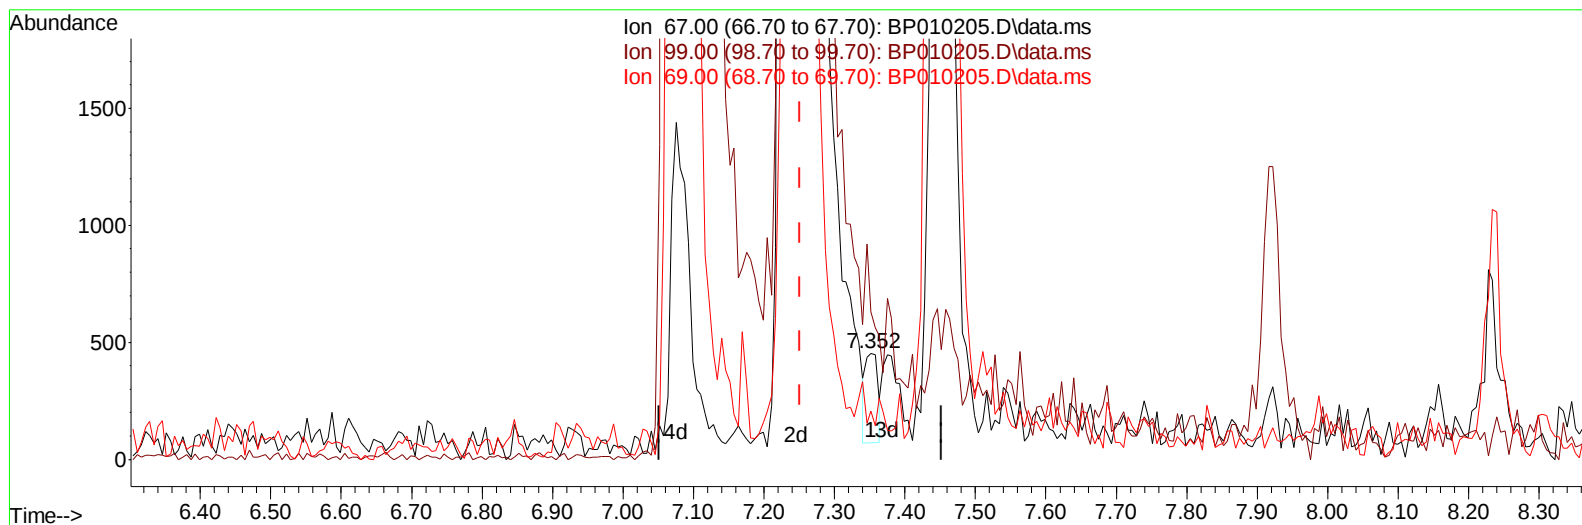

TIC: BP010205.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.352min (+ 0.100) 0.06 ng/u1

response 460

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	138.99
69.00	40.10	45.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010205.D
 Acq On : 03 May 2022 12:00
 Operator : CG/JU
 Sample : N2623-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFJ4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:09:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

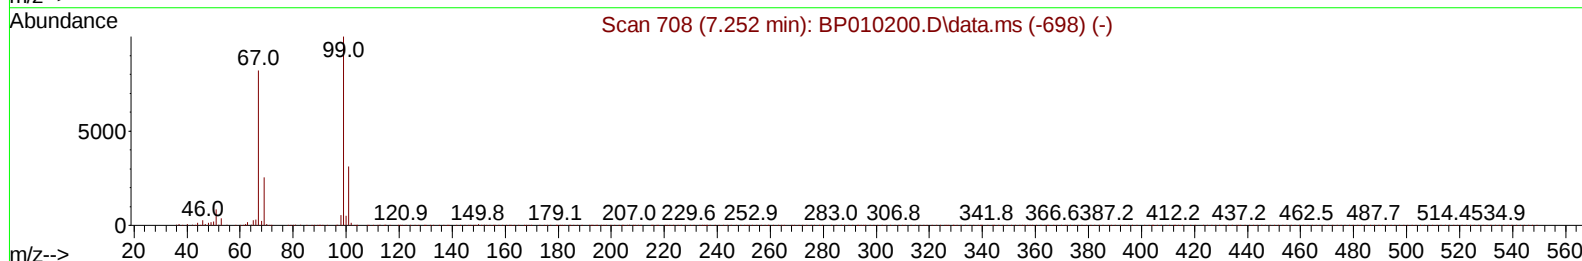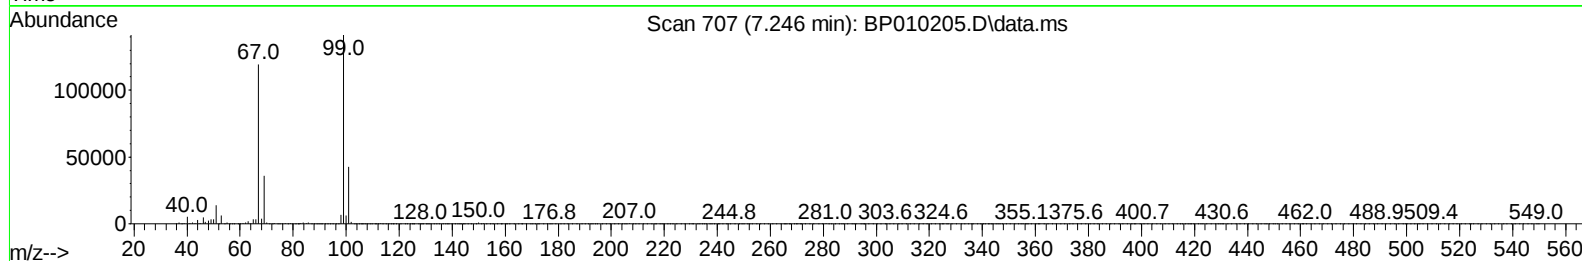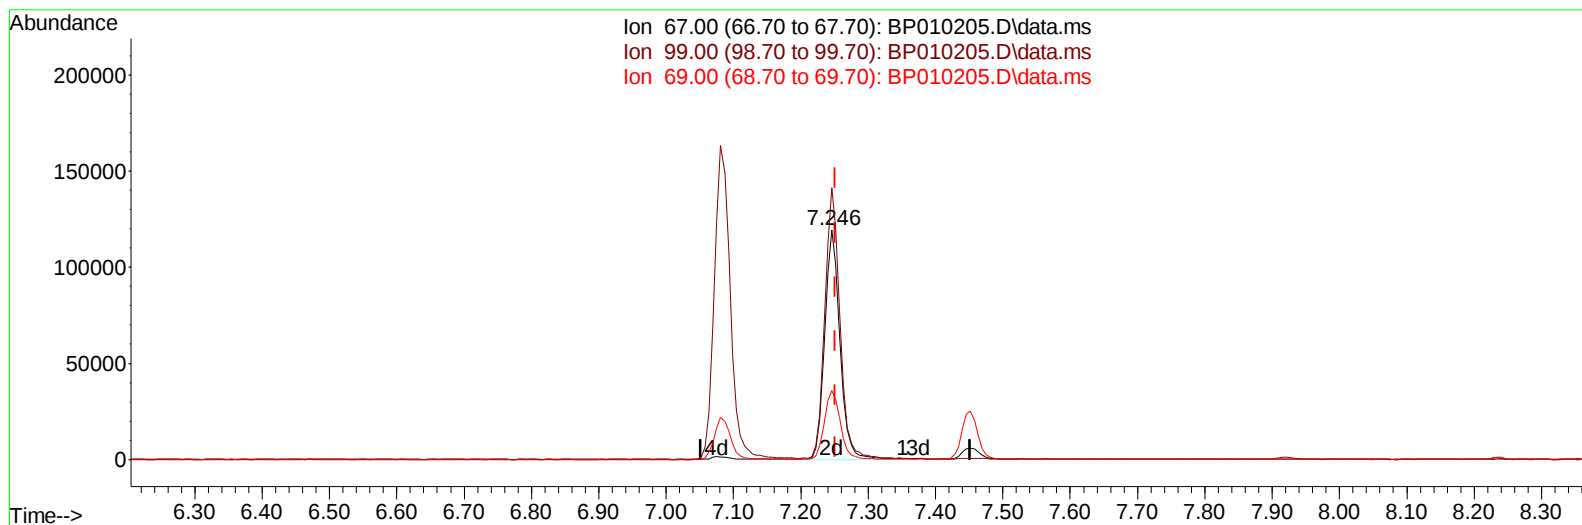

TIC: BP010205.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.246min (-0.006) 24.54 ng/ul m

response 188829

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	118.34#
69.00	40.10	30.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010205.D
Acq On : 03 May 2022 12:00
Operator : CG/JU
Sample : N2623-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFJ4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:09:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

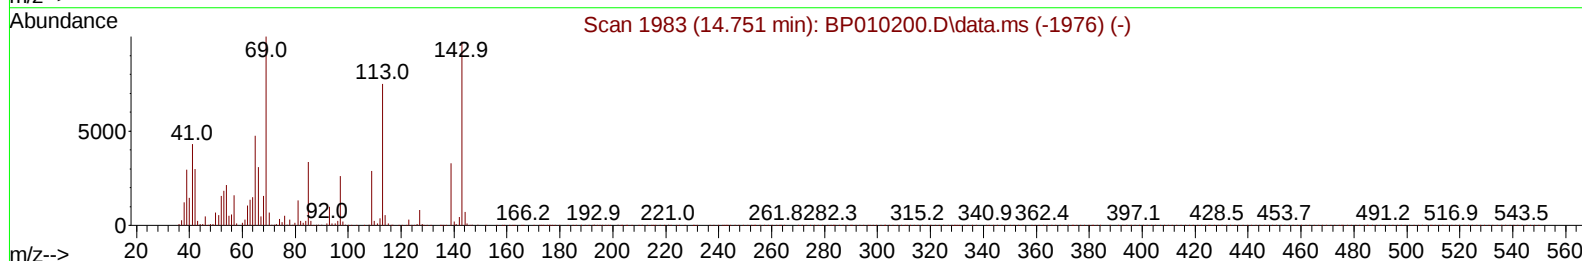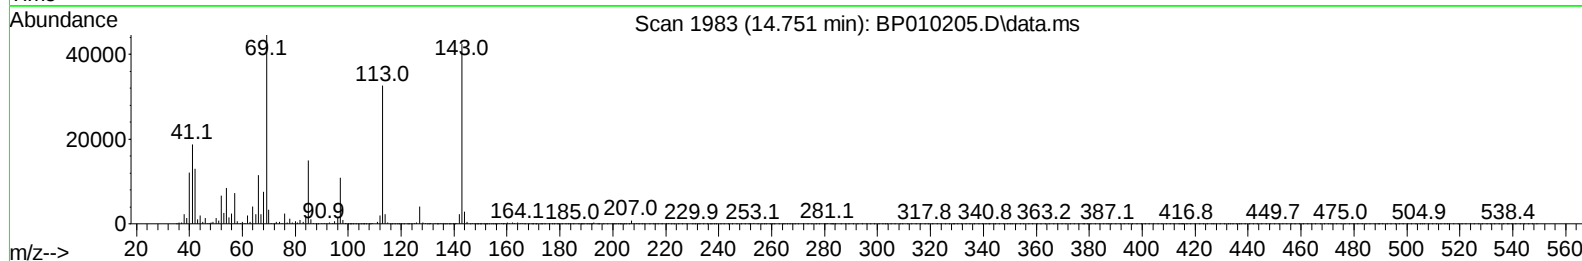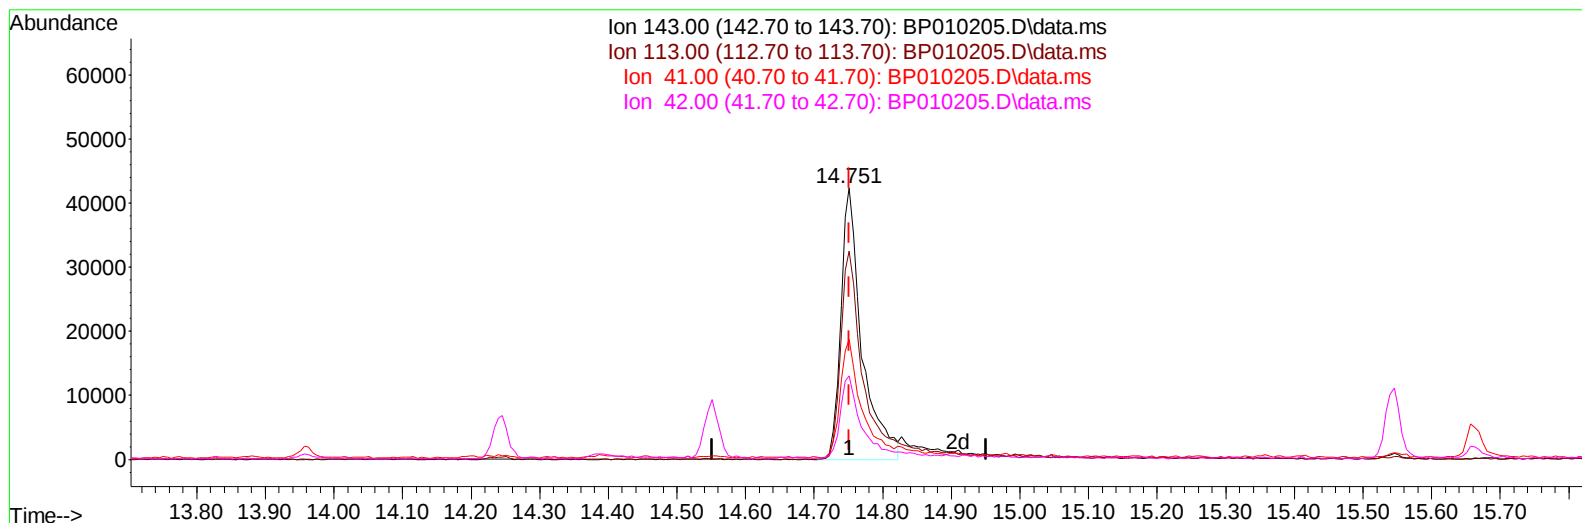

TIC: BP010205.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.000) 15.62 ng/u1

response 90067

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.81#
41.00	23.20	44.22#
42.00	18.00	30.74#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010205.D
 Acq On : 03 May 2022 12:00
 Operator : CG/JU
 Sample : N2623-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFJ4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:09:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

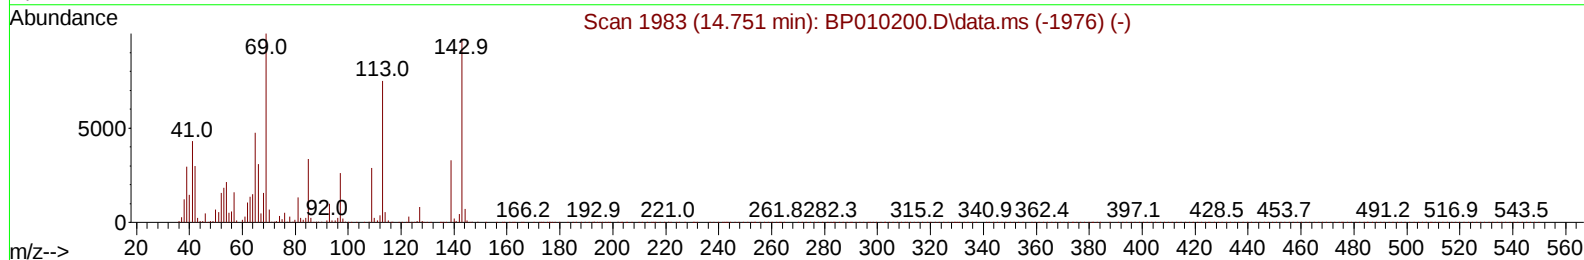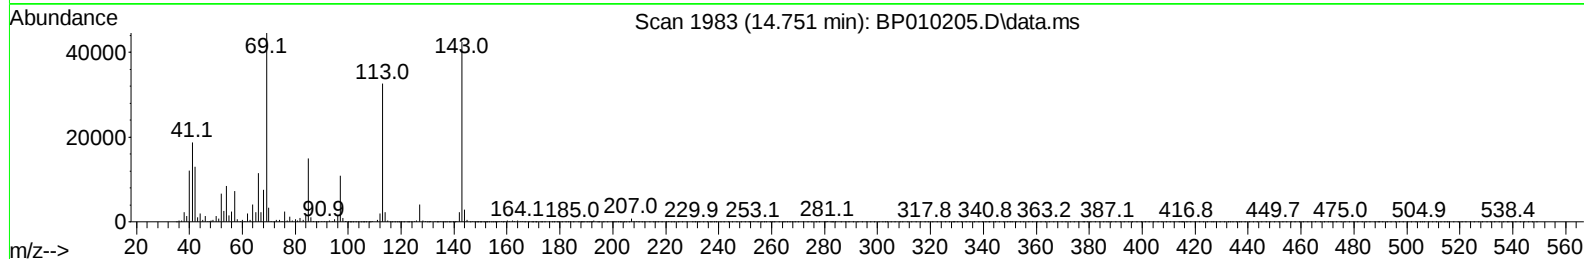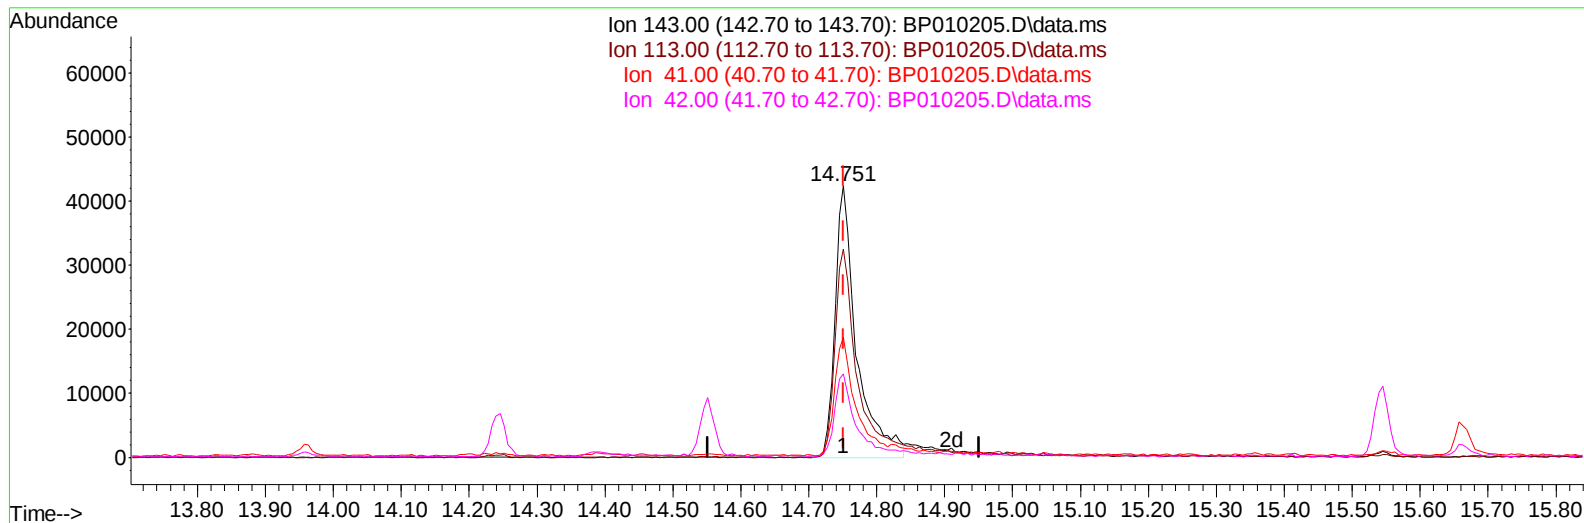

TIC: BP010205.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (-0.000) 16.13 ng/ul m

response 92962

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	76.81#
41.00	23.20	44.22#
42.00	18.00	30.74#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010205.D
Acq On : 03 May 2022 12:00
Operator : CG/JU
Sample : N2623-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFJ4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:09:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

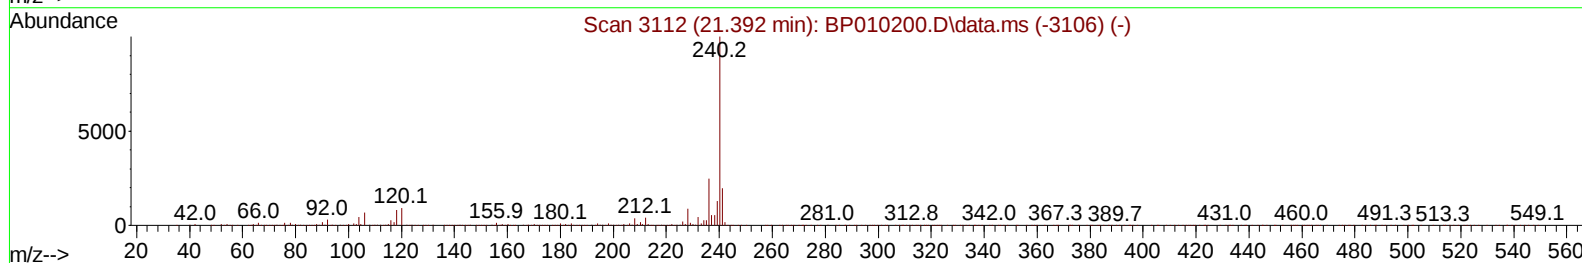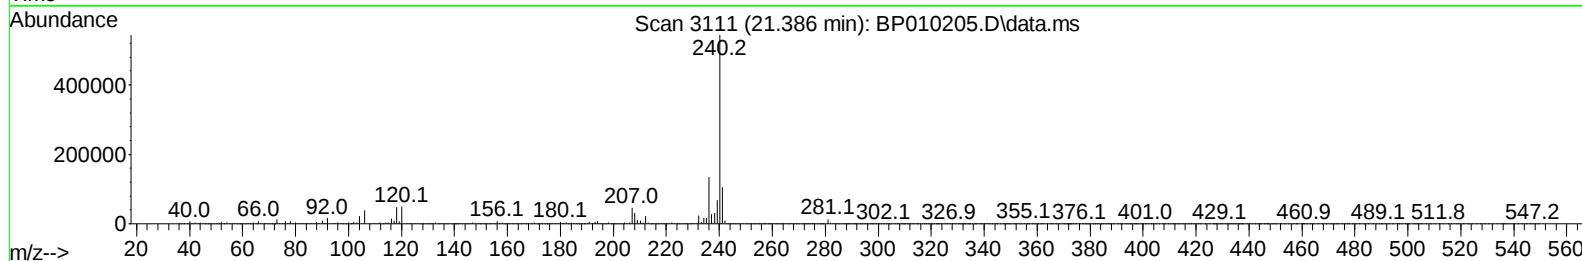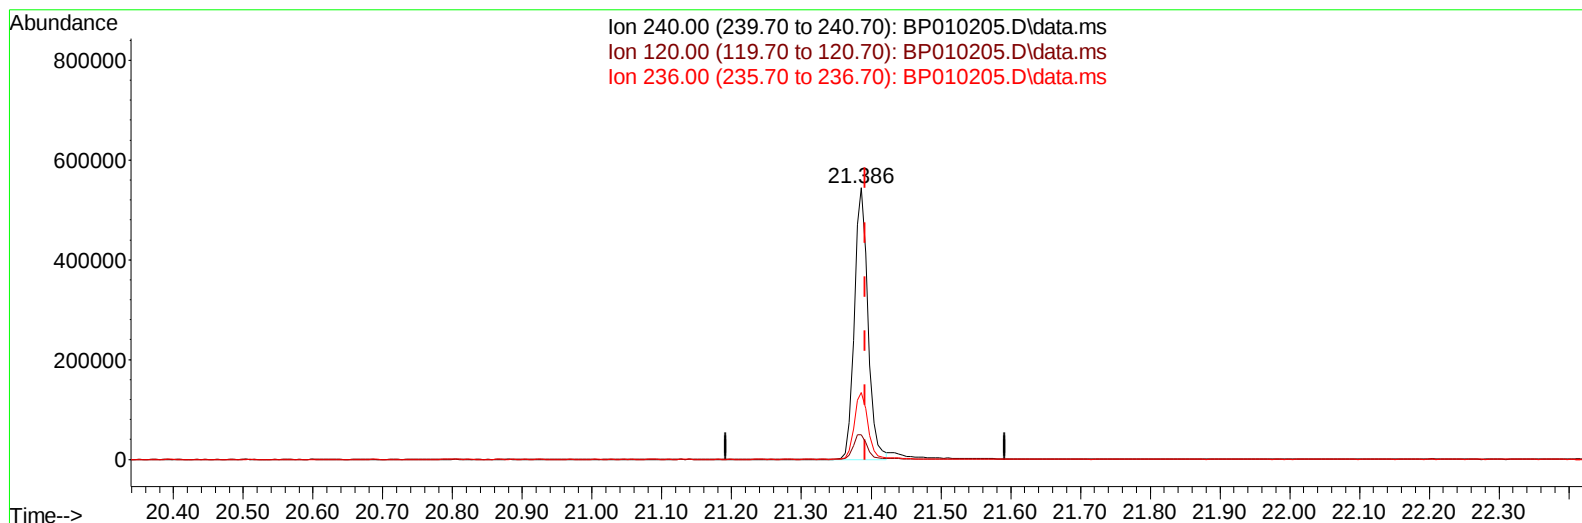

TIC: BP010205.D\data.ms

(79) Chrysene-d12 (I)

21.386min (-0.006) 20.00 ng/u1

response 732339

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	9.04
236.00	31.60	24.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010205.D
Acq On : 03 May 2022 12:00
Operator : CG/JU
Sample : N2623-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFJ4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:09:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

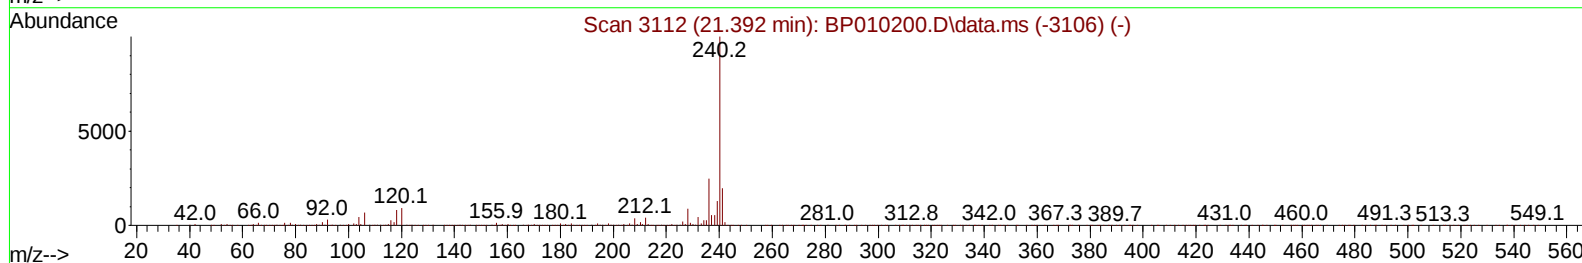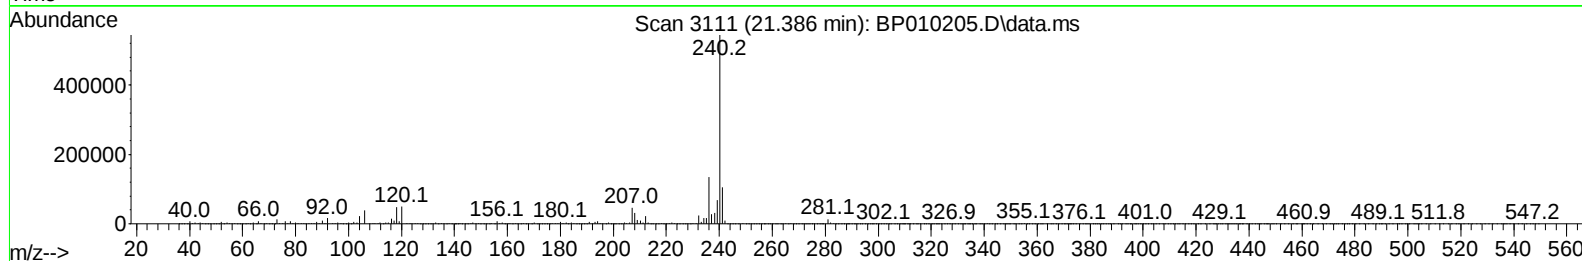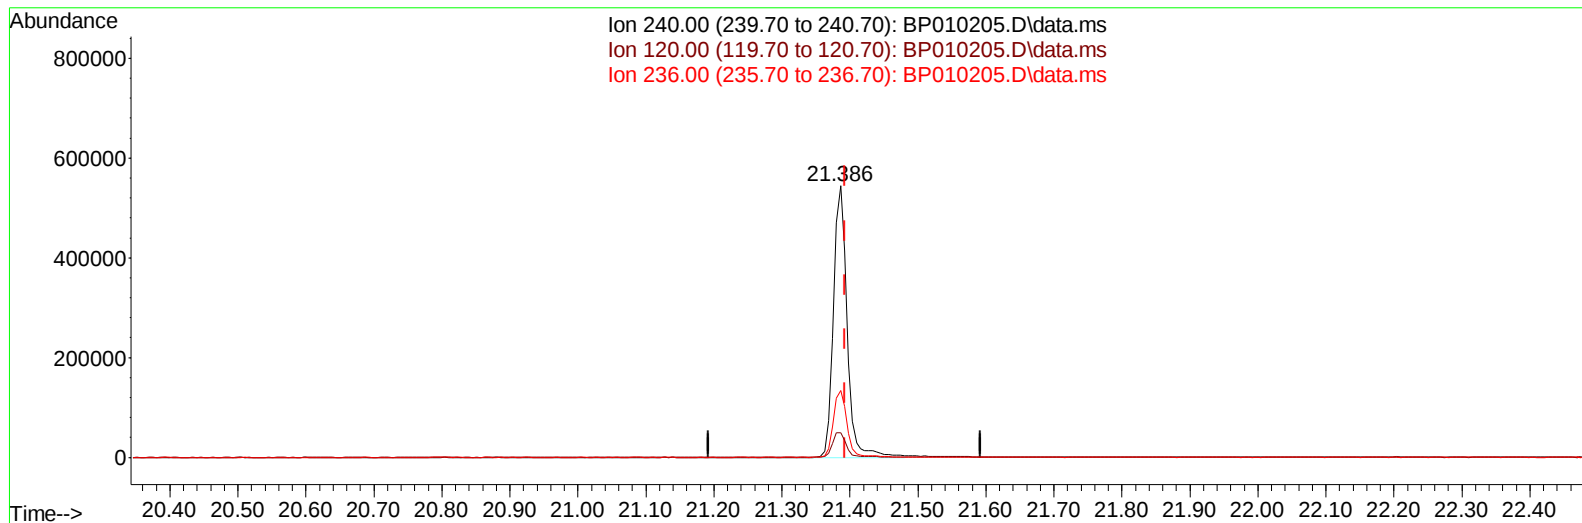

TIC: BP010205.D\data.ms

(79) Chrysene-d12 (I)

21.386min (-0.006) 20.00 ng/ul m

response 759836

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	9.04
236.00	31.60	24.67#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010205.D
 Acq On : 03 May 2022 12:00
 Operator : CG/JU
 Sample : N2623-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFFJ4

Manual IntegrationsAPPROVED

Quant Time: May 04 01:09:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	140973	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	599793	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	402538	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	822590	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	759836m	20.000	ng/ul	0.00
88) Perylene-d12	23.827	264	758854	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	12855	3.976	ng/uL	0.00
4) Pyridine-d5	3.781	84	82032	9.020	ng/ul	0.00
7) Phenol-d5	7.081	99	268653	20.951	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	188829m	24.542	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	224212	23.610	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	230460	21.692	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	115048	24.117	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	124462	23.889	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	213502	21.050	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	265566	18.261	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	751212	23.990	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	848195	22.381	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	92962m	16.126	ng/ul	0.00
60) Fluorene-d10	15.545	176	636910	23.646	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	88674	17.048	ng/ul	0.00
73) Anthracene-d10	17.404	188	988007	24.827	ng/ul	0.00
81) Pyrene-d10	19.633	212	1213323	28.078	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1061222	26.675	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010205.D
Acq On : 03 May 2022 12:00
Operator : CG/JU
Sample : N2623-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFFJ4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:09:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

