




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010210.D
 Acq On : 03 May 2022 16:43
 Operator : CG/JU
 Sample : N2615-18
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0D8

Manual IntegrationsAPPROVED

Quant Time: May 04 01:10:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

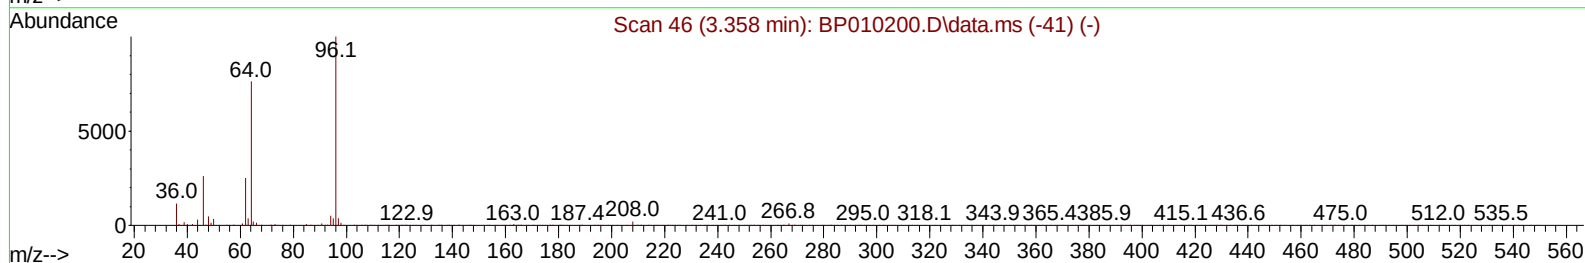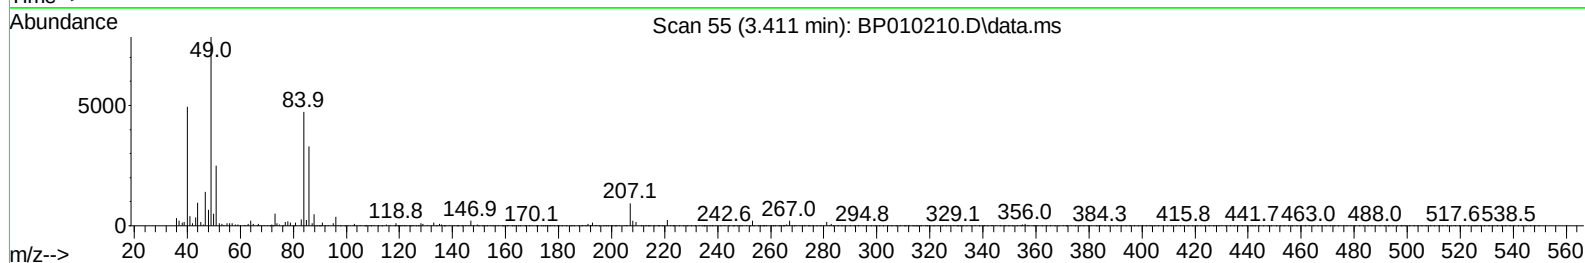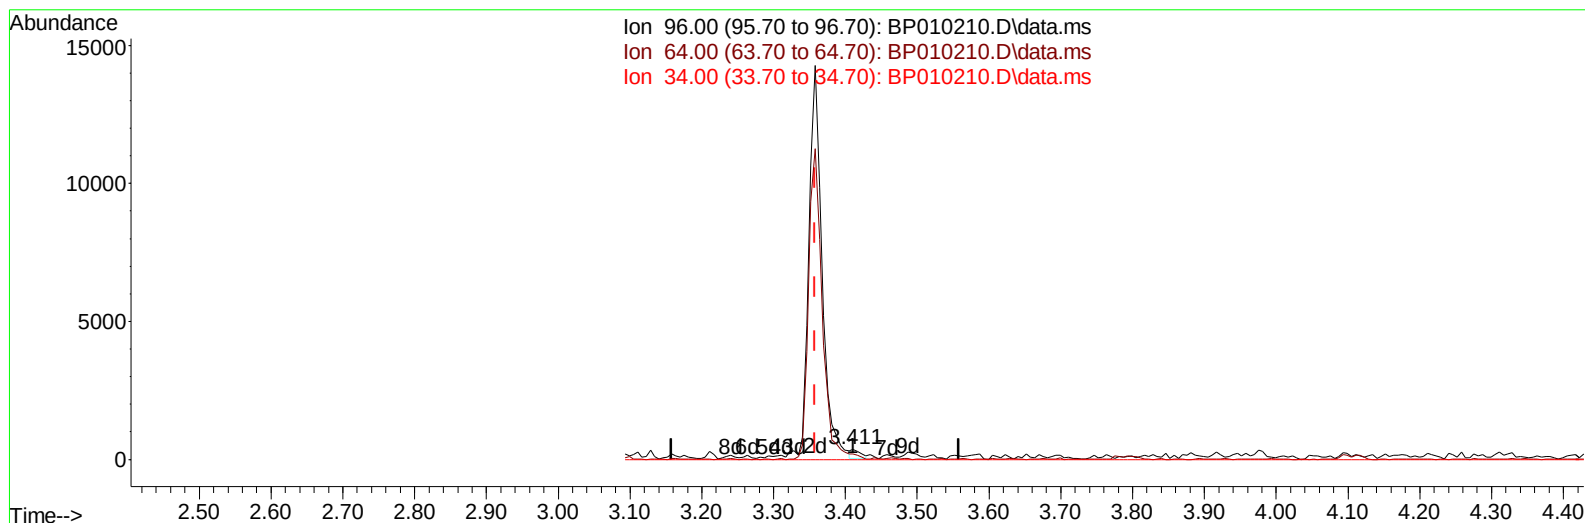

TIC: BP010210.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.411min (+ 0.053) 0.08 ng/uL

response 280

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	56.83
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010210.D
 Acq On : 03 May 2022 16:43
 Operator : CG/JU
 Sample : N2615-18
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0D8

Manual IntegrationsAPPROVED

Quant Time: May 04 01:10:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

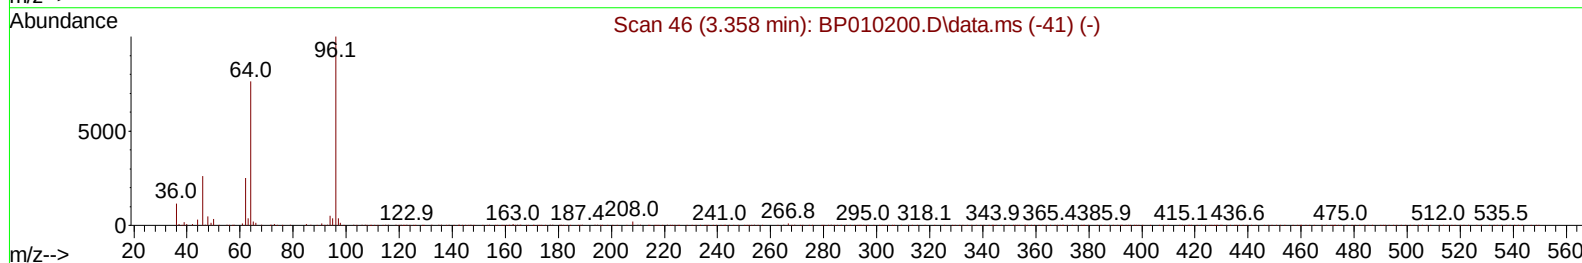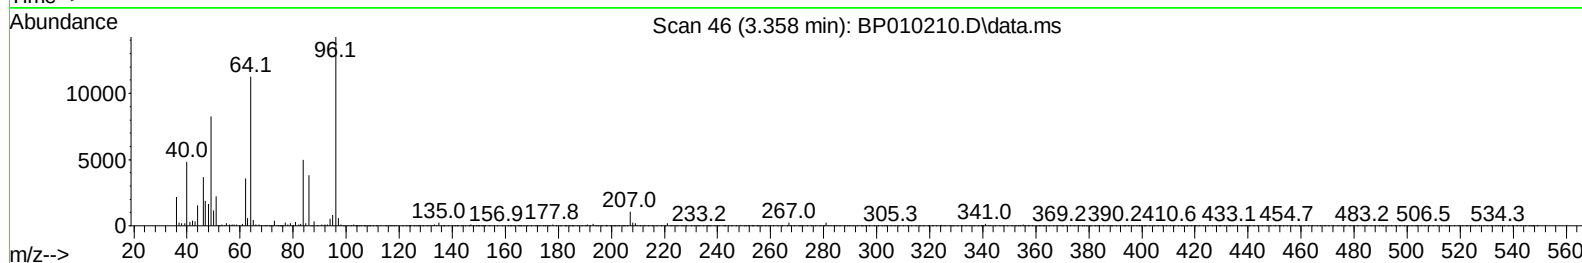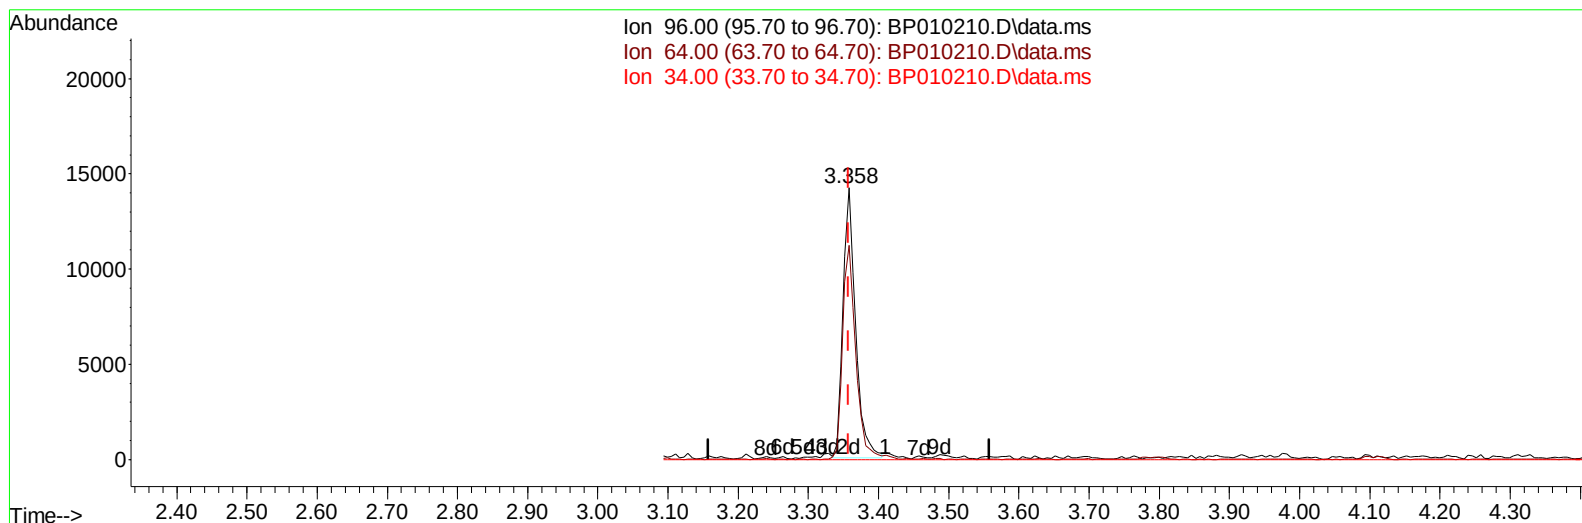

TIC: BP010210.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (+ 0.000) 4.83 ng/uL m

response 17736

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	78.98#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010210.D
Acq On : 03 May 2022 16:43
Operator : CG/JU
Sample : N2615-18
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0D8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:10:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

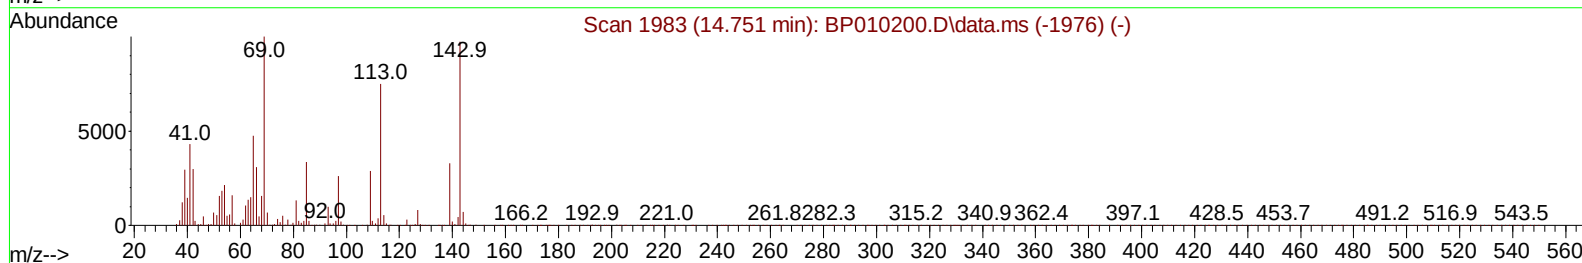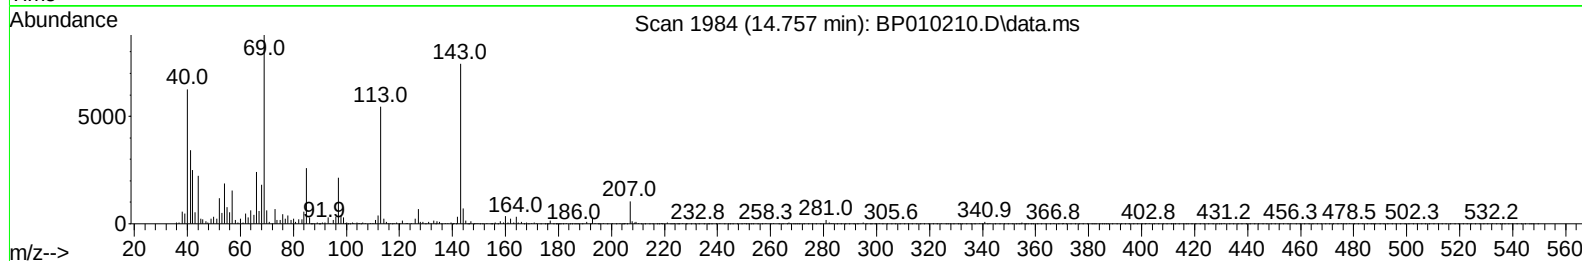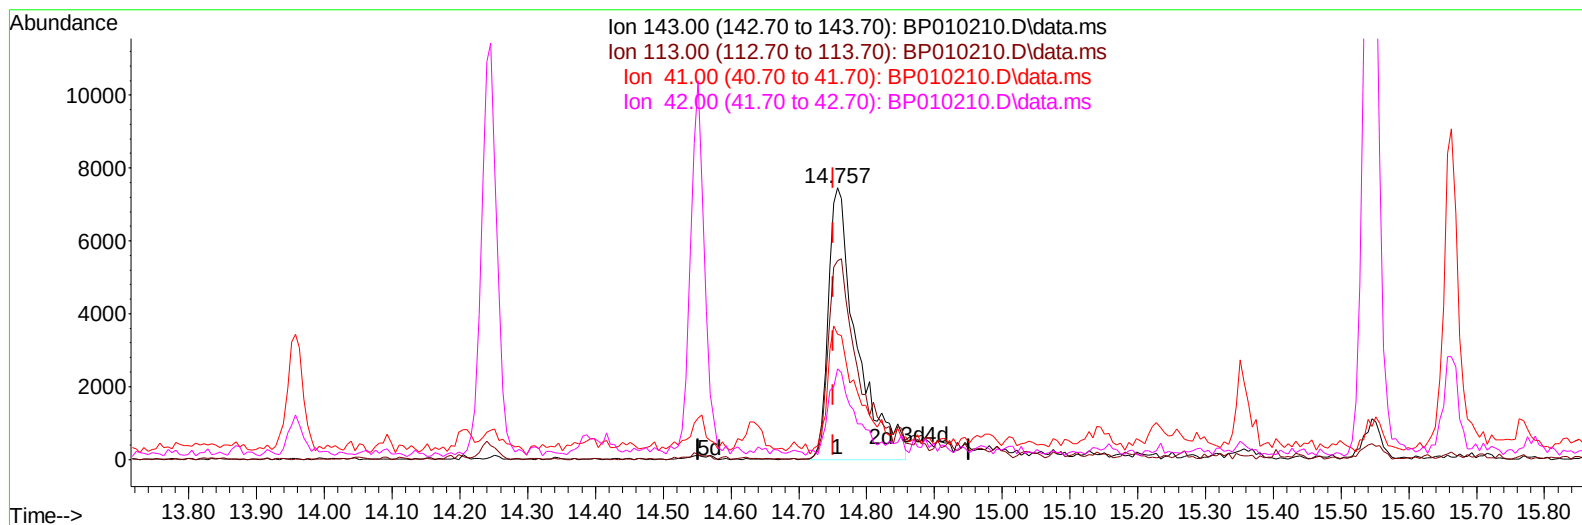

TIC: BP010210.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.006) 3.37 ng/ul m

response 21779

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	73.16#
41.00	23.20	46.16#
42.00	18.00	33.49#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010210.D
 Acq On : 03 May 2022 16:43
 Operator : CG/JU
 Sample : N2615-18
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0D8

Manual IntegrationsAPPROVED

Quant Time: May 04 01:10:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.916	152		160159	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136		689918	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164		451033	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188		848938	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240		642031	20.000	ng/ul	# 0.00
88) Perylene-d12	23.827	264		610164	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.358	96		17736m	4.829	ng/uL	0.00
4) Pyridine-d5	3.781	84		60143	5.821	ng/ul	0.00
7) Phenol-d5	7.081	99		81960	5.626	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67		310621	35.535	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132		269135	24.946	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113		176719	14.641	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128		191974	34.986	ng/ul	0.00
24) 2-Nitrophenol-d4	9.805	143		195467	32.617	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165		316773	27.152	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131		384351	22.977	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166		1236408	35.240	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160		1379165	32.479	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143		21779m	3.372	ng/ul	0.00
60) Fluorene-d10	15.545	176		1030955	34.160	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200		129773	24.176	ng/ul	0.00
73) Anthracene-d10	17.404	188		1595595	38.850	ng/ul	0.00
81) Pyrene-d10	19.633	212		1649054	45.164	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.674	264		1323108	41.362	ng/ul	0.00
Target Compounds							
						Qvalue	
16) Acetophenone	8.740	105		23721	1.260	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010210.D
Acq On : 03 May 2022 16:43
Operator : CG/JU
Sample : N2615-18
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0D8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:10:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

