




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 09:59:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

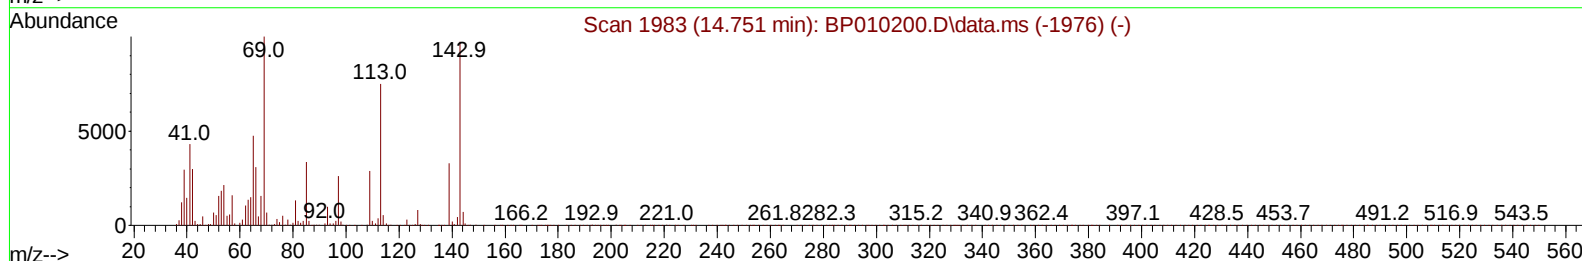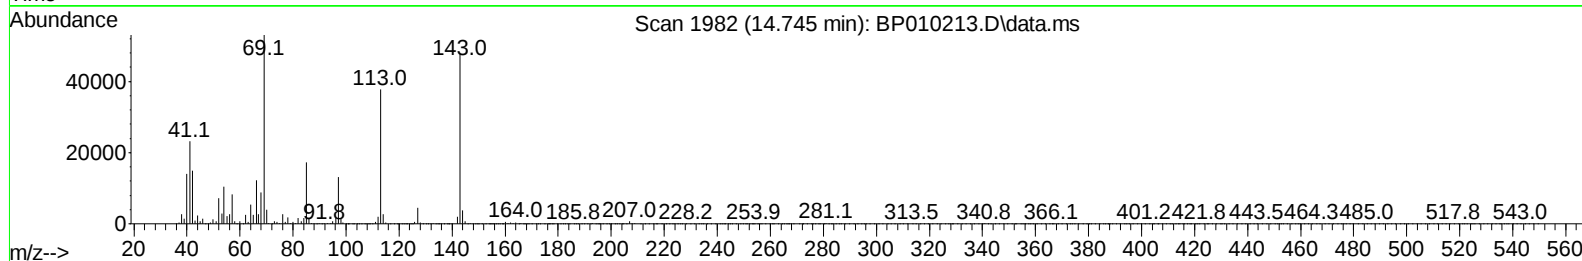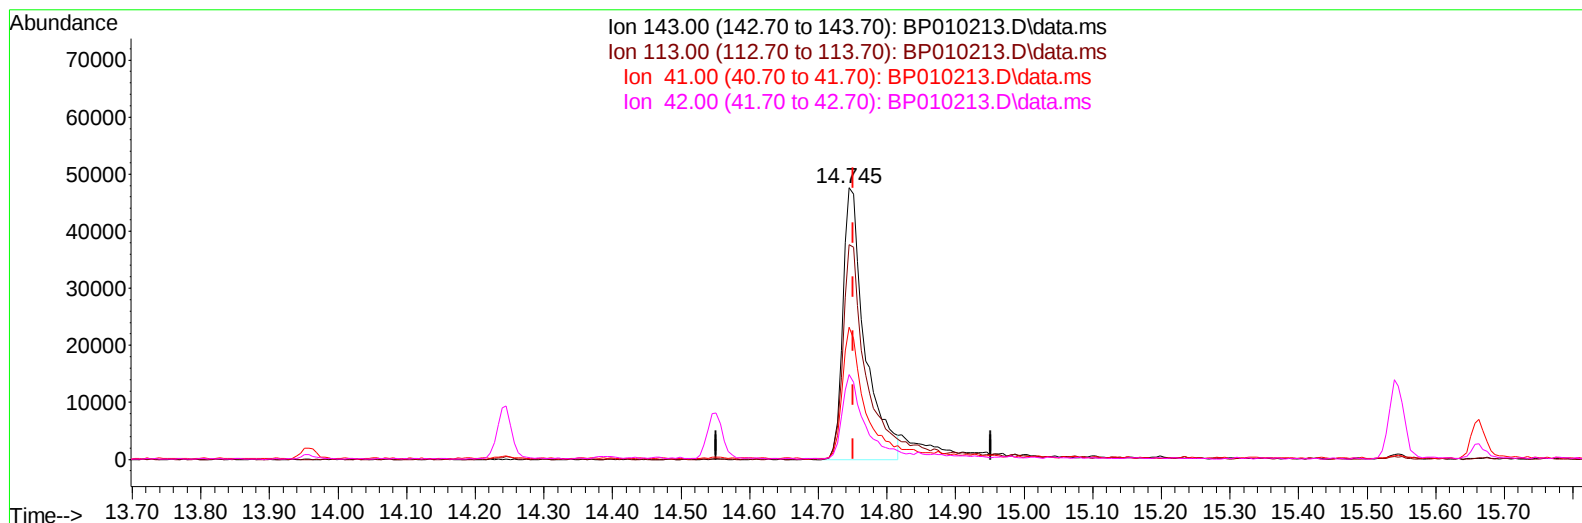

TIC: BP010213.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (-0.006) 18.52 ng/u1

response 106303

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.22#
41.00	23.20	48.59#
42.00	18.00	31.29#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 09:59:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

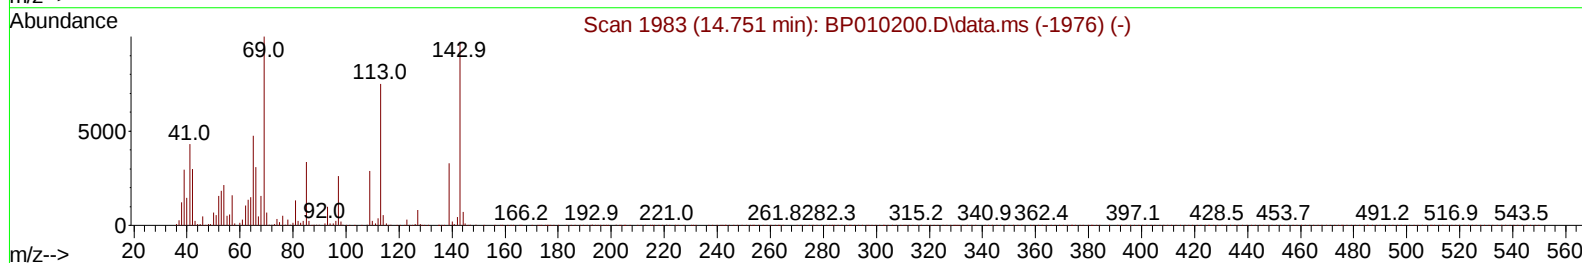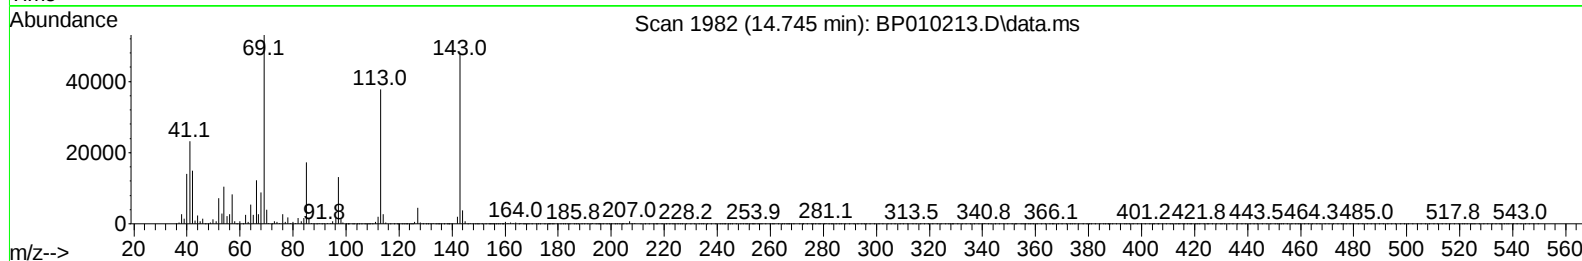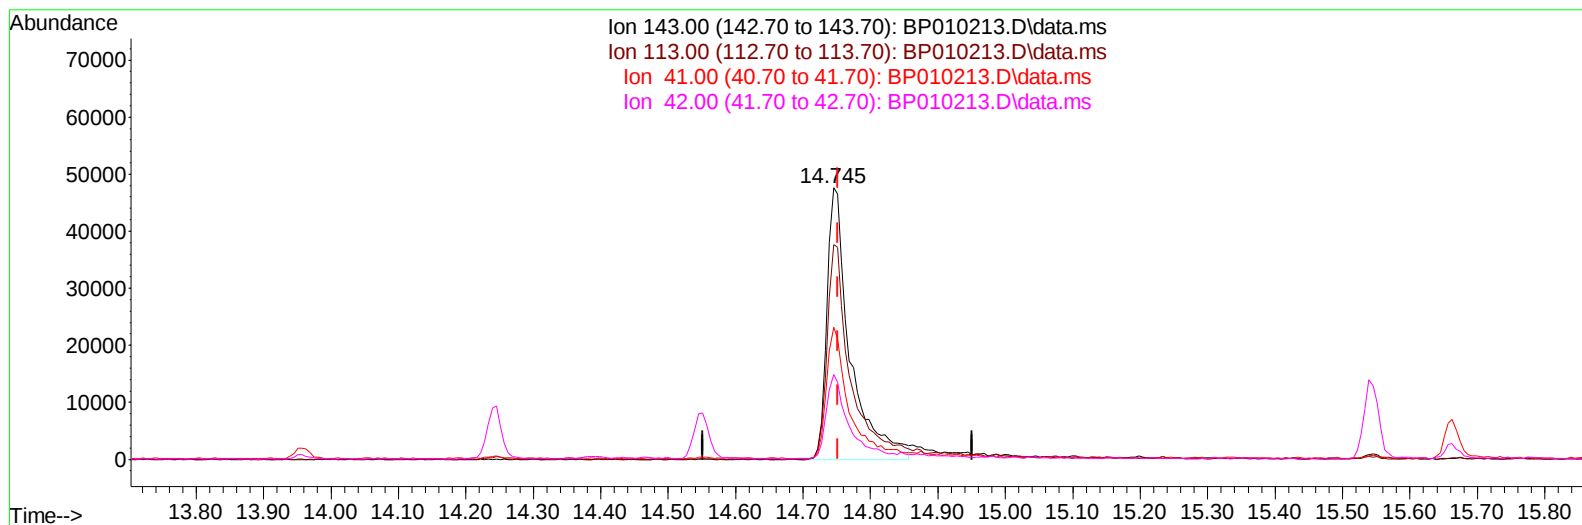

TIC: BP010213.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (-0.006) 19.86 ng/ul m

response 113954

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.22#
41.00	23.20	48.59#
42.00	18.00	31.29#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010213.D
 Acq On : 03 May 2022 18:24
 Operator : CG/JU
 Sample : PB144543BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 09:59:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	155390	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	642485	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	400717	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	819615	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	754501	20.000	ng/ul	# 0.00
88) Perylene-d12	23.827	264	706528	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	21604	6.063	ng/uL	0.00
4) Pyridine-d5	3.769	84	280442	27.975	ng/ul	0.00
7) Phenol-d5	7.081	99	349142	24.702	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	247854	29.224	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	292289	27.923	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	293594	25.071	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	145291	28.433	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	158163	28.341	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	268840	24.745	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	390978	25.098	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	898381	28.821	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1035232	27.441	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	113954m	19.858	ng/ul	0.00
60) Fluorene-d10	15.545	176	769785	28.709	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	106983	20.643	ng/ul	0.00
73) Anthracene-d10	17.404	188	1170845	29.528	ng/ul	0.00
81) Pyrene-d10	19.633	212	1369519	31.917	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1155627	31.199	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 09:59:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

