




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010216.D
 Acq On : 03 May 2022 20:38
 Operator : CG/JU
 Sample : PB144510BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK510

Manual IntegrationsAPPROVED

Quant Time: May 04 01:24:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

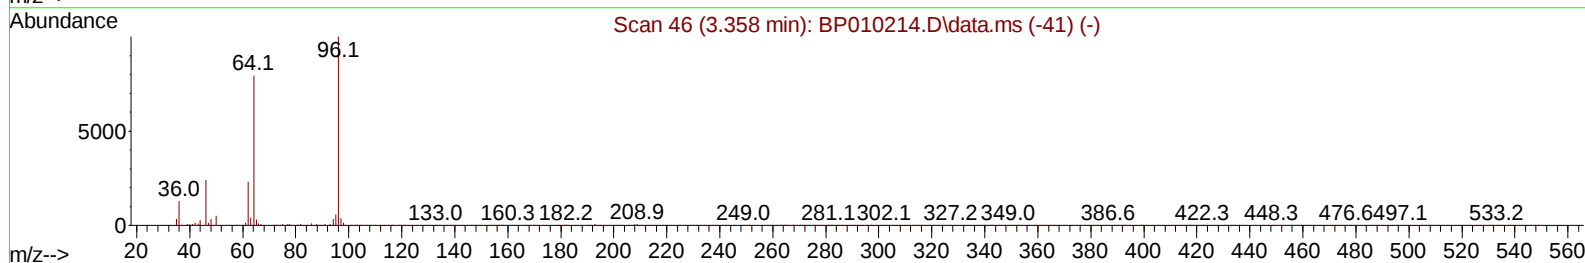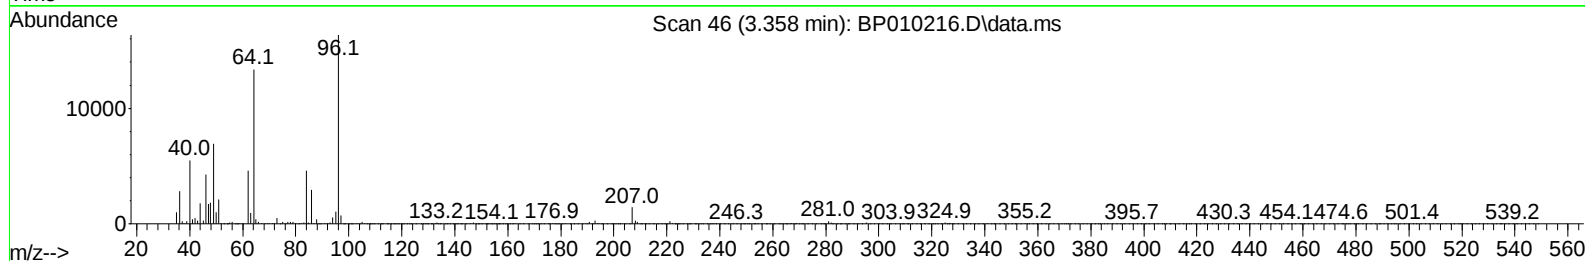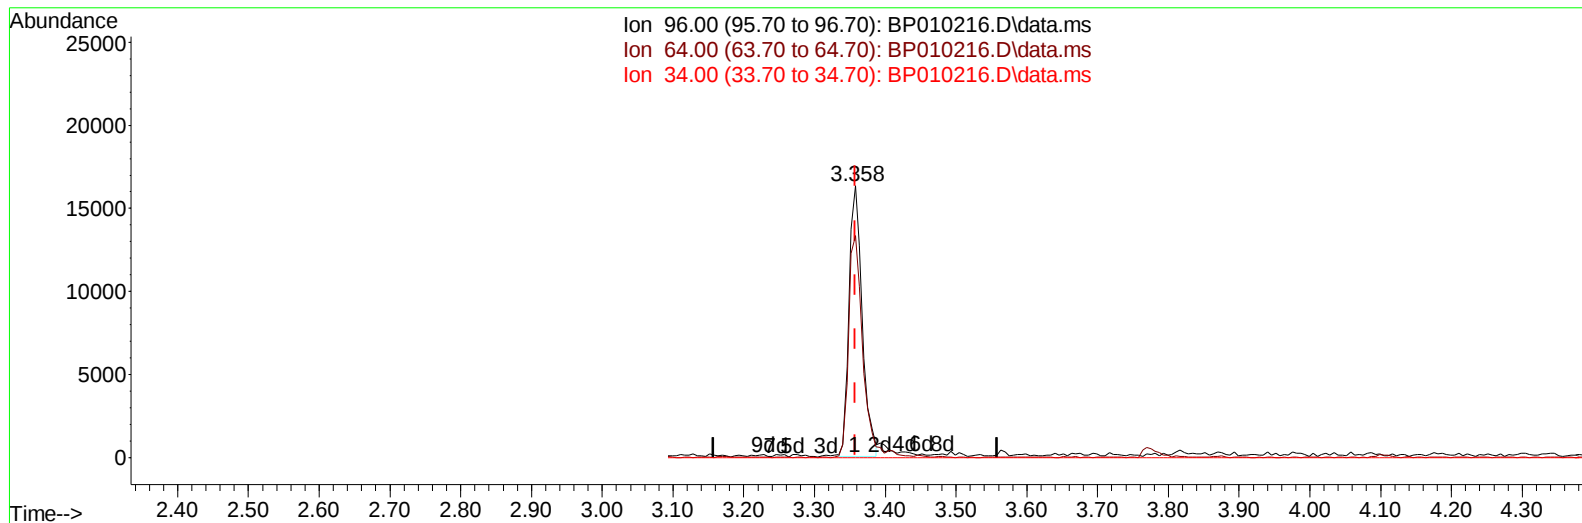

TIC: BP010216.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 5.35 ng/uL

response 21176

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	81.72#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010216.D
 Acq On : 03 May 2022 20:38
 Operator : CG/JU
 Sample : PB144510BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK510

Manual IntegrationsAPPROVED

Quant Time: May 04 01:24:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

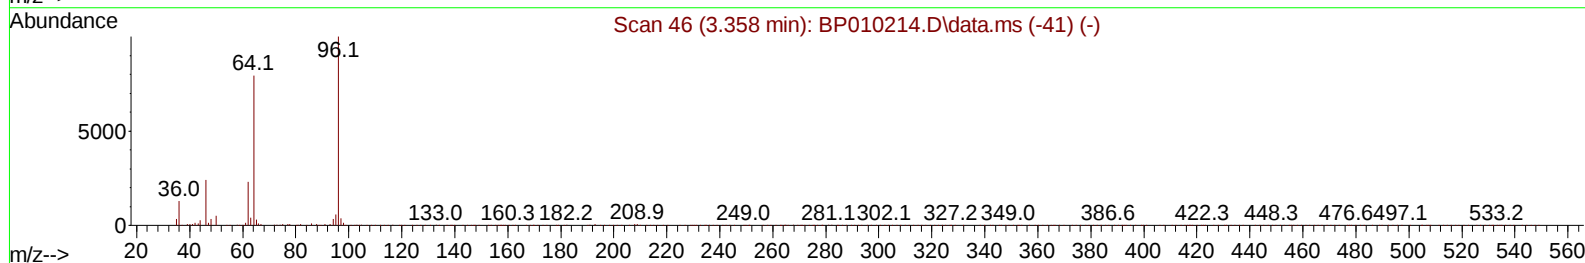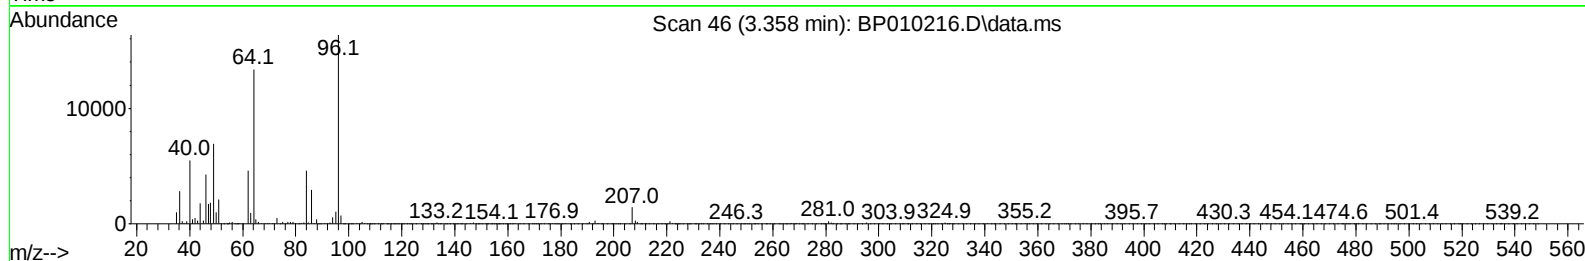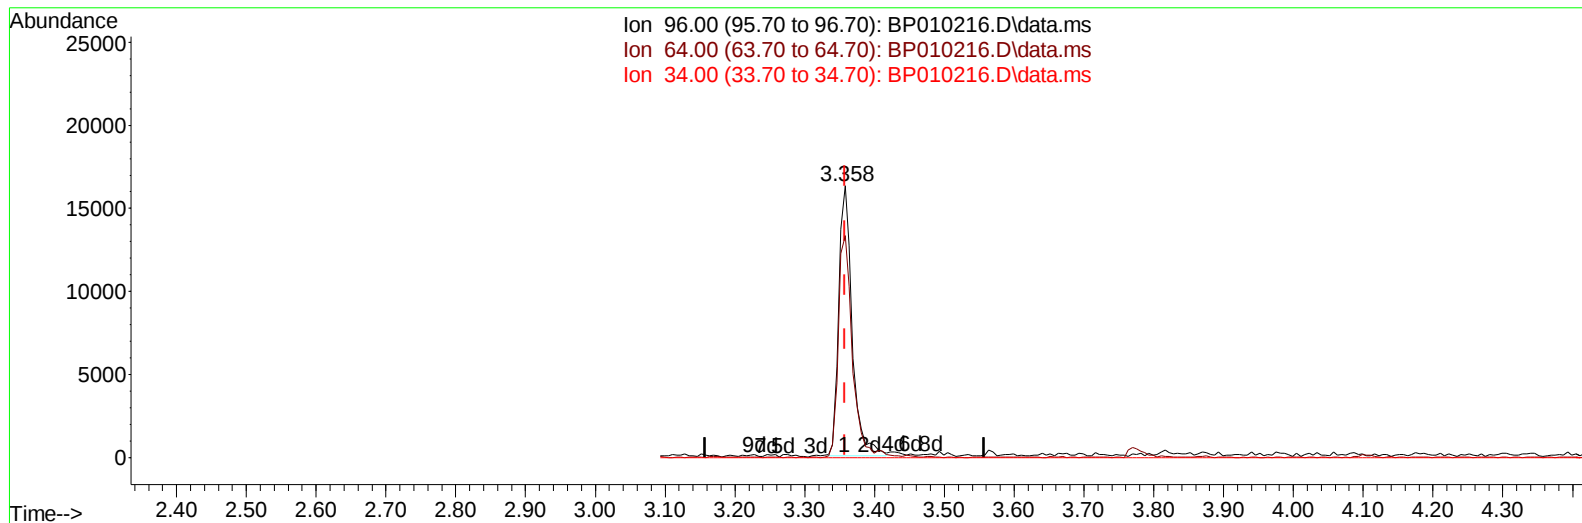

TIC: BP010216.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 5.49 ng/uL m

response 21720

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	81.72#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010216.D
 Acq On : 03 May 2022 20:38
 Operator : CG/JU
 Sample : PB144510BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK510

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:24:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	172612	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	731414	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	455795	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	855355	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.386	240	694671	20.000	ng/ul	# 0.00
88) Perylene-d12	23.827	264	668126	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	21720m	5.487	ng/uL	0.00
4) Pyridine-d5	3.769	84	306703	27.542	ng/ul	0.00
7) Phenol-d5	7.081	99	386921	24.644	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	281389	29.868	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	323043	27.782	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	332156	25.534	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	169415	29.123	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	183363	28.861	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.345	165	310020	25.066	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	443283	24.996	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1039365	29.314	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1178731	27.469	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	115537	17.701	ng/ul	0.00
60) Fluorene-d10	15.545	176	863559	28.314	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	111372	20.592	ng/ul	0.00
73) Anthracene-d10	17.404	188	1211160	29.268	ng/ul	0.00
81) Pyrene-d10	19.633	212	1328431	33.626	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1074708	30.682	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010216.D
Acq On : 03 May 2022 20:38
Operator : CG/JU
Sample : PB144510BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK510

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:24:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

