




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010219.D
 Acq On : 03 May 2022 22:19
 Operator : CG/JU
 Sample : N2670-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COW00

Manual IntegrationsAPPROVED

Quant Time: May 04 01:25:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

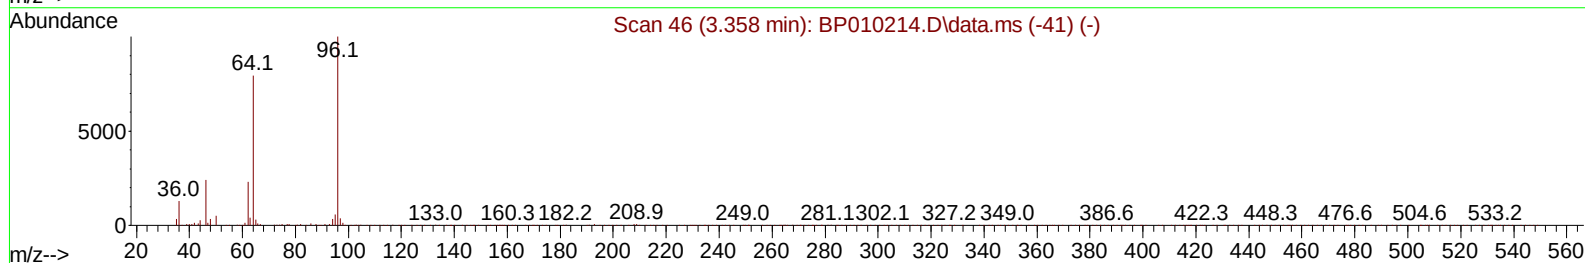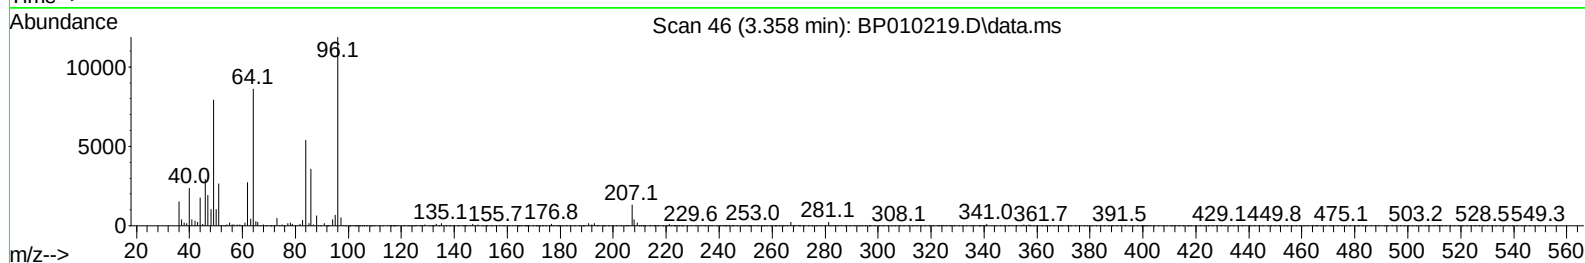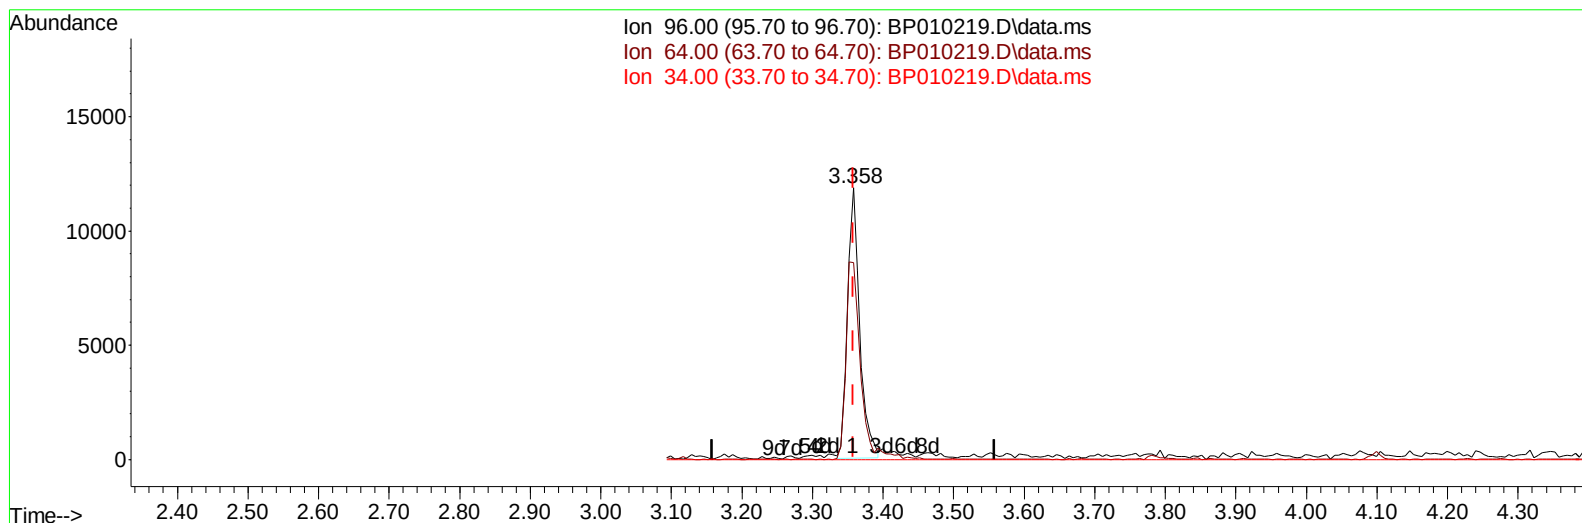

TIC: BP010219.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 4.31 ng/uL

response 14402

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	72.53#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010219.D
 Acq On : 03 May 2022 22:19
 Operator : CG/JU
 Sample : N2670-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COW00

Manual IntegrationsAPPROVED

Quant Time: May 04 01:25:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

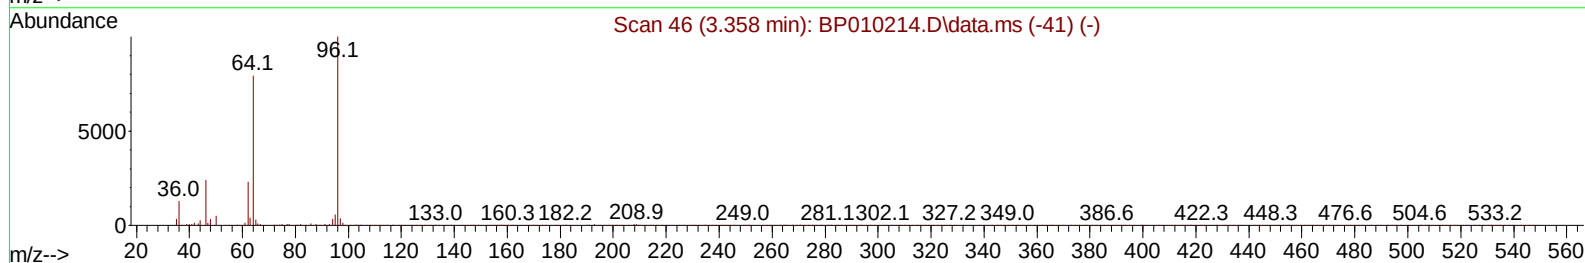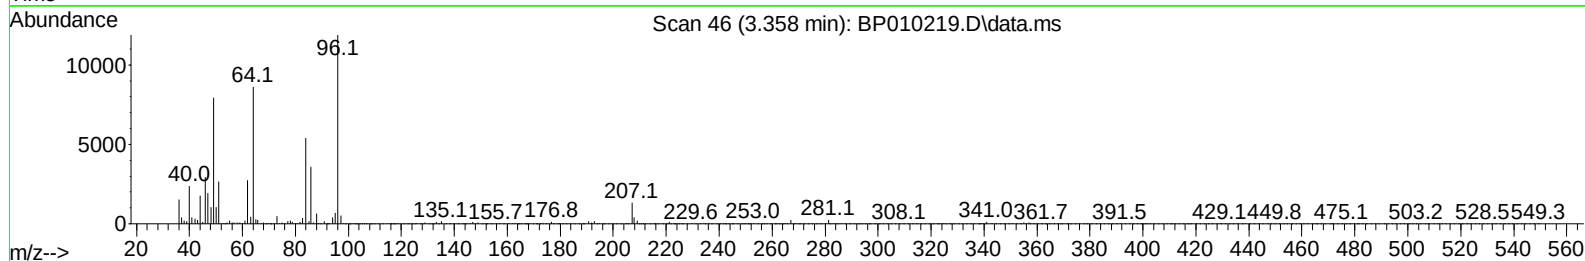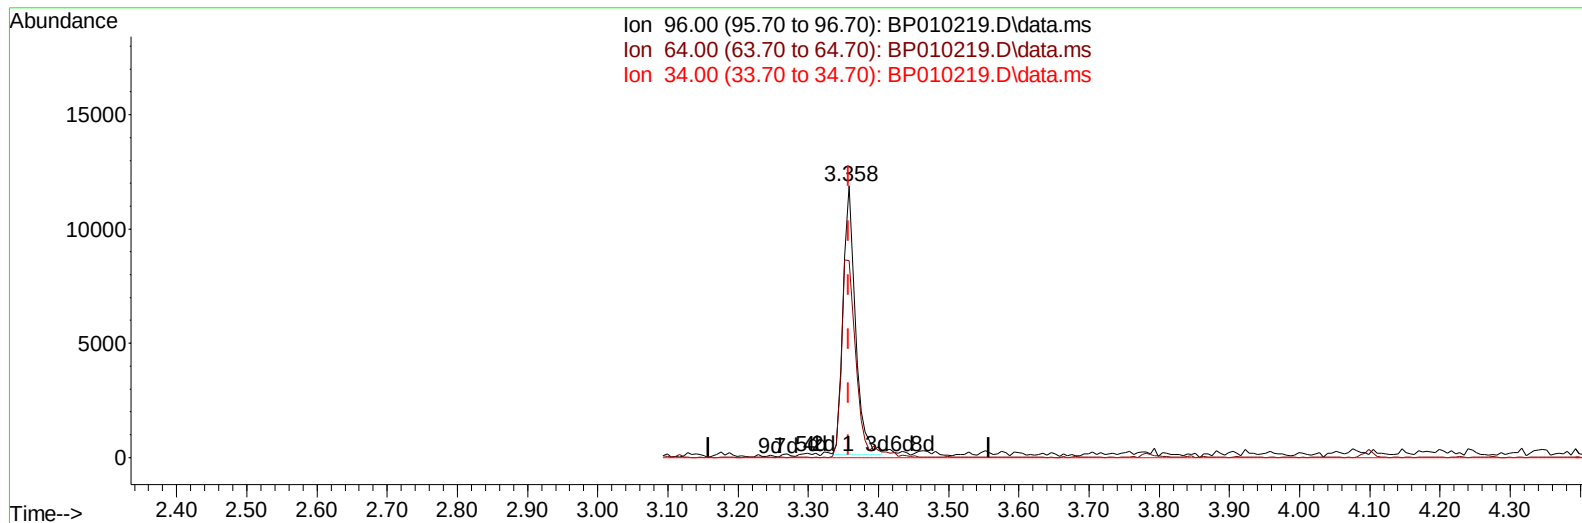

TIC: BP010219.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 4.30 ng/uL m

response 14361

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	72.53#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW00

Manual IntegrationsAPPROVED

Quant Time: May 04 01:25:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

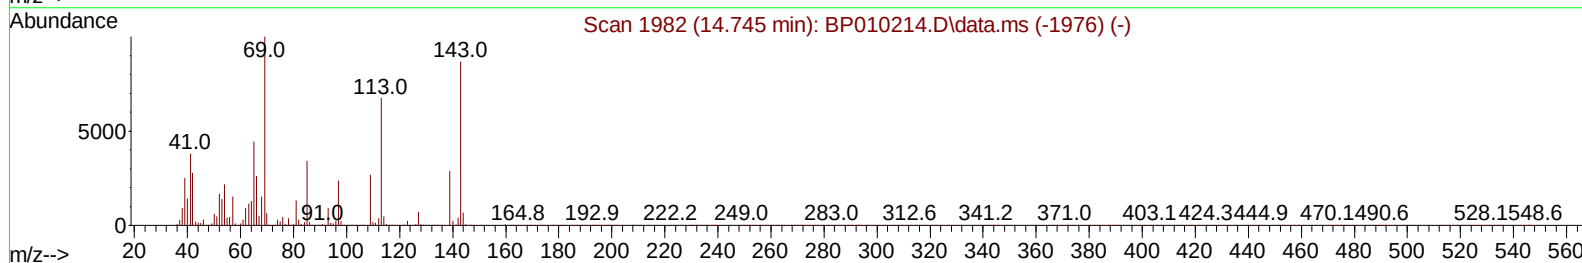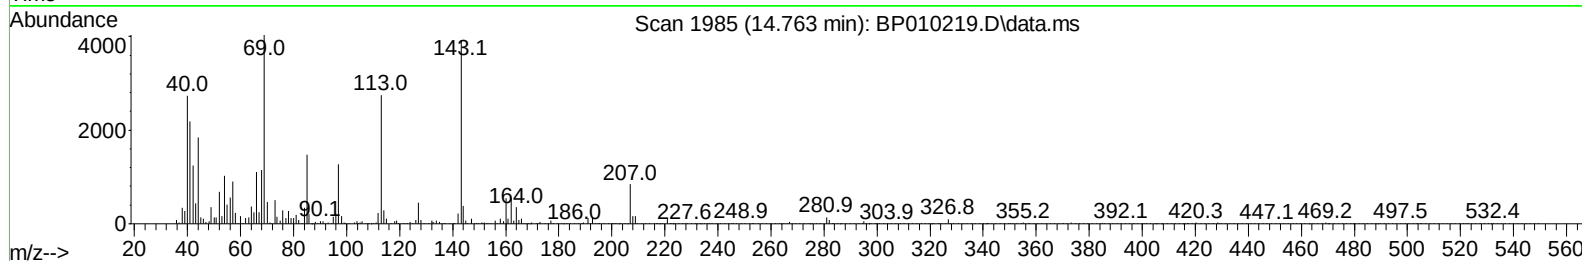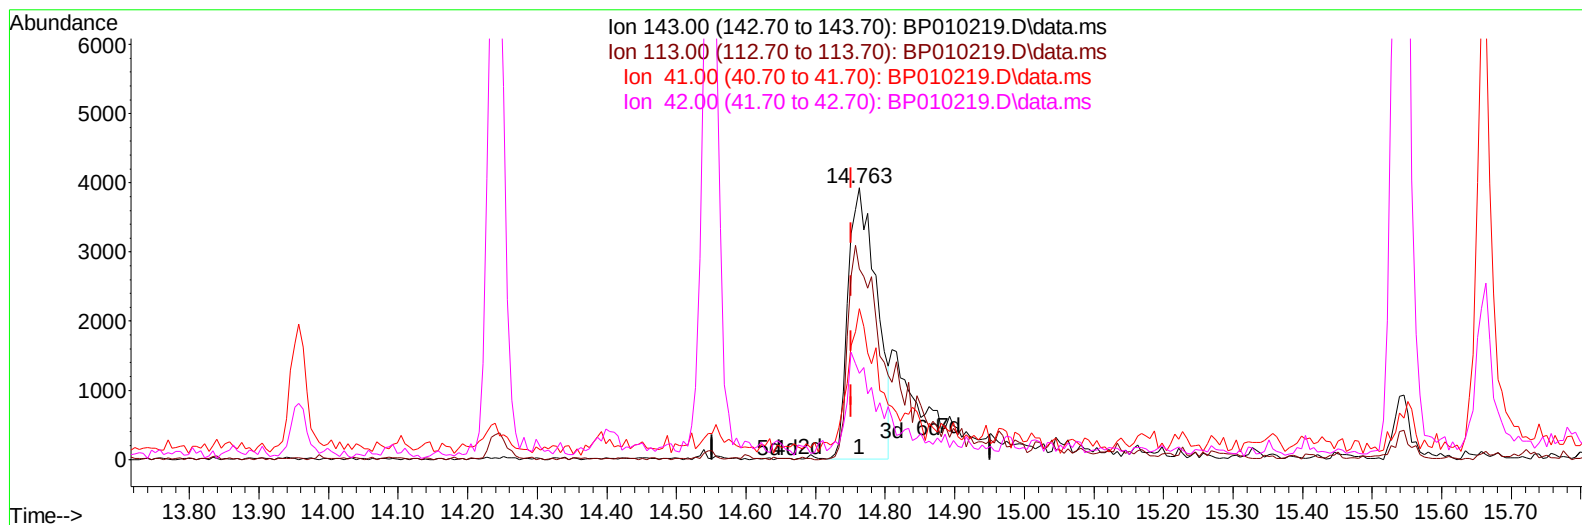

TIC: BP010219.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.012) 1.96 ng/ul

response 11123

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	70.10#
41.00	23.20	55.60#
42.00	18.00	31.81#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW00

Manual IntegrationsAPPROVED

Quant Time: May 04 01:25:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

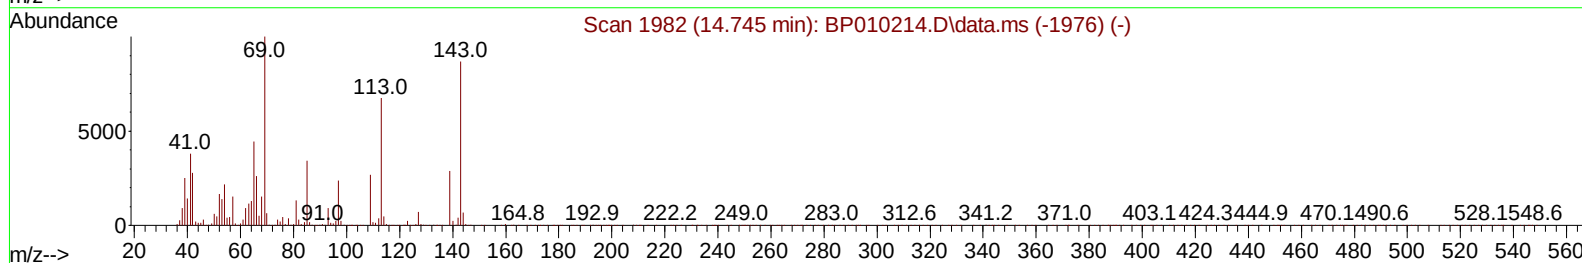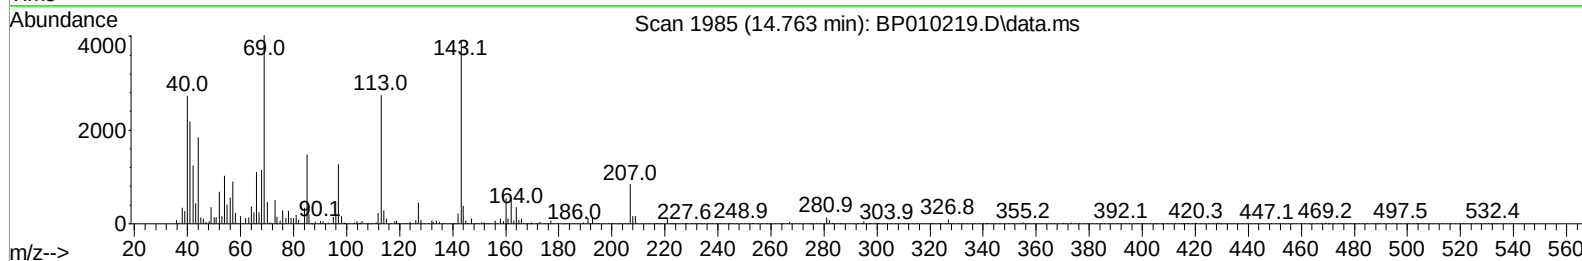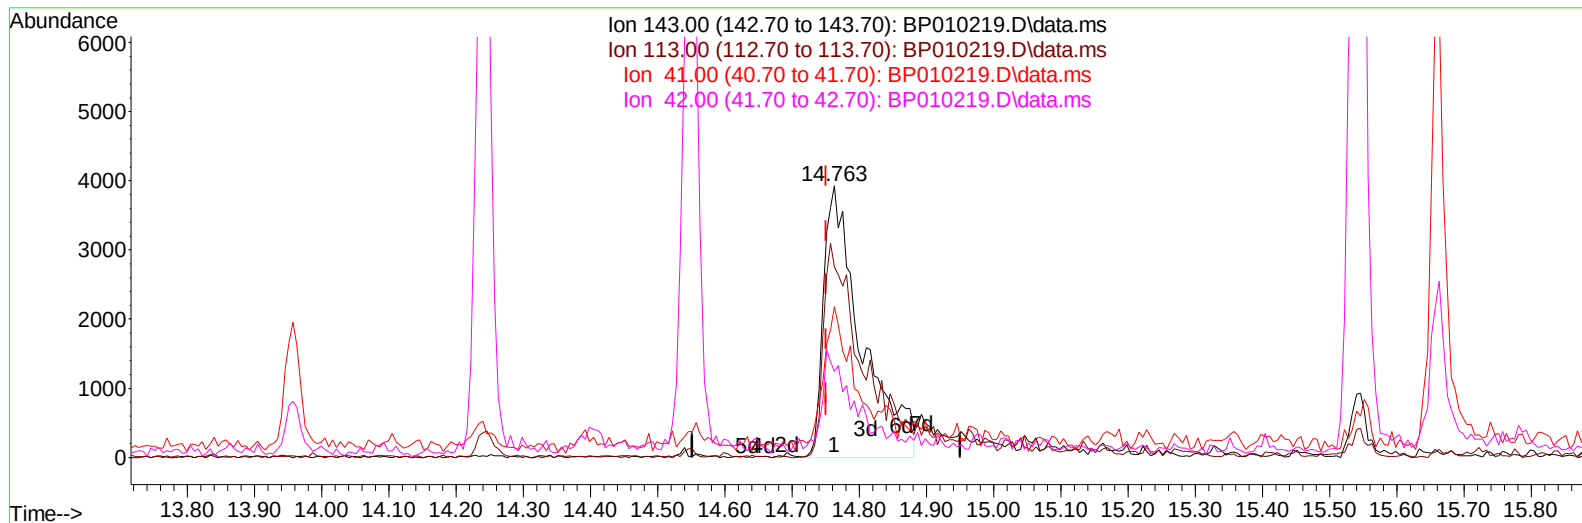

TIC: BP010219.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (+ 0.012) 2.71 ng/ul m

response 15409

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	70.10#
41.00	23.20	55.60#
42.00	18.00	31.81#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010219.D
 Acq On : 03 May 2022 22:19
 Operator : CG/JU
 Sample : N2670-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COW00

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:25:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	145665	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	603653	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	396604	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	816145	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.380	240	735967	20.000	ng/ul	#-0.01
88) Perylene-d12	23.827	264	707945	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	14361m	4.299	ng/uL	0.00
4) Pyridine-d5	3.781	84	56842	6.049	ng/ul	0.00
7) Phenol-d5	7.081	99	59080	4.459	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	239217	30.089	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	205266	20.919	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	123585	11.258	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	142169	29.612	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	141571	26.999	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	227067	22.245	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	284498	19.438	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	910779	29.522	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	1036743	27.766	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.763	143	15409m	2.713	ng/ul	0.01
60) Fluorene-d10	15.545	176	800631	30.169	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	106504	20.638	ng/ul	0.00
73) Anthracene-d10	17.398	188	1282588	32.484	ng/ul	-0.01
81) Pyrene-d10	19.633	212	1464789	34.997	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.668	264	1243681	33.509	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW00

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:25:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

