

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010170.D
 Acq On : 02 May 2022 13:36
 Operator : CG/JU
 Sample : N2562-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW476

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 03 01:07:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	149151	20.000	ng/u1	0.00
20) Naphthalene-d8	10.728	136	591376	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.557	164	346413	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	662764	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.392	240	618653	20.000	ng/u1	# 0.00
88) Perylene-d12	23.839	264	626290	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	15573m	4.553	ng/uL	0.00
4) Pyridine-d5	3.781	84	77588	8.063	ng/u1	0.00
7) Phenol-d5	7.087	99	268256	19.773	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.252	67	192243	23.615	ng/u1	0.00
11) 2-Chlorophenol-d4	7.458	132	228233	22.716	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	223179	19.855	ng/u1	0.00
21) Nitrobenzene-d5	9.081	128	111942	23.800	ng/u1	0.00
24) 2-Nitrophenol-d4	9.805	143	120584	23.474	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	195253	19.525	ng/u1	0.00
31) 4-Chloroaniline-d4	10.863	131	250972	17.503	ng/u1	0.00
46) Dimethylphthalate-d6	13.963	166	652482	24.213	ng/u1	0.00
49) Acenaphthylene-d8	14.251	160	732357	22.456	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	50513m	10.182	ng/u1	0.00
60) Fluorene-d10	15.551	176	550384	23.744	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	20423m	4.873	ng/u1	0.00
73) Anthracene-d10	17.410	188	812474	25.339	ng/u1	0.00
81) Pyrene-d10	19.639	212	970285	27.578	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	908905	27.682	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.298	149	28204	1.126	ng/u1#	Qvalue 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010170.D
Acq On : 02 May 2022 13:36
Operator : CG/JU
Sample : N2562-15
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EW476

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
Supervised By :Yogesh Patel 05/05/2022


Quant Time: May 03 01:07:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

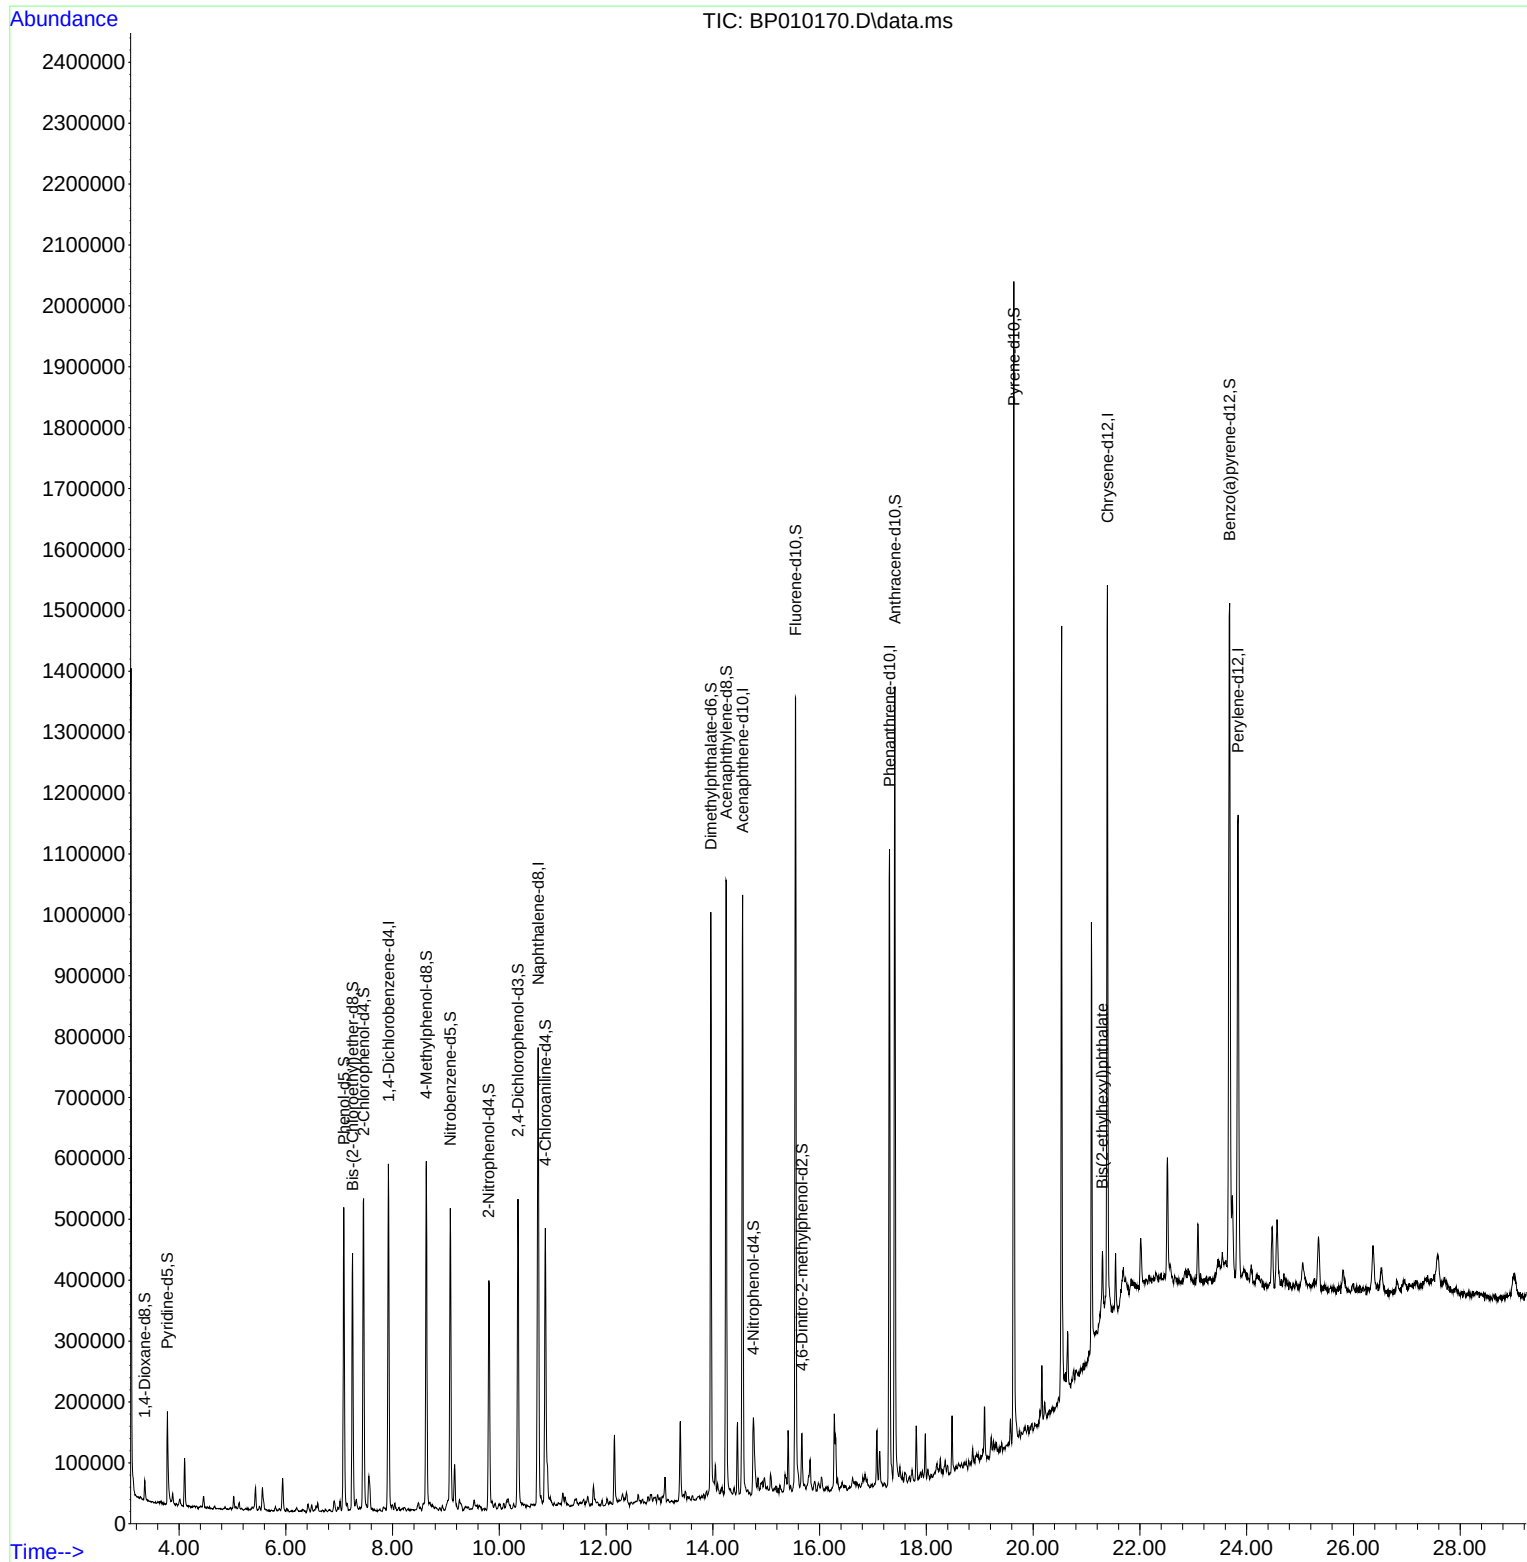

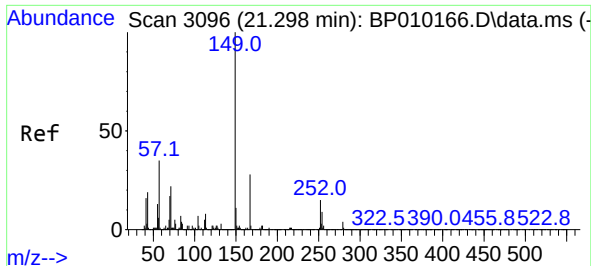

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.126 ng/ul
 RT: 21.298 min Scan# 3096
 Delta R.T. -0.000 min
 Lab File: BP010170.D
 Acq: 02 May 2022 13:36

Instrument :
 BNA_P
 ClientSampleId :
 EW476

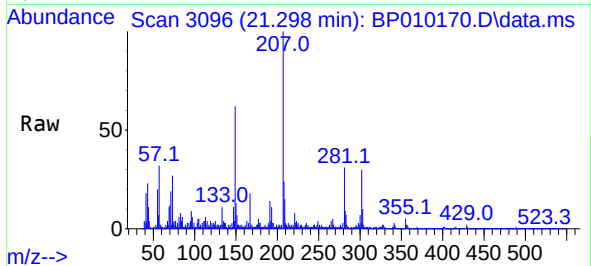

Tgt Ion:149 Resp: 28204

Ion	Ratio	Lower	Upper
149	100		
167	28.3	32.8	49.2
279	4.6	5.6	8.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/03/2022
 Supervised By :Yogesh Patel 05/05/2022

