

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010210.D
 Acq On : 03 May 2022 16:43
 Operator : CG/JU
 Sample : N2615-18
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0D8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 01:10:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 00:58:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	160159	20.000	ng/u1	0.00
20) Naphthalene-d8	10.722	136	689918	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.551	164	451033	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	848938	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.386	240	642031	20.000	ng/u1	# 0.00
88) Perylene-d12	23.827	264	610164	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	17736m	4.829	ng/uL	0.00
4) Pyridine-d5	3.781	84	60143	5.821	ng/u1	0.00
7) Phenol-d5	7.081	99	81960	5.626	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	310621	35.535	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	269135	24.946	ng/u1	0.00
15) 4-Methylphenol-d8	8.628	113	176719	14.641	ng/u1	0.00
21) Nitrobenzene-d5	9.075	128	191974	34.986	ng/u1	0.00
24) 2-Nitrophenol-d4	9.805	143	195467	32.617	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.346	165	316773	27.152	ng/u1	0.00
31) 4-Chloroaniline-d4	10.857	131	384351	22.977	ng/u1	0.00
46) Dimethylphthalate-d6	13.963	166	1236408	35.240	ng/u1	0.00
49) Acenaphthylene-d8	14.245	160	1379165	32.479	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	21779m	3.372	ng/u1	0.00
60) Fluorene-d10	15.545	176	1030955	34.160	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	129773	24.176	ng/u1	0.00
73) Anthracene-d10	17.404	188	1595595	38.850	ng/u1	0.00
81) Pyrene-d10	19.633	212	1649054	45.164	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.674	264	1323108	41.362	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.740	105	23721	1.260	ng/u1#	Qvalue 75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010210.D
Acq On : 03 May 2022 16:43
Operator : CG/JU
Sample : N2615-18
Misc :
ALS Vial : 46 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
BH0D8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022


Quant Time: May 04 01:10:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 00:58:32 2022
Response via : Initial Calibration

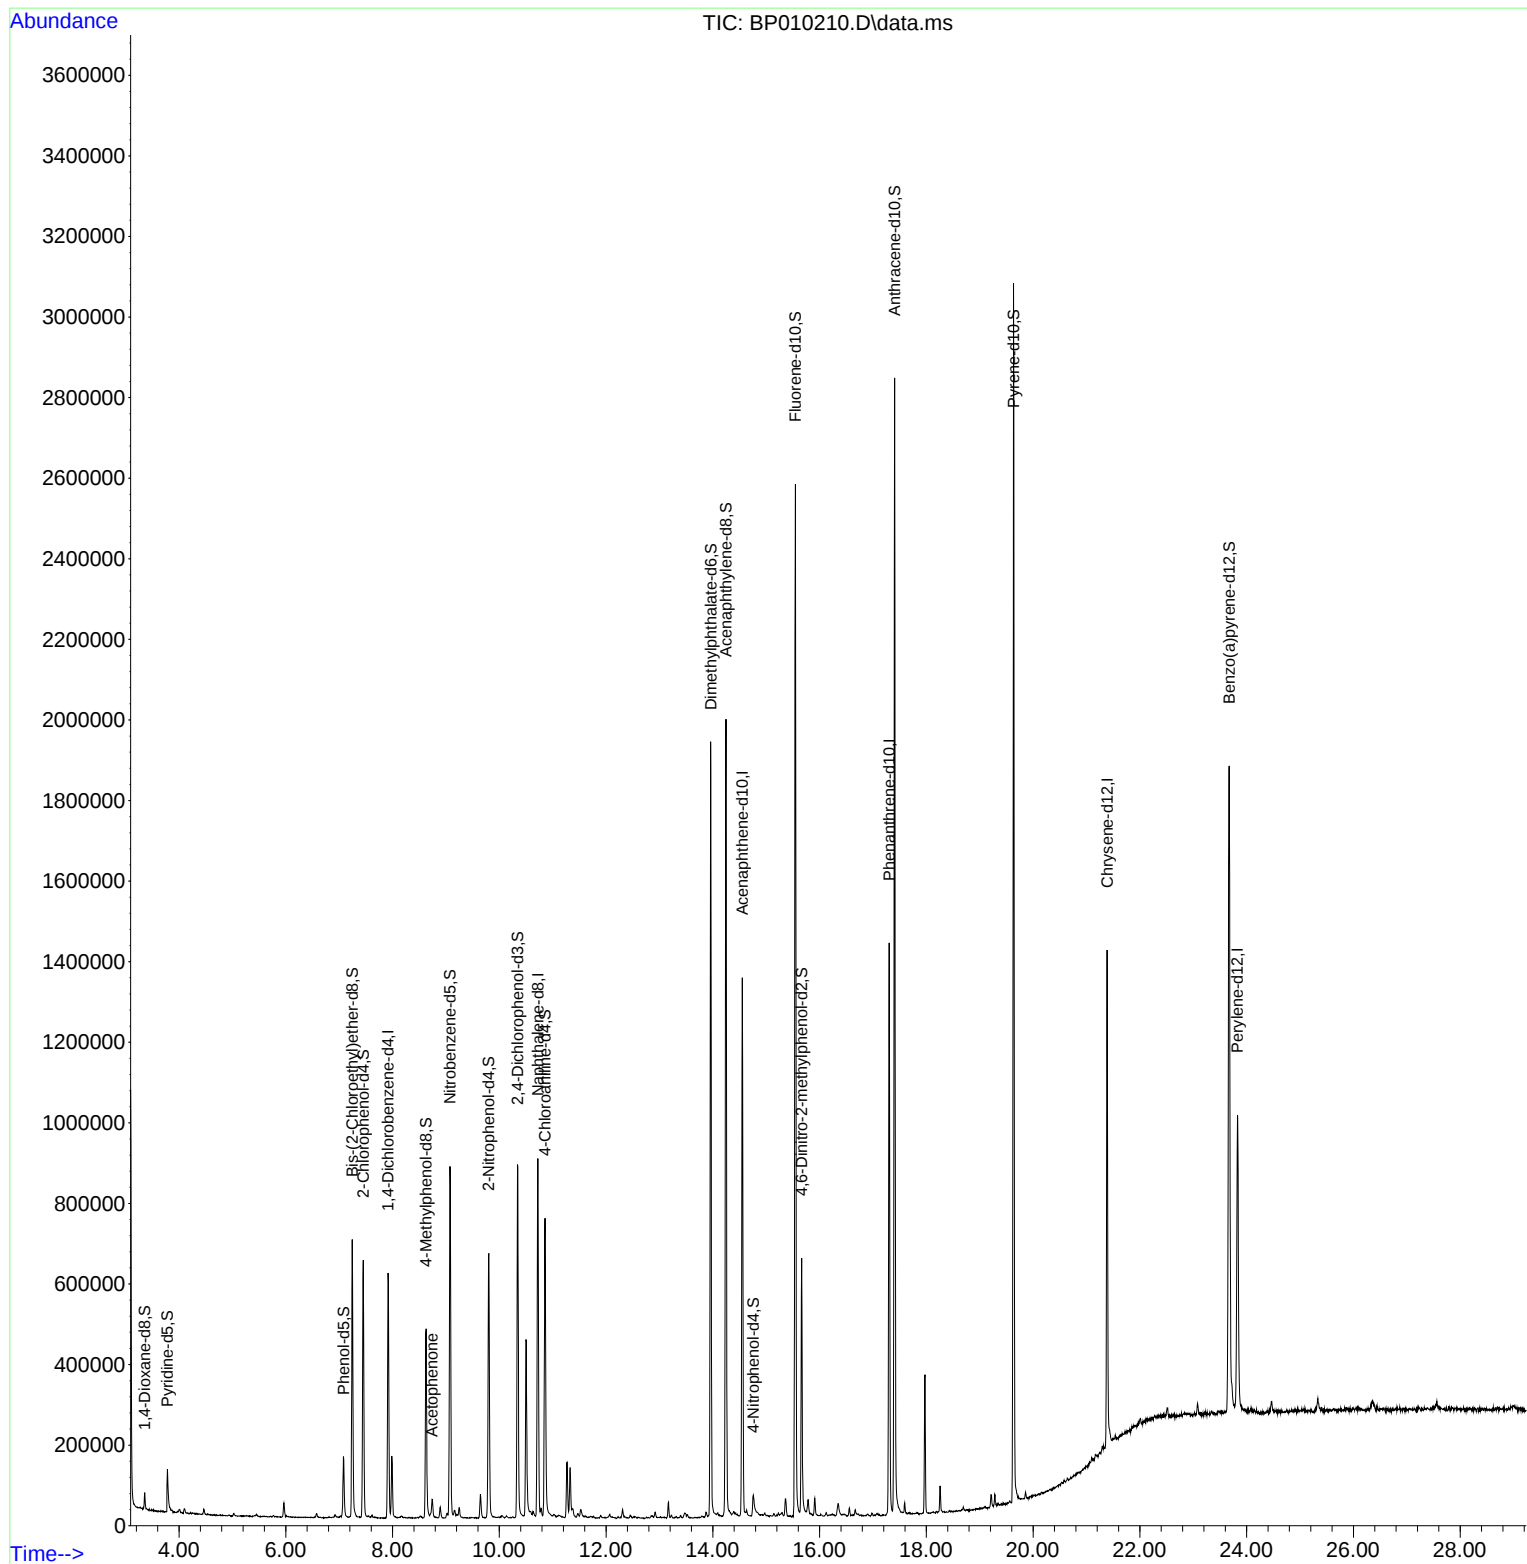

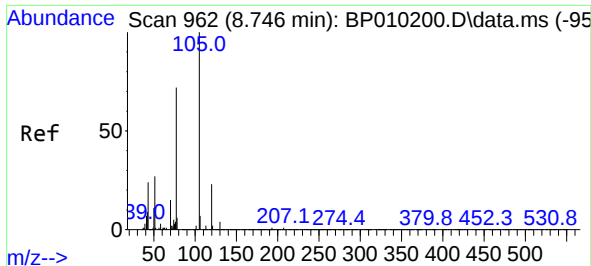

#16
Acetophenone
Concen: 1.260 ng/ul
RT: 8.740 min Scan# 90
Delta R.T. -0.006 min
Lab File: BP010210.D
Acq: 03 May 2022 16:43

Instrument :
BNA_P
ClientSampleId :
BH0D8

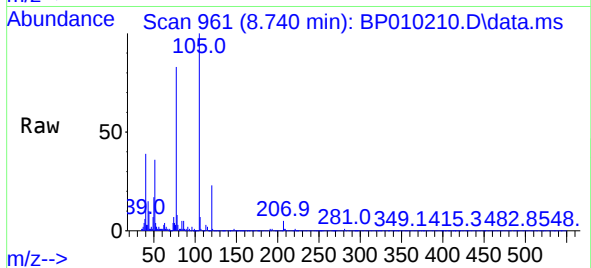

Tgt Ion:105 Resp: 2372
Ion Ratio Lower Upper
105 100
77 83.5 53.4 80.2
51 36.2 13.8 20.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

