

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	55	rVB	19568	28306	1.66%	0.135%
2	3.787	116	119	130	rBV	68735	110360	6.48%	0.528%
3	3.875	132	134	141	rVB3	13848	18468	1.08%	0.088%
4	4.017	153	158	163	rVB3	8642	14731	0.87%	0.070%
5	4.105	170	173	184	rVB4	13287	21432	1.26%	0.103%
6	4.334	207	212	216	rBV6	8191	12360	0.73%	0.059%
7	4.746	278	282	286	rBV7	2954	5304	0.31%	0.025%
8	4.799	289	291	293	rBV3	2544	2021	0.12%	0.010%
9	4.928	311	313	316	rBV4	2181	2297	0.13%	0.011%
10	5.022	325	329	337	rBV3	11145	17506	1.03%	0.084%
11	5.099	340	342	344	rBV3	2507	2353	0.14%	0.011%
12	5.128	344	347	348	rBV2	2304	2331	0.14%	0.011%
13	5.175	353	355	357	rVB3	2810	2231	0.13%	0.011%
14	5.481	405	407	410	rVB4	2502	2741	0.16%	0.013%
15	5.893	473	477	485	rVB4	2298	3178	0.19%	0.015%
16	6.028	495	500	501	rBV5	1869	2776	0.16%	0.013%
17	6.922	648	652	653	rBV4	2759	2532	0.15%	0.012%
18	6.946	653	656	658	rVB4	2388	2263	0.13%	0.011%
19	7.016	667	668	672	rBV3	1504	2130	0.13%	0.010%
20	7.087	672	680	693	rVV	275853	465216	27.33%	2.226%
21	7.252	701	708	719	rVV	243739	401382	23.58%	1.921%
22	7.328	719	721	728	rVB7	2554	5337	0.31%	0.026%
23	7.458	736	743	754	rBV	295357	488883	28.72%	2.339%
24	7.552	756	759	766	rVB6	6674	11027	0.65%	0.053%
25	7.705	783	785	790	rVV6	1395	2135	0.13%	0.010%
26	7.752	790	793	796	rVB5	2655	2227	0.13%	0.011%
27	7.852	806	810	812	rBV5	1549	2428	0.14%	0.012%
28	7.922	812	822	833	rBV	592335	968132	56.88%	4.632%
29	8.481	914	917	919	rVB4	2320	2687	0.16%	0.013%
30	8.634	935	943	954	rVV	275965	483069	28.38%	2.311%
31	8.746	958	962	971	rVV2	13343	27404	1.61%	0.131%
32	8.811	971	973	977	rVV5	2491	3054	0.18%	0.015%
33	9.081	1012	1019	1030	rBV	285296	497513	29.23%	2.381%
34	9.258	1045	1049	1053	rVV7	3568	6706	0.39%	0.032%
35	9.322	1056	1060	1062	rBV5	1652	2615	0.15%	0.013%
36	9.528	1091	1095	1101	rVB3	11932	19146	1.12%	0.092%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	9.810	1133	1143	1155	rBV	221086	404746	23.78%	1.937%
38	10.152	1199	1201	1205	rBV5	1665	2422	0.14%	0.012%
39	10.352	1225	1235	1245	rBV	304485	564074	33.14%	2.699%
40	10.728	1290	1299	1309	rBV	793865	1350094	79.32%	6.460%
41	10.799	1309	1311	1314	rVB4	2659	2230	0.13%	0.011%
42	10.863	1316	1322	1336	rBV	262533	516855	30.37%	2.473%
43	11.075	1355	1358	1362	rVB6	2170	3253	0.19%	0.016%
44	11.352	1403	1405	1408	rVB4	1778	2094	0.12%	0.010%
45	11.422	1414	1417	1421	rVB6	1684	2561	0.15%	0.012%
46	11.534	1432	1436	1437	rBV4	3805	4926	0.29%	0.024%
47	11.546	1437	1438	1448	rVB9	4441	8660	0.51%	0.041%
48	12.022	1512	1519	1524	rVB10	2317	4422	0.26%	0.021%
49	12.157	1536	1542	1551	rBV7	5884	10102	0.59%	0.048%
50	12.322	1564	1570	1573	rBV6	6465	11613	0.68%	0.056%
51	12.787	1643	1649	1650	rBV6	1789	2545	0.15%	0.012%
52	12.840	1653	1658	1659	rBV5	3427	5512	0.32%	0.026%
53	12.957	1677	1678	1686	rVB8	2241	3644	0.21%	0.017%
54	13.063	1692	1696	1698	rBV5	1779	2237	0.13%	0.011%
55	13.104	1701	1703	1709	rVB7	3380	4581	0.27%	0.022%
56	13.181	1713	1716	1718	rBV4	2452	2761	0.16%	0.013%
57	13.287	1731	1734	1738	rVB4	2137	3399	0.20%	0.016%
58	13.393	1747	1752	1758	rVB3	10979	18867	1.11%	0.090%
59	13.734	1806	1810	1811	rBV3	2372	2729	0.16%	0.013%
60	13.834	1824	1827	1829	rBV4	2101	2258	0.13%	0.011%
61	13.922	1836	1842	1843	rBV5	4101	5752	0.34%	0.028%
62	13.963	1843	1849	1861	rVV	578086	832510	48.91%	3.983%
63	14.051	1862	1864	1868	rVB5	4725	4180	0.25%	0.020%
64	14.169	1882	1884	1887	rVB4	2734	2065	0.12%	0.010%
65	14.251	1887	1898	1909	rBV	610583	975099	57.29%	4.666%
66	14.393	1917	1922	1926	rBV2	14089	25065	1.47%	0.120%
67	14.463	1932	1934	1940	rVB6	5133	6730	0.40%	0.032%
68	14.557	1942	1950	1961	rBV	1059276	1646860	96.75%	7.880%
69	14.763	1979	1985	2003	rBV	89496	244584	14.37%	1.170%
70	14.981	2016	2022	2026	rBV9	6588	13404	0.79%	0.064%
71	15.128	2041	2047	2050	rBV8	5506	9336	0.55%	0.045%
72	15.375	2083	2089	2093	rBV2	16787	26787	1.57%	0.128%
73	15.551	2112	2119	2133	rBV	797814	1238482	72.76%	5.926%
74	15.669	2133	2139	2146	rVV	113548	189800	11.15%	0.908%
75	15.792	2157	2160	2167	rVB8	9255	16145	0.95%	0.077%
76	15.922	2178	2182	2186	rVB7	3585	4276	0.25%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010171.D
 Acq On : 02 May 2022 14:10
 Operator : CG/JU
 Sample : N2562-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW470

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

77	16.204	2228	2230	2231	rBV2	2774	2055	0.12%	0.010%
78	16.275	2239	2242	2244	rVV4	3777	4872	0.29%	0.023%
79	16.340	2249	2253	2263	rVB4	8148	18299	1.08%	0.088%
80	16.704	2312	2315	2317	rBV3	2285	3156	0.19%	0.015%
81	16.781	2325	2328	2332	rBV6	2211	2873	0.17%	0.014%
82	16.851	2335	2340	2344	rBV5	14471	23251	1.37%	0.111%
83	16.963	2355	2359	2360	rBV4	2552	3066	0.18%	0.015%
84	17.081	2374	2379	2382	rBV6	7674	13302	0.78%	0.064%
85	17.222	2400	2403	2405	rBV4	3452	4755	0.28%	0.023%
86	17.310	2411	2418	2429	rBV	1077063	1702122	100.00%	8.144%
87	17.410	2429	2435	2447	rVB	718737	1142108	67.10%	5.465%
88	17.592	2465	2466	2472	rBV6	4957	5395	0.32%	0.026%
89	17.810	2501	2503	2509	rVB7	6828	8766	0.52%	0.042%
90	17.928	2519	2523	2528	rBV7	9603	16240	0.95%	0.078%
91	18.192	2565	2568	2571	rBV4	9104	10460	0.61%	0.050%
92	18.263	2576	2580	2584	rBV	23853	32924	1.93%	0.158%
93	18.475	2614	2616	2620	rBV4	6295	7969	0.47%	0.038%
94	19.086	2718	2720	2725	rVB5	8369	7670	0.45%	0.037%
95	19.216	2739	2742	2749	rBV7	15566	23436	1.38%	0.112%
96	19.639	2808	2814	2826	rBV	980530	1426359	83.80%	6.825%
97	21.092	3057	3061	3069	rBV	279362	372006	21.86%	1.780%
98	21.386	3107	3111	3118	rBV	1077453	1508021	88.60%	7.216%
99	23.674	3494	3500	3507	rBV2	574575	1170738	68.78%	5.602%
100	23.833	3521	3527	3540	rVB2	741808	1567342	92.08%	7.500%


Sum of corrected areas: 20899126

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010171.D
Acq On : 02 May 2022 14:10
Operator : CG/JU
Sample : N2562-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

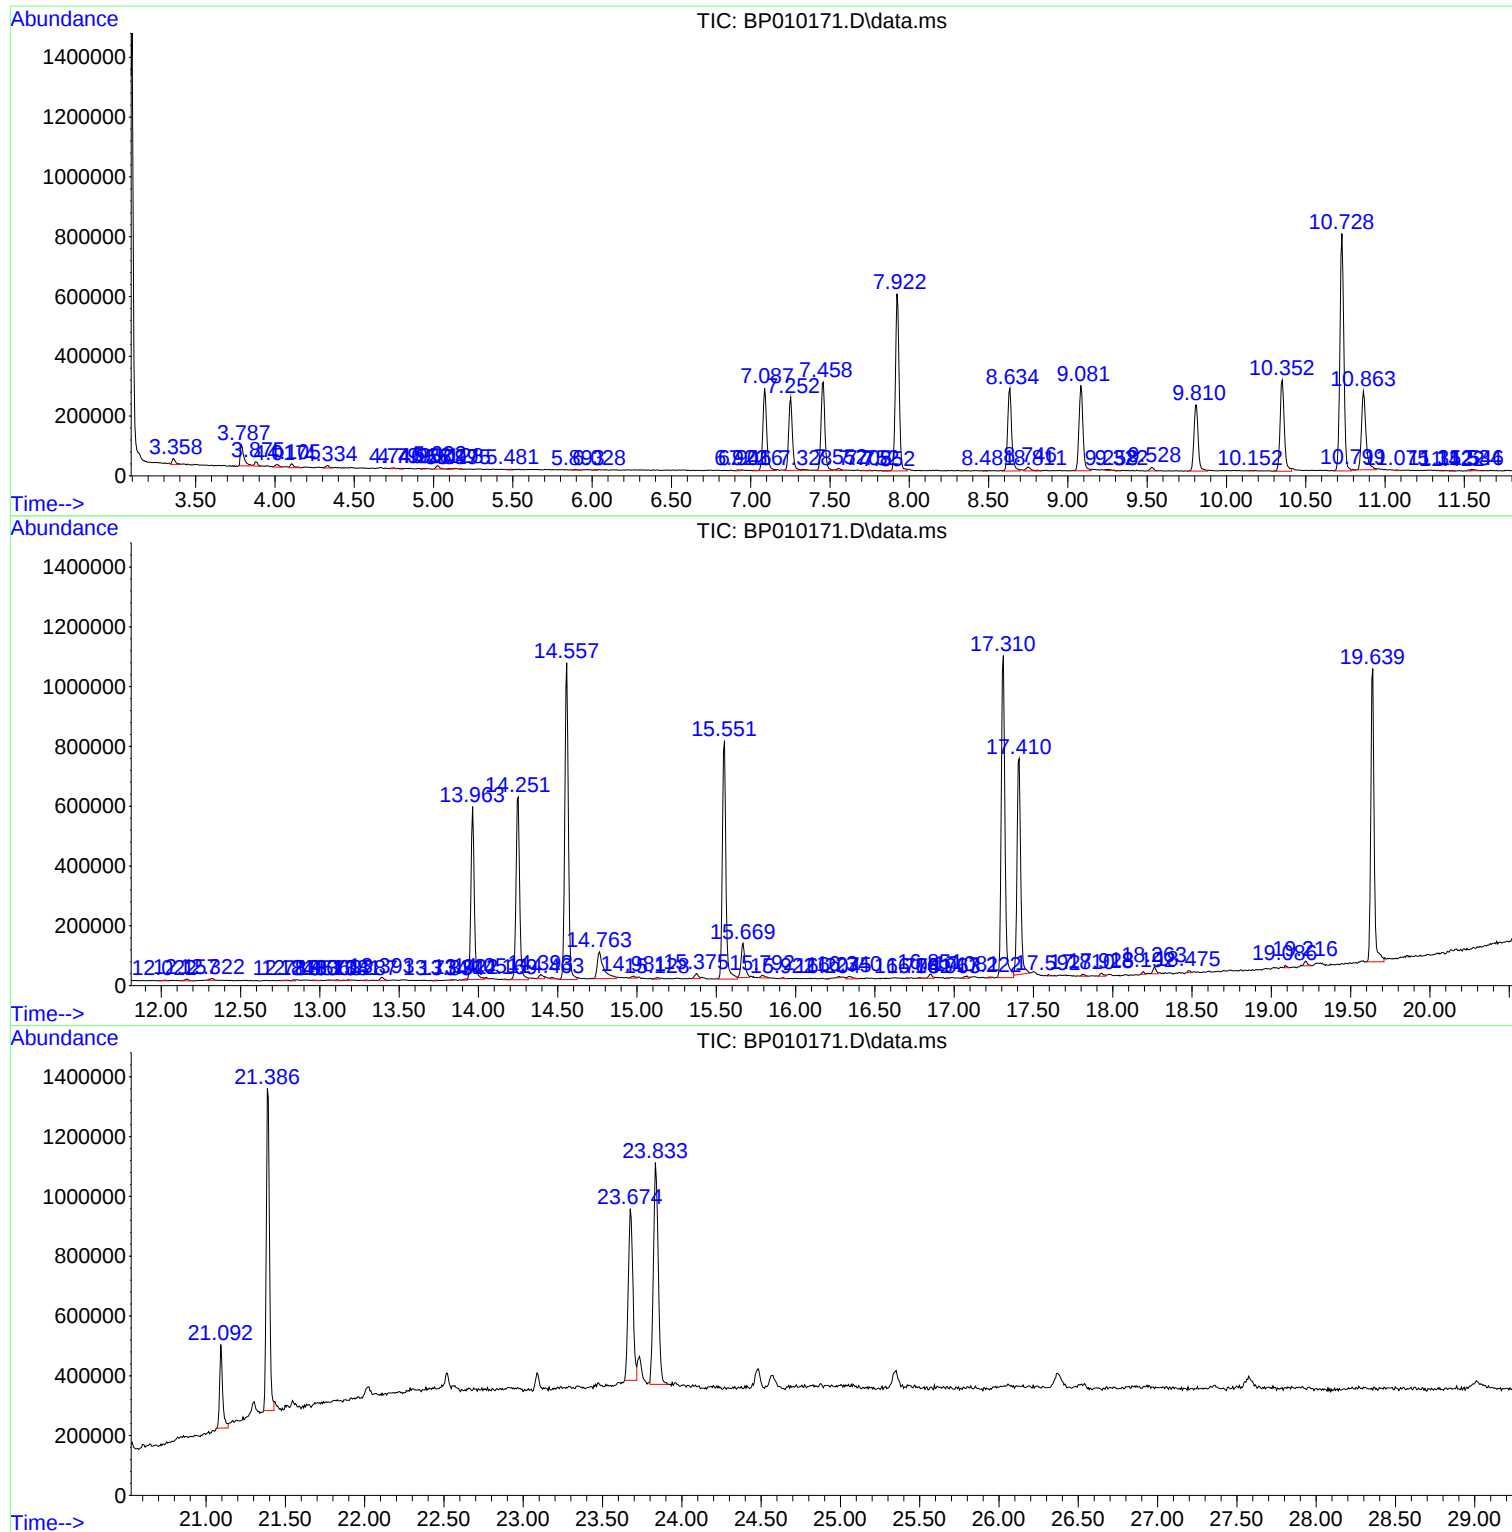

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010171.D
Acq On : 02 May 2022 14:10
Operator : CG/JU
Sample : N2562-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW470










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.092 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	4.93 ng/ul	372006	Chrysene-d12	21.386

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	99
2			1-Nonadecene	266	C19H38	018435-45-5	97
3			Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	94
4			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
5			1-Hexacosene	364	C26H52	018835-33-1	94

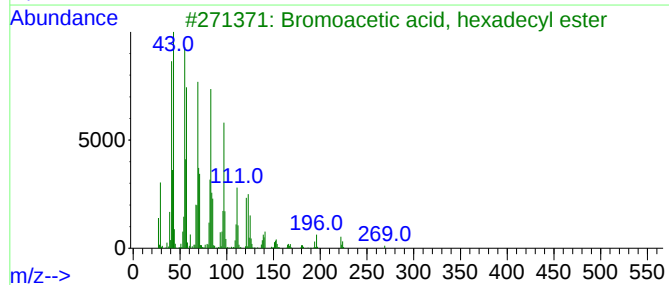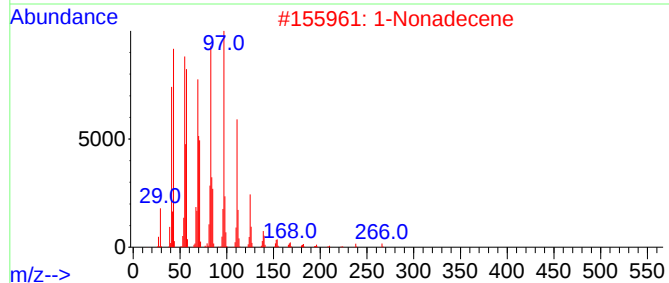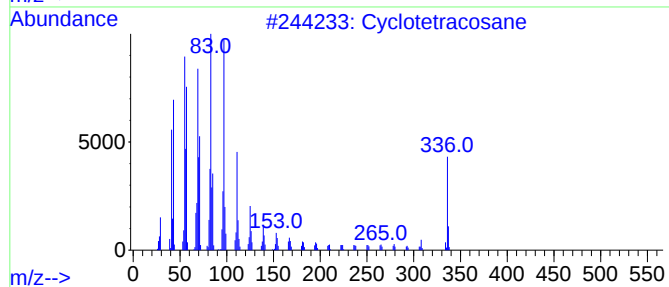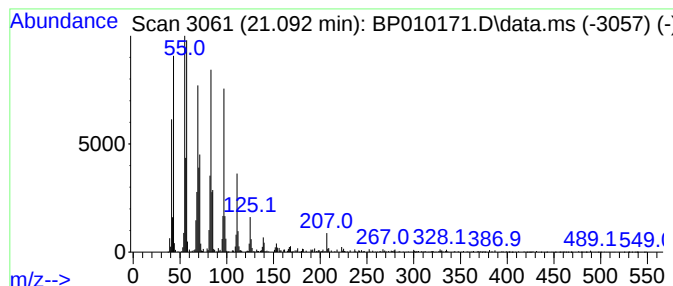

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010171.D
Acq On : 02 May 2022 14:10
Operator : CG/JU
Sample : N2562-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW470

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.092	4.9	ng/u1	372006	5	21.386	1508020	20.0