

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010177.D
 Acq On : 02 May 2022 17:32
 Operator : CG/JU
 Sample : N2562-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW478

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	54	rVB	31742	44700	1.59%	0.131%
2	3.775	114	117	142	rBV	334497	539026	19.21%	1.579%
3	4.105	170	173	178	rVB2	10966	14349	0.51%	0.042%
4	4.352	213	215	218	rVB3	3216	3336	0.12%	0.010%
5	4.375	218	219	223	rBV4	3020	3538	0.13%	0.010%
6	4.463	233	234	240	rBV6	2985	3698	0.13%	0.011%
7	5.022	327	329	336	rBV4	6867	9353	0.33%	0.027%
8	5.716	445	447	450	rBV4	2655	3111	0.11%	0.009%
9	6.140	515	519	522	rBV5	2574	3887	0.14%	0.011%
10	6.434	565	569	572	rVV6	2099	3356	0.12%	0.010%
11	6.463	572	574	578	rVB4	2415	2883	0.10%	0.008%
12	7.087	673	680	691	rBV	524783	864007	30.78%	2.530%
13	7.252	701	708	719	rBV	440947	709092	25.26%	2.077%
14	7.334	719	722	728	rVB2	4362	6812	0.24%	0.020%
15	7.451	733	742	754	rBV	534854	878918	31.32%	2.574%
16	7.922	815	822	832	rBV	553047	880931	31.39%	2.580%
17	7.993	832	834	841	rVB7	5602	8285	0.30%	0.024%
18	8.316	887	889	895	rVB7	2478	3141	0.11%	0.009%
19	8.628	932	942	956	rBV	690778	1177345	41.95%	3.448%
20	9.081	1012	1019	1033	rVV	565788	980800	34.95%	2.872%
21	9.251	1044	1048	1054	rVB7	5963	11486	0.41%	0.034%
22	9.534	1089	1096	1100	rBV4	13094	23790	0.85%	0.070%
23	9.804	1135	1142	1155	rBV	476855	824918	29.39%	2.416%
24	10.351	1227	1235	1251	rBV	641200	1187349	42.31%	3.477%
25	10.728	1290	1299	1309	rBV	767045	1299132	46.29%	3.804%
26	10.863	1313	1322	1339	rBV	635408	1217942	43.40%	3.567%
27	11.022	1347	1349	1353	rVB5	2732	3617	0.13%	0.011%
28	11.057	1353	1355	1358	rVB3	3019	3253	0.12%	0.010%
29	11.663	1455	1458	1461	rVV5	2900	4072	0.15%	0.012%
30	11.763	1473	1475	1479	rVB4	3159	4266	0.15%	0.012%
31	12.163	1538	1543	1548	rBV3	10887	17098	0.61%	0.050%
32	12.322	1563	1570	1578	rBV4	12168	27585	0.98%	0.081%
33	12.610	1615	1619	1621	rBV5	2716	2924	0.10%	0.009%
34	12.892	1663	1667	1669	rVB4	2964	3169	0.11%	0.009%
35	12.969	1676	1680	1683	rVB6	3963	4863	0.17%	0.014%
36	13.057	1692	1695	1697	rVB4	2988	2963	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010177.D
 Acq On : 02 May 2022 17:32
 Operator : CG/JU
 Sample : N2562-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW478

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	13.104	1701	1703	1710	rVB6	6292	7458	0.27%	0.022%
38	13.175	1710	1715	1718	rBV7	2430	4276	0.15%	0.013%
39	13.386	1746	1751	1755	rBV3	16715	24843	0.89%	0.073%
40	13.757	1808	1814	1818	rBV8	1635	3404	0.12%	0.010%
41	13.963	1842	1849	1861	rBV	1348035	1972350	70.27%	5.776%
42	14.045	1861	1863	1867	rVB5	4230	6072	0.22%	0.018%
43	14.245	1889	1897	1909	rBV	1470274	2237175	79.71%	6.551%
44	14.392	1917	1922	1930	rBV9	6308	13237	0.47%	0.039%
45	14.457	1931	1933	1941	rVB8	8244	13250	0.47%	0.039%
46	14.557	1943	1950	1961	rBV	1125594	1694285	60.37%	4.962%
47	14.633	1961	1963	1969	rVB7	3896	6060	0.22%	0.018%
48	14.751	1976	1983	1997	rBV	277514	626415	22.32%	1.834%
49	14.969	2017	2020	2024	rVB5	5086	7681	0.27%	0.022%
50	15.257	2065	2069	2072	rBV5	2655	3963	0.14%	0.012%
51	15.375	2085	2089	2092	rBV4	5687	8484	0.30%	0.025%
52	15.410	2092	2095	2101	rVB5	8237	10536	0.38%	0.031%
53	15.545	2111	2118	2133	rBV	1813405	2806625	100.00%	8.219%
54	15.663	2133	2138	2154	rVV	395472	623641	22.22%	1.826%
55	15.792	2155	2160	2169	rVB4	24114	50923	1.81%	0.149%
56	16.028	2198	2200	2202	rBV3	3044	3094	0.11%	0.009%
57	16.116	2209	2215	2216	rBV6	3575	6004	0.21%	0.018%
58	16.169	2222	2224	2228	rVB5	2418	2912	0.10%	0.009%
59	16.216	2228	2232	2233	rBV4	2766	3954	0.14%	0.012%
60	16.275	2238	2242	2244	rVV4	12039	18539	0.66%	0.054%
61	16.298	2244	2246	2249	rVV3	14005	17048	0.61%	0.050%
62	16.339	2249	2253	2259	rVB8	9398	16643	0.59%	0.049%
63	16.863	2338	2342	2345	rVB6	2411	3382	0.12%	0.010%
64	16.986	2358	2363	2367	rBV7	5504	10441	0.37%	0.031%
65	17.075	2372	2378	2381	rVV5	12281	21193	0.76%	0.062%
66	17.122	2383	2386	2392	rVB8	8470	13800	0.49%	0.040%
67	17.304	2410	2417	2428	rBV	1137662	1761683	62.77%	5.159%
68	17.404	2428	2434	2448	rVV2	1780179	2686366	95.72%	7.867%
69	17.598	2463	2467	2474	rVB10	4380	9482	0.34%	0.028%
70	17.686	2478	2482	2488	rBV9	3001	6843	0.24%	0.020%
71	17.810	2500	2503	2508	rVB2	11433	14684	0.52%	0.043%
72	17.904	2516	2519	2520	rBV3	2656	3043	0.11%	0.009%
73	17.974	2529	2531	2537	rVB6	8911	12187	0.43%	0.036%
74	18.192	2564	2568	2572	rBV5	19883	26799	0.95%	0.078%
75	18.263	2576	2580	2583	rBV	10392	13896	0.50%	0.041%
76	18.480	2614	2617	2620	rBV3	11854	12682	0.45%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010177.D
 Acq On : 02 May 2022 17:32
 Operator : CG/JU
 Sample : N2562-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW478

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

77	18.604	2636	2638	2643	rVB6	6799	7092	0.25%	0.021%
78	19.092	2717	2721	2726	rVB6	11676	18130	0.65%	0.053%
79	19.216	2738	2742	2749	rBV4	25359	36534	1.30%	0.107%
80	19.286	2750	2754	2761	rVV	18938	30975	1.10%	0.091%
81	19.639	2808	2814	2820	rBV	2073515	2804284	99.92%	8.212%
82	20.533	2962	2966	2970	rBV	70143	81507	2.90%	0.239%
83	21.092	3057	3061	3068	rBV	399563	496157	17.68%	1.453%
84	21.392	3107	3112	3120	rBV	1004800	1421682	50.65%	4.163%
85	23.674	3493	3500	3515	rVB2	1048343	2304628	82.11%	6.749%
86	23.833	3521	3527	3539	rVB2	651110	1382554	49.26%	4.049%




Sum of corrected areas: 34147891

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010177.D
Acq On : 02 May 2022 17:32
Operator : CG/JU
Sample : N2562-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW478

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

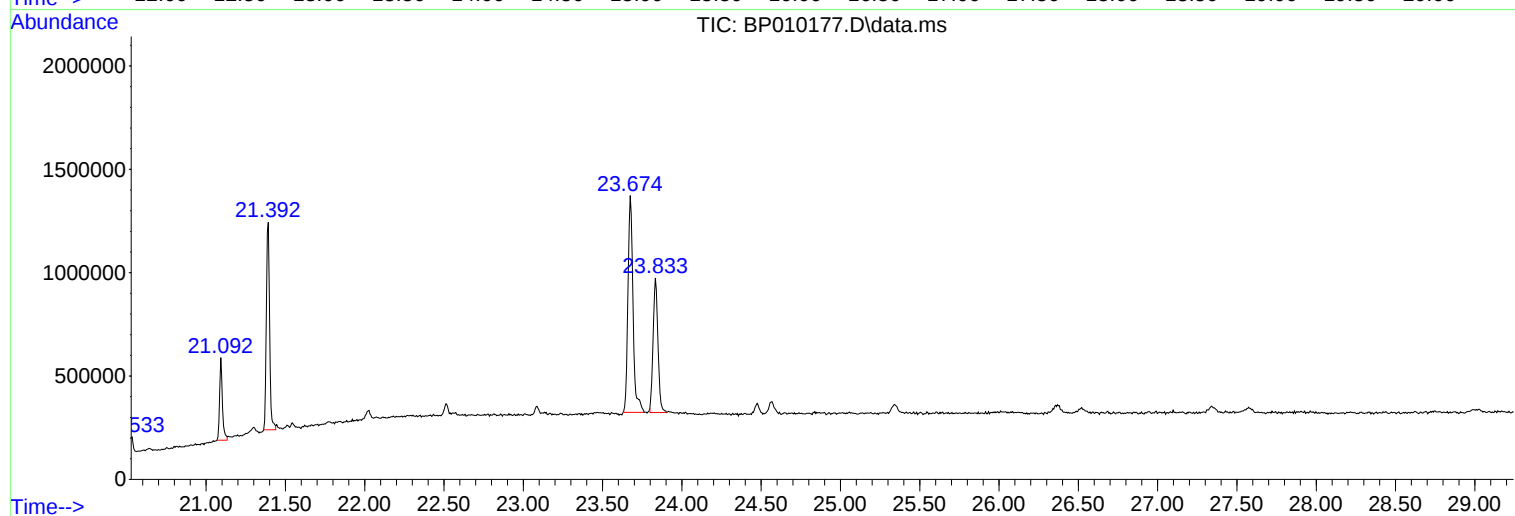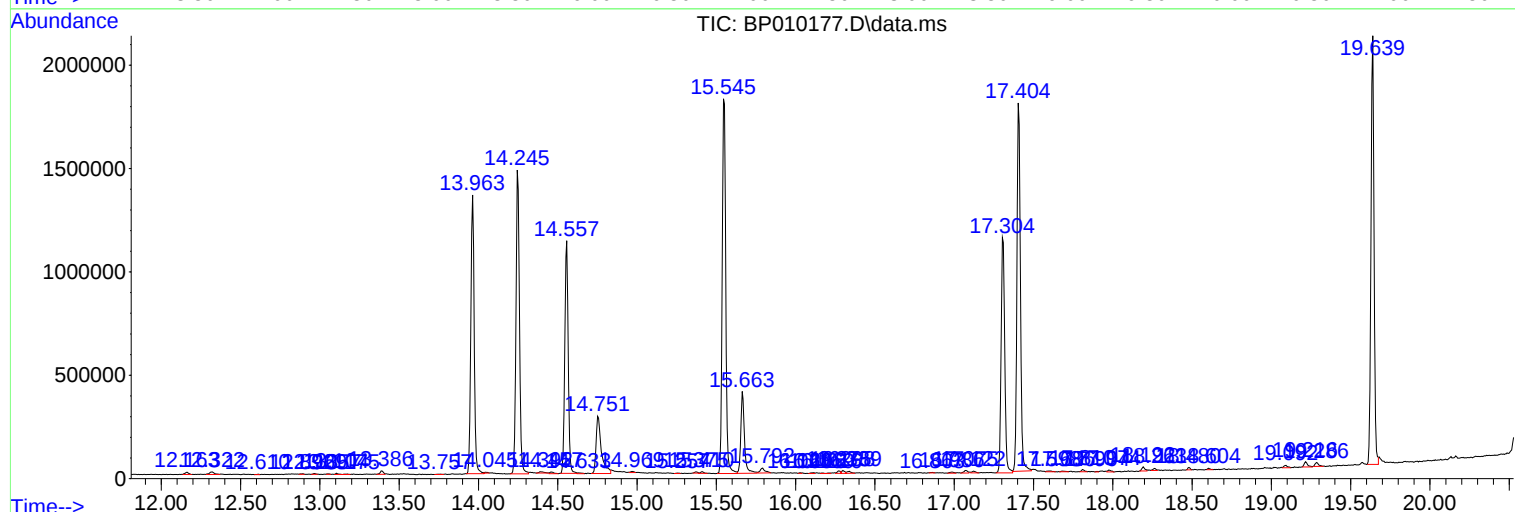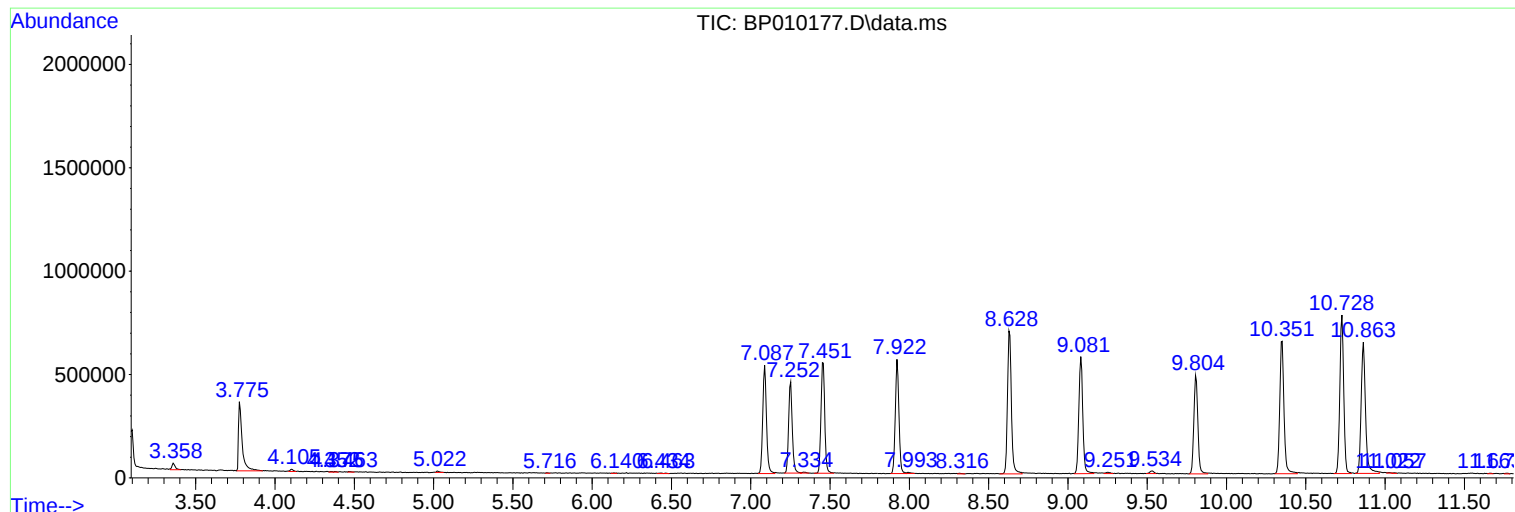

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010177.D
Acq On : 02 May 2022 17:32
Operator : CG/JU
Sample : N2562-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW478










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	6.98 ng/ul	496157	Chrysene-d12	21.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene			364	C26H52	018835-33-1	93
2	Pentacos-1-ene			350	C25H50	016980-85-1	91
3	Behenic alcohol			326	C22H46O	000661-19-8	91
4	1-Tetracosene			336	C24H48	010192-32-2	91
5	n-Tetracosanol-1			354	C24H50O	000506-51-4	91

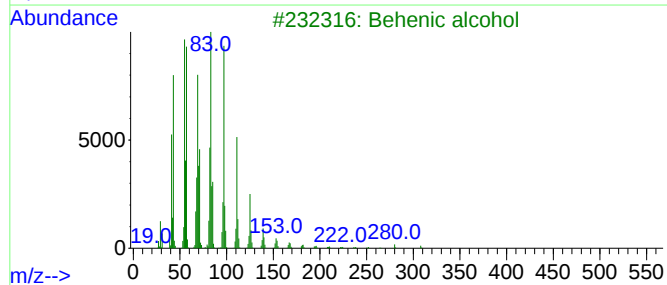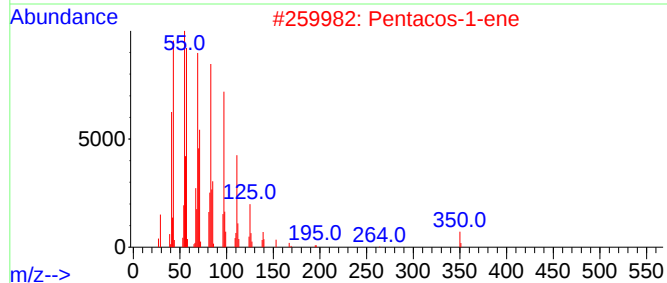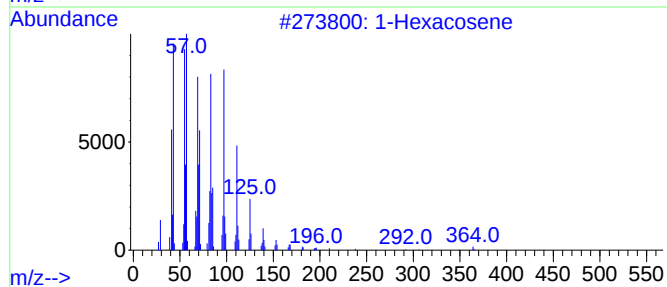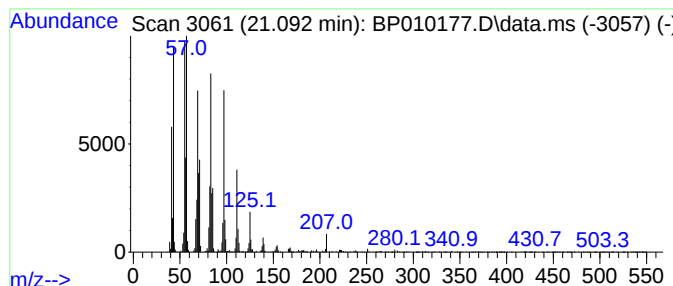

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010177.D
Acq On : 02 May 2022 17:32
Operator : CG/JU
Sample : N2562-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW478

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.092	7.0	ng/u1	496157	5	21.392	1421680	20.0