

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010180.D
 Acq On : 02 May 2022 19:13
 Operator : CG/JU
 Sample : N2562-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	41	47	54	rBV3	18747	30172	1.49%	0.121%
2	3.793	116	120	130	rBV	51031	91727	4.54%	0.368%
3	3.881	132	135	141	rVB4	14897	19482	0.96%	0.078%
4	4.010	152	157	161	rBV2	10870	19201	0.95%	0.077%
5	4.104	169	173	177	rBV	12953	19406	0.96%	0.078%
6	5.028	325	330	337	rBV5	12969	25450	1.26%	0.102%
7	5.122	340	346	352	rVV7	8614	15585	0.77%	0.063%
8	5.940	482	485	492	rVB4	12257	18724	0.93%	0.075%
9	6.481	572	577	585	rBV4	12117	23728	1.17%	0.095%
10	6.598	594	597	602	rVB5	11367	14639	0.72%	0.059%
11	6.922	648	652	657	rVB3	10003	14338	0.71%	0.058%
12	6.975	657	661	667	rVB7	6130	10125	0.50%	0.041%
13	7.087	672	680	690	rBV	271434	470762	23.30%	1.891%
14	7.251	702	708	715	rVV	239030	387916	19.20%	1.558%
15	7.451	735	742	750	rBV	277556	464455	22.99%	1.865%
16	7.557	755	760	768	rVV	37781	58793	2.91%	0.236%
17	7.922	814	822	831	rVV	589156	990610	49.03%	3.978%
18	7.998	831	835	843	rVB10	7707	15671	0.78%	0.063%
19	8.487	906	918	922	rBV9	10423	29563	1.46%	0.119%
20	8.522	922	924	929	rVV6	6795	9198	0.46%	0.037%
21	8.628	932	942	951	rBV	310394	548043	27.13%	2.201%
22	8.698	951	954	958	rVV4	13318	24707	1.22%	0.099%
23	8.745	958	962	969	rVV	23321	49021	2.43%	0.197%
24	9.010	1004	1007	1010	rBV5	7151	11899	0.59%	0.048%
25	9.081	1010	1019	1028	rVV	297752	520906	25.78%	2.092%
26	9.163	1028	1033	1044	rVB	61161	99518	4.93%	0.400%
27	9.251	1044	1048	1054	rBV8	10398	21473	1.06%	0.086%
28	9.416	1070	1076	1082	rVB9	5293	10291	0.51%	0.041%
29	9.528	1089	1095	1101	rBV6	12626	20947	1.04%	0.084%
30	9.581	1101	1104	1110	rVB7	7931	12749	0.63%	0.051%
31	9.639	1110	1114	1121	rBV10	5654	12016	0.59%	0.048%
32	9.804	1135	1142	1149	rBV	228033	406926	20.14%	1.634%
33	9.863	1150	1152	1157	rVV6	12124	17178	0.85%	0.069%
34	9.910	1157	1160	1166	rVB8	5733	10708	0.53%	0.043%
35	9.992	1169	1174	1182	rBV6	9995	27215	1.35%	0.109%
36	10.081	1185	1189	1196	rVB9	9203	17072	0.84%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010180.D
 Acq On : 02 May 2022 19:13
 Operator : CG/JU
 Sample : N2562-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	10.163	1196	1203	1211	rBV6	14671	34736	1.72%	0.139%
38	10.263	1214	1220	1225	rVB3	6459	9938	0.49%	0.040%
39	10.351	1226	1235	1243	rBV	313797	565544	27.99%	2.271%
40	10.728	1291	1299	1310	rBV	857624	1557258	77.08%	6.254%
41	10.863	1314	1322	1334	rBV2	271515	586565	29.03%	2.356%
42	11.192	1375	1378	1381	rVV5	7649	12031	0.60%	0.048%
43	11.233	1381	1385	1392	rVB7	14162	25236	1.25%	0.101%
44	11.410	1409	1415	1416	rBV5	9840	13966	0.69%	0.056%
45	11.575	1439	1443	1448	rVB8	7712	10629	0.53%	0.043%
46	11.657	1453	1457	1465	rVB5	12107	24109	1.19%	0.097%
47	11.763	1469	1475	1484	rVB2	36636	68232	3.38%	0.274%
48	11.922	1498	1502	1508	rVB7	9812	17222	0.85%	0.069%
49	12.016	1510	1518	1523	rBV7	13227	28040	1.39%	0.113%
50	12.086	1523	1530	1534	rBV9	6655	12021	0.59%	0.048%
51	12.157	1536	1542	1552	rBV	108684	173913	8.61%	0.698%
52	12.380	1576	1580	1585	rVB5	13161	19409	0.96%	0.078%
53	12.463	1588	1594	1597	rBV8	6297	11758	0.58%	0.047%
54	12.786	1644	1649	1653	rVV8	10864	18262	0.90%	0.073%
55	12.833	1653	1657	1664	rVB8	10808	25366	1.26%	0.102%
56	12.963	1675	1679	1683	rBV3	11283	16050	0.79%	0.064%
57	13.104	1697	1703	1708	rVB2	44928	75539	3.74%	0.303%
58	13.386	1745	1751	1759	rBV	110205	185253	9.17%	0.744%
59	13.480	1765	1767	1772	rVB4	14526	19190	0.95%	0.077%
60	13.839	1822	1828	1829	rBV6	9528	14535	0.72%	0.058%
61	13.963	1843	1849	1857	rVV	663731	948811	46.96%	3.810%
62	14.045	1860	1863	1867	rVV	65948	89790	4.44%	0.361%
63	14.086	1867	1870	1877	rVB6	23032	36257	1.79%	0.146%
64	14.174	1881	1885	1889	rVB3	17229	26745	1.32%	0.107%
65	14.245	1889	1897	1908	rBV	709329	1088279	53.86%	4.370%
66	14.398	1918	1923	1929	rBV10	9942	22924	1.13%	0.092%
67	14.457	1929	1933	1940	rVV	110326	160229	7.93%	0.643%
68	14.557	1942	1950	1963	rVV	1274016	1931307	95.59%	7.756%
69	14.763	1979	1985	1996	rBV	92215	229496	11.36%	0.922%
70	14.969	2015	2020	2025	rBV7	18393	36692	1.82%	0.147%
71	15.080	2036	2039	2046	rVB4	25699	44411	2.20%	0.178%
72	15.257	2066	2069	2073	rBV4	12466	18810	0.93%	0.076%
73	15.410	2091	2095	2100	rVB	88251	107552	5.32%	0.432%
74	15.545	2112	2118	2131	rVB	885678	1354616	67.05%	5.440%
75	15.669	2133	2139	2145	rBV	125153	200798	9.94%	0.806%
76	15.821	2157	2165	2170	rVB2	62625	112958	5.59%	0.454%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010180.D
 Acq On : 02 May 2022 19:13
 Operator : CG/JU
 Sample : N2562-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

77	15.910	2177	2180	2184	rVB6	10787	14624	0.72%	0.059%
78	16.033	2198	2201	2206	rVB5	28241	36675	1.82%	0.147%
79	16.274	2237	2242	2244	rBV	101956	143742	7.11%	0.577%
80	16.298	2244	2246	2251	rVB	125893	149410	7.40%	0.600%
81	16.621	2298	2301	2304	rBV5	9705	12187	0.60%	0.049%
82	16.839	2335	2338	2340	rBV4	10662	15832	0.78%	0.064%
83	17.068	2373	2377	2382	rBV	80677	107807	5.34%	0.433%
84	17.127	2383	2387	2396	rVB	63684	98118	4.86%	0.394%
85	17.310	2411	2418	2428	rBV	1285092	2020405	100.00%	8.114%
86	17.404	2428	2434	2447	rVB	871202	1351935	66.91%	5.429%
87	17.598	2464	2467	2474	rBV6	20374	37693	1.87%	0.151%
88	17.733	2487	2490	2495	rVB7	16393	22639	1.12%	0.091%
89	17.810	2499	2503	2507	rVV	77512	95620	4.73%	0.384%
90	17.963	2526	2529	2530	rBV3	9878	12337	0.61%	0.050%
91	18.027	2536	2540	2542	rBV4	12557	15773	0.78%	0.063%
92	18.480	2613	2617	2624	rBV	68106	88297	4.37%	0.355%
93	19.086	2717	2720	2728	rVB	60363	74011	3.66%	0.297%
94	19.633	2808	2813	2828	rBV	1122900	1657489	82.04%	6.656%
95	20.162	2900	2903	2907	rVB	46520	48161	2.38%	0.193%
96	20.527	2963	2965	2971	rVB	61764	65721	3.25%	0.264%
97	21.092	3058	3061	3067	rVB	190714	232298	11.50%	0.933%
98	21.386	3106	3111	3124	rVB2	1120409	1613608	79.87%	6.480%
99	23.674	3494	3500	3507	rBV2	515961	1054996	52.22%	4.237%
100	23.833	3521	3527	3537	rVB2	701667	1457284	72.13%	5.852%




Sum of corrected areas: 24901353

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

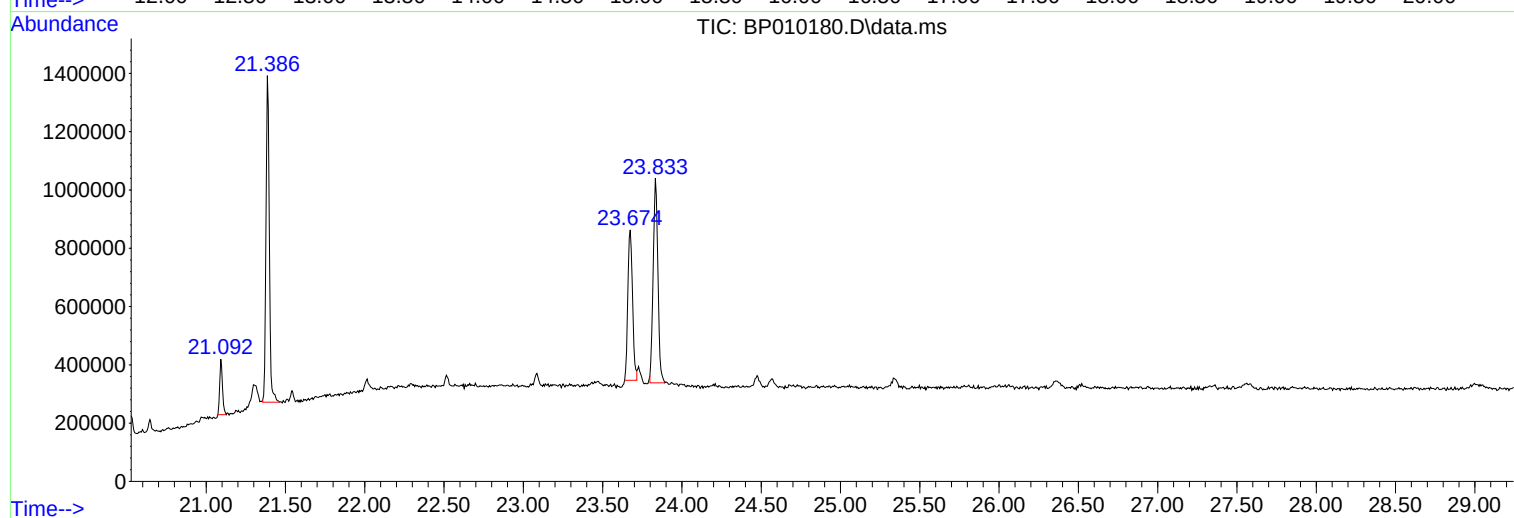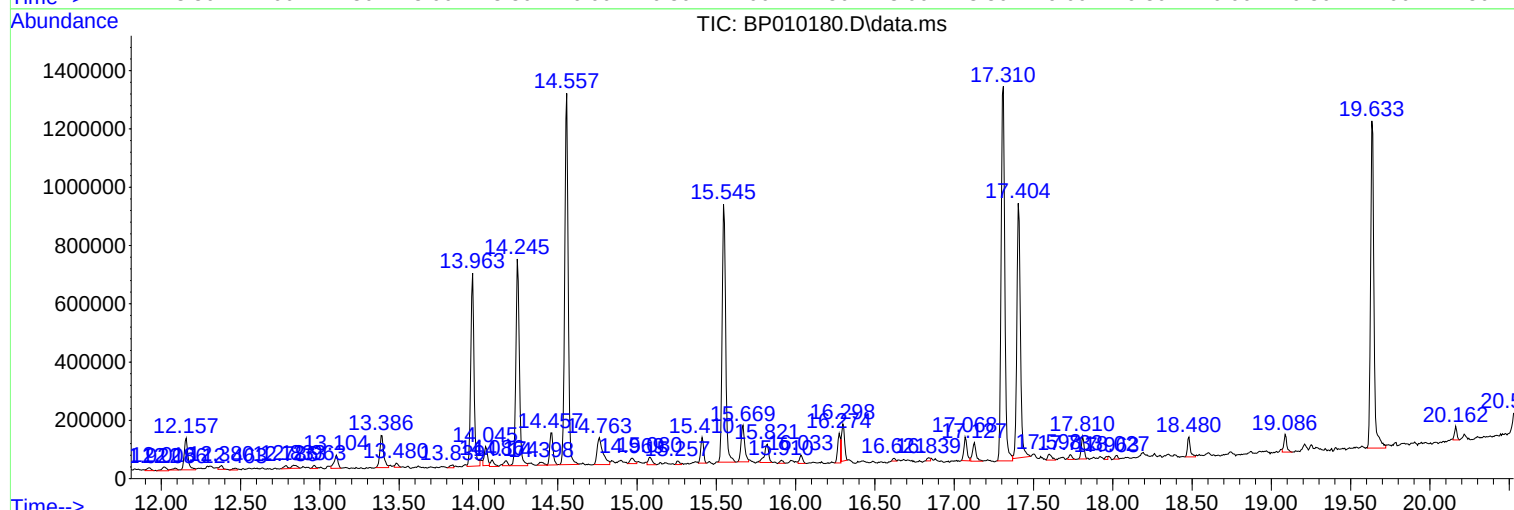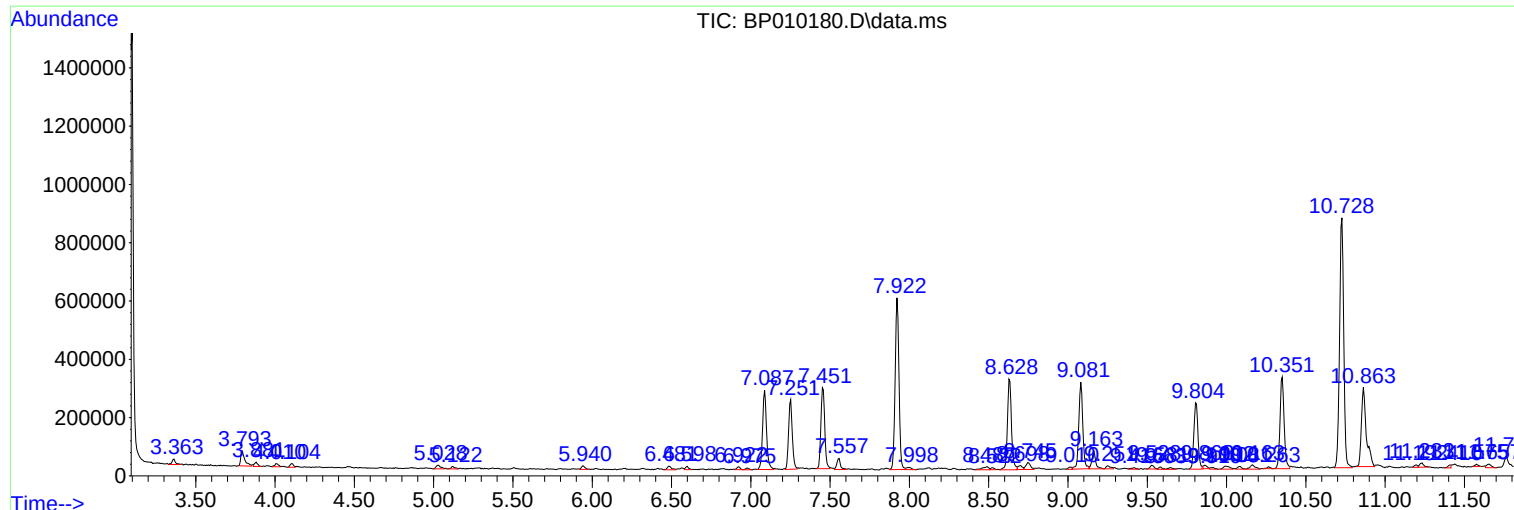

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010180.D
Acq On : 02 May 2022 19:13
Operator : CG/JU
Sample : N2562-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------