

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010184.D
 Acq On : 02 May 2022 22:02
 Operator : CG/JU
 Sample : PB144527BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK527

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	57	rVB	50263	70080	2.16%	0.183%
2	3.775	113	117	132	rBV	593909	924362	28.44%	2.420%
3	4.111	170	174	177	rVB	11126	16242	0.50%	0.043%
4	7.087	672	680	695	rBV	693455	1142961	35.16%	2.992%
5	7.252	701	708	720	rBV	581897	946755	29.13%	2.478%
6	7.452	735	742	755	rBV	726458	1196523	36.81%	3.132%
7	7.922	815	822	833	rBV	572736	947522	29.15%	2.480%
8	8.628	935	942	958	rBV	860488	1472089	45.29%	3.853%
9	9.081	1009	1019	1031	rBV	729295	1241665	38.20%	3.250%
10	9.805	1134	1142	1158	rVV	591276	1029357	31.67%	2.694%
11	10.346	1225	1234	1252	rBV	805473	1447773	44.54%	3.790%
12	10.728	1290	1299	1313	rBV	795265	1372582	42.23%	3.593%
13	10.857	1313	1321	1340	rBV	764826	1487222	45.75%	3.893%
14	11.557	1434	1440	1443	rBV8	1844	3589	0.11%	0.009%
15	11.975	1505	1511	1513	rBV5	1780	3256	0.10%	0.009%
16	12.322	1563	1570	1577	rVB4	12982	27858	0.86%	0.073%
17	12.528	1603	1605	1613	rVB9	2241	4651	0.14%	0.012%
18	13.287	1731	1734	1739	rBV7	2212	4105	0.13%	0.011%
19	13.916	1837	1841	1842	rBV3	3523	4562	0.14%	0.012%
20	13.963	1842	1849	1860	rVV	1476341	2073904	63.80%	5.428%
21	14.246	1890	1897	1917	rBV	1609406	2413110	74.24%	6.316%
22	14.393	1917	1922	1927	rVV6	6801	12730	0.39%	0.033%
23	14.557	1942	1950	1959	rBV	1047671	1692014	52.05%	4.429%
24	14.751	1976	1983	2001	rBV	332409	796441	24.50%	2.085%
25	15.128	2041	2047	2049	rBV6	2729	4761	0.15%	0.012%
26	15.545	2111	2118	2132	rBV	1933347	2952977	90.85%	7.729%
27	15.663	2133	2138	2155	rVV	539059	844907	25.99%	2.212%
28	15.787	2155	2159	2168	rVB2	26798	47604	1.46%	0.125%
29	16.328	2248	2251	2256	rBV7	7821	13400	0.41%	0.035%
30	16.822	2330	2335	2337	rVV6	1926	3484	0.11%	0.009%
31	16.987	2360	2363	2366	rVB5	4219	5281	0.16%	0.014%
32	17.092	2377	2381	2383	rBV5	3004	3350	0.10%	0.009%
33	17.304	2411	2417	2428	rBV	1189012	1779086	54.73%	4.657%
34	17.404	2428	2434	2454	rVB	1877969	2916627	89.73%	7.634%
35	18.257	2577	2579	2585	rVB5	5988	8094	0.25%	0.021%
36	18.786	2667	2669	2671	rBV3	3860	3305	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010184.D
Acq On : 02 May 2022 22:02
Operator : CG/JU
Sample : PB144527BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	19.210	2738	2741	2747	rVB4	22386	34959	1.08%	0.092%
38	19.286	2750	2754	2761	rVB	19753	30078	0.93%	0.079%
39	19.633	2807	2813	2832	rBV	2321705	3250503	100.00%	8.508%
40	21.386	3106	3111	3125	rBV	1139087	1645279	50.62%	4.306%
41	23.674	3493	3500	3515	rVB2	1288709	2782795	85.61%	7.284%
42	23.833	3520	3527	3538	rVB	712243	1546799	47.59%	4.049%




Sum of corrected areas: 38204642

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010184.D
Acq On : 02 May 2022 22:02
Operator : CG/JU
Sample : PB144527BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

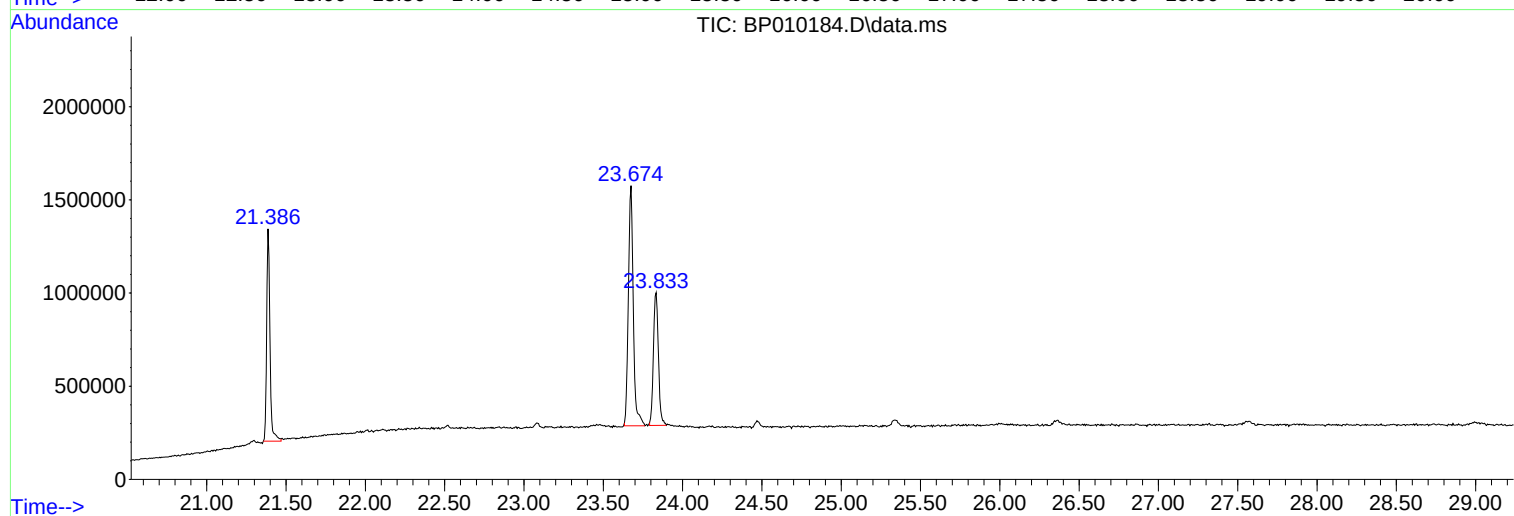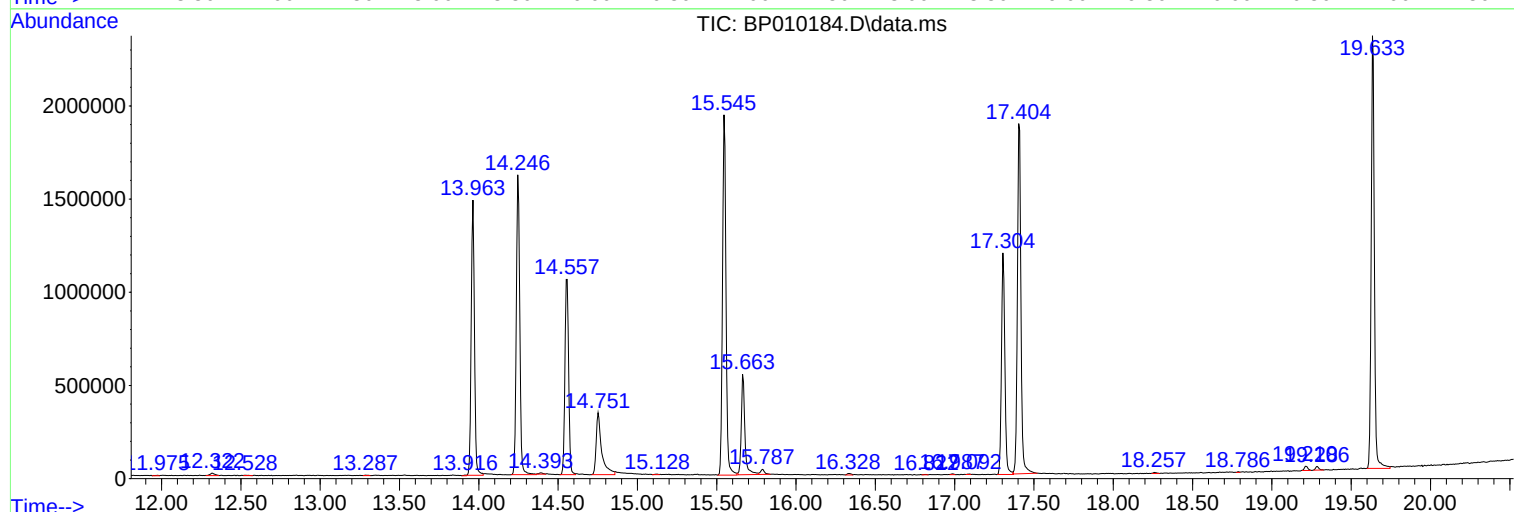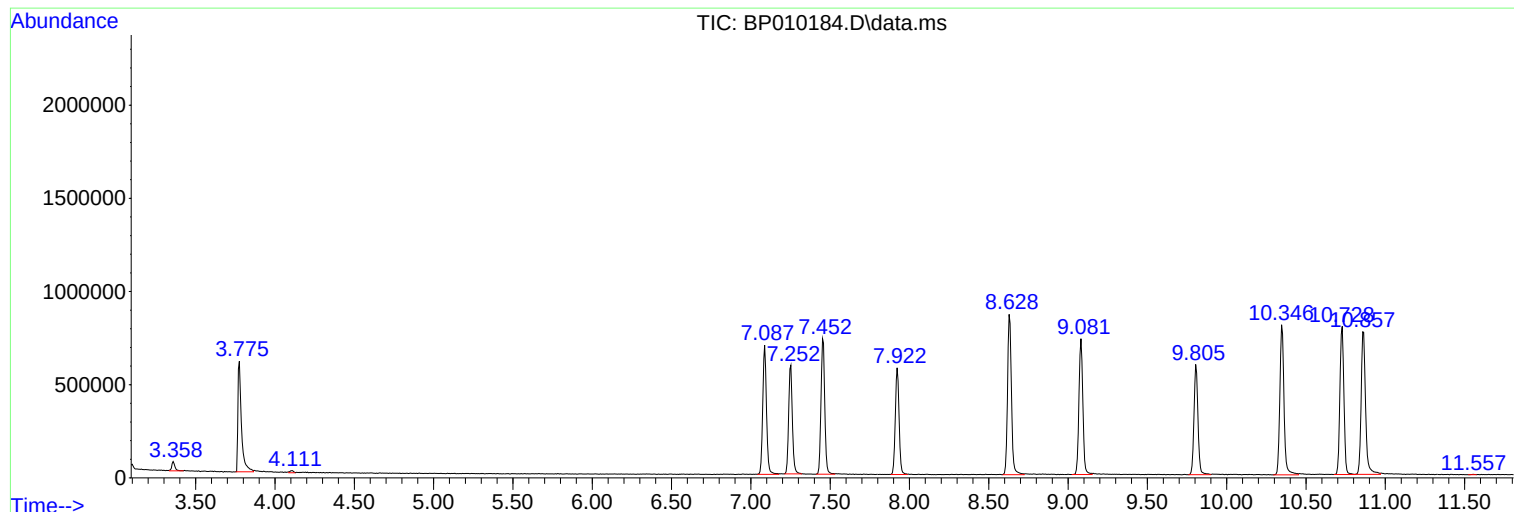

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010184.D
Acq On : 02 May 2022 22:02
Operator : CG/JU
Sample : PB144527BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010184.D
Acq On : 02 May 2022 22:02
Operator : CG/JU
Sample : PB144527BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------