

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010191.D
 Acq On : 03 May 2022 01:57
 Operator : CG/JU
 Sample : N2615-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	54	rBV	36144	45250	1.10%	0.120%
2	3.787	115	119	130	rBV	80575	141625	3.45%	0.375%
3	4.105	169	173	178	rVB2	10997	14087	0.34%	0.037%
4	4.358	212	216	219	rBV6	4939	6061	0.15%	0.016%
5	4.416	221	226	231	rBV9	4246	7747	0.19%	0.021%
6	5.022	326	329	333	rBV3	5850	8399	0.20%	0.022%
7	7.087	672	680	690	rBV	148271	254004	6.18%	0.673%
8	7.246	701	707	728	rVB	594046	975182	23.74%	2.583%
9	7.452	733	742	752	rBV	584328	947134	23.05%	2.509%
10	7.552	757	759	764	rVB5	4967	6176	0.15%	0.016%
11	7.922	815	822	833	rBV	493421	811455	19.75%	2.150%
12	8.628	935	942	954	rBV2	462468	780530	19.00%	2.068%
13	9.081	1010	1019	1032	rBV	763726	1294834	31.52%	3.430%
14	9.240	1044	1046	1052	rVV5	2981	4892	0.12%	0.013%
15	9.322	1055	1060	1065	rVV2	10380	17099	0.42%	0.045%
16	9.534	1092	1096	1100	rVB3	6231	9066	0.22%	0.024%
17	9.804	1133	1142	1155	rBV	591630	1028473	25.03%	2.725%
18	10.346	1226	1234	1252	rBV	783440	1403800	34.17%	3.719%
19	10.722	1289	1298	1308	rBV	678272	1191851	29.01%	3.157%
20	10.857	1314	1321	1340	rBV	589262	1120170	27.27%	2.967%
21	11.028	1347	1350	1356	rVB7	3196	5141	0.13%	0.014%
22	11.298	1394	1396	1400	rVB5	3182	4223	0.10%	0.011%
23	12.316	1563	1569	1574	rBV3	13764	25574	0.62%	0.068%
24	12.928	1668	1673	1678	rVB6	2916	6635	0.16%	0.018%
25	13.534	1771	1776	1780	rBV8	2793	5480	0.13%	0.015%
26	13.834	1824	1827	1831	rBV7	3121	4210	0.10%	0.011%
27	13.963	1842	1849	1864	rBV	1706168	2442319	59.45%	6.470%
28	14.245	1886	1897	1911	rBV	1749453	2673411	65.08%	7.082%
29	14.392	1918	1922	1924	rBV4	6619	8603	0.21%	0.023%
30	14.434	1924	1929	1940	rVB3	18887	42483	1.03%	0.113%
31	14.551	1942	1949	1959	rBV	973645	1479577	36.02%	3.920%
32	14.757	1977	1984	1993	rBV2	66070	165552	4.03%	0.439%
33	15.081	2034	2039	2043	rBV	23338	34155	0.83%	0.090%
34	15.216	2057	2062	2065	rVB6	10869	16927	0.41%	0.045%
35	15.298	2072	2076	2083	rVB9	2940	6526	0.16%	0.017%
36	15.363	2083	2087	2090	rBV6	4331	7270	0.18%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010191.D
 Acq On : 03 May 2022 01:57
 Operator : CG/JU
 Sample : N2615-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0D2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	15.545	2111	2118	2132	rBV	2316151	3374790	82.15%	8.940%
38	15.663	2132	2138	2154	rVV	744691	1129942	27.50%	2.993%
39	15.786	2154	2159	2167	rVB4	29489	57050	1.39%	0.151%
40	16.333	2247	2252	2257	rVB5	9758	16513	0.40%	0.044%
41	16.639	2299	2304	2306	rBV5	2580	4136	0.10%	0.011%
42	16.980	2359	2362	2366	rVB6	4832	6529	0.16%	0.017%
43	17.033	2366	2371	2374	rBV7	3820	6161	0.15%	0.016%
44	17.304	2410	2417	2426	rBV	1044226	1521231	37.03%	4.030%
45	17.404	2427	2434	2453	rVB	2555727	3803027	92.57%	10.075%
46	17.622	2470	2471	2477	rVB6	5417	5518	0.13%	0.015%
47	18.186	2564	2567	2575	rBV9	18332	29825	0.73%	0.079%
48	18.257	2577	2579	2583	rVB3	9104	10567	0.26%	0.028%
49	18.475	2613	2616	2619	rBV4	5527	7590	0.18%	0.020%
50	19.216	2738	2742	2747	rBV2	30433	45833	1.12%	0.121%
51	19.280	2749	2753	2760	rVV	26889	40948	1.00%	0.108%
52	19.633	2807	2813	2827	rBV	2972214	4108175	100.00%	10.883%
53	21.092	3057	3061	3070	rBV	215015	302395	7.36%	0.801%
54	21.386	3106	3111	3118	rBV	969061	1341531	32.66%	3.554%
55	23.674	3492	3500	3507	rBV2	1719157	3600039	87.63%	9.537%
56	23.827	3520	3526	3536	rVB2	610001	1341059	32.64%	3.553%




Sum of corrected areas: 37748780

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010191.D
Acq On : 03 May 2022 01:57
Operator : CG/JU
Sample : N2615-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0D2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

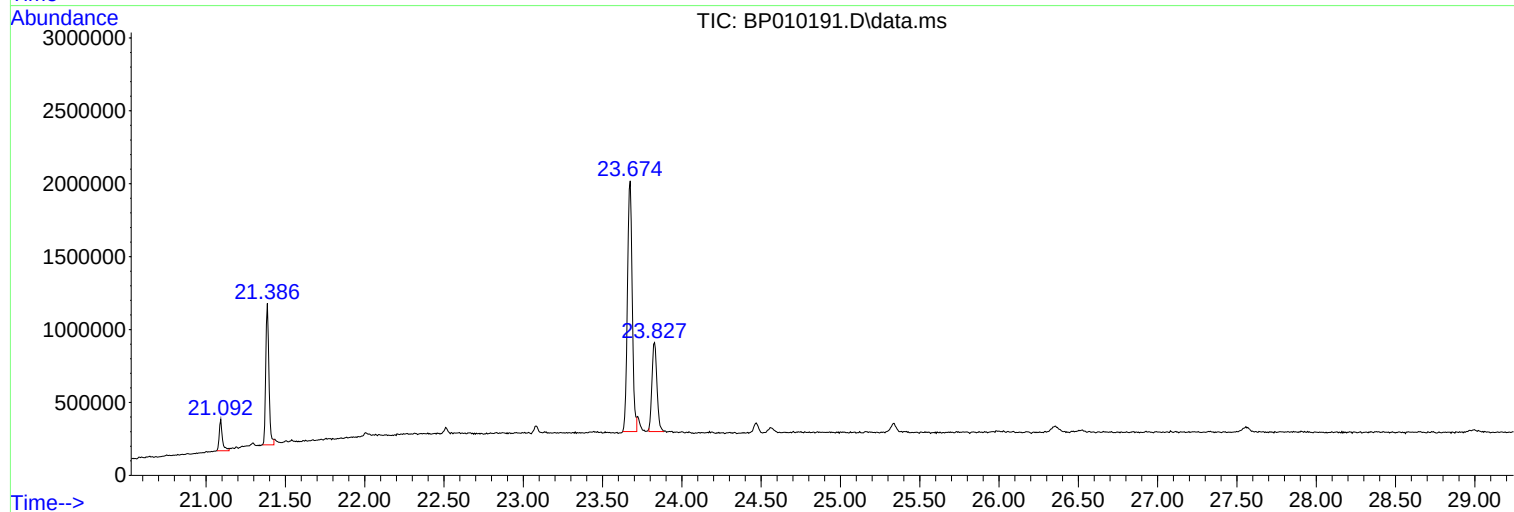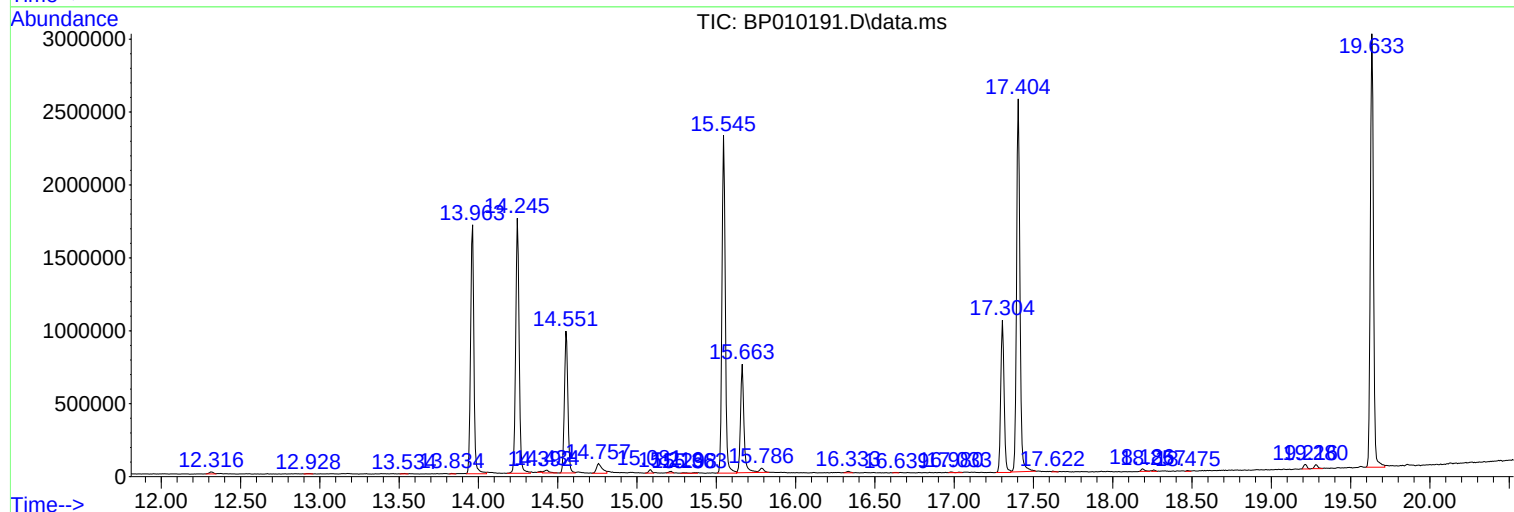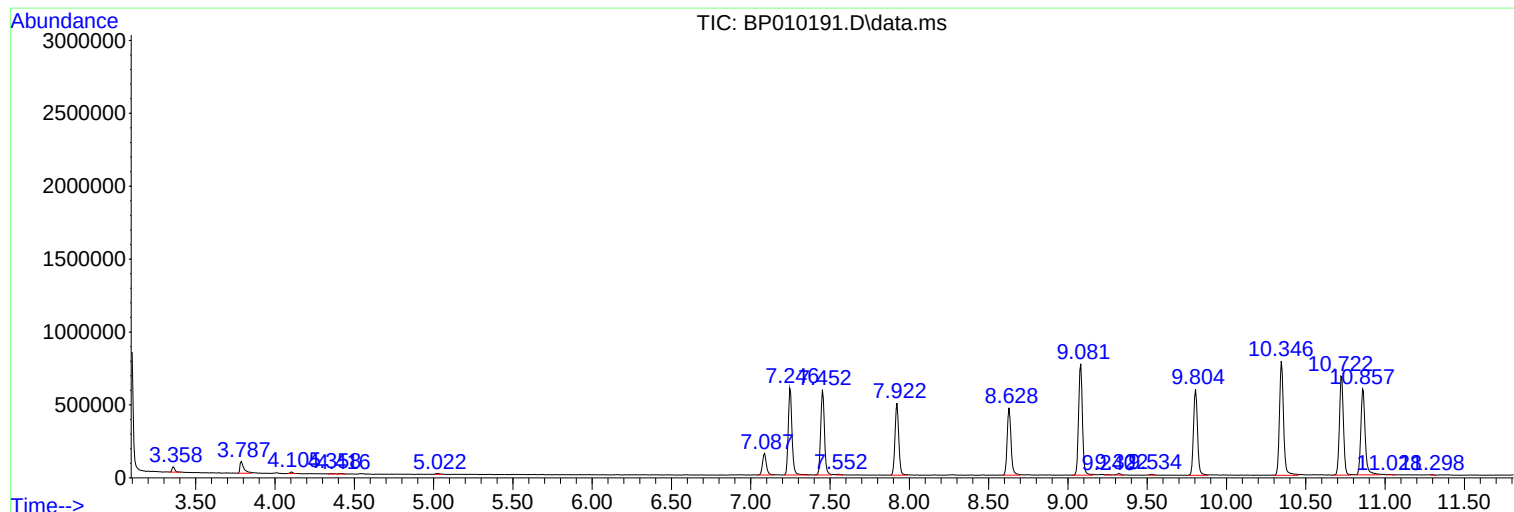

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010191.D
Acq On : 03 May 2022 01:57
Operator : CG/JU
Sample : N2615-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0D2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010191.D
Acq On : 03 May 2022 01:57
Operator : CG/JU
Sample : N2615-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0D2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc