

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010192.D
 Acq On : 03 May 2022 02:31
 Operator : CG/JU
 Sample : N2615-15
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	43	46	55	rVB	42031	54287	1.25%	0.137%
2	3.781	115	118	135	rBV	188122	317809	7.33%	0.800%
3	4.104	170	173	178	rBV3	8662	10997	0.25%	0.028%
4	5.022	325	329	336	rBV4	6836	11968	0.28%	0.030%
5	6.928	648	653	660	rBV4	3693	7405	0.17%	0.019%
6	7.087	673	680	696	rBV	159090	269881	6.22%	0.679%
7	7.245	699	707	720	rBV	655981	1091336	25.16%	2.746%
8	7.451	734	742	752	rBV	640842	1038981	23.96%	2.614%
9	7.551	756	759	765	rVB7	5968	9923	0.23%	0.025%
10	7.922	814	822	832	rBV	496178	828800	19.11%	2.085%
11	7.992	832	834	839	rVB6	4498	7232	0.17%	0.018%
12	8.628	934	942	956	rBV	482197	816182	18.82%	2.054%
13	9.081	1009	1019	1036	rBV	848647	1439414	33.19%	3.622%
14	9.534	1090	1096	1098	rBV4	7077	10759	0.25%	0.027%
15	9.804	1134	1142	1158	rBV	657164	1125191	25.94%	2.831%
16	10.345	1223	1234	1253	rBV	839222	1491548	34.39%	3.753%
17	10.728	1292	1299	1311	rVB	675698	1168145	26.94%	2.939%
18	10.857	1314	1321	1336	rBV	712749	1344496	31.00%	3.383%
19	11.292	1391	1395	1399	rVB7	2771	4796	0.11%	0.012%
20	12.163	1538	1543	1549	rVB7	4618	9214	0.21%	0.023%
21	12.316	1559	1569	1577	rBV3	15077	32348	0.75%	0.081%
22	12.928	1668	1673	1676	rVV7	3689	4741	0.11%	0.012%
23	13.110	1701	1704	1709	rVB6	2986	4791	0.11%	0.012%
24	13.175	1709	1715	1720	rBV9	4818	9848	0.23%	0.025%
25	13.392	1748	1752	1757	rVB5	8162	12031	0.28%	0.030%
26	13.527	1770	1775	1780	rVB9	3461	5536	0.13%	0.014%
27	13.963	1842	1849	1863	rBV	1720113	2536285	58.48%	6.382%
28	14.080	1867	1869	1878	rVB7	8524	18859	0.43%	0.047%
29	14.245	1887	1897	1916	rBV	1888172	2871886	66.22%	7.226%
30	14.386	1918	1921	1925	rBV4	7613	10931	0.25%	0.028%
31	14.551	1943	1949	1961	rBV	955973	1434539	33.08%	3.610%
32	14.757	1977	1984	2001	rBV2	61626	174680	4.03%	0.440%
33	14.969	2018	2020	2026	rVB7	4248	6022	0.14%	0.015%
34	15.086	2034	2040	2043	rBV4	9206	12794	0.30%	0.032%
35	15.210	2052	2061	2068	rBV5	17100	27502	0.63%	0.069%
36	15.363	2083	2087	2091	rBV6	8070	13783	0.32%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010192.D
 Acq On : 03 May 2022 02:31
 Operator : CG/JU
 Sample : N2615-15
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	15.545	2111	2118	2132	rBV	2356586	3612336	83.29%	9.089%
38	15.663	2132	2138	2152	rVV	739358	1130245	26.06%	2.844%
39	15.786	2155	2159	2166	rVB	28608	48300	1.11%	0.122%
40	15.904	2174	2179	2181	rBV6	2348	4478	0.10%	0.011%
41	16.110	2209	2214	2220	rBV8	3183	7127	0.16%	0.018%
42	16.333	2247	2252	2255	rBV6	9807	14401	0.33%	0.036%
43	16.986	2358	2363	2369	rVB10	5621	10698	0.25%	0.027%
44	17.068	2373	2377	2379	rVV5	4245	5901	0.14%	0.015%
45	17.098	2381	2382	2389	rVB6	3528	6068	0.14%	0.015%
46	17.304	2409	2417	2427	rBV	1032847	1522087	35.10%	3.830%
47	17.404	2427	2434	2451	rVV	2566479	3823642	88.17%	9.621%
48	17.592	2464	2466	2470	rVB5	5610	6924	0.16%	0.017%
49	17.927	2519	2523	2525	rBV5	4224	6355	0.15%	0.016%
50	18.186	2564	2567	2573	rBV8	7952	12708	0.29%	0.032%
51	18.257	2575	2579	2583	rBV2	10461	15221	0.35%	0.038%
52	18.604	2634	2638	2641	rVB4	16454	21036	0.49%	0.053%
53	19.210	2738	2741	2747	rVB	31220	43300	1.00%	0.109%
54	19.280	2749	2753	2760	rBV	28023	43966	1.01%	0.111%
55	19.633	2807	2813	2828	rBV	3245105	4336887	100.00%	10.913%
56	21.092	3058	3061	3065	rBV2	64710	75930	1.75%	0.191%
57	21.386	3106	3111	3118	rBV	1028194	1414214	32.61%	3.558%
58	23.674	3492	3500	3518	rVV	1836002	3941713	90.89%	9.918%
59	23.827	3520	3526	3539	rVB	645451	1403467	32.36%	3.531%




Sum of corrected areas: 39741944

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010192.D
Acq On : 03 May 2022 02:31
Operator : CG/JU
Sample : N2615-15
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

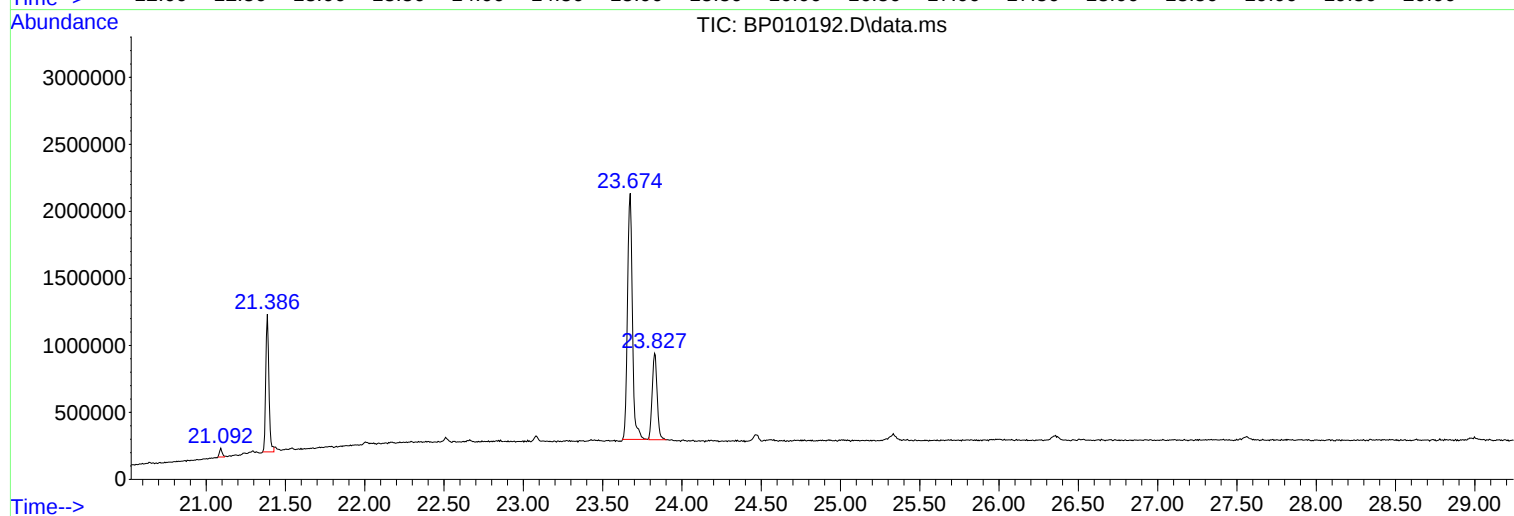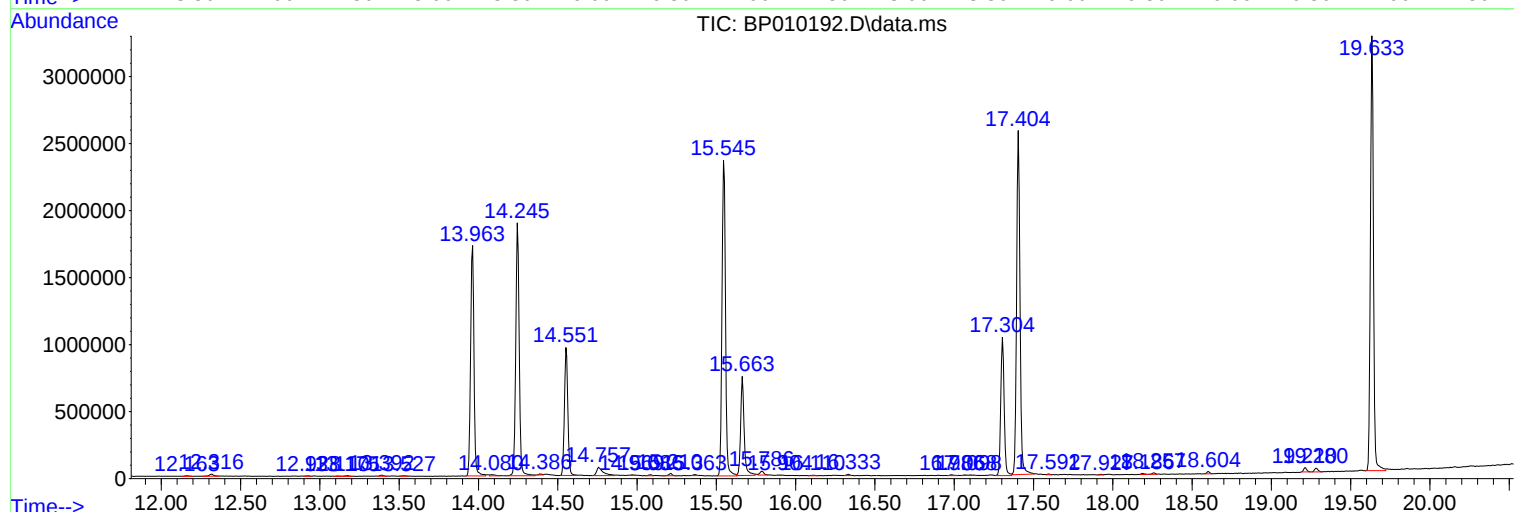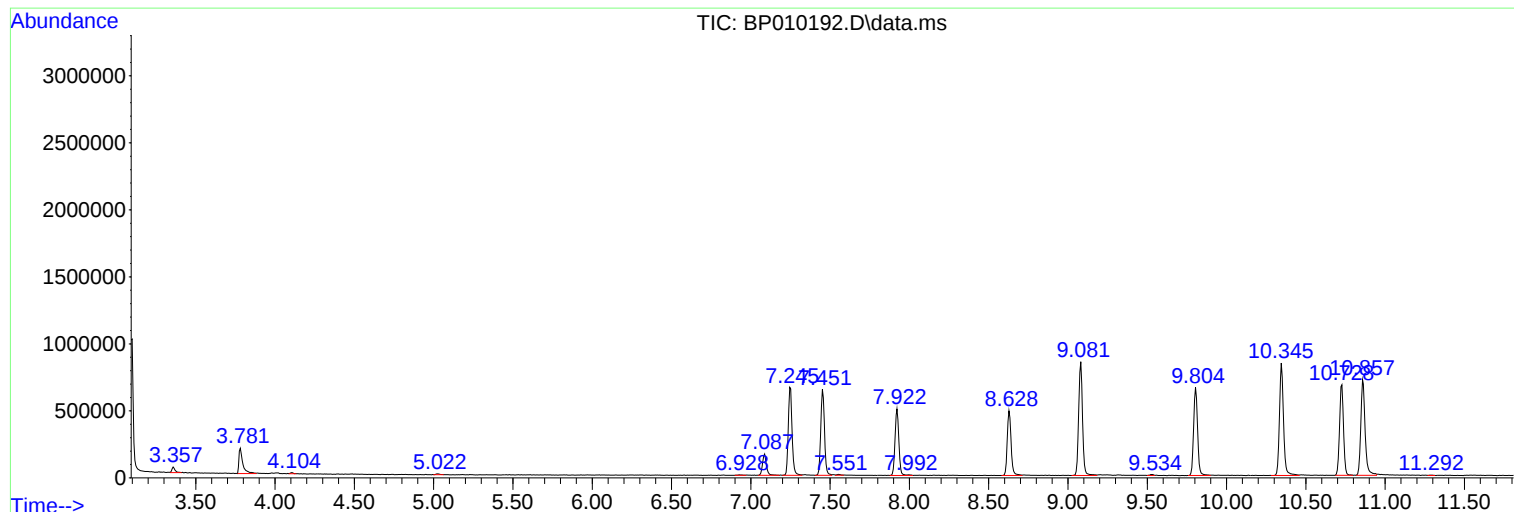

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010192.D
Acq On : 03 May 2022 02:31
Operator : CG/JU
Sample : N2615-15
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010192.D
Acq On : 03 May 2022 02:31
Operator : CG/JU
Sample : N2615-15
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
