

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010196.D
 Acq On : 03 May 2022 04:45
 Operator : CG/JU
 Sample : N2615-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	53	rVB	41176	50471	1.18%	0.128%
2	3.787	116	119	128	rBV	65743	109365	2.56%	0.277%
3	4.111	170	174	179	rVB3	11807	18316	0.43%	0.046%
4	5.022	325	329	336	rBV5	6386	13810	0.32%	0.035%
5	7.087	673	680	691	rBV	151219	256812	6.01%	0.651%
6	7.246	701	707	722	rBV	616758	1005429	23.54%	2.548%
7	7.452	735	742	756	rBV	614985	984015	23.04%	2.493%
8	7.552	756	759	763	rVB6	6063	8589	0.20%	0.022%
9	7.922	815	822	833	rBV	596314	977870	22.90%	2.478%
10	8.269	876	881	889	rVB2	11039	19345	0.45%	0.049%
11	8.628	933	942	956	rBV	447882	758176	17.75%	1.921%
12	8.846	974	979	982	rBV6	6166	9398	0.22%	0.024%
13	9.081	1010	1019	1031	rBV	739862	1293938	30.30%	3.279%
14	9.199	1037	1039	1044	rVV5	5859	8823	0.21%	0.022%
15	9.252	1047	1048	1054	rVB6	3846	4287	0.10%	0.011%
16	9.322	1054	1060	1066	rVB	22833	37639	0.88%	0.095%
17	9.528	1091	1095	1101	rVB8	3396	6894	0.16%	0.017%
18	9.657	1115	1117	1124	rVB7	3311	5362	0.13%	0.014%
19	9.804	1133	1142	1160	rBV	595985	1033878	24.21%	2.620%
20	10.346	1226	1234	1252	rBV	758239	1350149	31.61%	3.421%
21	10.722	1289	1298	1308	rBV	798576	1394811	32.66%	3.534%
22	10.857	1313	1321	1339	rBV	475035	927239	21.71%	2.350%
23	11.022	1346	1349	1355	rVB8	4304	6887	0.16%	0.017%
24	11.151	1368	1371	1377	rVB6	2535	4302	0.10%	0.011%
25	11.346	1400	1404	1409	rBV7	3893	7336	0.17%	0.019%
26	11.398	1409	1413	1418	rVB7	3100	6079	0.14%	0.015%
27	11.504	1426	1431	1433	rBV4	4730	7231	0.17%	0.018%
28	11.728	1465	1469	1472	rBV6	3563	5546	0.13%	0.014%
29	12.134	1535	1538	1542	rBV6	2557	4312	0.10%	0.011%
30	12.316	1560	1569	1578	rBV5	13871	33042	0.77%	0.084%
31	13.175	1709	1715	1718	rBV8	5427	8661	0.20%	0.022%
32	13.534	1771	1776	1777	rBV5	3262	4675	0.11%	0.012%
33	13.610	1783	1789	1792	rBV8	3225	5925	0.14%	0.015%
34	13.963	1842	1849	1859	rBV	1599018	2329792	54.55%	5.904%
35	14.245	1886	1897	1913	rBV	1691712	2535173	59.36%	6.424%
36	14.387	1916	1921	1924	rBV5	9954	17789	0.42%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010196.D
 Acq On : 03 May 2022 04:45
 Operator : CG/JU
 Sample : N2615-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	14.428	1924	1928	1932	rVV3	11747	16286	0.38%	0.041%
38	14.551	1943	1949	1960	rVV	1134605	1692918	39.64%	4.290%
39	14.757	1978	1984	2002	rBV3	63813	187445	4.39%	0.475%
40	14.975	2018	2021	2026	rVB7	4161	6466	0.15%	0.016%
41	15.363	2083	2087	2092	rVB6	9614	15056	0.35%	0.038%
42	15.545	2111	2118	2132	rBV	2220876	3313521	77.58%	8.396%
43	15.663	2132	2138	2154	rVV	702399	1110313	26.00%	2.814%
44	15.786	2155	2159	2166	rVB	31045	48695	1.14%	0.123%
45	16.333	2247	2252	2255	rBV5	8534	15037	0.35%	0.038%
46	16.981	2359	2362	2368	rBV8	7163	11399	0.27%	0.029%
47	17.304	2410	2417	2427	rBV	1286434	1889135	44.23%	4.787%
48	17.404	2427	2434	2453	rVB	2515154	3732200	87.38%	9.457%
49	17.969	2528	2530	2535	rVB6	5203	6019	0.14%	0.015%
50	18.186	2564	2567	2571	rBV6	14871	21171	0.50%	0.054%
51	18.257	2576	2579	2585	rVB2	8847	13560	0.32%	0.034%
52	18.604	2635	2638	2643	rVB6	6363	7370	0.17%	0.019%
53	19.210	2737	2741	2748	rBV4	33349	50432	1.18%	0.128%
54	19.280	2750	2753	2760	rVV	29257	42774	1.00%	0.108%
55	19.633	2807	2813	2827	rBV	3139510	4271073	100.00%	10.823%
56	21.092	3057	3061	3066	rBV2	98837	142183	3.33%	0.360%
57	21.386	3106	3111	3126	rBV	1347664	1849485	43.30%	4.687%
58	23.668	3492	3499	3518	rVV2	1887468	3926832	91.94%	9.951%
59	23.827	3520	3526	3542	rVB	832324	1842684	43.14%	4.669%




Sum of corrected areas: 39463420

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010196.D
Acq On : 03 May 2022 04:45
Operator : CG/JU
Sample : N2615-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

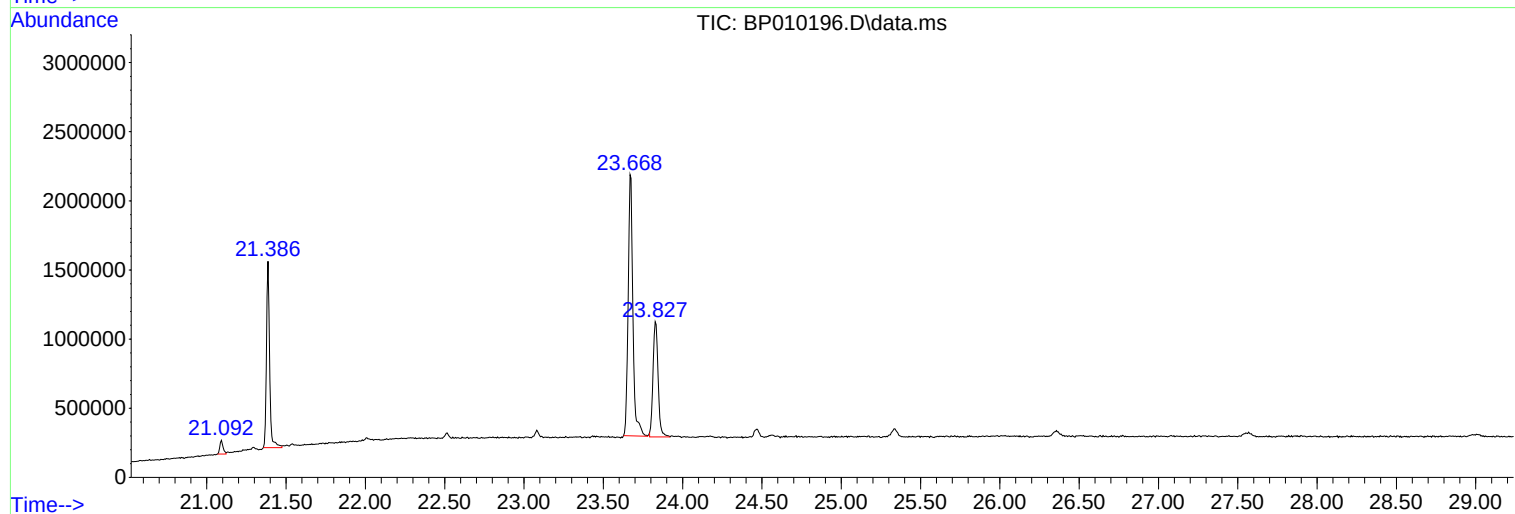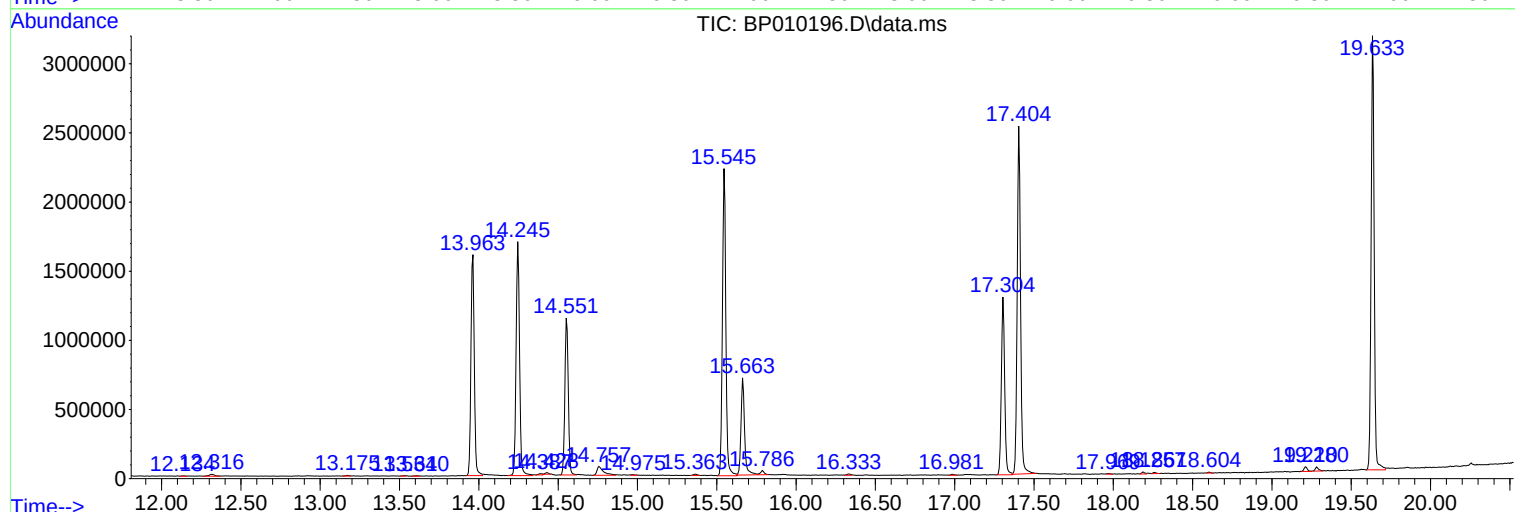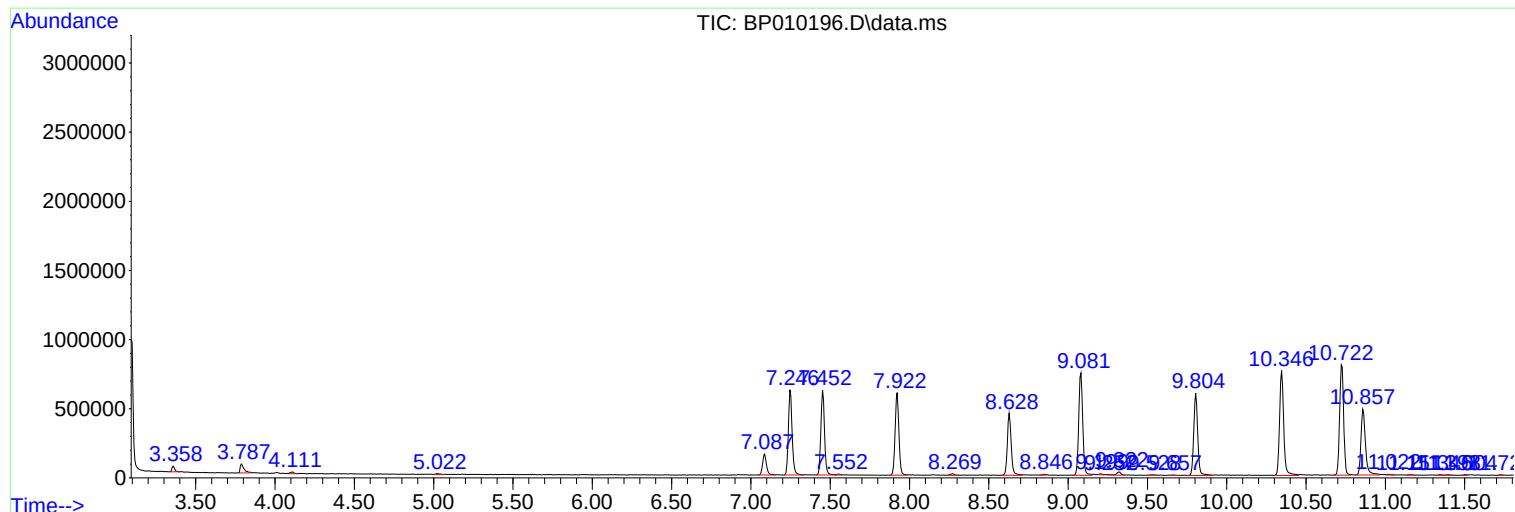

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010196.D
Acq On : 03 May 2022 04:45
Operator : CG/JU
Sample : N2615-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010196.D
Acq On : 03 May 2022 04:45
Operator : CG/JU
Sample : N2615-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc