

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010201.D
 Acq On : 03 May 2022 09:46
 Operator : CG/JU
 Sample : PB144528BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	56	rVB	41692	55219	1.77%	0.162%
2	3.775	113	117	137	rBV	470767	761318	24.34%	2.234%
3	4.105	169	173	178	rVB5	10715	17266	0.55%	0.051%
4	5.275	368	372	378	rBV9	2019	5377	0.17%	0.016%
5	5.575	419	423	426	rBV6	2498	4231	0.14%	0.012%
6	7.081	672	679	692	rBV	545910	907723	29.02%	2.663%
7	7.246	699	707	719	rBV	488628	776288	24.82%	2.278%
8	7.452	734	742	758	rVV	601073	966386	30.90%	2.835%
9	7.922	814	822	830	rBV	506892	842495	26.94%	2.472%
10	8.628	933	942	960	rBV	689678	1171739	37.47%	3.438%
11	8.775	964	967	970	rVB4	3468	3876	0.12%	0.011%
12	9.075	1010	1018	1040	rBV	567437	988183	31.60%	2.899%
13	9.805	1133	1142	1152	rBV	455824	801584	25.63%	2.352%
14	10.346	1225	1234	1258	rBV	628261	1168324	37.36%	3.428%
15	10.722	1290	1298	1313	rBV	690931	1199119	38.34%	3.518%
16	10.857	1313	1321	1340	rBV	615908	1172561	37.49%	3.440%
17	12.322	1566	1570	1577	rBV5	8773	16478	0.53%	0.048%
18	13.140	1705	1709	1713	rBV7	2554	5629	0.18%	0.017%
19	13.957	1842	1848	1862	rBV	1168496	1745520	55.81%	5.121%
20	14.245	1890	1897	1906	rBV	1312192	1988674	63.59%	5.835%
21	14.393	1917	1922	1930	rVB7	8244	19485	0.62%	0.057%
22	14.551	1942	1949	1962	rBV	1031224	1535944	49.11%	4.507%
23	14.751	1976	1983	2005	rBV	281493	713840	22.83%	2.094%
24	15.545	2111	2118	2130	rVV	1711355	2563441	81.97%	7.521%
25	15.663	2132	2138	2155	rVV	458390	732084	23.41%	2.148%
26	15.787	2155	2159	2167	rVB3	22133	40781	1.30%	0.120%
27	16.128	2215	2217	2222	rVB5	3110	4238	0.14%	0.012%
28	16.169	2222	2224	2229	rBV6	3003	5056	0.16%	0.015%
29	16.334	2246	2252	2256	rBV8	7451	12396	0.40%	0.036%
30	16.981	2360	2362	2366	rVB5	4078	4285	0.14%	0.013%
31	17.304	2410	2417	2427	rBV	1189035	1782940	57.01%	5.231%
32	17.404	2428	2434	2454	rVB	1797304	2737993	87.55%	8.033%
33	17.675	2479	2480	2486	rBV5	2747	4612	0.15%	0.014%
34	18.145	2556	2560	2563	rBV5	2217	4282	0.14%	0.013%
35	18.522	2621	2624	2628	rBV6	3359	3983	0.13%	0.012%
36	19.216	2738	2742	2747	rVB4	21244	30699	0.98%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010201.D
Acq On : 03 May 2022 09:46
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	19.281	2750	2753	2759	rVV	18620	24166	0.77%	0.071%
38	19.633	2807	2813	2828	rBV	2167304	3127405	100.00%	9.176%
39	21.386	3106	3111	3122	rBV	1193519	1734216	55.45%	5.088%
40	23.669	3492	3499	3514	rBV2	1263959	2741980	87.68%	8.045%
41	23.827	3520	3526	3541	rVB2	768180	1661023	53.11%	4.873%




Sum of corrected areas: 34082839

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010201.D
Acq On : 03 May 2022 09:46
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

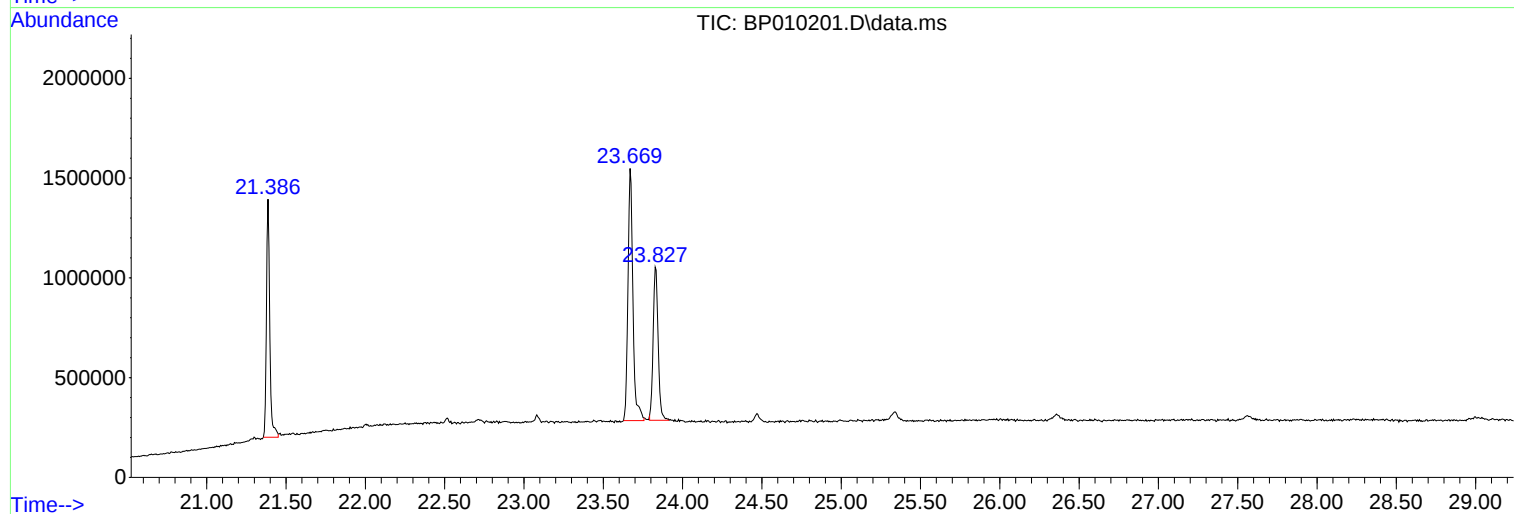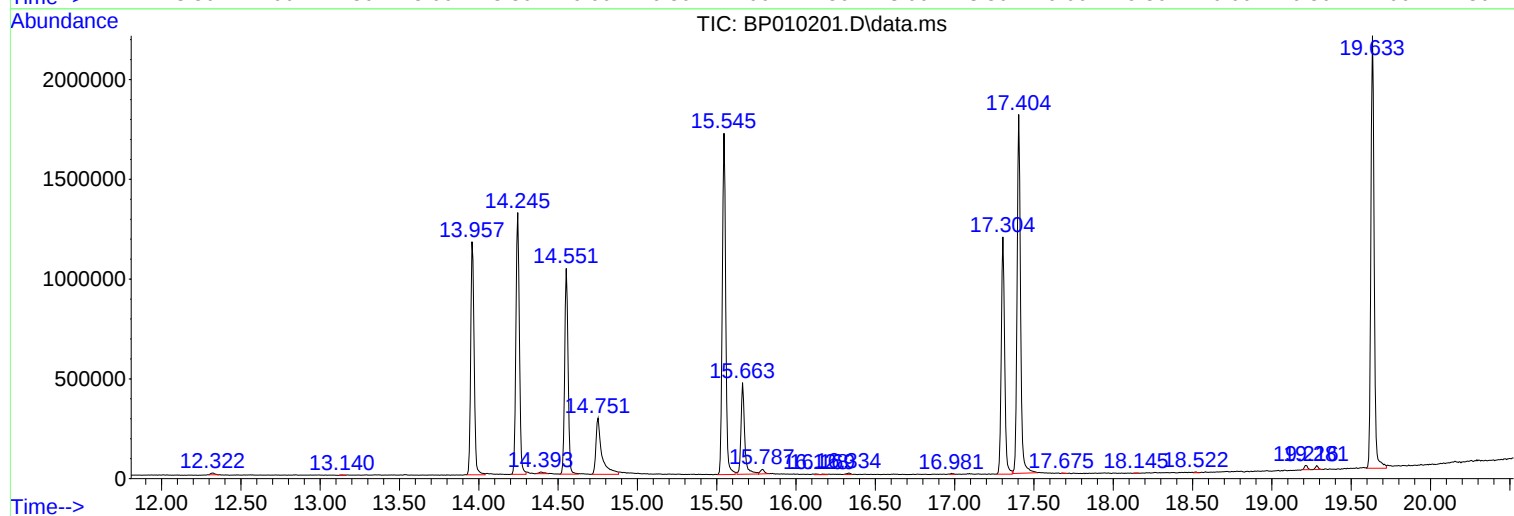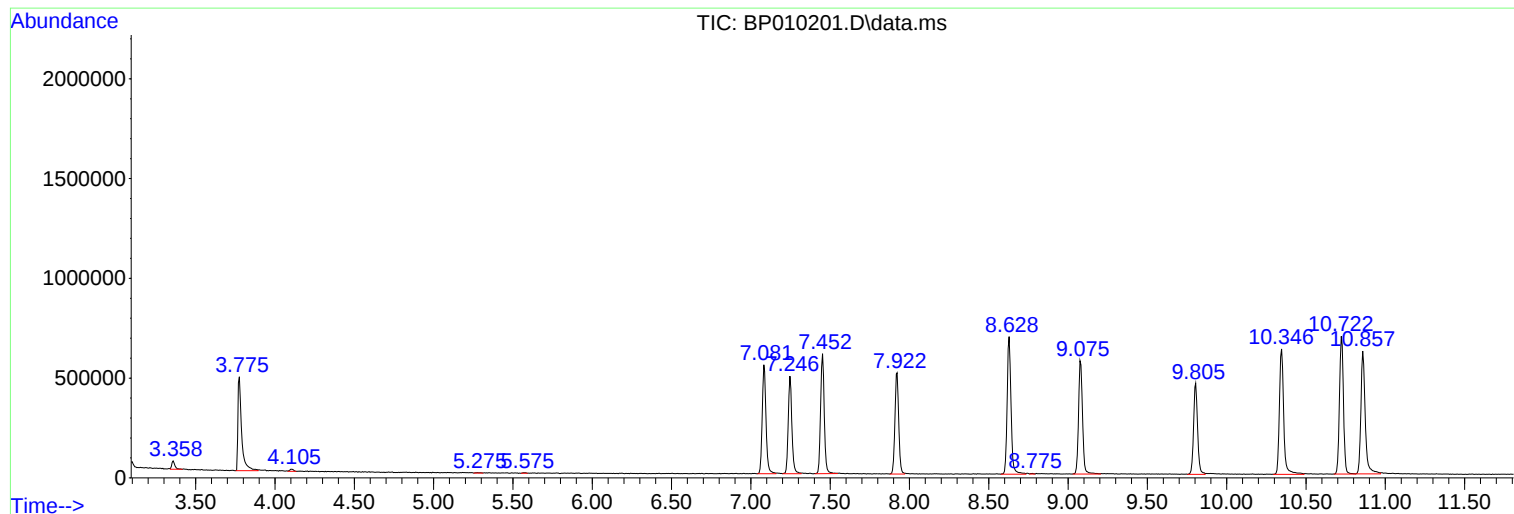

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010201.D
Acq On : 03 May 2022 09:46
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010201.D
Acq On : 03 May 2022 09:46
Operator : CG/JU
Sample : PB144528BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc