

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010202.D
 Acq On : 03 May 2022 10:20
 Operator : CG/JU
 Sample : PB144510BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	51	rVB	40543	49024	1.67%	0.155%
2	3.775	114	117	135	rBV	452710	718505	24.53%	2.270%
3	4.105	170	173	178	rVB3	9837	13526	0.46%	0.043%
4	4.428	226	228	232	rVB5	3454	3348	0.11%	0.011%
5	6.240	533	536	540	rVB6	2489	3128	0.11%	0.010%
6	6.840	635	638	642	rBV5	2688	3794	0.13%	0.012%
7	6.963	656	659	662	rVB5	2399	3604	0.12%	0.011%
8	7.081	672	679	689	rBV	514790	847191	28.92%	2.677%
9	7.246	701	707	719	rBV	440401	715100	24.41%	2.260%
10	7.452	734	742	756	rBV	551540	904856	30.89%	2.859%
11	7.922	815	822	832	rBV	471219	781182	26.67%	2.468%
12	8.628	934	942	956	rBV	632960	1078843	36.83%	3.409%
13	9.081	1008	1019	1028	rBV	524893	921241	31.45%	2.911%
14	9.804	1132	1142	1155	rBV	444048	764588	26.10%	2.416%
15	9.893	1155	1157	1161	rVB5	3422	4714	0.16%	0.015%
16	10.346	1225	1234	1252	rBV	593713	1079422	36.85%	3.411%
17	10.722	1291	1298	1310	rBV	637237	1102430	37.64%	3.484%
18	10.857	1313	1321	1341	rBV	558068	1092162	37.29%	3.451%
19	11.422	1412	1417	1419	rVB6	2024	2984	0.10%	0.009%
20	12.328	1565	1571	1576	rBV4	8929	20593	0.70%	0.065%
21	13.293	1730	1735	1738	rBV7	2447	3587	0.12%	0.011%
22	13.963	1842	1849	1862	rBV	1056365	1608330	54.91%	5.082%
23	14.245	1890	1897	1912	rBV	1239483	1843914	62.95%	5.827%
24	14.392	1917	1922	1926	rBV6	6305	12913	0.44%	0.041%
25	14.551	1942	1949	1965	rBV	948218	1414726	48.30%	4.470%
26	14.751	1976	1983	2003	rBV	253048	665113	22.71%	2.102%
27	15.545	2111	2118	2132	rVV	1572134	2359206	80.54%	7.455%
28	15.663	2132	2138	2154	rVV	401272	683663	23.34%	2.160%
29	15.786	2155	2159	2165	rVV3	23386	41303	1.41%	0.131%
30	16.334	2248	2252	2256	rVB6	6330	9974	0.34%	0.032%
31	16.439	2267	2270	2273	rVB5	2143	3079	0.11%	0.010%
32	16.981	2358	2362	2366	rBV6	5052	8411	0.29%	0.027%
33	17.086	2375	2380	2382	rBV5	3679	6049	0.21%	0.019%
34	17.304	2410	2417	2428	rBV	1114366	1645861	56.19%	5.201%
35	17.404	2428	2434	2455	rVB	1624510	2533827	86.50%	8.007%
36	17.681	2477	2481	2483	rBV4	3663	4194	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010202.D
 Acq On : 03 May 2022 10:20
 Operator : CG/JU
 Sample : PB144510BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	18.233	2573	2575	2579	rBV4	3215	5588	0.19%	0.018%
38	18.486	2613	2618	2619	rBV5	3330	3303	0.11%	0.010%
39	18.710	2651	2656	2657	rBV5	4044	6425	0.22%	0.020%
40	19.216	2738	2742	2747	rVB4	20174	27092	0.92%	0.086%
41	19.286	2750	2754	2760	rVB	20059	26733	0.91%	0.084%
42	19.563	2799	2801	2805	rBV5	5854	6903	0.24%	0.022%
43	19.633	2807	2813	2829	rVV	2096716	2929218	100.00%	9.256%
44	21.386	3106	3111	3128	rBV	1140974	1719848	58.71%	5.435%
45	23.674	3493	3500	3508	rBV	1178632	2458958	83.95%	7.770%
46	23.833	3520	3527	3535	rVB2	697746	1507797	51.47%	4.765%


Sum of corrected areas: 31646250

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010202.D
Acq On : 03 May 2022 10:20
Operator : CG/JU
Sample : PB144510BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

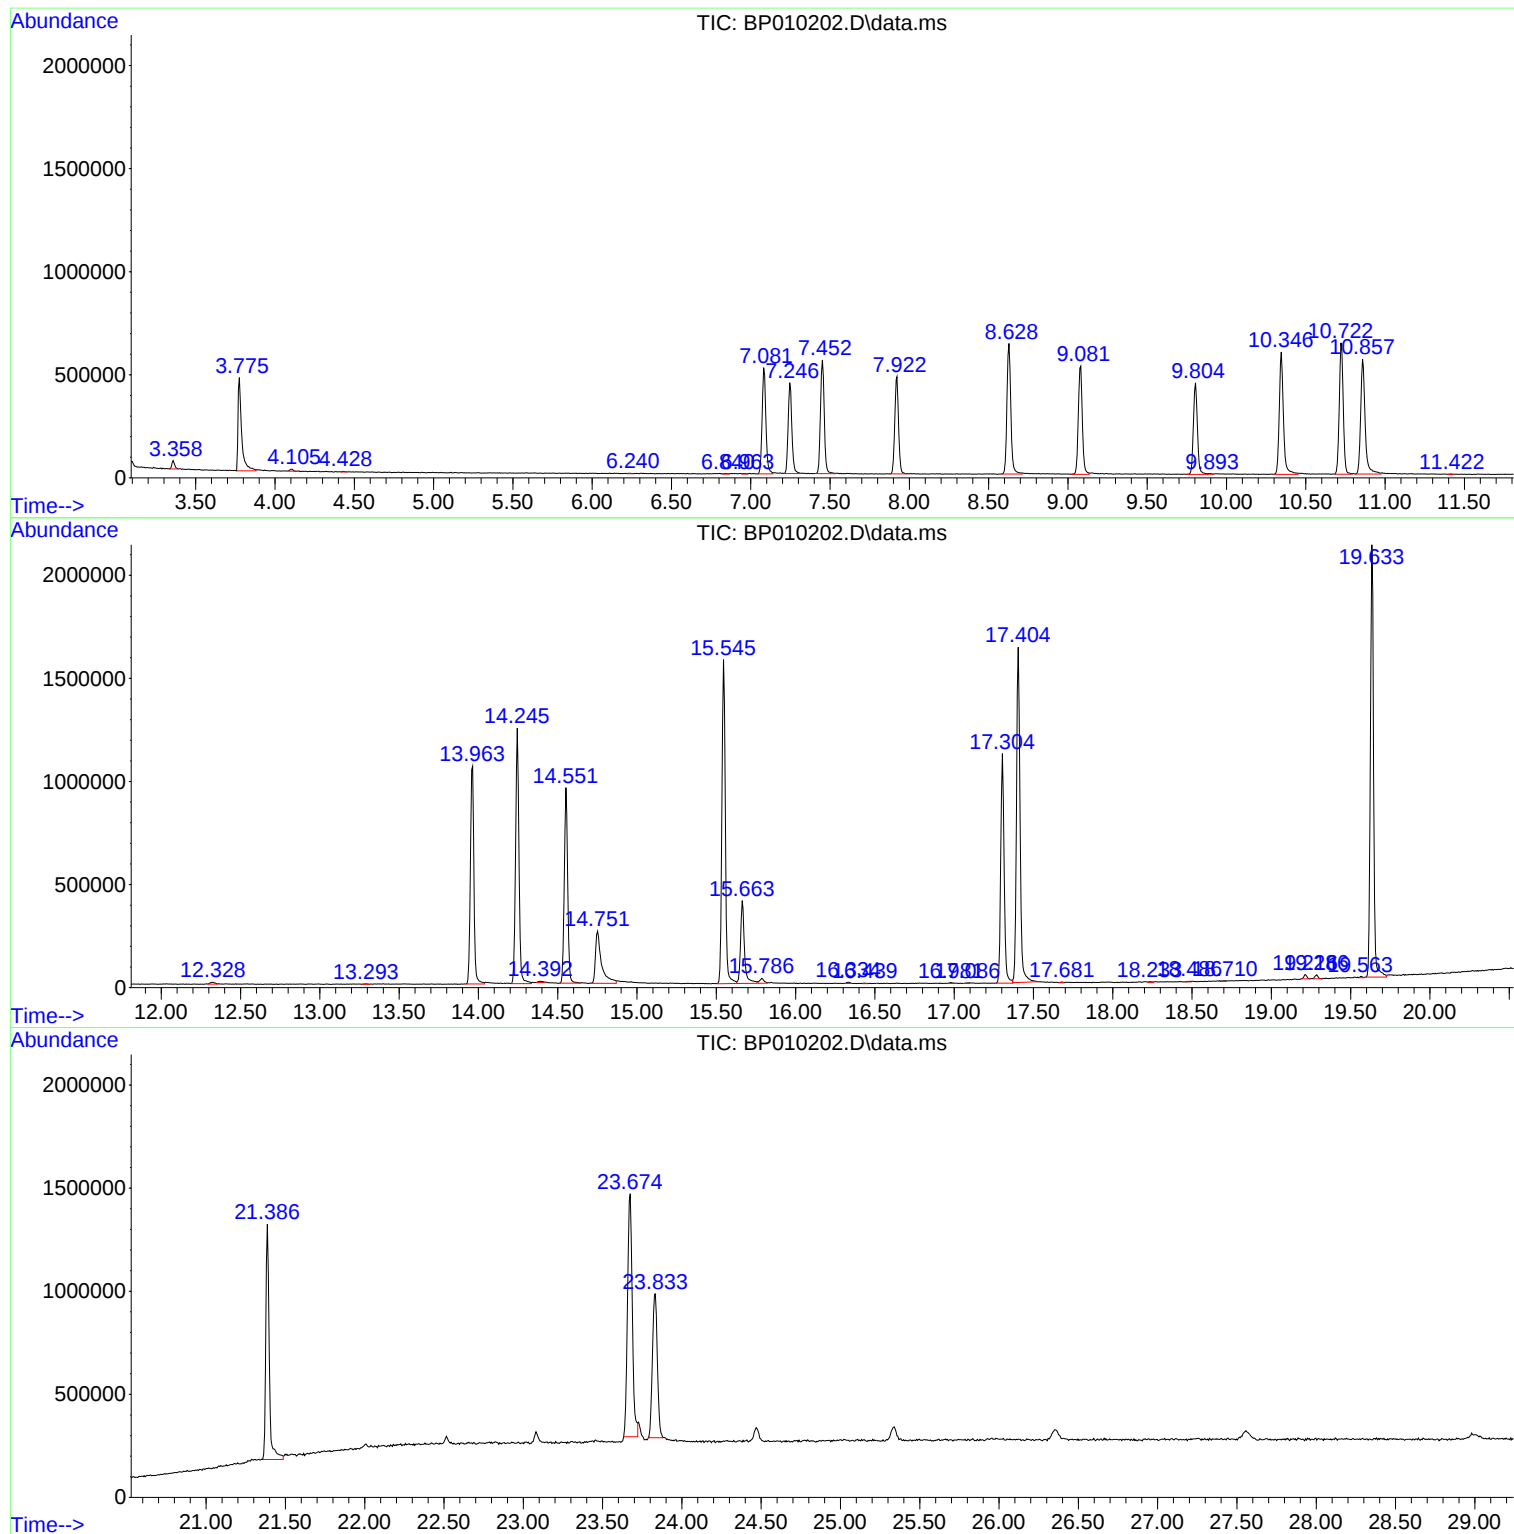

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010202.D
Acq On : 03 May 2022 10:20
Operator : CG/JU
Sample : PB144510BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010202.D
Acq On : 03 May 2022 10:20
Operator : CG/JU
Sample : PB144510BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc