

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010208.D
 Acq On : 03 May 2022 14:18
 Operator : CG/JU
 Sample : N2652-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.846	127	129	130	rBV2	3255	1818	0.12%	0.023%
2	4.099	169	172	177	rVV4	10749	15105	0.97%	0.189%
3	4.140	177	179	182	rVB4	2877	2352	0.15%	0.029%
4	4.646	264	265	267	rBV2	2652	1614	0.10%	0.020%
5	4.740	279	281	284	rBV4	1734	1603	0.10%	0.020%
6	4.864	300	302	306	rVB4	2857	2478	0.16%	0.031%
7	4.899	306	308	312	rVB5	1887	2188	0.14%	0.027%
8	4.946	315	316	324	rVB7	1815	2633	0.17%	0.033%
9	5.022	327	329	332	rBV4	1985	1761	0.11%	0.022%
10	5.334	380	382	384	rVB3	2669	2038	0.13%	0.026%
11	5.352	384	385	388	rBV3	2287	2820	0.18%	0.035%
12	5.740	449	451	454	rBV4	2418	2811	0.18%	0.035%
13	5.781	454	458	460	rVV5	1822	2891	0.18%	0.036%
14	5.805	460	462	466	rVB4	1597	1906	0.12%	0.024%
15	5.969	486	490	491	rBV4	1859	2326	0.15%	0.029%
16	6.087	508	510	513	rVB4	1795	2052	0.13%	0.026%
17	6.152	519	521	524	rBV4	1370	1655	0.11%	0.021%
18	6.234	533	535	538	rVB3	2323	2541	0.16%	0.032%
19	6.699	611	614	618	rVB6	1448	2068	0.13%	0.026%
20	6.887	644	646	649	rVB4	2248	1800	0.12%	0.023%
21	6.922	649	652	655	rBV4	1417	1959	0.13%	0.025%
22	6.999	663	665	668	rVB4	1364	1578	0.10%	0.020%
23	7.034	668	671	674	rVV4	2102	2221	0.14%	0.028%
24	7.075	677	678	681	rVB3	2501	2061	0.13%	0.026%
25	7.805	800	802	806	rVB5	1815	2279	0.15%	0.029%
26	7.922	813	822	836	rBV	472364	820714	52.48%	10.287%
27	8.363	895	897	899	rVB2	1954	1740	0.11%	0.022%
28	8.440	909	910	915	rBV5	1907	3006	0.19%	0.038%
29	8.493	917	919	922	rBV4	2145	2131	0.14%	0.027%
30	8.752	961	963	965	rBV3	1493	1680	0.11%	0.021%
31	8.816	973	974	976	rBV2	2764	2034	0.13%	0.025%
32	9.022	1006	1009	1010	rBV3	2291	2086	0.13%	0.026%
33	9.081	1017	1019	1020	rBV2	2062	1631	0.10%	0.020%
34	9.228	1040	1044	1045	rBV3	1944	2000	0.13%	0.025%
35	9.328	1059	1061	1065	rVB5	2107	1646	0.11%	0.021%
36	9.487	1085	1088	1090	rBV4	1501	1979	0.13%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010208.D
 Acq On : 03 May 2022 14:18
 Operator : CG/JU
 Sample : N2652-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	9.634	1109	1113	1114	rBV4	1536	1626	0.10%	0.020%
38	9.734	1129	1130	1133	rVB3	1930	1615	0.10%	0.020%
39	9.810	1142	1143	1148	rVB4	1382	1977	0.13%	0.025%
40	10.322	1228	1230	1233	rVB2	2054	1664	0.11%	0.021%
41	10.357	1233	1236	1237	rBV3	2228	2303	0.15%	0.029%
42	10.722	1291	1298	1313	rBV	613906	1129497	72.22%	14.157%
43	10.869	1322	1323	1328	rVB4	3361	3548	0.23%	0.044%
44	10.916	1328	1331	1336	rVB7	1270	1604	0.10%	0.020%
45	11.110	1362	1364	1367	rVB3	1523	1625	0.10%	0.020%
46	11.134	1367	1368	1373	rVV5	1654	2069	0.13%	0.026%
47	11.204	1377	1380	1382	rVV4	1580	1654	0.11%	0.021%
48	11.228	1382	1384	1387	rVB4	2428	1596	0.10%	0.020%
49	11.463	1423	1424	1428	rVB4	1722	1596	0.10%	0.020%
50	11.634	1452	1453	1457	rVV4	1785	1823	0.12%	0.023%
51	11.716	1463	1467	1469	rVV5	1283	2177	0.14%	0.027%
52	11.740	1469	1471	1474	rVB4	1721	1591	0.10%	0.020%
53	11.869	1490	1493	1497	rVB6	1385	2090	0.13%	0.026%
54	11.951	1504	1507	1509	rBV3	1754	2222	0.14%	0.028%
55	12.010	1513	1517	1519	rBV5	1250	1659	0.11%	0.021%
56	12.251	1555	1558	1561	rBV4	1738	2325	0.15%	0.029%
57	12.334	1568	1572	1573	rBV4	1729	1933	0.12%	0.024%
58	12.828	1653	1656	1660	rVB5	1560	2174	0.14%	0.027%
59	12.869	1660	1663	1666	rVB4	2181	2187	0.14%	0.027%
60	12.892	1666	1667	1671	rBV4	1659	2120	0.14%	0.027%
61	12.928	1671	1673	1676	rBV3	1536	1628	0.10%	0.020%
62	12.957	1676	1678	1681	rVB4	1444	1852	0.12%	0.023%
63	12.992	1681	1684	1686	rBV3	1726	1831	0.12%	0.023%
64	13.128	1704	1707	1709	rBV3	1352	1582	0.10%	0.020%
65	13.292	1731	1735	1736	rBV3	2443	2414	0.15%	0.030%
66	13.345	1739	1744	1745	rBV4	1636	1605	0.10%	0.020%
67	13.622	1788	1791	1793	rBV4	1330	1617	0.10%	0.020%
68	13.710	1802	1806	1811	rBV6	1158	2206	0.14%	0.028%
69	14.169	1881	1884	1886	rVB4	1638	1572	0.10%	0.020%
70	14.222	1888	1893	1895	rBV4	1806	2064	0.13%	0.026%
71	14.404	1917	1924	1927	rBV6	8154	18162	1.16%	0.228%
72	14.481	1936	1937	1940	rVB3	3019	1873	0.12%	0.023%
73	14.551	1942	1949	1961	rBV	877775	1367372	87.43%	17.139%
74	14.981	2020	2022	2027	rVB3	1355	1972	0.13%	0.025%
75	15.175	2052	2055	2058	rBV5	1818	2804	0.18%	0.035%
76	15.269	2070	2071	2076	rVB5	1416	1579	0.10%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010208.D
 Acq On : 03 May 2022 14:18
 Operator : CG/JU
 Sample : N2652-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

77	15.316	2076	2079	2082	rBV4	1463	2205	0.14%	0.028%
78	15.386	2088	2091	2093	rVB4	1807	1892	0.12%	0.024%
79	15.422	2093	2097	2098	rBV4	1900	2247	0.14%	0.028%
80	15.557	2117	2120	2122	rBV4	1637	2148	0.14%	0.027%
81	16.151	2219	2221	2223	rBV3	2083	2145	0.14%	0.027%
82	16.210	2228	2231	2234	rBV2	2136	2470	0.16%	0.031%
83	16.316	2245	2249	2250	rBV3	2158	2224	0.14%	0.028%
84	16.528	2282	2285	2289	rBV6	2376	3092	0.20%	0.039%
85	16.598	2296	2297	2301	rVB3	2257	2000	0.13%	0.025%
86	16.639	2301	2304	2305	rBV3	1929	1774	0.11%	0.022%
87	16.963	2357	2359	2362	rBV4	1850	2284	0.15%	0.029%
88	17.145	2389	2390	2393	rBV3	1365	1565	0.10%	0.020%
89	17.222	2401	2403	2406	rVB4	1954	2374	0.15%	0.030%
90	17.304	2409	2417	2445	rBV	732788	1563899	100.00%	19.602%
91	17.628	2470	2472	2474	rBV3	2099	2240	0.14%	0.028%
92	17.669	2478	2479	2482	rVB3	2783	1613	0.10%	0.020%
93	17.716	2484	2487	2488	rBV2	1901	2041	0.13%	0.026%
94	18.563	2629	2631	2634	rBV4	2345	2767	0.18%	0.035%
95	21.386	3106	3111	3123	rBV	997792	1515294	96.89%	18.993%
96	23.833	3520	3527	3541	rVB2	606731	1367913	87.47%	17.146%




Sum of corrected areas: 7978200

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010208.D
Acq On : 03 May 2022 14:18
Operator : CG/JU
Sample : N2652-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

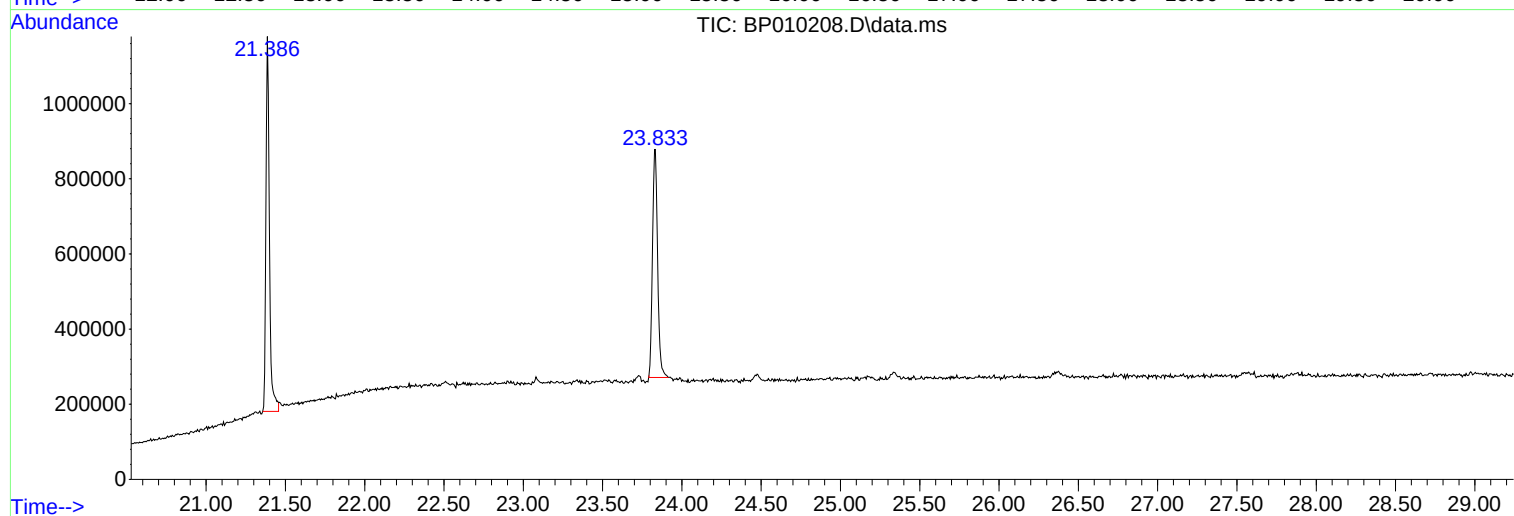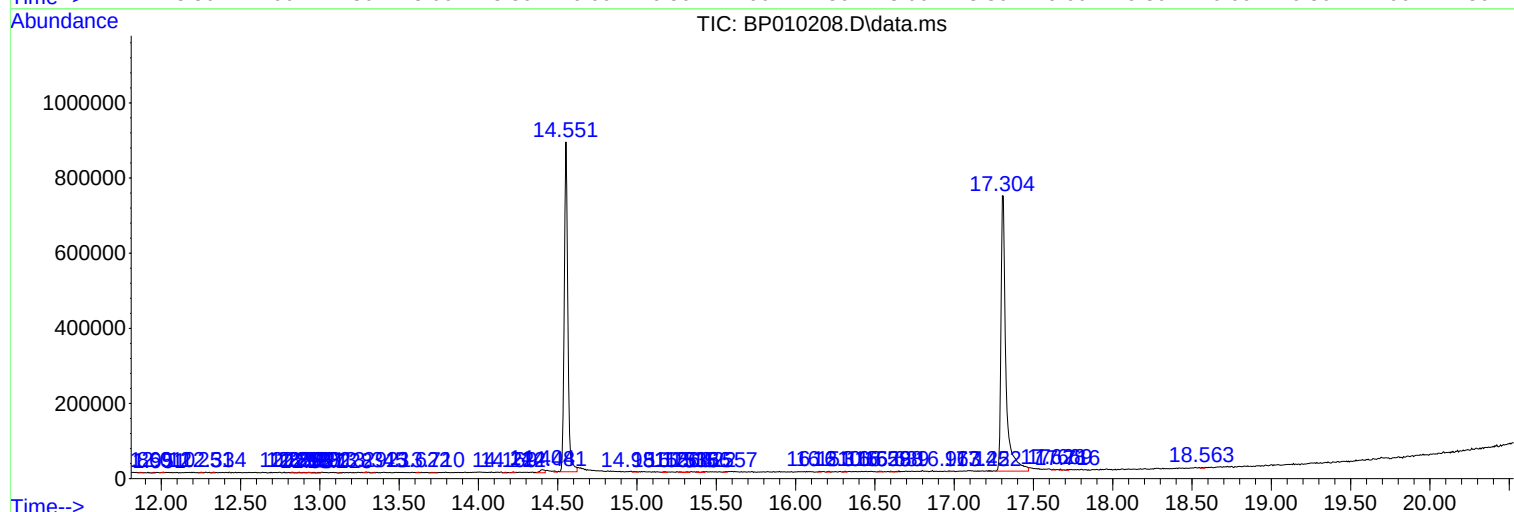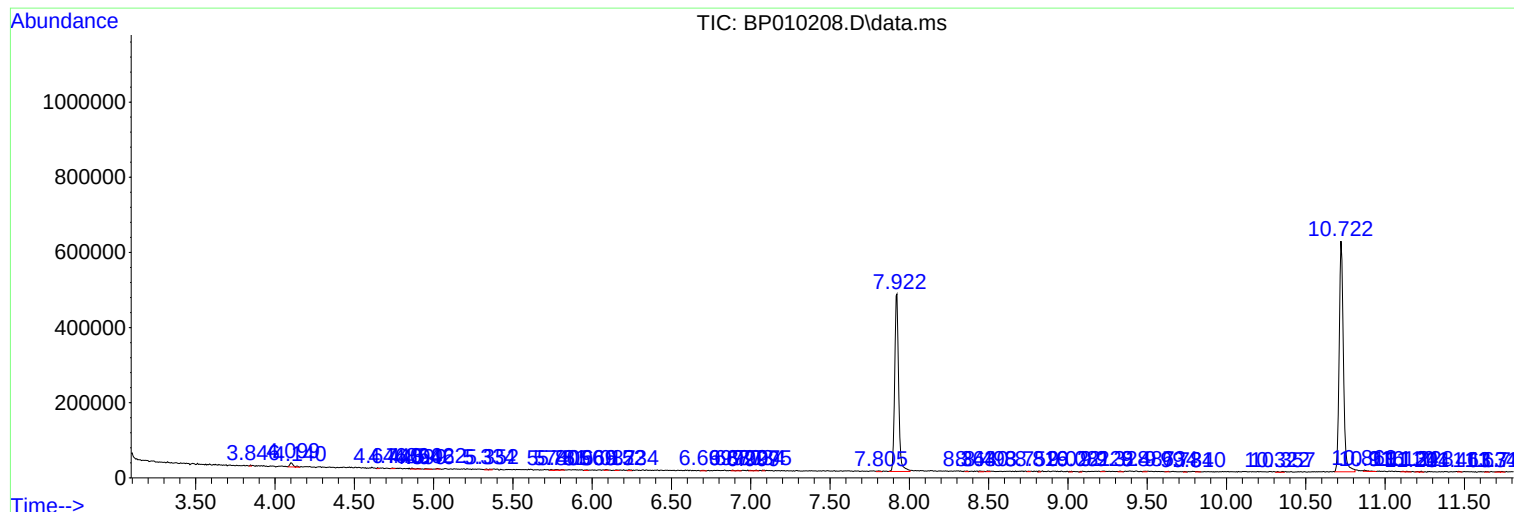

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010208.D
Acq On : 03 May 2022 14:18
Operator : CG/JU
Sample : N2652-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010208.D
Acq On : 03 May 2022 14:18
Operator : CG/JU
Sample : N2652-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------