

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010213.D
 Acq On : 03 May 2022 18:24
 Operator : CG/JU
 Sample : PB144543BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	52	rBV	47843	60802	1.74%	0.159%
2	3.769	113	116	131	rBV	542237	859352	24.57%	2.243%
3	4.105	170	173	178	rVB2	12094	14139	0.40%	0.037%
4	4.793	287	290	292	rBV3	3585	3844	0.11%	0.010%
5	7.081	672	679	692	rBV	635756	1040856	29.76%	2.716%
6	7.246	701	707	717	rBV	543960	868652	24.84%	2.267%
7	7.451	734	742	754	rBV	686626	1112047	31.80%	2.902%
8	7.916	813	821	835	rBV	584425	966539	27.64%	2.522%
9	8.628	934	942	956	rBV	791414	1324102	37.86%	3.456%
10	9.075	1011	1018	1027	rBV	647190	1112984	31.82%	2.905%
11	9.804	1133	1142	1162	rBV	523494	924898	26.45%	2.414%
12	10.345	1226	1234	1248	rBV	701369	1309444	37.44%	3.417%
13	10.722	1290	1298	1307	rBV	795322	1363868	39.00%	3.559%
14	10.857	1313	1321	1341	rBV	699891	1337461	38.24%	3.490%
15	12.322	1564	1570	1575	rBV5	10521	23544	0.67%	0.061%
16	12.522	1600	1604	1606	rBV5	2901	4320	0.12%	0.011%
17	13.357	1743	1746	1750	rVB6	2278	4090	0.12%	0.011%
18	13.957	1842	1848	1863	rBV	1339311	1969576	56.32%	5.140%
19	14.086	1868	1870	1875	rVB5	3922	5835	0.17%	0.015%
20	14.245	1889	1897	1911	rBV	1451527	2276717	65.10%	5.942%
21	14.392	1916	1922	1928	rVV10	6050	14775	0.42%	0.039%
22	14.551	1942	1949	1965	rBV	1202549	1733489	49.57%	4.524%
23	14.745	1975	1982	2005	rBV	331813	822370	23.51%	2.146%
24	15.363	2083	2087	2092	rVB8	2183	4111	0.12%	0.011%
25	15.545	2111	2118	2132	rVV	1892087	2875402	82.22%	7.504%
26	15.663	2132	2138	2151	rVV	518913	821007	23.48%	2.143%
27	15.786	2154	2159	2168	rVB2	24815	49158	1.41%	0.128%
28	16.333	2247	2252	2256	rVB5	6760	9448	0.27%	0.025%
29	16.986	2360	2363	2367	rVB6	4417	5796	0.17%	0.015%
30	17.092	2374	2381	2386	rBV6	4178	10661	0.30%	0.028%
31	17.304	2410	2417	2427	rBV	1358844	1994244	57.02%	5.205%
32	17.404	2427	2434	2451	rVB	1974926	3043312	87.02%	7.942%
33	18.410	2602	2605	2608	rBV5	3244	5109	0.15%	0.013%
34	18.798	2669	2671	2673	rBV3	3789	3680	0.11%	0.010%
35	19.210	2738	2741	2749	rVB4	25781	33939	0.97%	0.089%
36	19.280	2749	2753	2760	rBV	25323	35246	1.01%	0.092%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	19.633	2807	2813	2829	rBV	2567925	3497258	100.00%	9.127%
38	21.386	3106	3111	3126	rBV	1358384	1991321	56.94%	5.197%
39	23.668	3492	3499	3506	rBV2	1399773	2898504	82.88%	7.564%
40	23.827	3519	3526	3540	rVB2	873384	1885692	53.92%	4.921%




Sum of corrected areas: 38317592

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

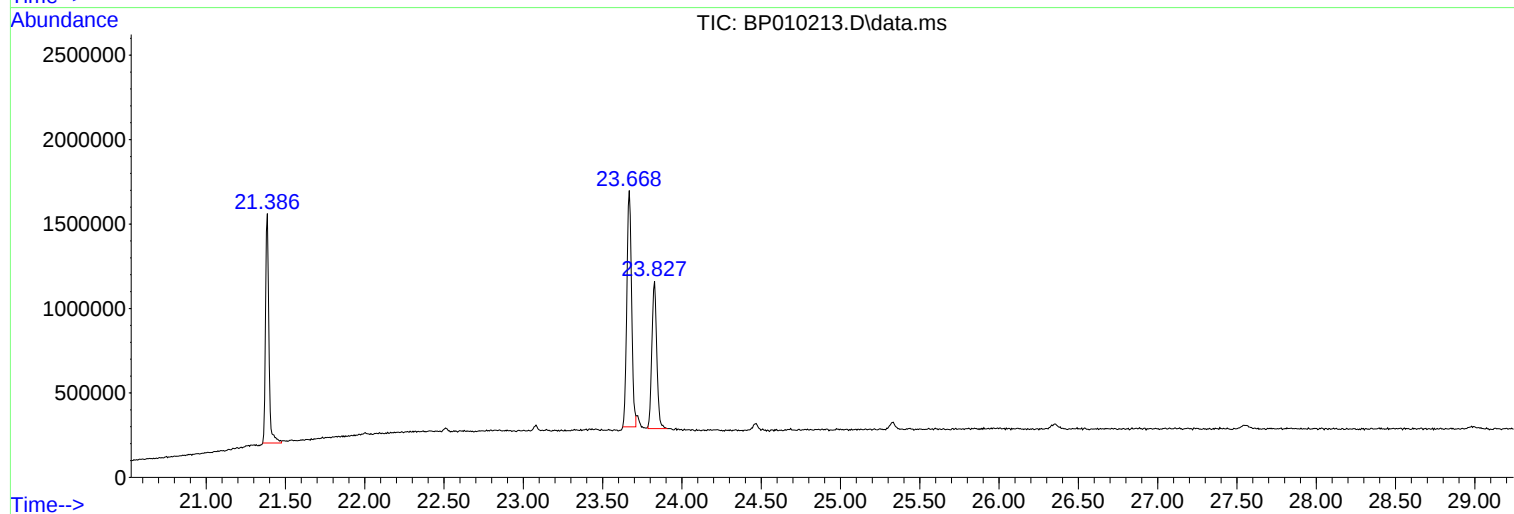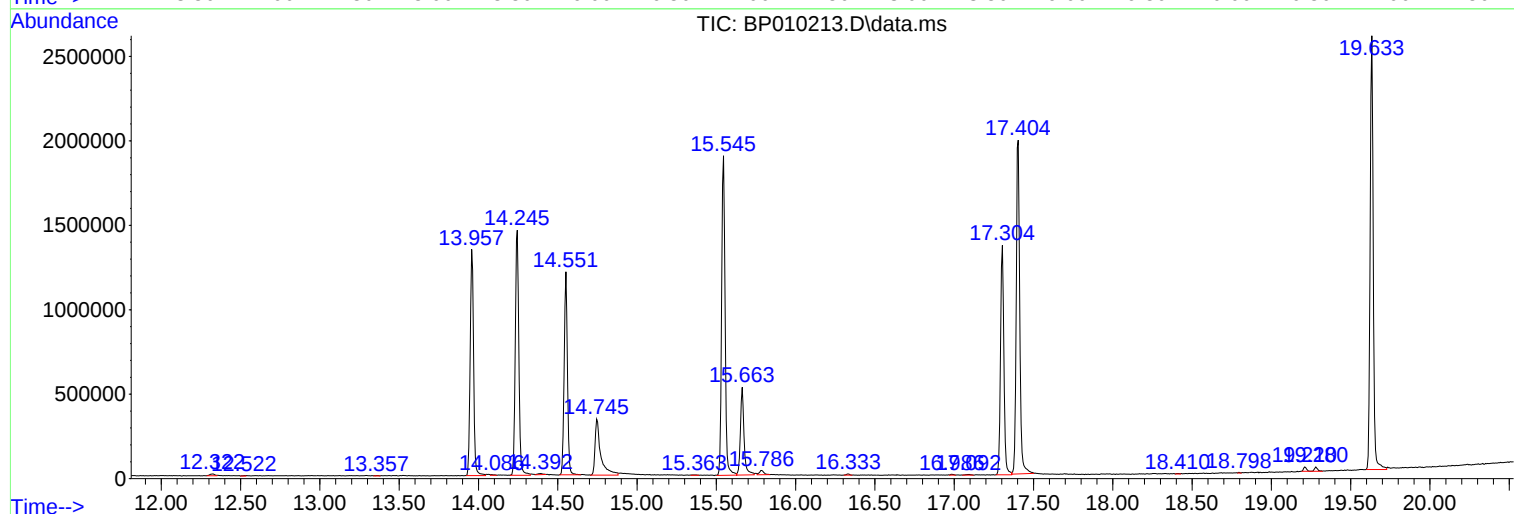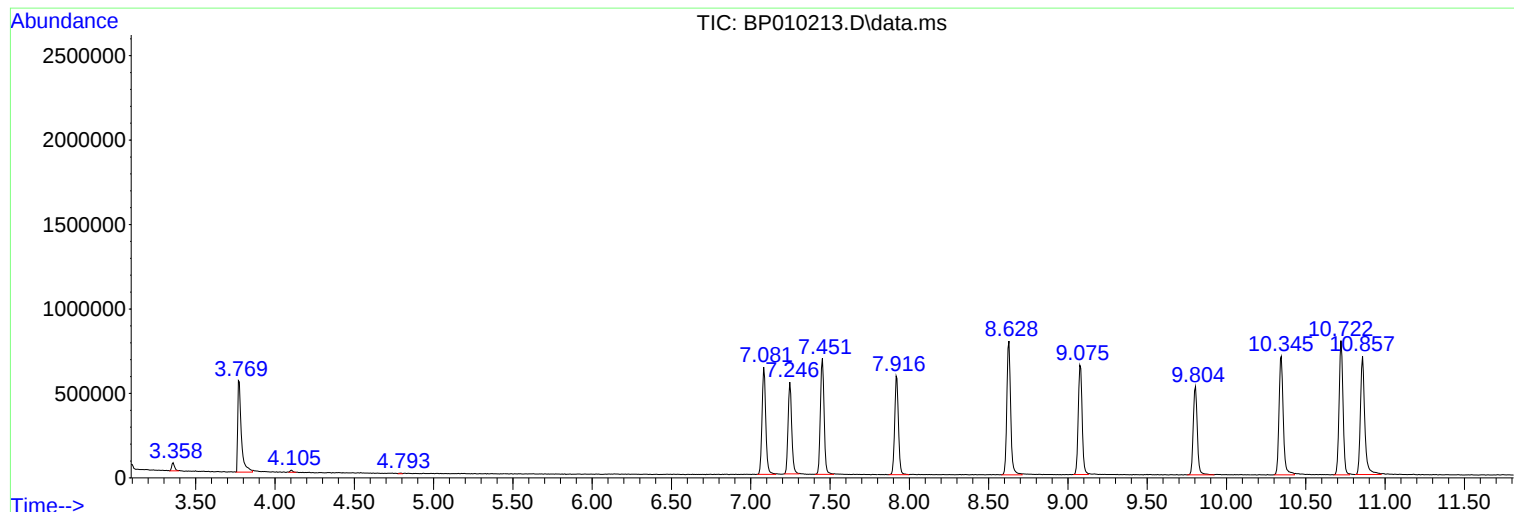

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010213.D
Acq On : 03 May 2022 18:24
Operator : CG/JU
Sample : PB144543BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc