

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010215.D
 Acq On : 03 May 2022 20:05
 Operator : CG/JU
 Sample : PB144558BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK558

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	51	rVB	45164	57822	1.76%	0.155%
2	3.770	113	116	135	rBV	527965	845745	25.74%	2.267%
3	4.105	169	173	178	rVB	17250	22845	0.70%	0.061%
4	6.640	600	604	607	rBV4	2027	3498	0.11%	0.009%
5	7.081	671	679	693	rBV	635343	1047670	31.88%	2.808%
6	7.246	701	707	722	rVB	551577	884273	26.91%	2.370%
7	7.452	734	742	756	rBV	676223	1103680	33.59%	2.959%
8	7.675	778	780	782	rBV3	3384	4003	0.12%	0.011%
9	7.916	813	821	836	rBV	593731	1007489	30.66%	2.701%
10	8.252	875	878	883	rVB6	2066	3424	0.10%	0.009%
11	8.628	933	942	958	rBV	769912	1325839	40.35%	3.554%
12	9.075	1009	1018	1028	rBV	649734	1128001	34.33%	3.024%
13	9.799	1134	1141	1158	rBV	513439	921817	28.05%	2.471%
14	10.340	1226	1233	1251	rBV	680884	1304516	39.70%	3.497%
15	10.722	1290	1298	1309	rBV	844976	1420838	43.24%	3.809%
16	10.857	1313	1321	1345	rVV	670143	1307124	39.78%	3.504%
17	12.316	1563	1569	1576	rBV5	10804	24218	0.74%	0.065%
18	13.534	1771	1776	1778	rBV5	2964	4304	0.13%	0.012%
19	13.957	1841	1848	1861	rBV	1295883	1939439	59.02%	5.199%
20	14.240	1888	1896	1914	rBV	1426582	2221380	67.60%	5.955%
21	14.398	1917	1923	1927	rVV9	4985	11769	0.36%	0.032%
22	14.551	1942	1949	1963	rBV	1193697	1792824	54.56%	4.806%
23	14.745	1976	1982	2005	rBV	300219	742191	22.59%	1.990%
24	15.363	2084	2087	2091	rBV5	2436	3909	0.12%	0.010%
25	15.545	2111	2118	2130	rVV	1780272	2765839	84.17%	7.414%
26	15.663	2132	2138	2155	rVV	473288	768267	23.38%	2.059%
27	15.787	2155	2159	2165	rVB3	22907	36876	1.12%	0.099%
28	16.334	2244	2252	2257	rBV9	6910	14308	0.44%	0.038%
29	16.981	2357	2362	2366	rVB8	4318	7356	0.22%	0.020%
30	17.186	2395	2397	2401	rBV4	2814	3636	0.11%	0.010%
31	17.304	2410	2417	2427	rBV	1318075	1998863	60.83%	5.358%
32	17.404	2427	2434	2452	rVB	1885262	2910531	88.57%	7.802%
33	18.133	2556	2558	2560	rBV2	3534	3907	0.12%	0.010%
34	18.751	2661	2663	2666	rBV4	3289	3881	0.12%	0.010%
35	19.210	2737	2741	2746	rBV4	25396	38950	1.19%	0.104%
36	19.280	2750	2753	2758	rVV	20344	27481	0.84%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010215.D
Acq On : 03 May 2022 20:05
Operator : CG/JU
Sample : PB144558BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	19.633	2807	2813	2827	rBV	2332328	3285978	100.00%	8.809%
38	21.386	3106	3111	3117	rBV	1323572	1838131	55.94%	4.927%
39	23.668	3492	3499	3506	rBV2	1324910	2718971	82.74%	7.289%
40	23.827	3519	3526	3536	rBV2	854679	1752126	53.32%	4.697%




Sum of corrected areas: 37303719

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010215.D
Acq On : 03 May 2022 20:05
Operator : CG/JU
Sample : PB144558BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

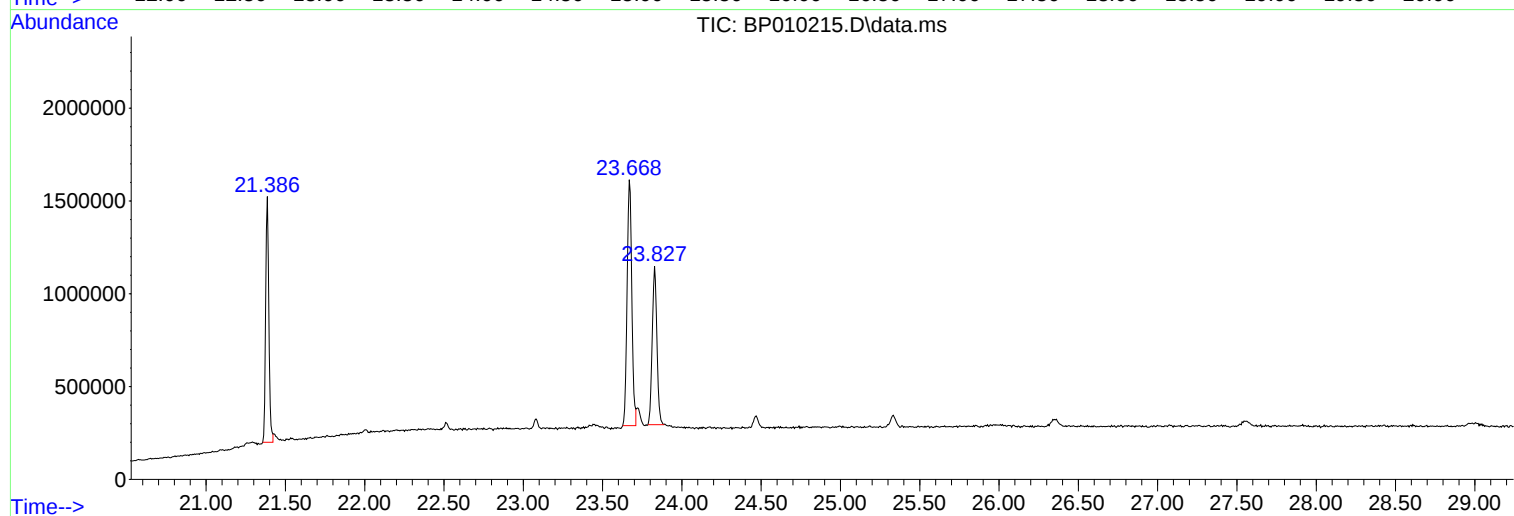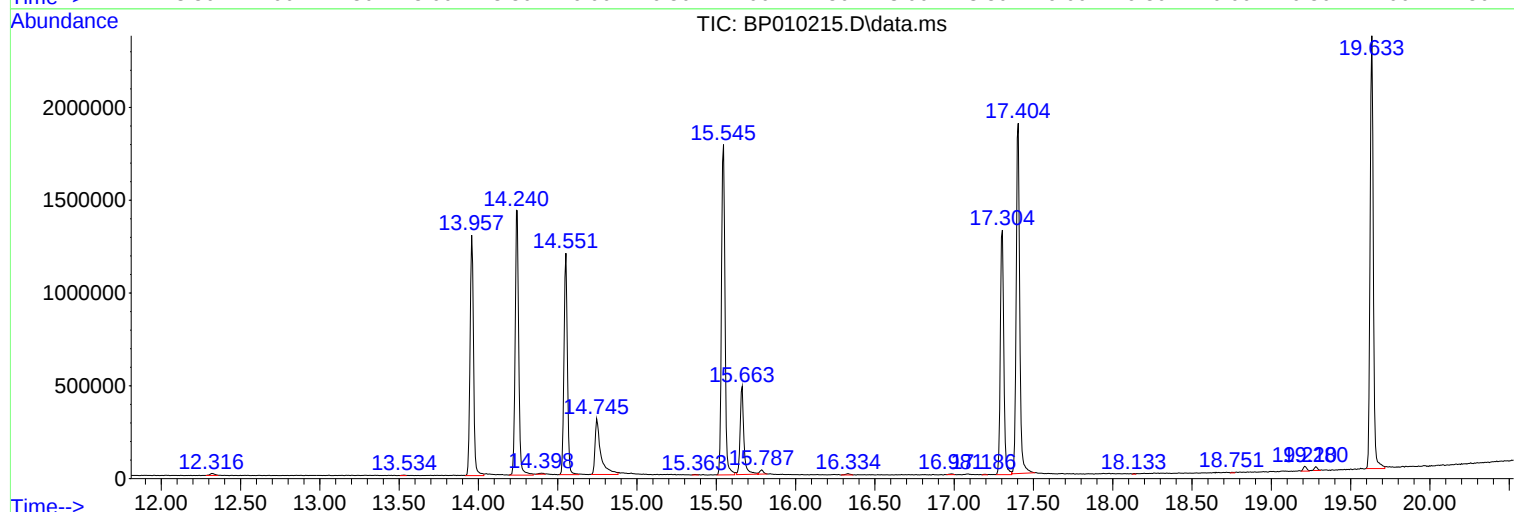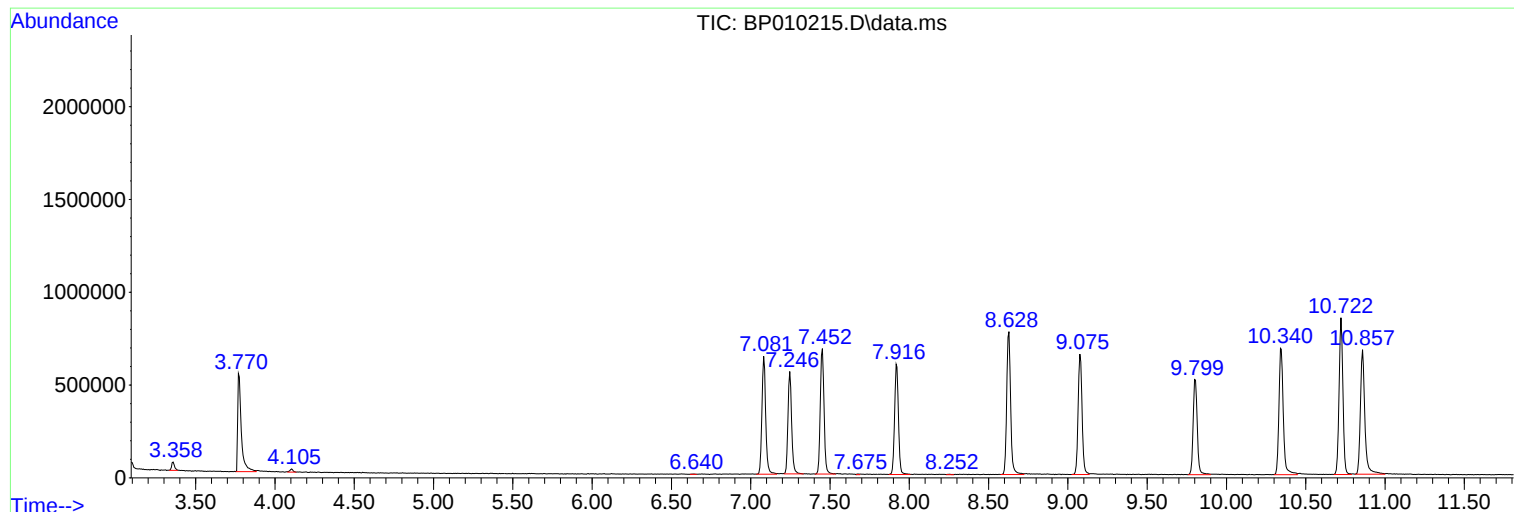

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010215.D
Acq On : 03 May 2022 20:05
Operator : CG/JU
Sample : PB144558BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010215.D
Acq On : 03 May 2022 20:05
Operator : CG/JU
Sample : PB144558BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK558

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc