

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010219.D
 Acq On : 03 May 2022 22:19
 Operator : CG/JU
 Sample : N2670-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COW00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	53	rVB	33036	45230	1.21%	0.128%
2	3.781	115	118	132	rBV	105730	178949	4.80%	0.505%
3	4.011	155	157	160	rVB4	5682	6126	0.16%	0.017%
4	4.105	169	173	182	rVB	36233	53335	1.43%	0.150%
5	7.081	672	679	690	rBV	107013	184485	4.95%	0.520%
6	7.246	700	707	720	rBV	516678	835176	22.39%	2.355%
7	7.452	735	742	756	rBV	475066	790330	21.19%	2.228%
8	7.552	756	759	764	rVB5	3939	5930	0.16%	0.017%
9	7.916	814	821	832	rBV	543037	892521	23.93%	2.516%
10	8.628	933	942	952	rBV	321302	571116	15.31%	1.610%
11	9.075	1008	1018	1031	rBV	637410	1095336	29.36%	3.088%
12	9.522	1090	1094	1102	rVB5	7989	14440	0.39%	0.041%
13	9.804	1130	1142	1155	rBV	468616	853101	22.87%	2.405%
14	10.346	1224	1234	1248	rBV	609944	1133877	30.40%	3.197%
15	10.722	1290	1298	1312	rBV	743731	1287972	34.53%	3.631%
16	10.857	1314	1321	1346	rVV	508684	1001328	26.84%	2.823%
17	12.022	1514	1519	1524	rVB7	5616	9143	0.25%	0.026%
18	12.316	1565	1569	1578	rBV3	11393	21708	0.58%	0.061%
19	13.528	1770	1775	1777	rBV6	3260	4975	0.13%	0.014%
20	13.957	1841	1848	1862	rBV	1425719	2041055	54.71%	5.755%
21	14.240	1889	1896	1913	rBV	1484468	2297045	61.58%	6.476%
22	14.392	1917	1922	1932	rVB	5069	16823	0.45%	0.047%
23	14.551	1941	1949	1959	rBV	1097590	1708422	45.80%	4.817%
24	14.757	1978	1984	2002	rBV3	28908	95831	2.57%	0.270%
25	14.969	2016	2020	2022	rBV5	2832	3778	0.10%	0.011%
26	15.545	2110	2118	2132	rBV	1896845	3012749	80.76%	8.494%
27	15.663	2132	2138	2153	rVV	517350	846600	22.69%	2.387%
28	15.787	2155	2159	2174	rVB2	28498	59284	1.59%	0.167%
29	16.328	2248	2251	2257	rVB8	7893	12679	0.34%	0.036%
30	16.986	2359	2363	2368	rVB7	4196	7686	0.21%	0.022%
31	17.298	2410	2416	2427	rBV	1293600	1984425	53.20%	5.595%
32	17.398	2427	2433	2456	rVB	2067747	3327663	89.21%	9.382%
33	18.263	2578	2580	2584	rVB5	4491	4229	0.11%	0.012%
34	19.210	2737	2741	2746	rBV2	27154	38996	1.05%	0.110%
35	19.280	2750	2753	2759	rVB	21496	30309	0.81%	0.085%
36	19.633	2807	2813	2827	rBV	2667652	3730343	100.00%	10.517%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW00

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	21.380	3105	3110	3122	rBV	1364535	2014798	54.01%	5.681%
38	23.668	3491	3499	3516	rVV	1550583	3369242	90.32%	9.499%
39	23.827	3519	3526	3542	rVB2	861459	1881333	50.43%	5.304%




Sum of corrected areas: 35468368

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

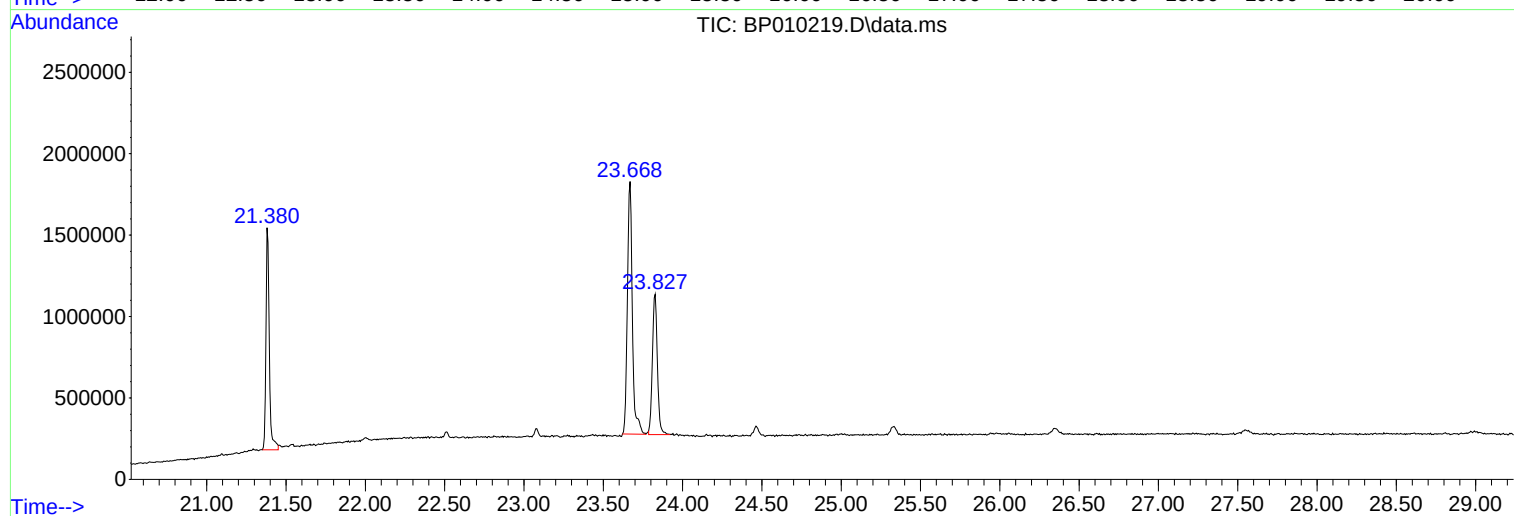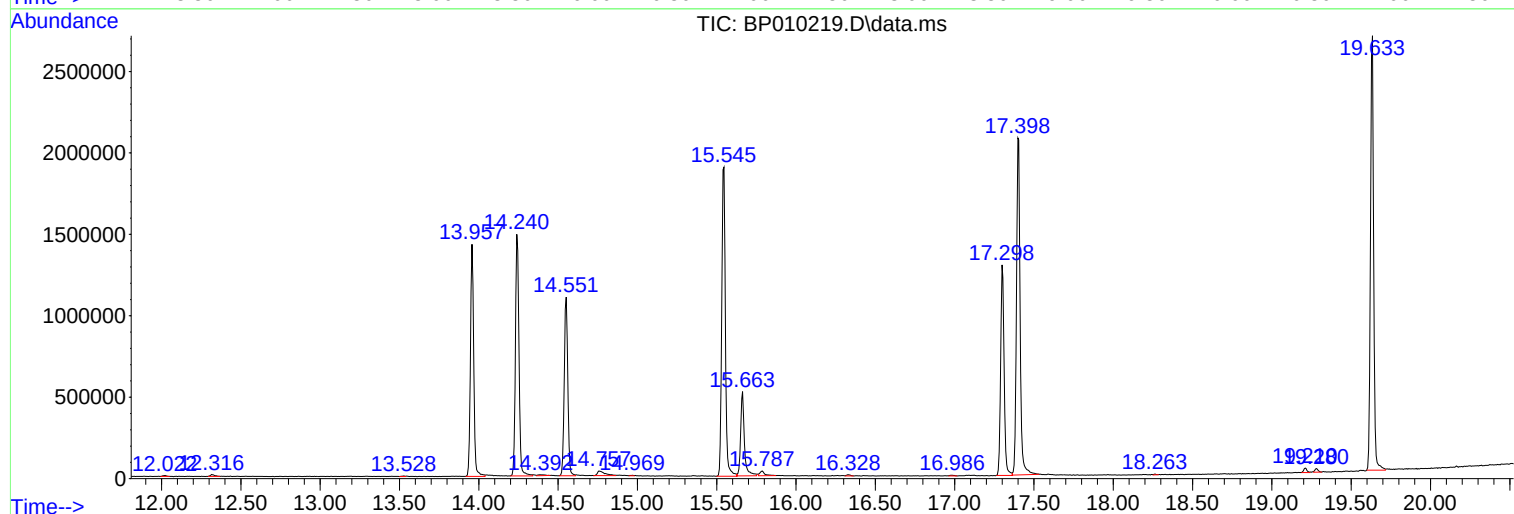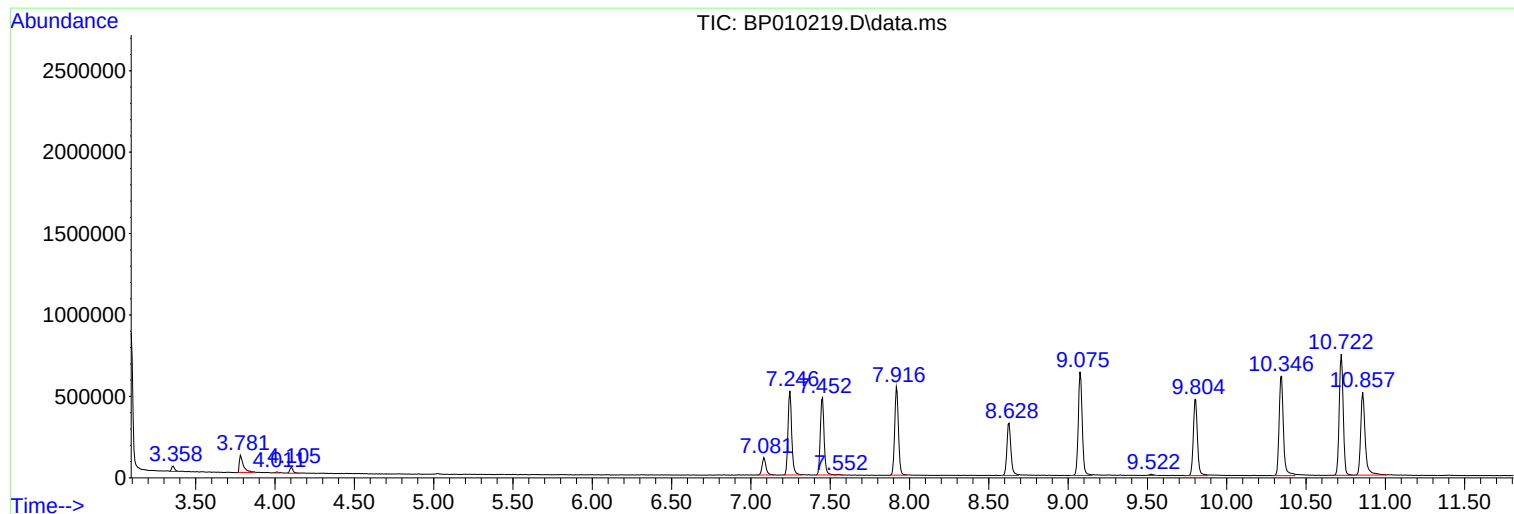

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010219.D
Acq On : 03 May 2022 22:19
Operator : CG/JU
Sample : N2670-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0W00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc