

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
 Data File : BP010220.D
 Acq On : 03 May 2022 22:53
 Operator : CG/JU
 Sample : N2670-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COW02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	55	rVB	42696	58357	1.43%	0.145%
2	3.781	115	118	132	rBV	138969	224071	5.50%	0.558%
3	4.011	154	157	167	rVB5	8408	16464	0.40%	0.041%
4	4.105	169	173	180	rVB	18580	28719	0.71%	0.071%
5	5.022	324	329	333	rBV3	5750	8377	0.21%	0.021%
6	7.081	673	679	688	rBV	160767	274964	6.75%	0.684%
7	7.246	700	707	726	rVB	695782	1112024	27.31%	2.768%
8	7.452	734	742	756	rBV	633270	1081583	26.56%	2.692%
9	7.552	756	759	764	rVB7	4845	7043	0.17%	0.018%
10	7.652	772	776	781	rVB8	3968	7261	0.18%	0.018%
11	7.916	814	821	838	rVB	591595	959959	23.57%	2.389%
12	8.622	934	941	956	rBV	465796	819036	20.11%	2.038%
13	9.075	1009	1018	1033	rBV	862816	1477499	36.28%	3.677%
14	9.528	1089	1095	1099	rVB6	5478	10500	0.26%	0.026%
15	9.799	1133	1141	1154	rBV	639962	1142637	28.06%	2.844%
16	10.340	1226	1233	1252	rBV	829229	1514732	37.20%	3.770%
17	10.722	1289	1298	1312	rBV	821662	1401602	34.42%	3.488%
18	10.857	1313	1321	1347	rVV	742418	1422497	34.93%	3.540%
19	12.022	1513	1519	1524	rVB3	6968	11113	0.27%	0.028%
20	12.322	1562	1570	1578	rBV3	13706	31863	0.78%	0.079%
21	13.957	1839	1848	1863	rBV	1730774	2458374	60.37%	6.118%
22	14.240	1887	1896	1918	rBV	1785266	2841466	69.78%	7.072%
23	14.551	1941	1949	1963	rBV	1121827	1739474	42.72%	4.329%
24	14.757	1978	1984	2006	rBV3	43766	155738	3.82%	0.388%
25	15.351	2082	2085	2087	rBV3	3561	4168	0.10%	0.010%
26	15.545	2109	2118	2131	rBV	2245458	3536746	86.85%	8.802%
27	15.663	2132	2138	2154	rVV	639569	1033465	25.38%	2.572%
28	15.786	2155	2159	2165	rVB2	28666	47243	1.16%	0.118%
29	16.328	2245	2251	2257	rBV8	9673	17061	0.42%	0.042%
30	16.981	2356	2362	2366	rBV9	5986	9359	0.23%	0.023%
31	17.086	2375	2380	2382	rBV6	3886	5694	0.14%	0.014%
32	17.298	2410	2416	2427	rBV	1197365	1845303	45.31%	4.593%
33	17.398	2427	2433	2456	rVB2	2263635	3697765	90.80%	9.203%
34	17.933	2520	2524	2527	rBV6	2887	4898	0.12%	0.012%
35	19.210	2737	2741	2746	rBV2	31768	45530	1.12%	0.113%
36	19.280	2749	2753	2757	rVV	23524	33192	0.82%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010220.D
Acq On : 03 May 2022 22:53
Operator : CG/JU
Sample : N2670-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW02

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	19.633	2807	2813	2830	rBV	2958472	4072215	100.00%	10.135%
38	21.386	3105	3111	3121	rBV	1194700	1790383	43.97%	4.456%
39	23.668	3491	3499	3506	rBV2	1730621	3564042	87.52%	8.870%
40	23.827	3519	3526	3536	rVB2	782881	1668146	40.96%	4.152%


Sum of corrected areas: 40180563

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010220.D
Acq On : 03 May 2022 22:53
Operator : CG/JU
Sample : N2670-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COW02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

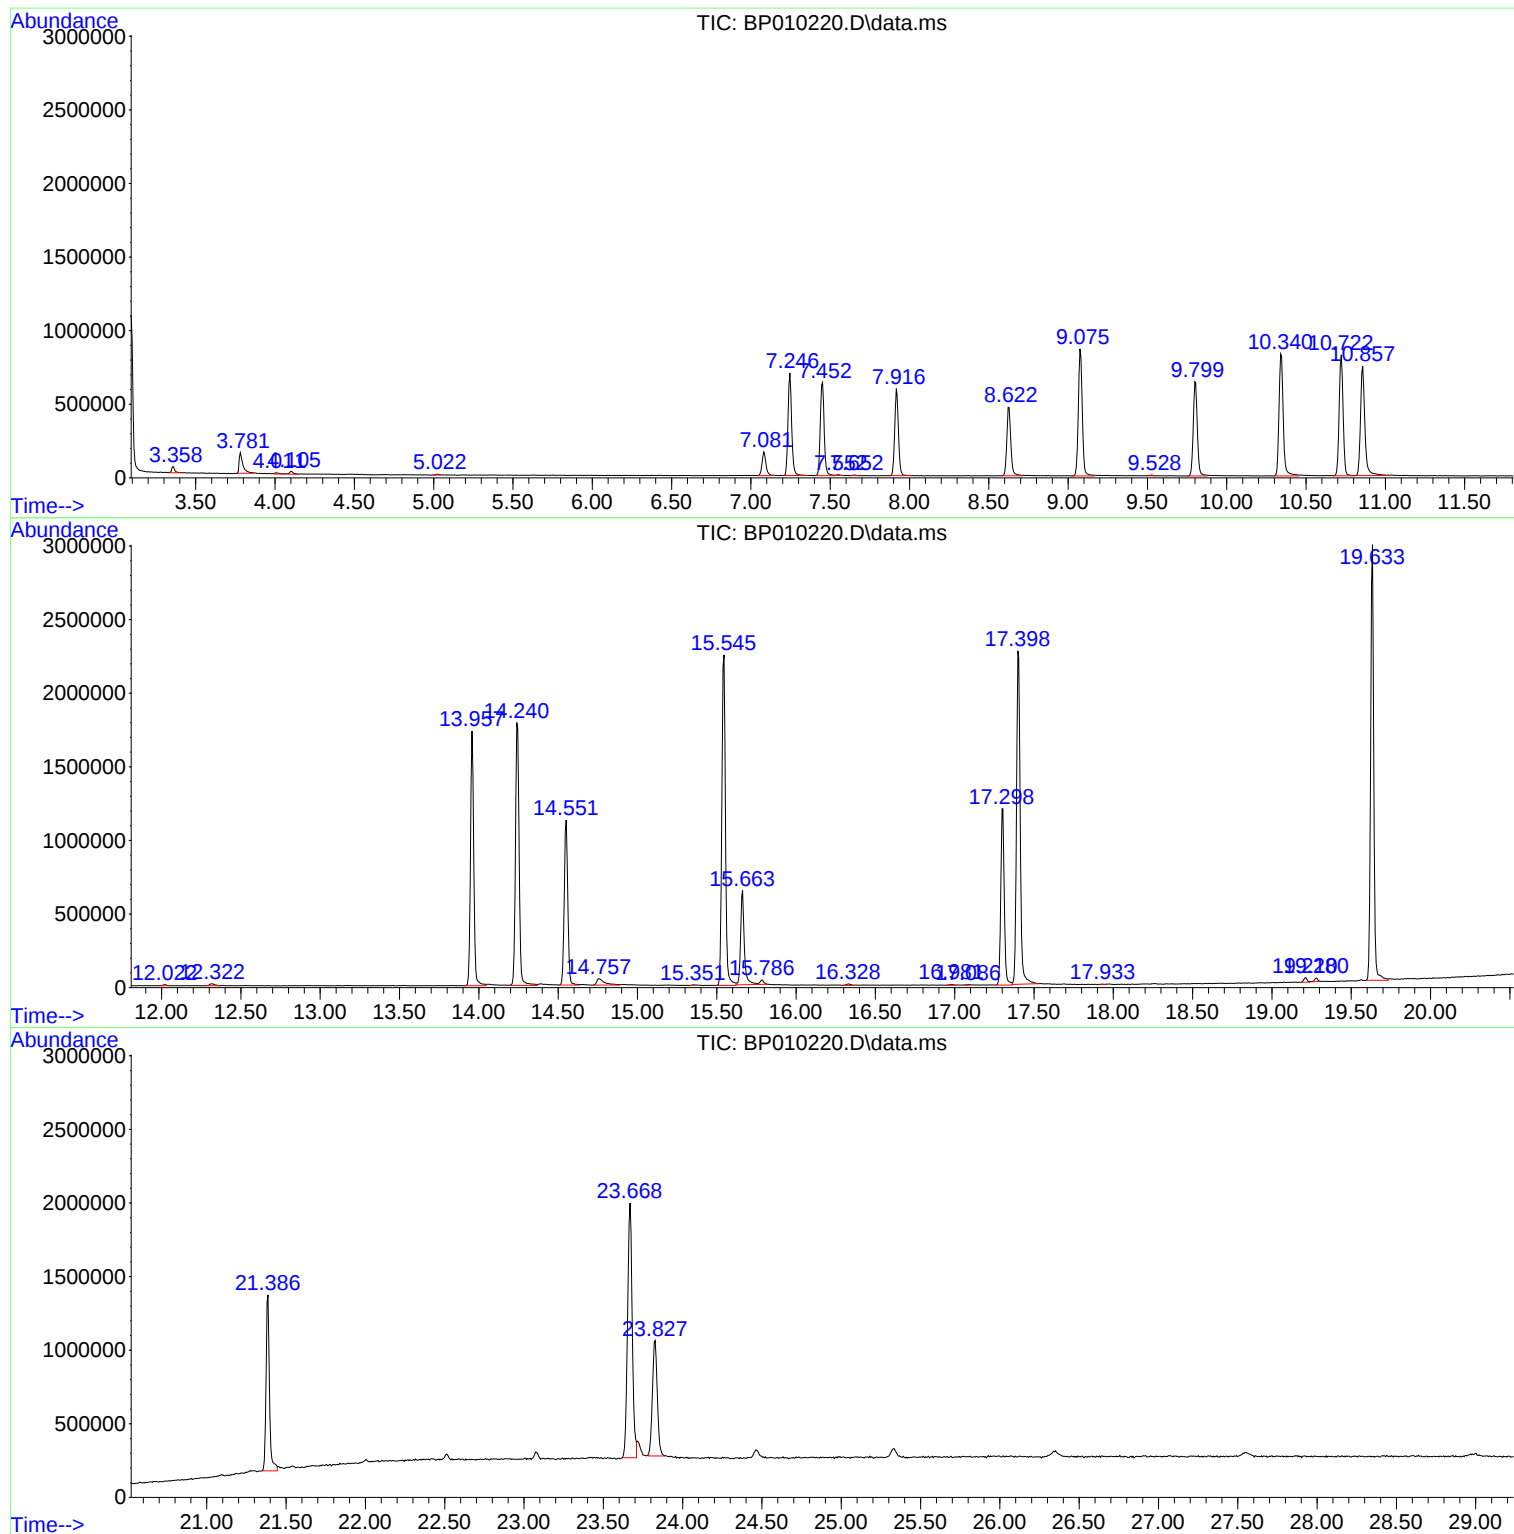

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010220.D
Acq On : 03 May 2022 22:53
Operator : CG/JU
Sample : N2670-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0W02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050222\
Data File : BP010220.D
Acq On : 03 May 2022 22:53
Operator : CG/JU
Sample : N2670-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0W02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc