




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020156.D
 Acq On : 02 May 2024 22:12
 Operator : MA/JU
 Sample : P2251-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AR3

Manual IntegrationsAPPROVED

Quant Time: May 03 00:44:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

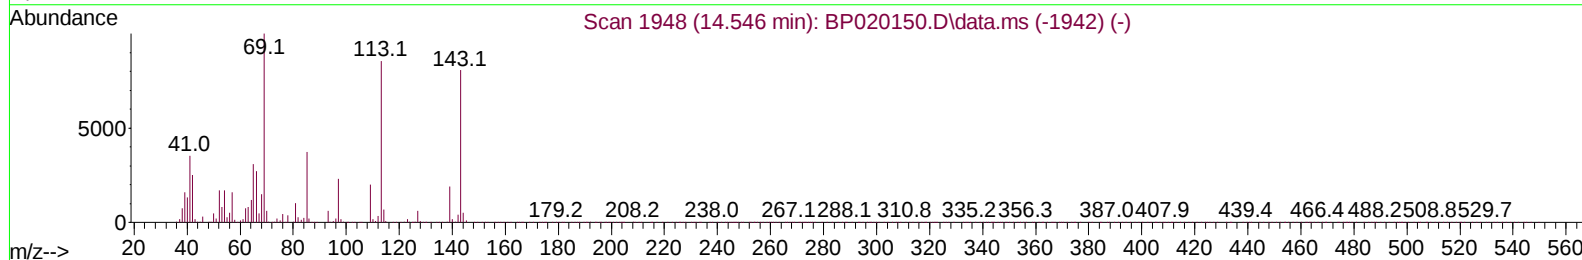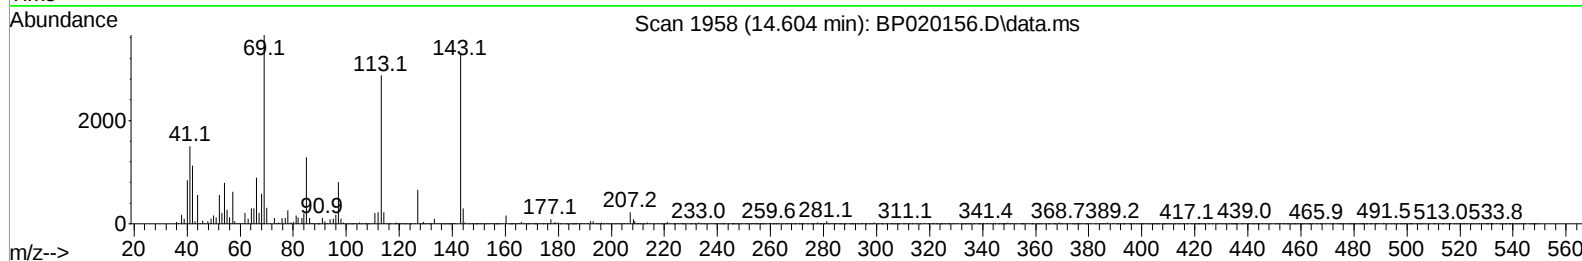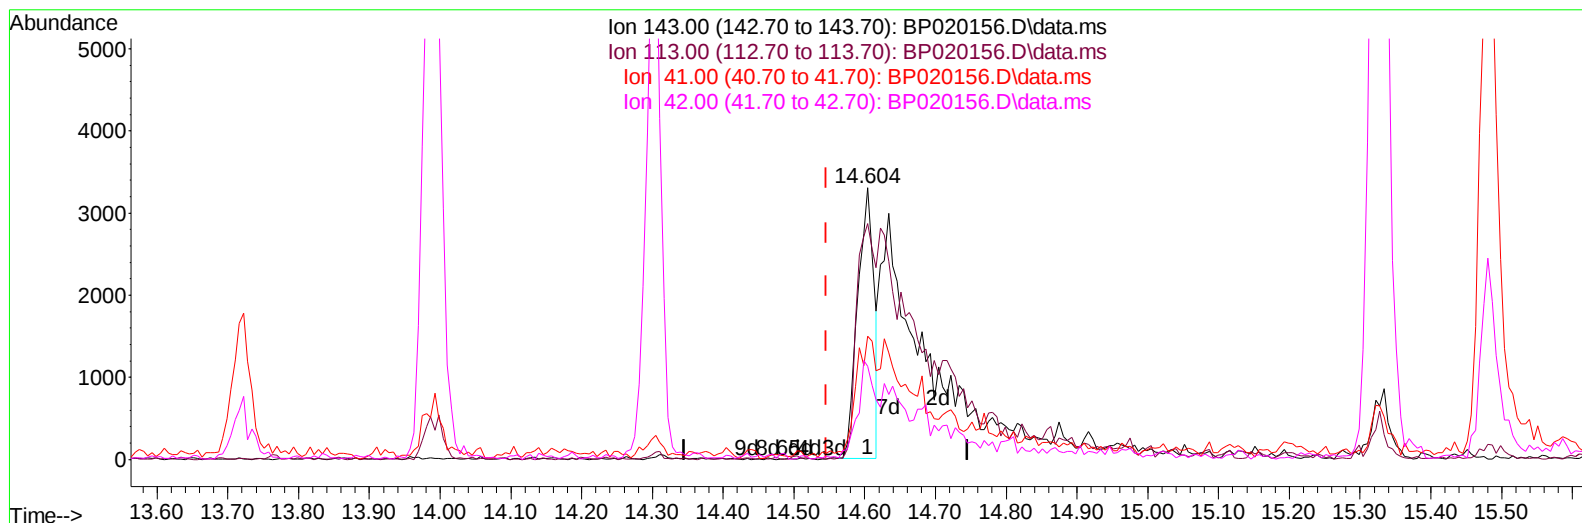

TIC: BP020156.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.604min (+ 0.059) 1.91 ng/u1

response 5300

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	86.90
41.00	50.30	45.40
42.00	32.50	34.27




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020156.D
Acq On : 02 May 2024 22:12
Operator : MA/JU
Sample : P2251-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AR3

Manual IntegrationsAPPROVED

Quant Time: May 03 00:44:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 00:38:56 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
Supervised By :mohammad ahmed 05/06/2024

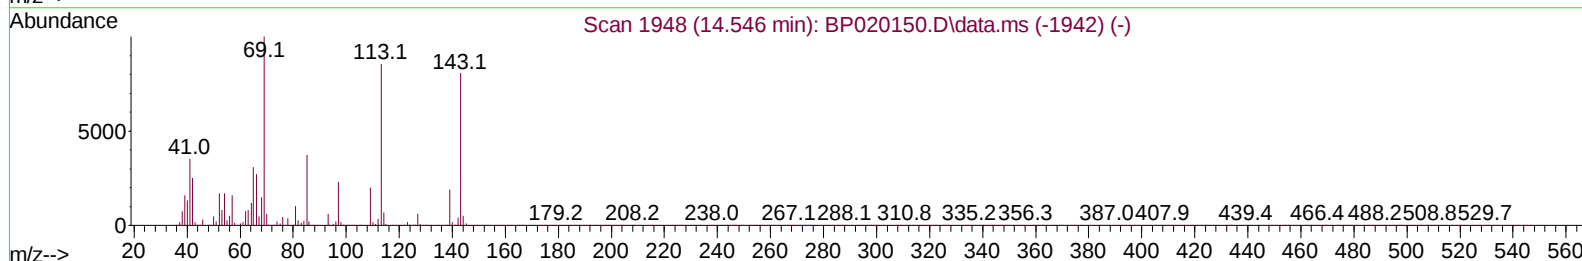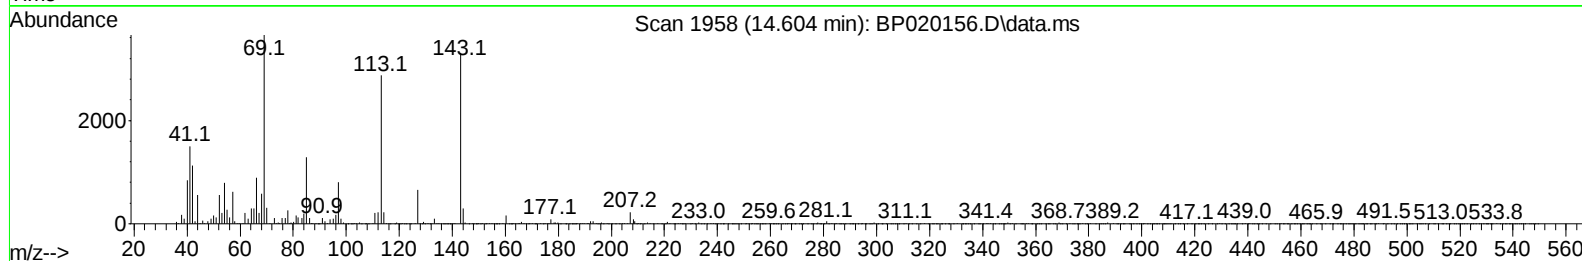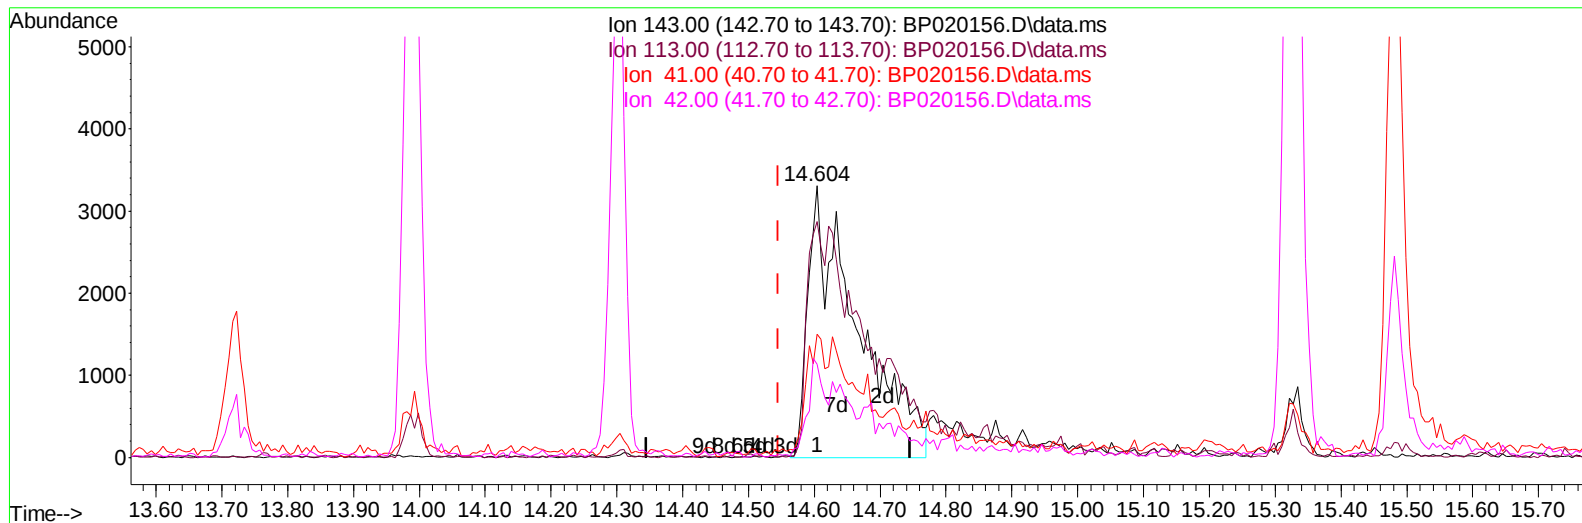

TIC: BP020156.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.604min (+ 0.059) 6.16 ng/ul m

response 17147

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	86.90
41.00	50.30	45.40
42.00	32.50	34.27

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020156.D
 Acq On : 02 May 2024 22:12
 Operator : MA/JU
 Sample : P2251-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AR3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 03 01:53:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	84465	20.000	ng/ul	0.00
20) Naphthalene-d8	10.399	136	350977	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	247849	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.145	188	547597	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	466124	20.000	ng/ul	0.00
88) Perylene-d12	24.992	264	416498	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	9694	4.847	ng/uL	0.00
4) Pyridine-d5	3.646	84	19999	3.441	ng/ul	0.02
7) Phenol-d5	6.822	99	52362	7.219	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.981	67	179161	40.659	ng/ul	0.00
11) 2-Chlorophenol-d4	7.164	132	160104	30.875	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	103931	17.722	ng/ul	0.01
21) Nitrobenzene-d5	8.787	128	109877	41.807	ng/ul	0.00
24) 2-Nitrophenol-d4	9.499	143	121137	40.249	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	182977	33.315	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	193187	25.132	ng/ul	0.01
46) Dimethylphthalate-d6	13.722	166	793514	43.842	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160	851094	42.568	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	17147m	6.164	ng/ul	0.06
60) Fluorene-d10	15.328	176	673535	44.616	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	131627	37.879	ng/ul	0.00
73) Anthracene-d10	17.245	188	1120939	47.318	ng/ul	0.00
81) Pyrene-d10	19.645	212	1311640	48.138	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.769	264	955454	47.445	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020156.D
Acq On : 02 May 2024 22:12
Operator : MA/JU
Sample : P2251-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AR3

Manual IntegrationsAPPROVED

Quant Time: May 03 01:53:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 00:38:56 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
Supervised By :mohammad ahmed 05/06/2024

