




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020162.D
 Acq On : 03 May 2024 02:37
 Operator : MA/JU
 Sample : P2279-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORR7

Manual IntegrationsAPPROVED

Quant Time: May 03 04:12:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

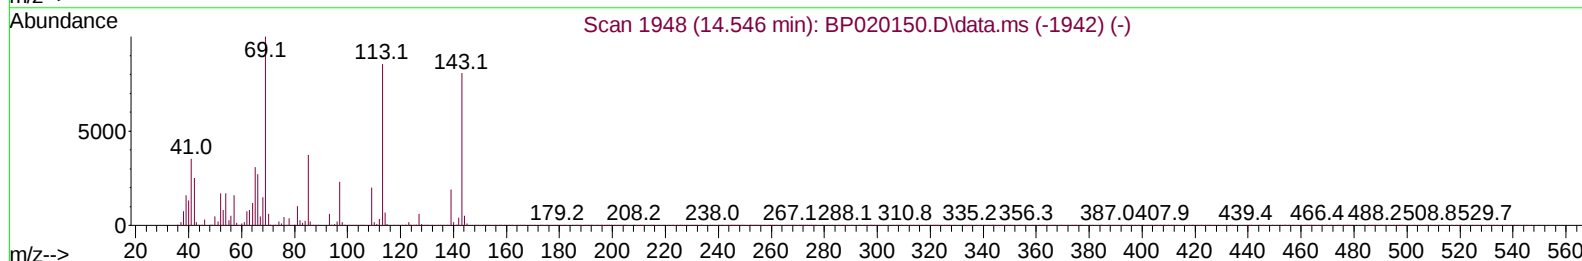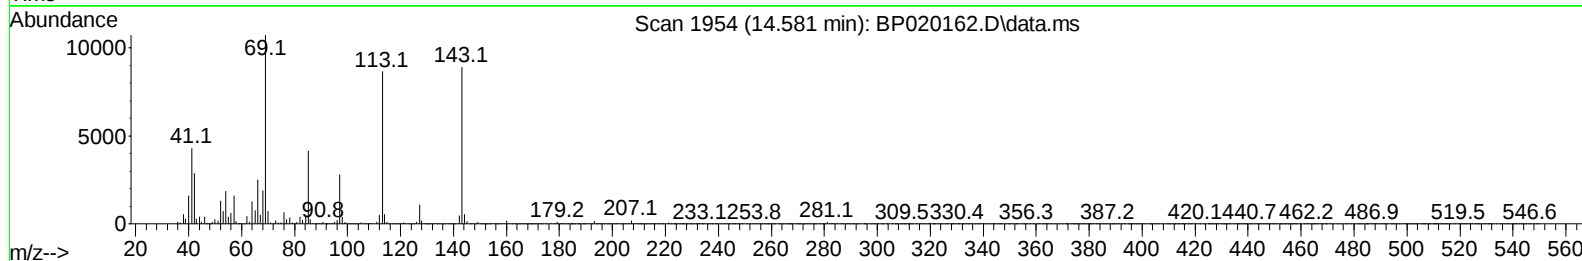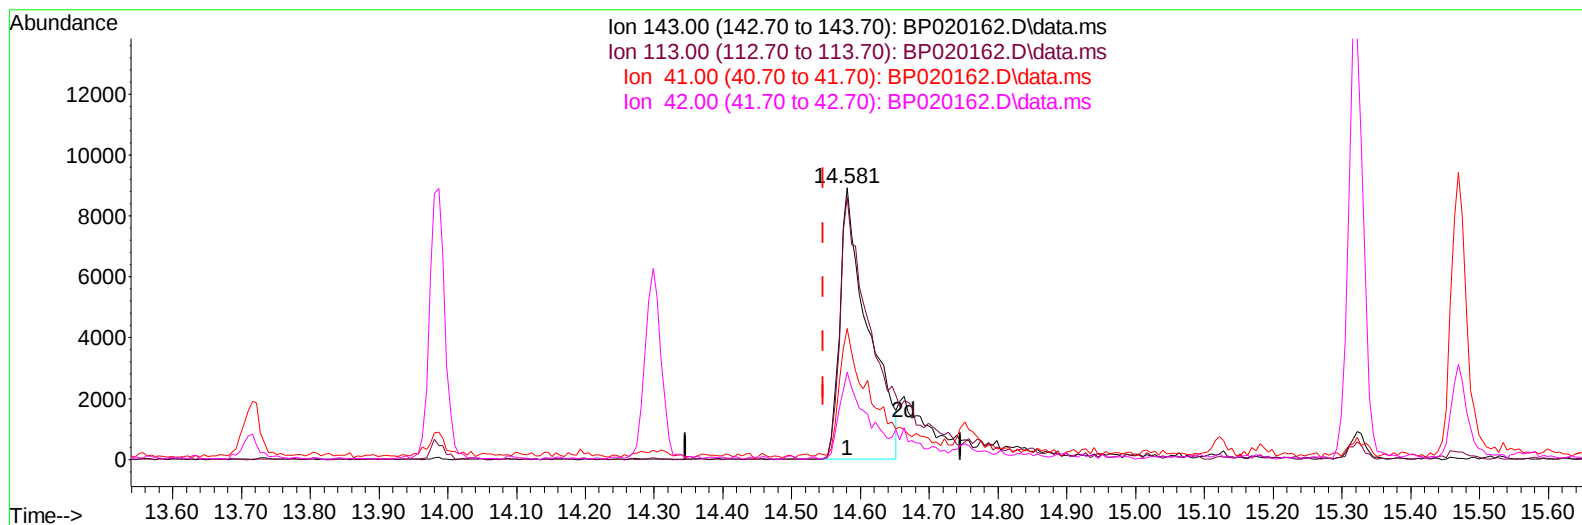

TIC: BP020162.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 8.57 ng/u1

response 25256

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	96.90
41.00	50.30	48.31
42.00	32.50	32.21




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020162.D
 Acq On : 03 May 2024 02:37
 Operator : MA/JU
 Sample : P2279-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORR7

Manual IntegrationsAPPROVED

Quant Time: May 03 04:12:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

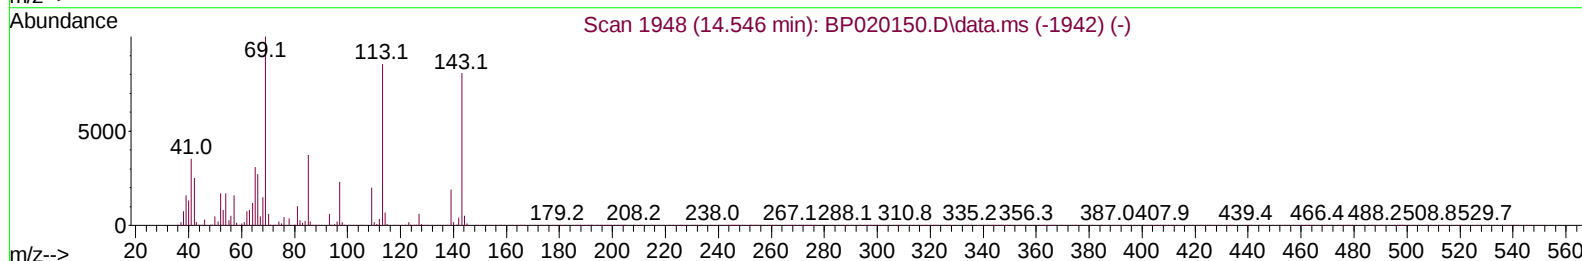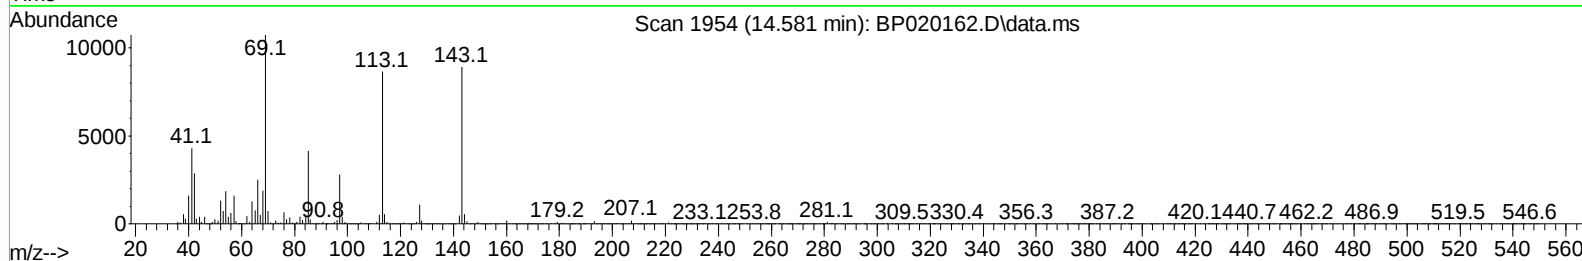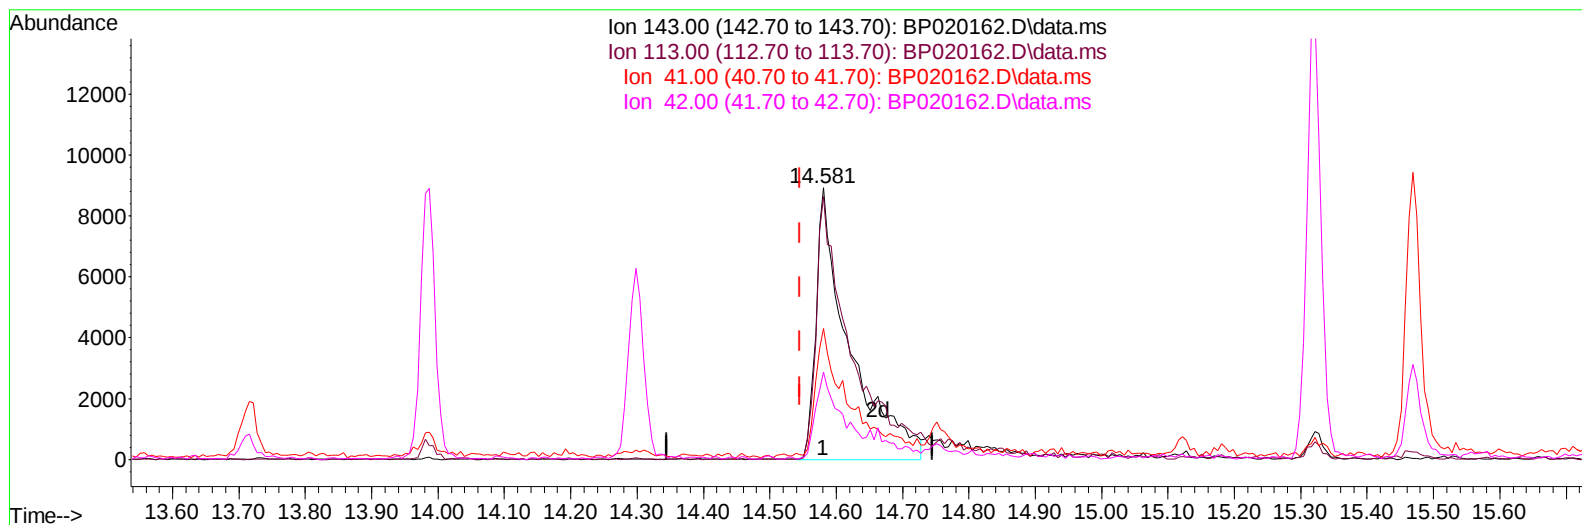

TIC: BP020162.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 10.50 ng/ul m

response 30941

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	96.90
41.00	50.30	48.31
42.00	32.50	32.21

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020162.D
 Acq On : 03 May 2024 02:37
 Operator : MA/JU
 Sample : P2279-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORR7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 03 04:13:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	74867	20.000	ng/ul	0.00
20) Naphthalene-d8	10.404	136	343364	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164	262434	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	603088	20.000	ng/ul	-0.01
79) Chrysene-d12	21.627	240	625187	20.000	ng/ul	-0.01
88) Perylene-d12	24.992	264	645193	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	9109	5.139	ng/uL	0.00
4) Pyridine-d5	3.634	84	40662	7.894	ng/ul	0.01
7) Phenol-d5	6.816	99	57267	8.907	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	157607	40.353	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132	145774	31.716	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	106651	20.517	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	100442	39.064	ng/ul	0.00
24) 2-Nitrophenol-d4	9.499	143	115131	39.101	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	181465	33.773	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	198025	26.333	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166	898150	46.865	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160	880663	41.599	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	30941m	10.505	ng/ul	0.04
60) Fluorene-d10	15.322	176	740820	46.345	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	167196	43.688	ng/ul	0.00
73) Anthracene-d10	17.239	188	1300439	49.844	ng/ul	0.00
81) Pyrene-d10	19.639	212	1648153	45.099	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.768	264	1573767	50.448	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020162.D
Acq On : 03 May 2024 02:37
Operator : MA/JU
Sample : P2279-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0RR7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2024
Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 03 04:13:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 00:38:56 2024
Response via : Initial Calibration

