




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020163.D
 Acq On : 03 May 2024 03:21
 Operator : MA/JU
 Sample : P2279-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORR8

Manual IntegrationsAPPROVED

Quant Time: May 03 04:15:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

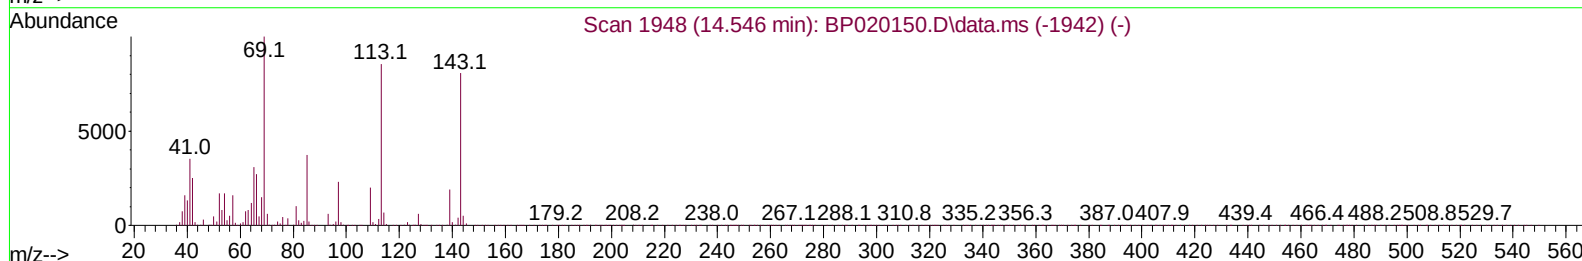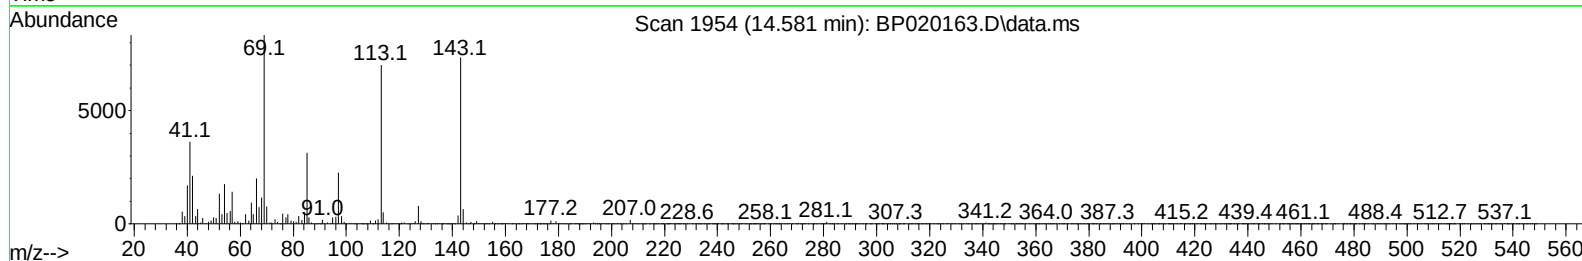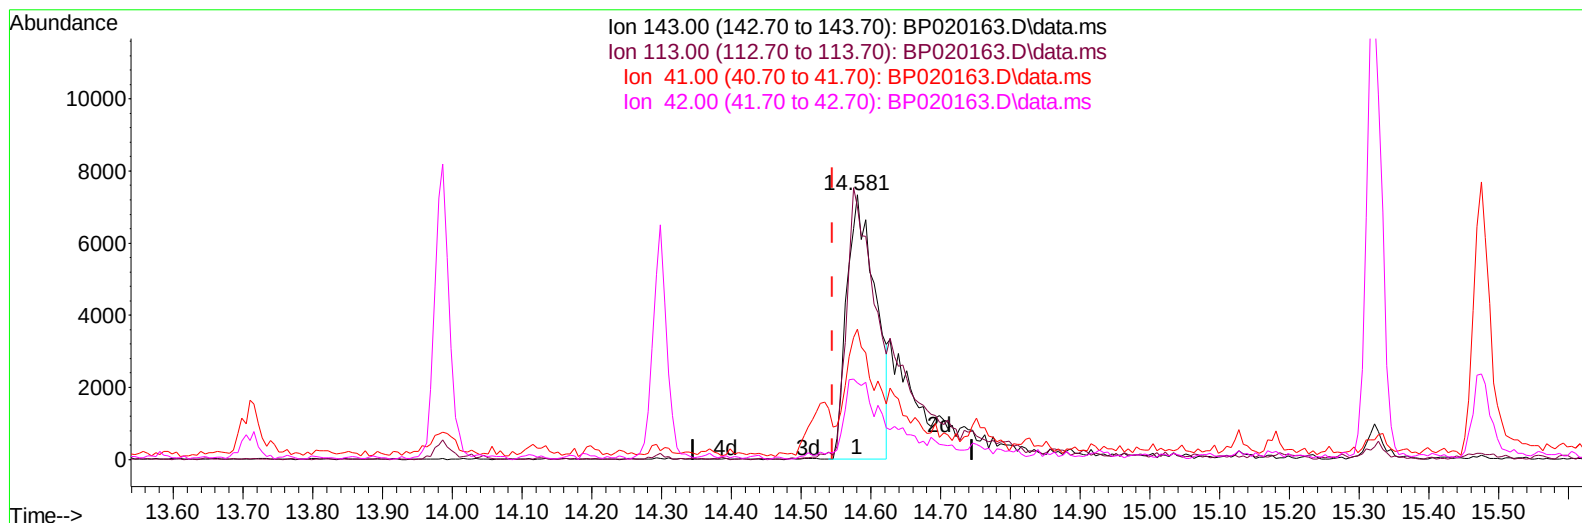

TIC: BP020163.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 7.63 ng/ul

response 20977

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	95.44
41.00	50.30	49.11
42.00	32.50	28.81




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020163.D
 Acq On : 03 May 2024 03:21
 Operator : MA/JU
 Sample : P2279-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORR8

Manual IntegrationsAPPROVED

Quant Time: May 03 04:15:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

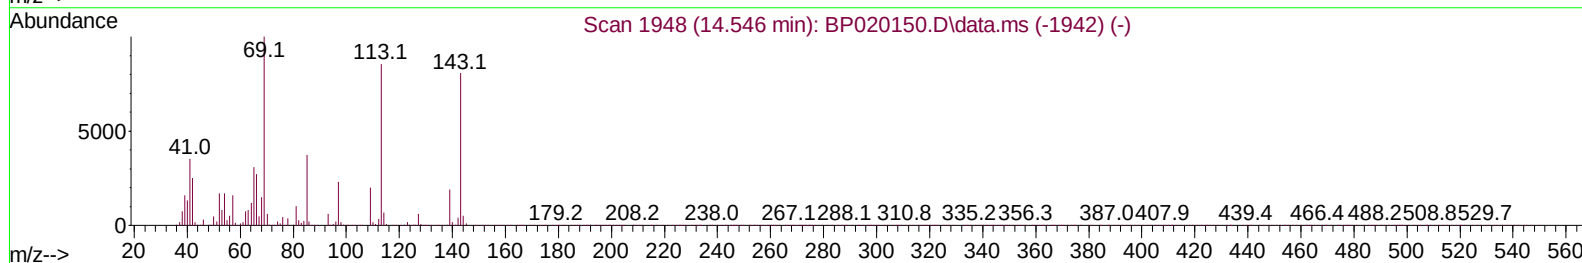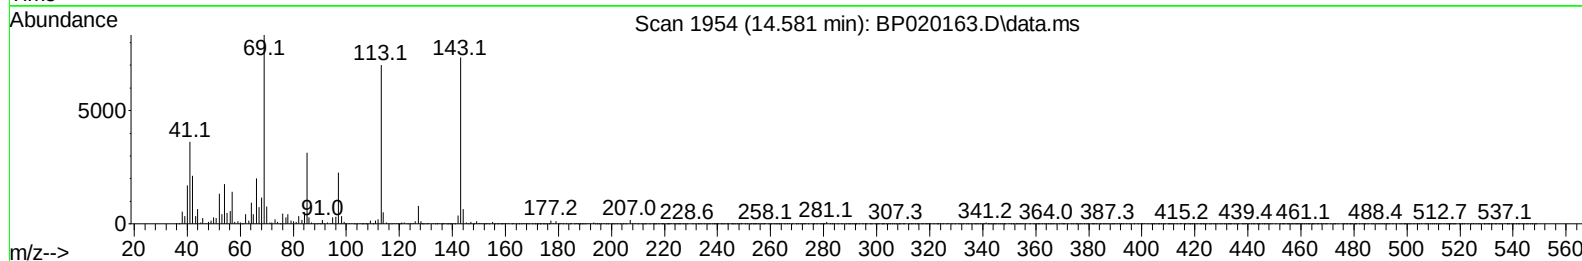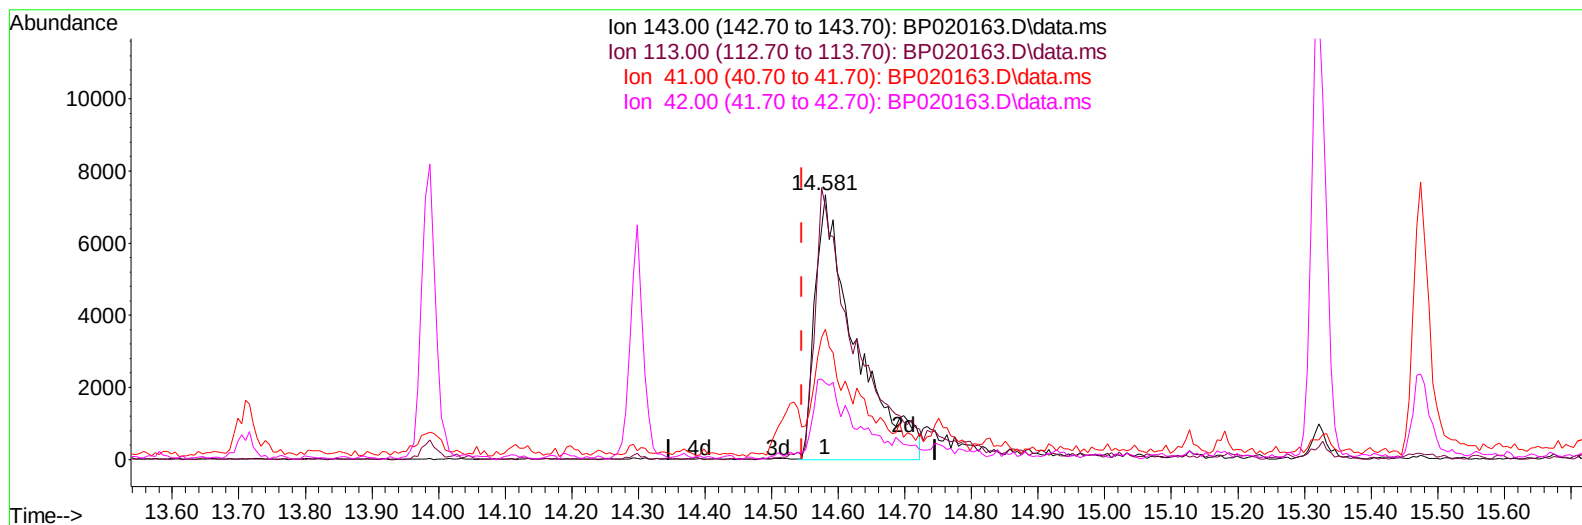

TIC: BP020163.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 11.19 ng/ul m

response 30760

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	95.44
41.00	50.30	49.11
42.00	32.50	28.81

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020163.D
 Acq On : 03 May 2024 03:21
 Operator : MA/JU
 Sample : P2279-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CORR8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/03/2024
 Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 03 04:16:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 00:38:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	74787	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	325124	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164	244846	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	570988	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	568134	20.000	ng/ul	0.00
88) Perylene-d12	24.992	264	585776	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	8703	4.915	ng/uL	0.00
4) Pyridine-d5	3.634	84	42710	8.301	ng/ul	0.01
7) Phenol-d5	6.816	99	56686	8.826	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	138492	35.497	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132	135445	29.500	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	110918	21.361	ng/ul	0.01
21) Nitrobenzene-d5	8.787	128	88914	36.521	ng/ul	0.00
24) 2-Nitrophenol-d4	9.498	143	100868	36.179	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	175004	34.397	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	195204	27.414	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	783389	43.813	ng/ul	0.00
49) Acenaphthylene-d8	13.986	160	775288	39.252	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	30760m	11.193	ng/ul	0.04
60) Fluorene-d10	15.322	176	643175	43.127	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	146724	40.494	ng/ul	0.00
73) Anthracene-d10	17.239	188	1106705	44.804	ng/ul	0.00
81) Pyrene-d10	19.639	212	1465770	44.136	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.745	264	1353303	47.781	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020163.D
Acq On : 03 May 2024 03:21
Operator : MA/JU
Sample : P2279-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0RR8

Manual IntegrationsAPPROVED

Quant Time: May 03 04:16:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 00:38:56 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/03/2024
Supervised By :mohammad ahmed 05/06/2024

