




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020185.D
 Acq On : 03 May 2024 21:27
 Operator : MA/JU
 Sample : P2350-05
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08Q3

Manual IntegrationsAPPROVED

Quant Time: May 03 23:07:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 06:07:25 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/04/2024
 Supervised By :mohammad ahmed 05/06/2024

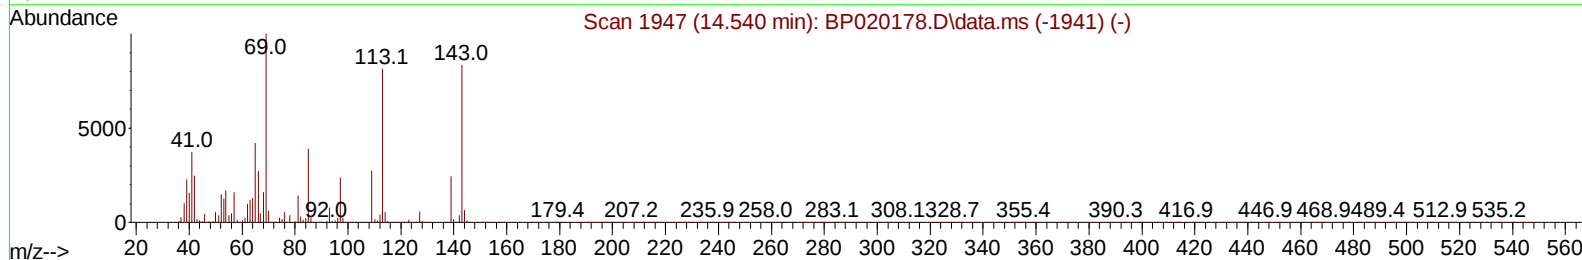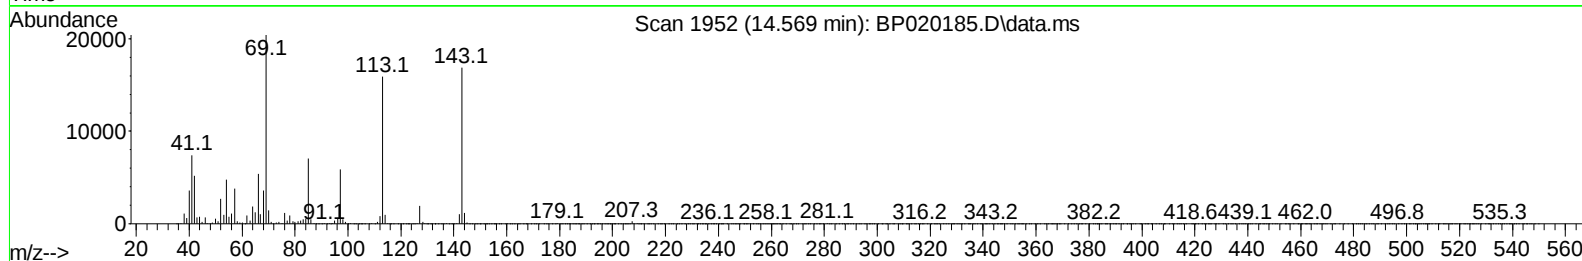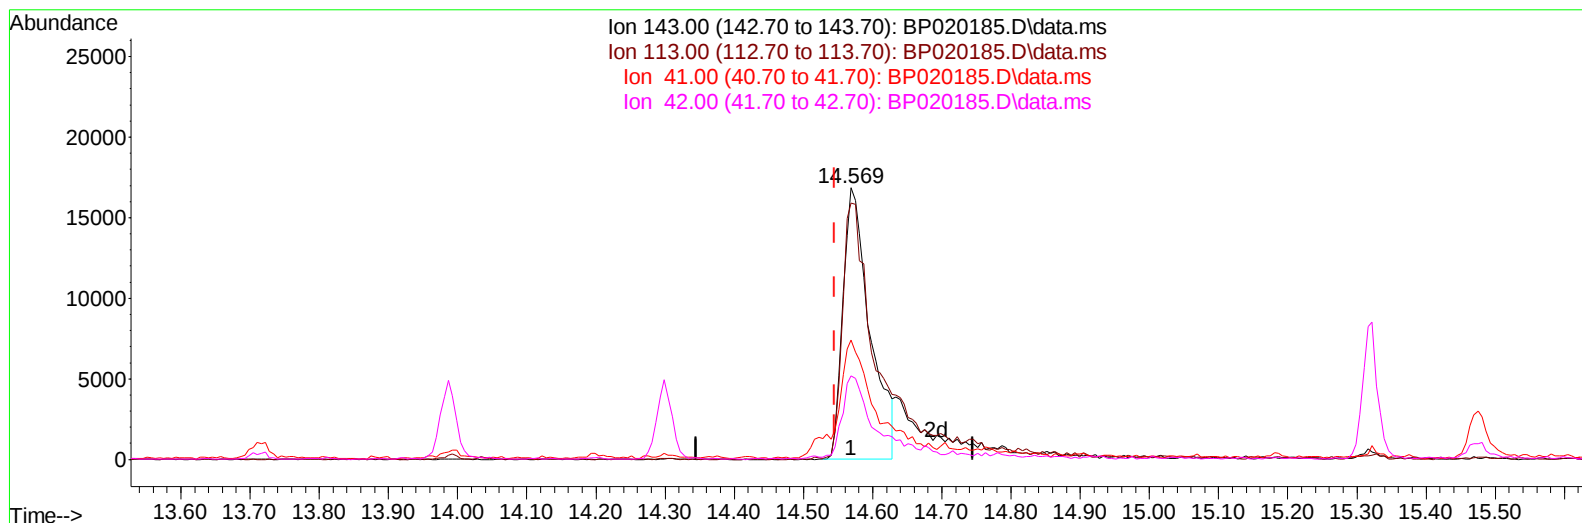

TIC: BP020185.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.024) 19.69 ng/u1

response 45450

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	94.32
41.00	50.30	44.01
42.00	32.50	30.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020185.D
Acq On : 03 May 2024 21:27
Operator : MA/JU
Sample : P2350-05
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08Q3

Manual IntegrationsAPPROVED

Quant Time: May 03 23:07:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 06:07:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/04/2024
Supervised By :mohammad ahmed 05/06/2024

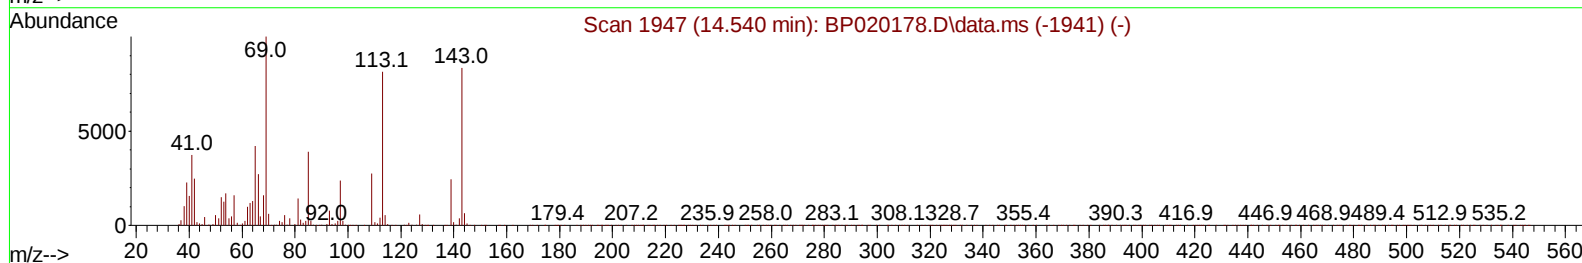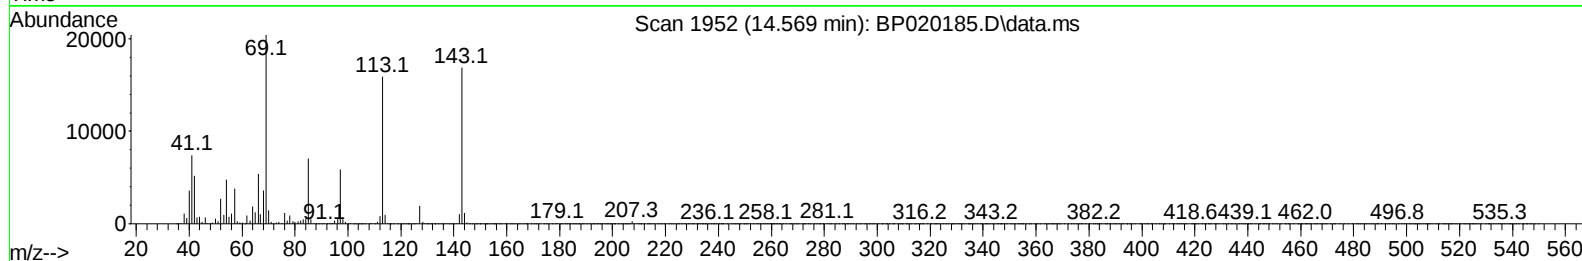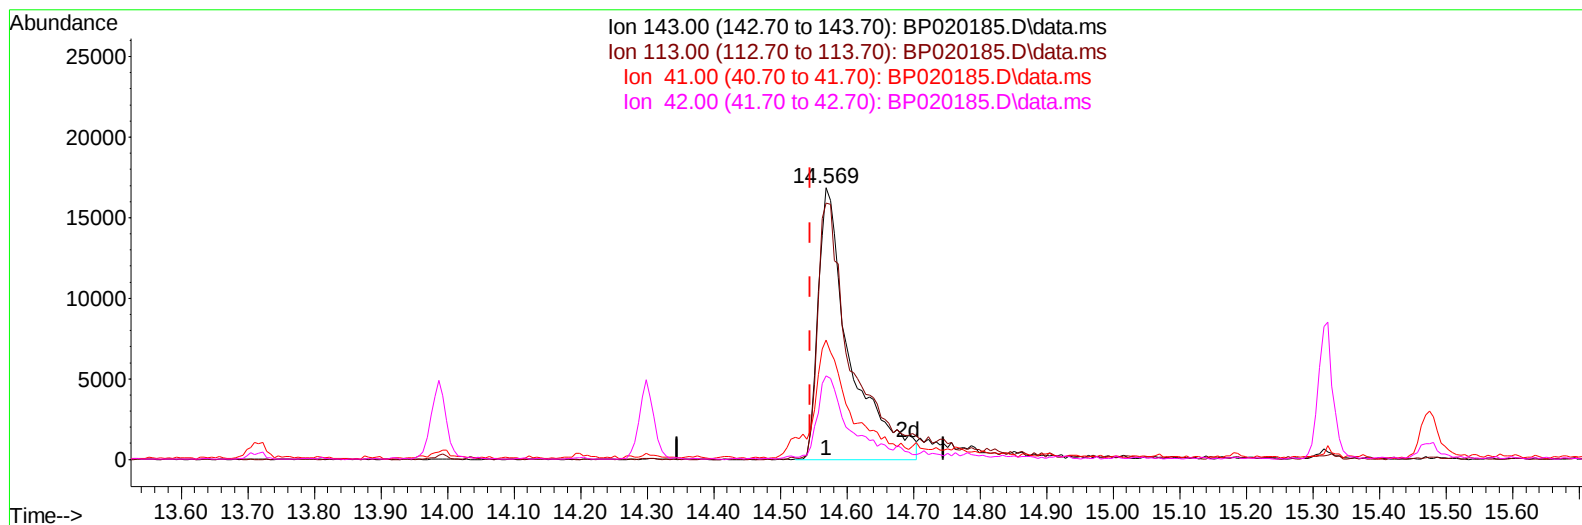

TIC: BP020185.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.024) 23.95 ng/ul m

response 55271

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	94.32
41.00	50.30	44.01
42.00	32.50	30.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020185.D
 Acq On : 03 May 2024 21:27
 Operator : MA/JU
 Sample : P2350-05
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08Q3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/04/2024
 Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 03 23:17:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 06:07:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	71136	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	288644	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164	205632	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	441038	20.000	ng/ul	0.00
79) Chrysene-d12	21.628	240	316165	20.000	ng/ul	0.00
88) Perylene-d12	24.980	264	317259	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	7772	4.614	ng/uL	0.00
4) Pyridine-d5	3.623	84	105418	21.539	ng/ul	0.00
7) Phenol-d5	6.811	99	151134	24.739	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	95571	25.753	ng/ul	0.00
11) 2-Chlorophenol-d4	7.164	132	115948	26.549	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	124413	25.190	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	61621	28.509	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	66735	26.961	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	120940	26.775	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	175840	27.815	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166	490758	32.681	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160	495041	29.843	ng/ul	0.00
54) 4-Nitrophenol-d4	14.569	143	55271m	23.948	ng/ul	0.02
60) Fluorene-d10	15.322	176	399249	31.876	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	62645	22.384	ng/ul	0.00
73) Anthracene-d10	17.234	188	628691	32.951	ng/ul	0.00
81) Pyrene-d10	19.634	212	689474	37.306	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.739	264	505038	32.923	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020185.D
Acq On : 03 May 2024 21:27
Operator : MA/JU
Sample : P2350-05
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08Q3

Manual IntegrationsAPPROVED

Quant Time: May 03 23:17:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 06:07:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/04/2024
Supervised By :mohammad ahmed 05/06/2024

