

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020189.D
 Acq On : 04 May 2024 00:24
 Operator : MA/JU
 Sample : P2238-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1CX6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/04/2024
 Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 04 01:43:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 03 06:07:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	68955	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	294288	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	209515	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.122	188	496886	20.000	ng/ul	-0.01
79) Chrysene-d12	21.610	240	542527	20.000	ng/ul	-0.01
88) Perylene-d12	24.969	264	535980	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	9809	6.008	ng/uL	0.00
4) Pyridine-d5	3.623	84	131569	27.733	ng/ul	0.00
7) Phenol-d5	6.817	99	106804	18.036	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	125384	34.855	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	31099	7.346	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	142813	29.830	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	77871	35.336	ng/ul	0.00
24) 2-Nitrophenol-d4	9.511	143	7334	2.906	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.046	165	15966m	3.467	ng/ul	0.02
31) 4-Chloroaniline-d4	10.552	131	227423	35.285	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	587564	38.403	ng/ul	-0.01
49) Acenaphthylene-d8	13.975	160	643246	38.059	ng/ul	0.00
54) 4-Nitrophenol-d4	14.534	143	25	0.011	ng/ul	-0.01
60) Fluorene-d10	15.310	176	536187	42.016	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.463	200	8	0.003	ng/ul	-0.01
73) Anthracene-d10	17.222	188	846159	39.364	ng/ul	-0.02
81) Pyrene-d10	19.628	212	1164638	36.724	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.739	264	1093287	42.187	ng/ul	-0.01
Target Compounds						
					Qvalue	
72) Phenanthrene	17.163	178	106107	4.185	ng/ul	99
80) Fluoranthene	19.275	202	191404	5.128	ng/ul	98
82) Pyrene	19.651	202	180236	4.641	ng/ul	99
85) Benzo(a)anthracene	21.592	228	156829	4.262	ng/ul	99
87) Chrysene	21.663	228	171322	5.023	ng/ul	97
90) Benzo(b)fluoranthene	23.910	252	382251	11.989	ng/ul	98
91) Benzo(k)fluoranthene	23.974	252	119766	3.686	ng/ul#	96
93) Benzo(a)pyrene	24.804	252	285121	9.398	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	28.780	276	227856	6.127	ng/ul	99
95) Dibenzo(a,h)anthracene	28.862	278	51455m	1.673	ng/ul	
96) Benzo(g,h,i)perylene	29.951	276	234171	7.807	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020189.D
Acq On : 04 May 2024 00:24
Operator : MA/JU
Sample : P2238-02
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
E1CX6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/04/2024
Supervised By :mohammad ahmed 05/06/2024

Quant Time: May 04 01:43:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 03 06:07:25 2024
Response via : Initial Calibration

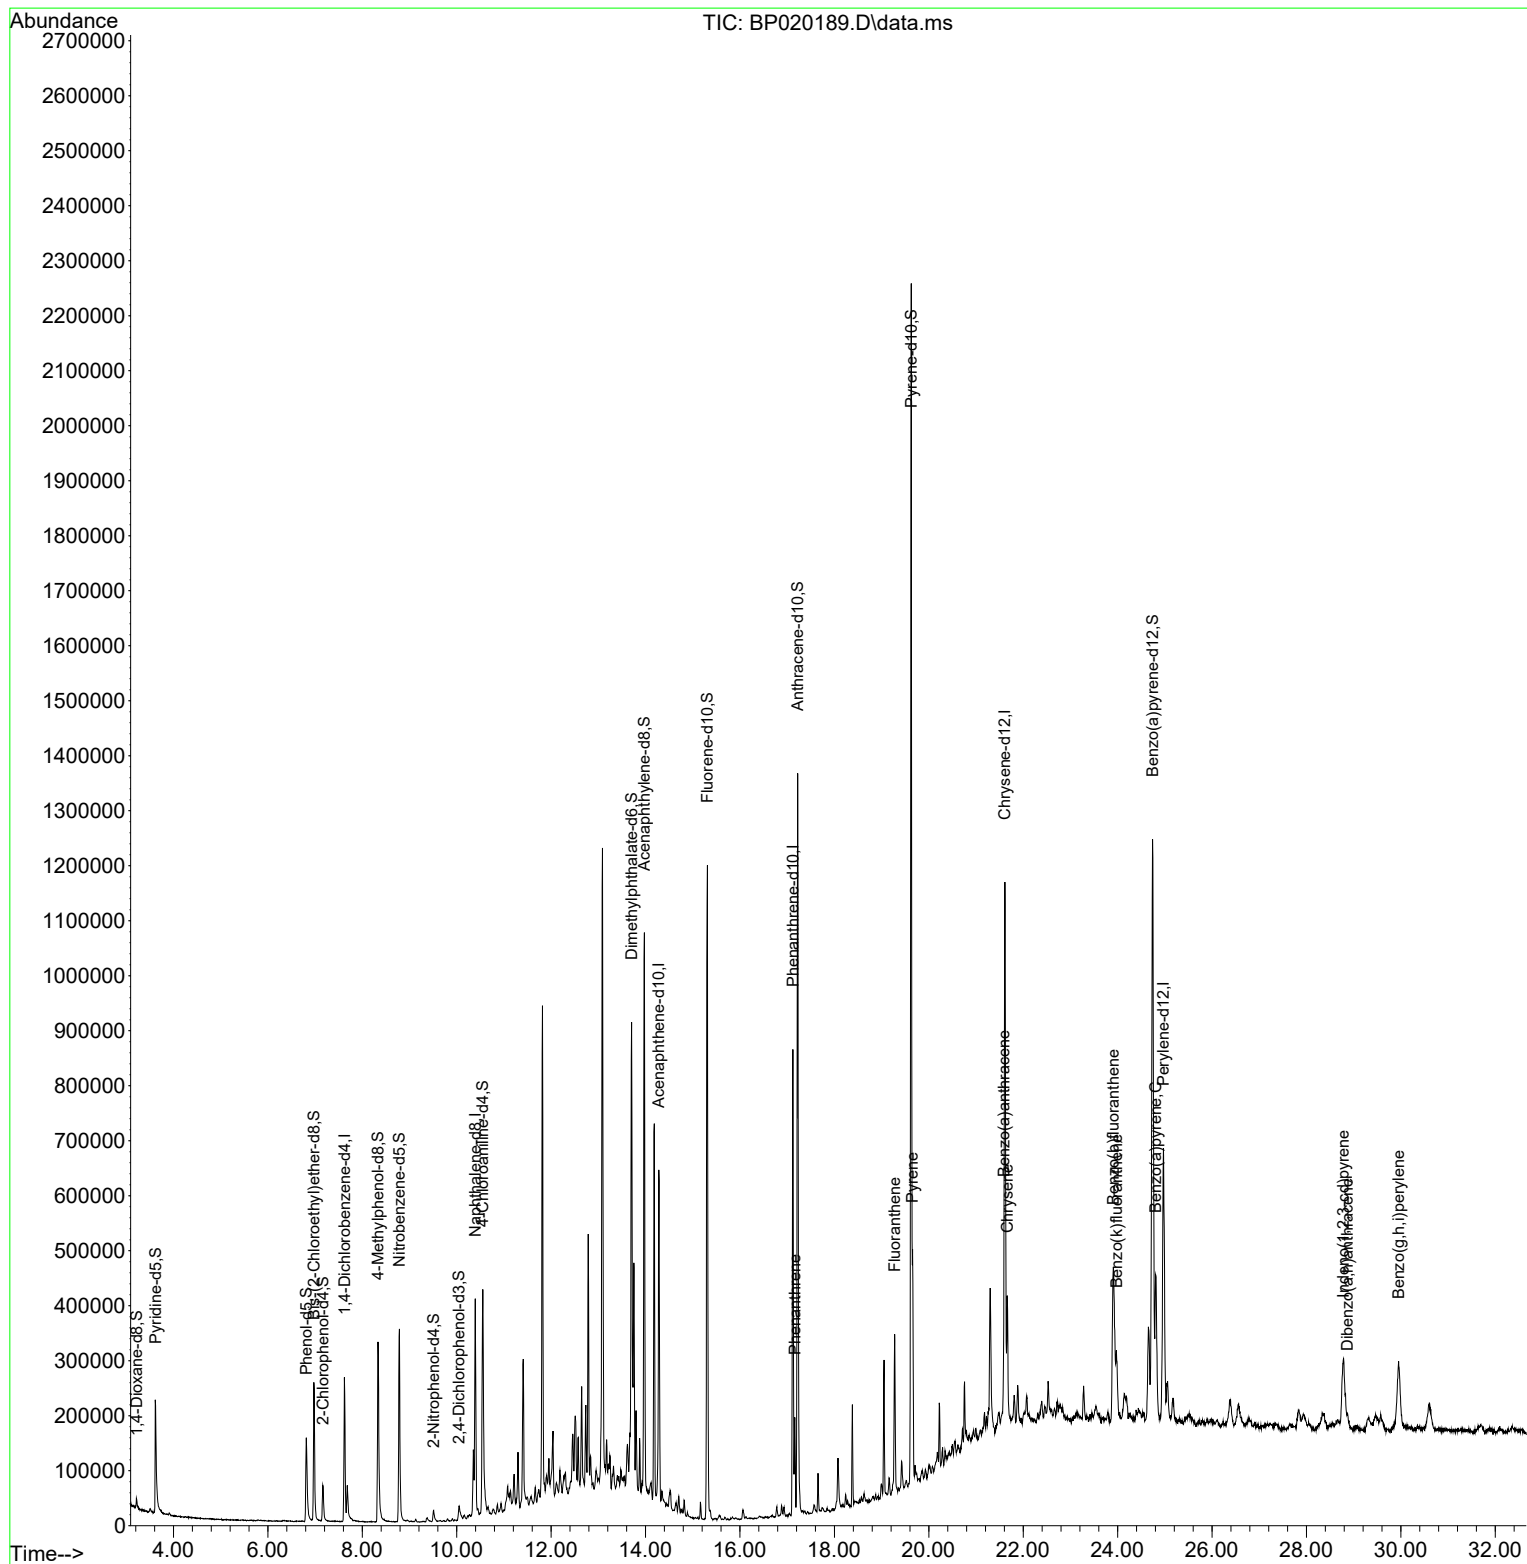



#72

Phenanthrene

Concen: 4.185 ng/ul

RT: 17.163 min Scan# 21

Delta R.T. -0.011 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Instrument :

BNA_P

ClientSampleId :

E1CX6

Tgt Ion:178 Resp: 10610

Ion Ratio Lower Upper

178 100

179 16.3 13.0 19.6





176 18.2 15.2 22.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2024

Supervised By :mohammad ahmed 05/06/2024

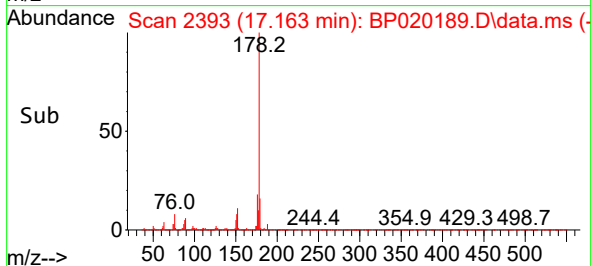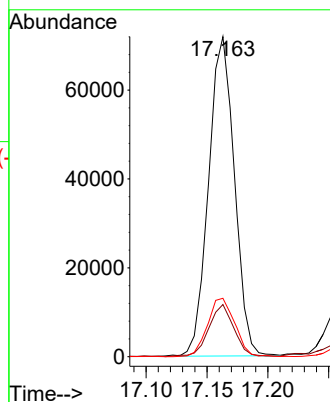

#80

Fluoranthene

Concen: 5.128 ng/ul

RT: 19.275 min Scan# 2752

Delta R.T. -0.011 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24




Tgt Ion:202 Resp: 191404


Ion Ratio Lower Upper

202 100

101 9.4 7.0 10.4

100 7.3 5.5 8.3

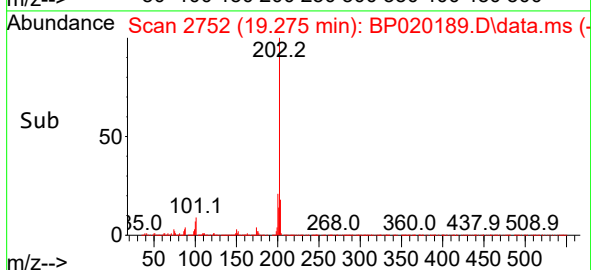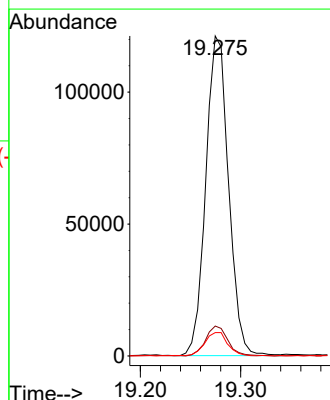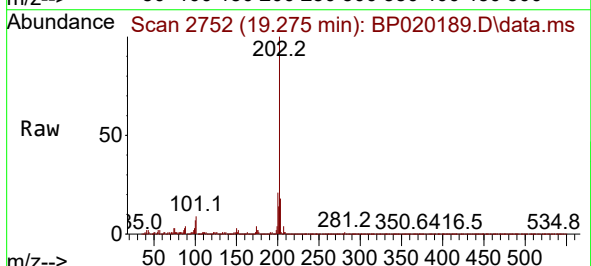



#82

Pyrene

Concen: 4.641 ng/ul

RT: 19.651 min Scan# 2816

Delta R.T. -0.017 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Instrument :

BNA_P

ClientSampleId :

E1CX6





Tgt Ion:	202	Resp:	180230
Ion Ratio	Lower	Upper	
202	100		
101	10.5	8.1	12.1
100	9.2	6.8	10.2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2024

Supervised By :mohammad ahmed 05/06/2024

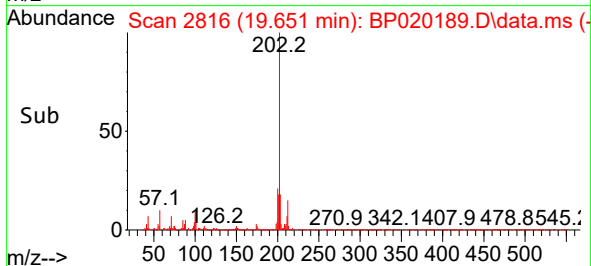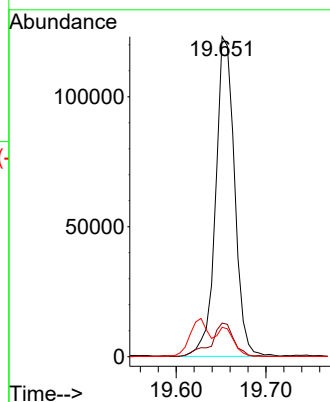

#85

Benzo(a)anthracene

Concen: 4.262 ng/ul




RT: 21.592 min Scan# 3146


Delta R.T. -0.011 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Tgt Ion:	228	Resp:	156829
Ion Ratio	Lower	Upper	
228	100		
229	19.5	15.8	23.8
226	27.3	21.5	32.3

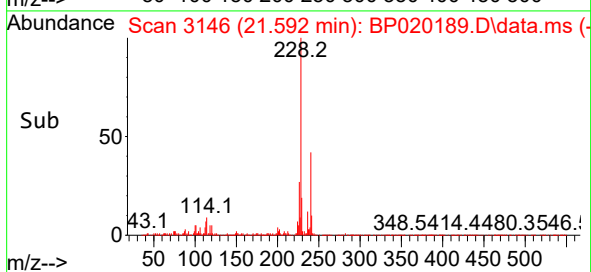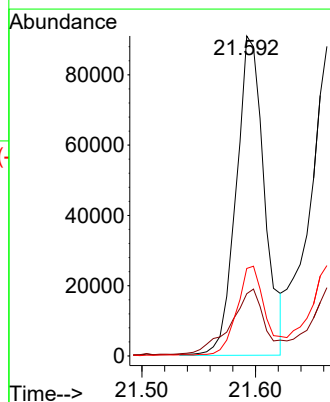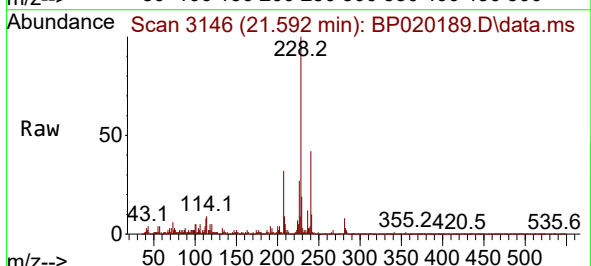



#87

Chrysene

Concen: 5.023 ng/ul

RT: 21.663 min Scan# 31

Delta R.T. -0.005 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Instrument :

BNA_P

ClientSampleId :

E1CX6





Tgt Ion:228	Resp: 17132
Ion Ratio	Lower Upper
228 100	
226 29.2	24.2 36.4
229 22.0	15.9 23.9

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2024

Supervised By :mohammad ahmed 05/06/2024

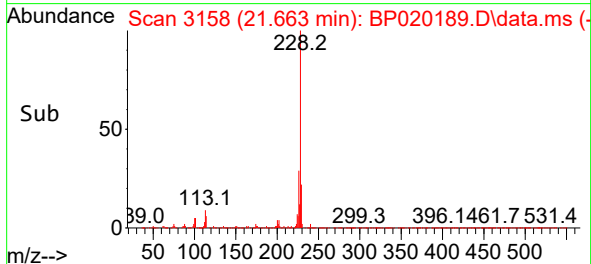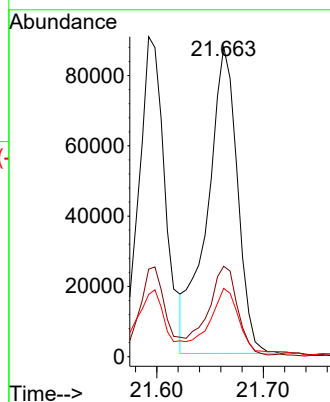

#90

Benzo(b)fluoranthene

Concen: 11.989 ng/ul




RT: 23.910 min Scan# 3540


Delta R.T. 0.000 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Tgt Ion:252	Resp: 382251
Ion Ratio	Lower Upper
252 100	
253 23.6	17.9 26.9
125 8.5	6.2 9.2

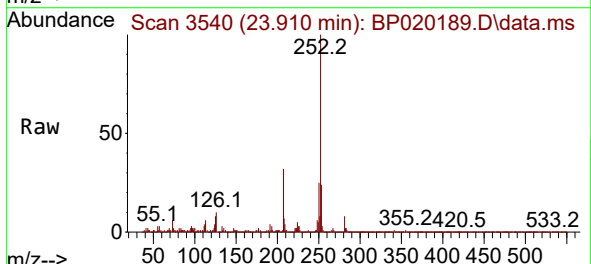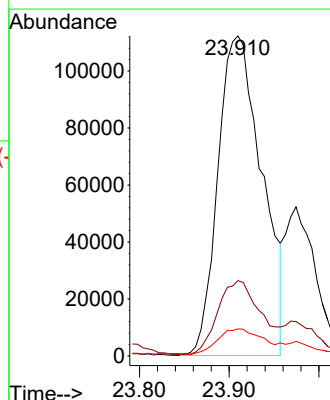



#91

Benzo(k)fluoranthene

Concen: 3.686 ng/ul

RT: 23.974 min Scan# 3554

Delta R.T. -0.011 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Instrument :

BNA_P

ClientSampleId :

E1CX6

Tgt Ion:252 Resp: 119760

Ion Ratio Lower Upper

252 100

253 23.1 17.3 25.9





125 9.8 5.6 8.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2024

Supervised By :mohammad ahmed 05/06/2024

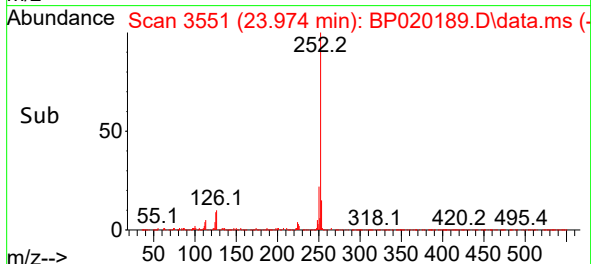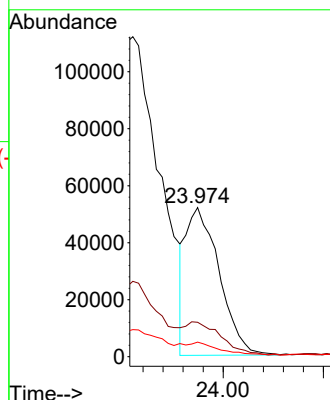

#93

Benzo(a)pyrene

Concen: 9.398 ng/ul

RT: 24.804 min Scan# 3692

Delta R.T. -0.011 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24




Tgt Ion:252 Resp: 285121


Ion Ratio Lower Upper

252 100

253 23.3 17.4 26.0

125 9.0 6.6 10.0

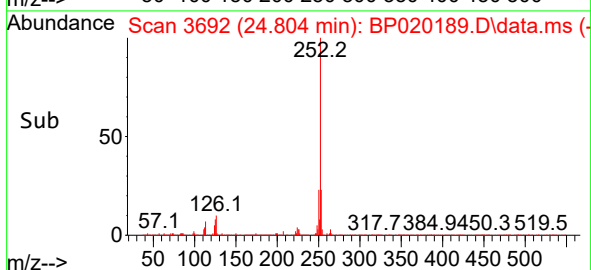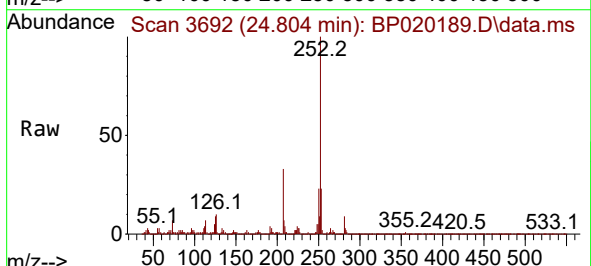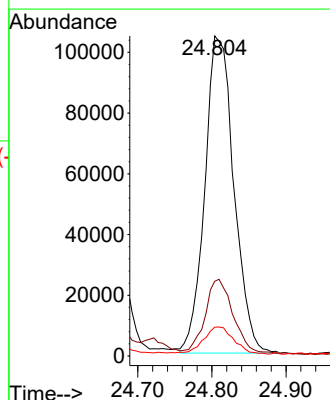



#94

Indeno(1,2,3-cd)pyrene

Concen: 6.127 ng/ul

RT: 28.780 min Scan# 4367

Delta R.T. 0.012 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24

Instrument :

BNA_P

ClientSampleId :

E1CX6

Tgt Ion:276 Resp: 22785

Ion Ratio Lower Upper

276 100

138 15.2 12.3 18.5





277 22.9 19.0 28.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/04/2024

Supervised By :mohammad ahmed 05/06/2024

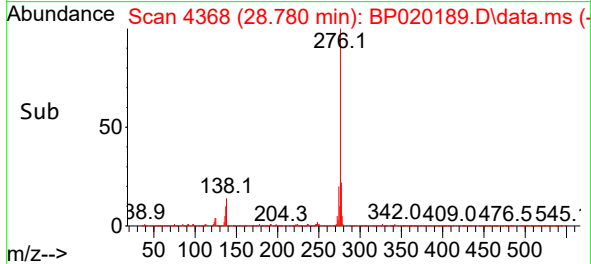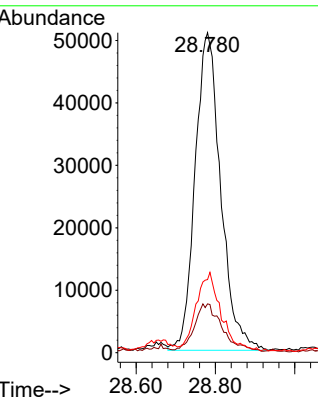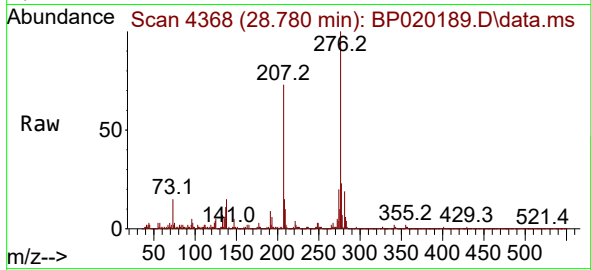

#95

Dibenzo(a,h)anthracene

Concen: 1.673 ng/ul m

RT: 28.862 min Scan# 4382

Delta R.T. 0.006 min

Lab File: BP020189.D

Acq: 04 May 2024 00:24




Tgt Ion:278 Resp: 51455


Ion Ratio Lower Upper

278 100

139 15.3 10.2 15.2#


279 25.6 19.3 28.9

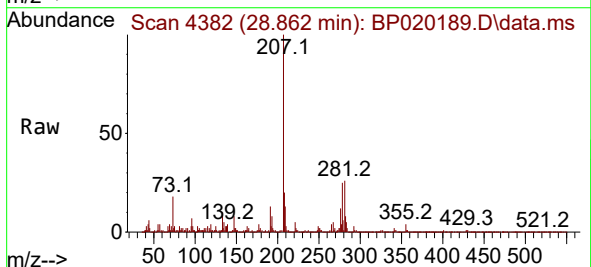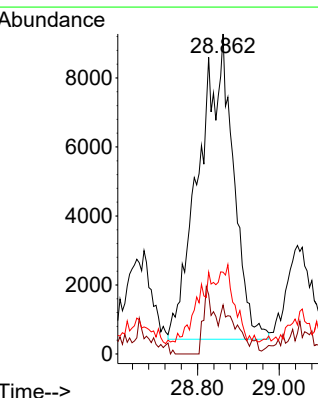

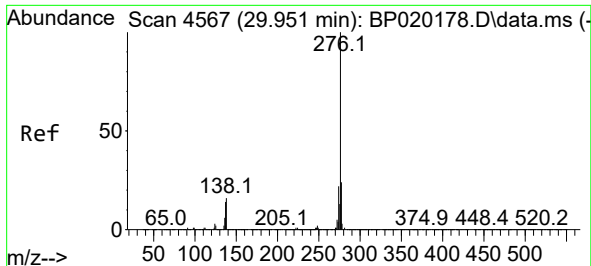

#96
 Benzo(g,h,i)perylene
 Concen: 7.807 ng/ul
 RT: 29.951 min Scan# 4567
 Delta R.T. -0.011 min
 Lab File: BP020189.D
 Acq: 04 May 2024 00:24

Instrument :
 BNA_P
 ClientSampleId :
 E1CX6

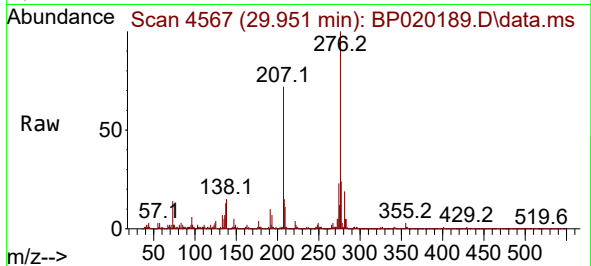

Tgt Ion: 276 Resp: 23417
 Ion Ratio Lower Upper
 276 100
 138 14.5 11.6 17.4
 277 23.5 19.4 29.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/04/2024
 Supervised By :mohammad ahmed 05/06/2024

