

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020177.D
 Acq On : 03 May 2024 15:35
 Operator : MA/JU
 Sample : P2305-01DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AL2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	31	rVB3	7172	11726	0.58%	0.063%
2	3.634	89	93	112	rBV2	24590	66310	3.28%	0.357%
3	3.899	134	138	142	rBV2	6231	8489	0.42%	0.046%
4	4.987	318	323	327	rVV5	5725	10682	0.53%	0.057%
5	5.028	327	330	338	rVB3	7822	13912	0.69%	0.075%
6	6.111	511	514	520	rVB3	5438	8502	0.42%	0.046%
7	6.822	627	635	649	rBV3	18404	54665	2.71%	0.294%
8	6.964	654	659	669	rVV	74211	143213	7.09%	0.771%
9	7.152	683	691	705	rBV	75654	163938	8.12%	0.882%
10	7.611	760	769	783	rBV	375071	697270	34.54%	3.752%
11	7.969	823	830	837	rBV3	7012	14341	0.71%	0.077%
12	8.146	853	860	865	rBV7	3168	6531	0.32%	0.035%
13	8.334	886	892	908	rVV	61884	148806	7.37%	0.801%
14	8.775	960	967	982	rBV	95789	207532	10.28%	1.117%
15	8.952	990	997	1003	rVB	2935	7551	0.37%	0.041%
16	9.058	1006	1015	1016	rBV7	3584	5909	0.29%	0.032%
17	9.199	1035	1039	1046	rVB8	3150	5852	0.29%	0.031%
18	9.487	1081	1088	1099	rBV	78797	171046	8.47%	0.920%
19	9.640	1108	1114	1122	rVB	5431	14077	0.70%	0.076%
20	9.810	1133	1143	1152	rBV	6574	23558	1.17%	0.127%
21	9.887	1152	1156	1159	rBV5	3674	5542	0.27%	0.030%
22	9.928	1159	1163	1169	rVB7	5216	9539	0.47%	0.051%
23	10.040	1172	1182	1200	rBV2	82402	260500	12.90%	1.402%
24	10.381	1226	1240	1246	rBV	547496	1021600	50.61%	5.497%
25	10.434	1246	1249	1257	rVB2	77933	136341	6.75%	0.734%
26	10.563	1263	1271	1281	rBV	67218	170102	8.43%	0.915%
27	10.675	1288	1290	1297	rVB8	6416	11217	0.56%	0.060%
28	10.804	1309	1312	1319	rVB8	3224	6449	0.32%	0.035%
29	10.993	1338	1344	1352	rVV3	20114	45660	2.26%	0.246%
30	11.157	1366	1372	1375	rBV8	2732	6499	0.32%	0.035%
31	11.346	1401	1404	1410	rVB7	3503	5881	0.29%	0.032%
32	11.510	1423	1432	1441	rBV2	17762	40245	1.99%	0.217%
33	11.716	1461	1467	1473	rBV2	6144	14974	0.74%	0.081%
34	11.828	1481	1486	1490	rBV3	6261	11136	0.55%	0.060%
35	11.963	1501	1509	1513	rBV5	19851	45464	2.25%	0.245%
36	12.087	1526	1530	1534	rVB6	4778	8101	0.40%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020177.D
 Acq On : 03 May 2024 15:35
 Operator : MA/JU
 Sample : P2305-01DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAL2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

37	12.134	1534	1538	1542	rBV8	3140	6164	0.31%	0.033%
38	12.246	1550	1557	1562	rBV4	19665	49052	2.43%	0.264%
39	12.428	1581	1588	1593	rBV7	17625	39688	1.97%	0.214%
40	12.504	1597	1601	1611	rVB9	7253	20088	1.00%	0.108%
41	12.610	1613	1619	1624	rBV6	7830	16106	0.80%	0.087%
42	12.693	1627	1633	1640	rBV3	11319	25323	1.25%	0.136%
43	12.787	1645	1649	1662	rVB8	16627	36493	1.81%	0.196%
44	12.904	1665	1669	1673	rVB5	3972	5333	0.26%	0.029%
45	12.951	1673	1677	1680	rVB6	3058	4867	0.24%	0.026%
46	12.998	1680	1685	1688	rBV7	4566	8044	0.40%	0.043%
47	13.093	1690	1701	1705	rBV10	11851	36151	1.79%	0.195%
48	13.157	1710	1712	1722	rVB3	19210	38321	1.90%	0.206%
49	13.334	1736	1742	1750	rVB2	50770	93355	4.62%	0.502%
50	13.469	1754	1765	1775	rBV7	17677	71209	3.53%	0.383%
51	13.622	1785	1791	1793	rBV7	14255	23488	1.16%	0.126%
52	13.710	1799	1806	1818	rVB	277352	484928	24.02%	2.609%
53	13.840	1823	1828	1831	rBV	32678	49452	2.45%	0.266%
54	13.869	1831	1833	1838	rVB3	23283	32390	1.60%	0.174%
55	13.987	1845	1853	1859	rBV	282584	528807	26.20%	2.845%
56	14.110	1868	1874	1884	rVB	13343	32411	1.61%	0.174%
57	14.298	1899	1906	1912	rVV	854367	1412696	69.98%	7.601%
58	14.363	1912	1917	1926	rVB	1333355	2018606	100.00%	10.862%
59	14.504	1938	1941	1945	rBV5	4866	5873	0.29%	0.032%
60	14.622	1955	1961	1966	rBV3	39299	76602	3.79%	0.412%
61	14.728	1974	1979	1983	rVB4	14780	25005	1.24%	0.135%
62	14.793	1986	1990	1994	rVB7	4497	8985	0.45%	0.048%
63	14.940	2010	2015	2024	rVB9	14770	36627	1.81%	0.197%
64	15.287	2068	2074	2075	rBV6	6163	11450	0.57%	0.062%
65	15.328	2075	2081	2086	rVV	401869	643585	31.88%	3.463%
66	15.381	2086	2090	2101	rVB	403316	591535	29.30%	3.183%
67	15.492	2101	2109	2116	rBV4	110054	304884	15.10%	1.641%
68	15.604	2124	2128	2138	rVB8	20599	40295	2.00%	0.217%
69	15.810	2161	2163	2164	rBV2	7000	4901	0.24%	0.026%
70	15.845	2164	2169	2180	rVV2	46288	106992	5.30%	0.576%
71	15.928	2181	2183	2188	rVB4	9659	13334	0.66%	0.072%
72	16.098	2207	2212	2222	rVB2	44362	95330	4.72%	0.513%
73	16.204	2225	2230	2235	rBV3	34805	54491	2.70%	0.293%
74	16.310	2243	2248	2253	rBV5	22679	35259	1.75%	0.190%
75	16.369	2254	2258	2260	rBV5	9235	14368	0.71%	0.077%
76	16.575	2290	2293	2296	rVB2	11115	15401	0.76%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020177.D
 Acq On : 03 May 2024 15:35
 Operator : MA/JU
 Sample : P2305-01DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AL2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

77	16.869	2339	2343	2344	rBV3	5522	8029	0.40%	0.043%
78	16.951	2349	2357	2360	rBV2	28836	75465	3.74%	0.406%
79	16.992	2361	2364	2368	rBV2	18051	30037	1.49%	0.162%
80	17.045	2369	2373	2376	rBV3	19075	35942	1.78%	0.193%
81	17.134	2382	2388	2400	rVB	1165073	1712350	84.83%	9.214%
82	17.245	2401	2407	2412	rBV	431311	677232	33.55%	3.644%
83	17.357	2421	2426	2432	rVB3	20553	40745	2.02%	0.219%
84	17.539	2452	2457	2459	rBV3	33982	50679	2.51%	0.273%
85	17.575	2459	2463	2468	rVB	49314	90007	4.46%	0.484%
86	17.845	2502	2509	2513	rBV6	19406	42209	2.09%	0.227%
87	18.039	2537	2542	2546	rBV3	29296	54074	2.68%	0.291%
88	18.092	2547	2551	2561	rVB4	99425	202487	10.03%	1.090%
89	18.198	2566	2569	2574	rVB	48453	65608	3.25%	0.353%
90	18.257	2575	2579	2589	rVB	72833	112172	5.56%	0.604%
91	18.386	2596	2601	2606	rBV6	22766	50831	2.52%	0.274%
92	18.481	2613	2617	2621	rBV6	17538	25108	1.24%	0.135%
93	18.528	2623	2625	2631	rVB4	23091	30484	1.51%	0.164%
94	19.286	2750	2754	2761	rVB	158736	224156	11.10%	1.206%
95	19.451	2777	2782	2788	rBV8	26018	52635	2.61%	0.283%
96	19.639	2809	2814	2823	rVB2	579532	898754	44.52%	4.836%
97	20.175	2900	2905	2914	rBV	51047	103230	5.11%	0.555%
98	21.633	3146	3153	3160	rBV	803754	1501859	74.40%	8.081%
99	24.763	3679	3685	3698	rVB2	193768	533805	26.44%	2.872%
100	25.010	3717	3727	3737	rVB3	385093	1265828	62.71%	6.811%




Sum of corrected areas: 18584775

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020177.D
Acq On : 03 May 2024 15:35
Operator : MA/JU
Sample : P2305-01DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

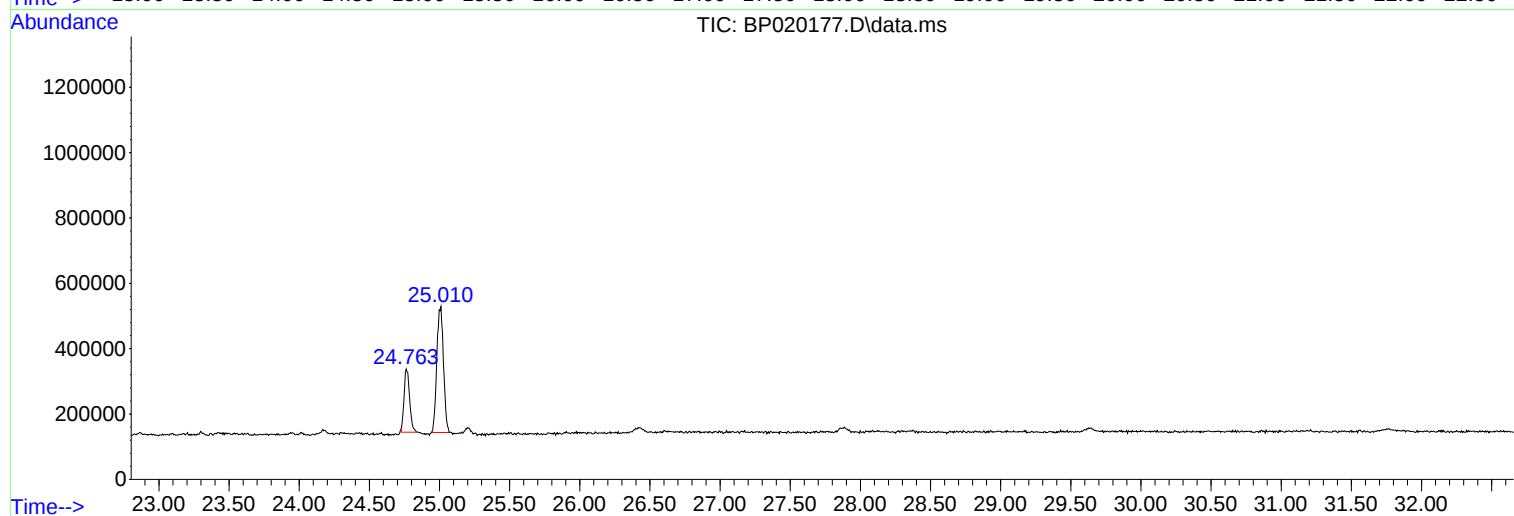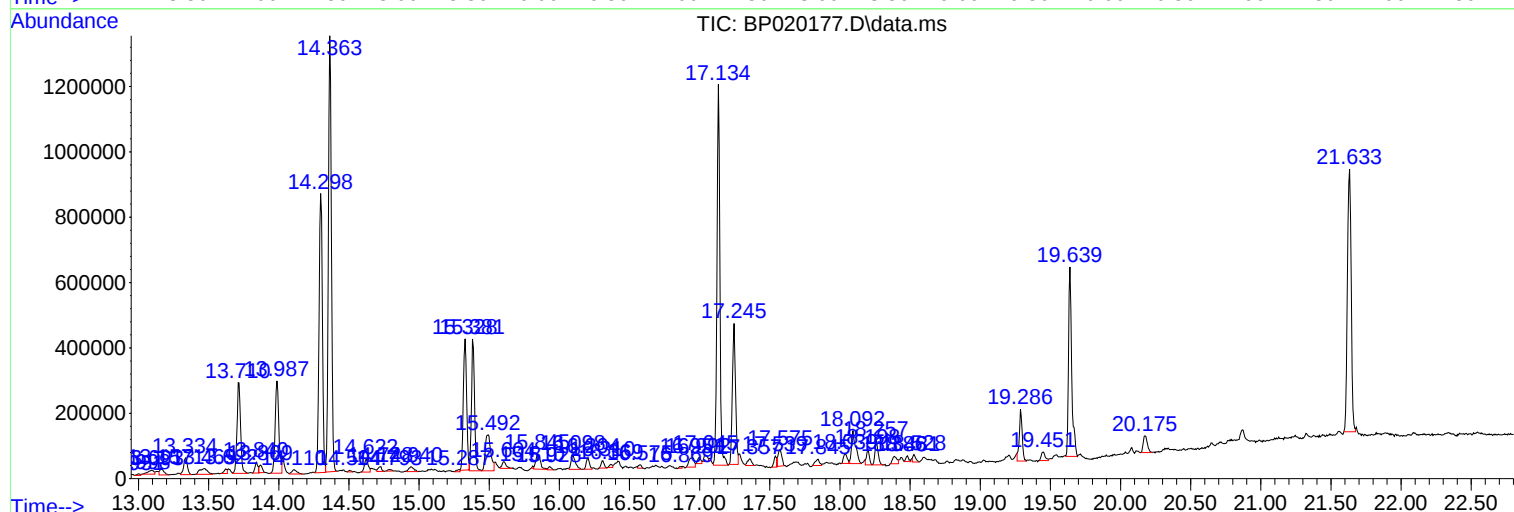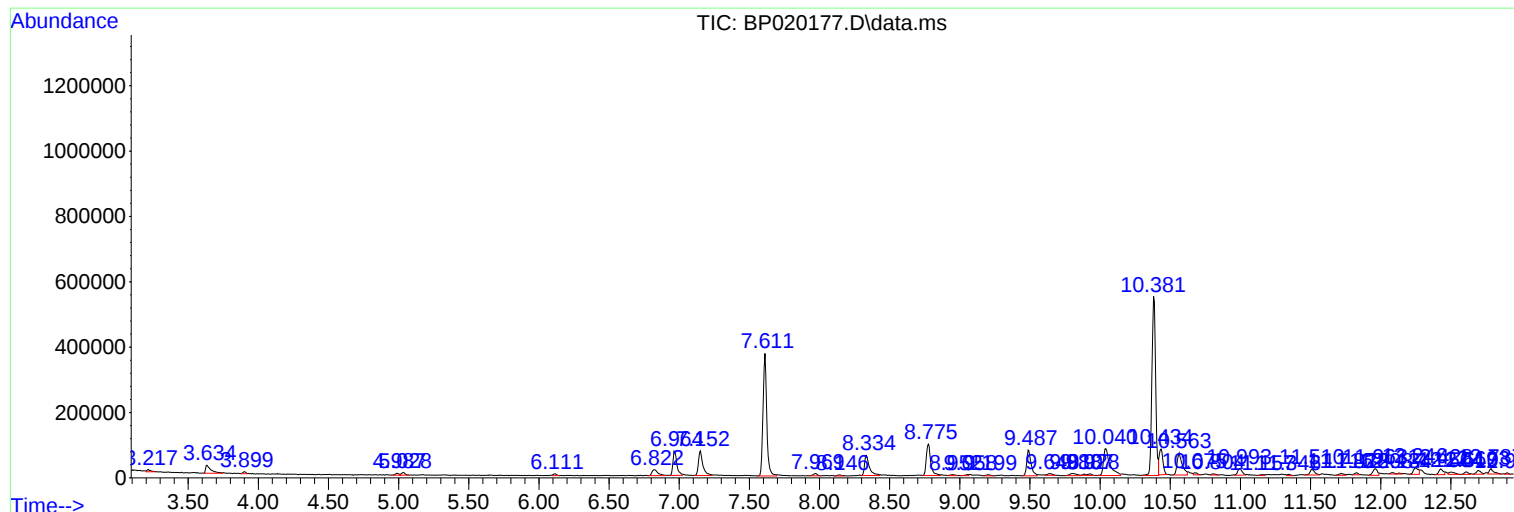

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020177.D
Acq On : 03 May 2024 15:35
Operator : MA/JU
Sample : P2305-01DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL2DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 .beta.-(1-Naphthyl)acrylic ... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.092	2.37 ng/ul	202487	Phenanthrene-d10	17.134

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		.beta.-(1-Naphthyl)acrylic acid	198	C13H10O2	013026-12-5	76
2		.beta.-(1-Naphthyl)acrylic acid	198	C13H10O2	013026-12-5	76
3		Benzeneacetonitrile, 3,4-difluoro-	153	C8H5F2N	000658-99-1	49
4		2(1H)-Pyridinethione, 1-ethyl-6-...	153	C8H11NS	019006-73-6	47
5		Benzenethiol, p-(dimethylamino)-	153	C8H11NS	004946-22-9	47

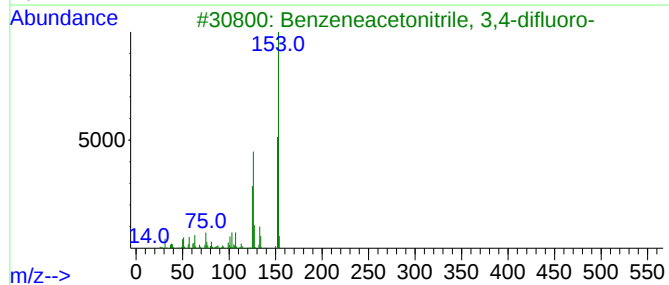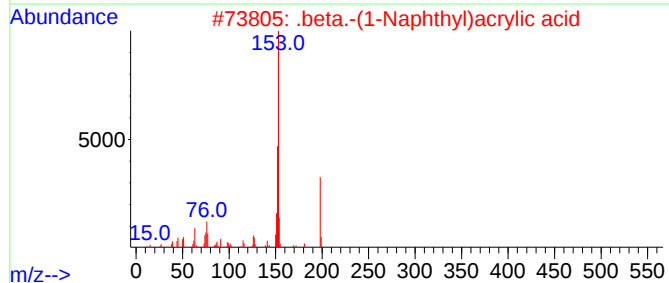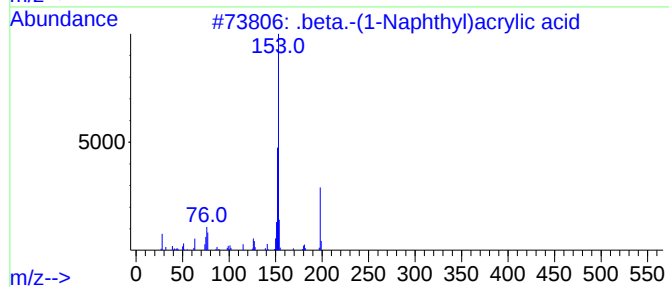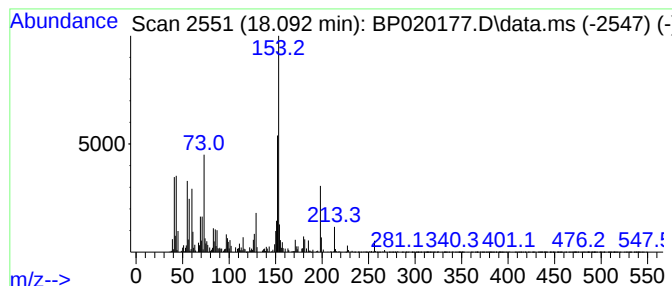

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020177.D
Acq On : 03 May 2024 15:35
Operator : MA/JU
Sample : P2305-01DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
.beta.-(1-Napht...	18.092	2.4	ng/u1	202487	4	17.134	1712350	20.0