

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
 Data File : BP020194.D
 Acq On : 04 May 2024 04:49
 Operator : MA/JU
 Sample : PB160586BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK586

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	32	rVB	28061	41757	1.48%	0.145%
2	3.616	87	90	112	rBV	268996	488558	17.30%	1.696%
3	3.916	137	141	151	rVB3	13446	20869	0.74%	0.072%
4	4.275	200	202	207	rVB6	2587	3155	0.11%	0.011%
5	6.810	626	633	651	rBV	331424	658592	23.32%	2.286%
6	6.975	655	661	675	rVB	282417	481789	17.06%	1.673%
7	7.163	686	693	709	rBV	376336	662590	23.46%	2.300%
8	7.622	762	771	783	rBV	345923	603177	21.36%	2.094%
9	8.328	883	891	908	rBV	431852	843362	29.86%	2.928%
10	8.651	941	946	950	rBV8	1529	2851	0.10%	0.010%
11	8.781	959	968	982	rBV	376255	704332	24.94%	2.445%
12	9.492	1078	1089	1106	rBV	323269	642538	22.75%	2.231%
13	10.028	1172	1180	1202	rBV	387940	872974	30.91%	3.031%
14	10.392	1234	1242	1257	rVB	483747	883603	31.29%	3.067%
15	10.551	1261	1269	1292	rBV	374274	923746	32.71%	3.207%
16	12.022	1513	1519	1525	rBV6	5483	12093	0.43%	0.042%
17	13.175	1709	1715	1722	rBV4	9654	19048	0.67%	0.066%
18	13.704	1798	1805	1817	rBV	1028244	1600361	56.66%	5.556%
19	13.975	1841	1851	1868	rBV	1164502	1711727	60.61%	5.942%
20	14.286	1897	1904	1918	rBV	886692	1355879	48.01%	4.707%
21	14.551	1942	1949	1964	rBV	245791	681682	24.14%	2.366%
22	15.316	2072	2079	2096	rBV	1417742	2171643	76.89%	7.539%
23	15.469	2099	2105	2118	rBV	467823	834952	29.56%	2.899%
24	15.569	2119	2122	2126	rVB5	8759	12729	0.45%	0.044%
25	16.045	2199	2203	2208	rBV8	1427	2951	0.10%	0.010%
26	16.127	2213	2217	2224	rVB8	2911	5600	0.20%	0.019%
27	16.798	2327	2331	2334	rBV6	3024	3453	0.12%	0.012%
28	16.904	2343	2349	2351	rBV5	2758	4308	0.15%	0.015%
29	17.127	2379	2387	2397	rBV	1203987	1757009	62.21%	6.099%
30	17.227	2397	2404	2423	rVB	1577872	2451558	86.80%	8.511%
31	18.110	2550	2554	2559	rBV7	3677	7252	0.26%	0.025%
32	18.245	2574	2577	2580	rBV4	5206	5859	0.21%	0.020%
33	19.180	2730	2736	2741	rBV4	21382	34013	1.20%	0.118%
34	19.257	2744	2749	2754	rBV3	16236	30862	1.09%	0.107%
35	19.627	2806	2812	2827	rBV	1845707	2824328	100.00%	9.805%
36	21.615	3144	3150	3168	rVB	1115709	1789921	63.38%	6.214%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020194.D
Acq On : 04 May 2024 04:49
Operator : MA/JU
Sample : PB160586BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Title : SVOA CALIBRATION

37	24.733	3670	3680	3694	rVB	731747	2149063	76.09%	7.461%
38	24.962	3711	3719	3735	rVB	560098	1505606	53.31%	5.227%




Sum of corrected areas: 28805790

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020194.D
Acq On : 04 May 2024 04:49
Operator : MA/JU
Sample : PB160586BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

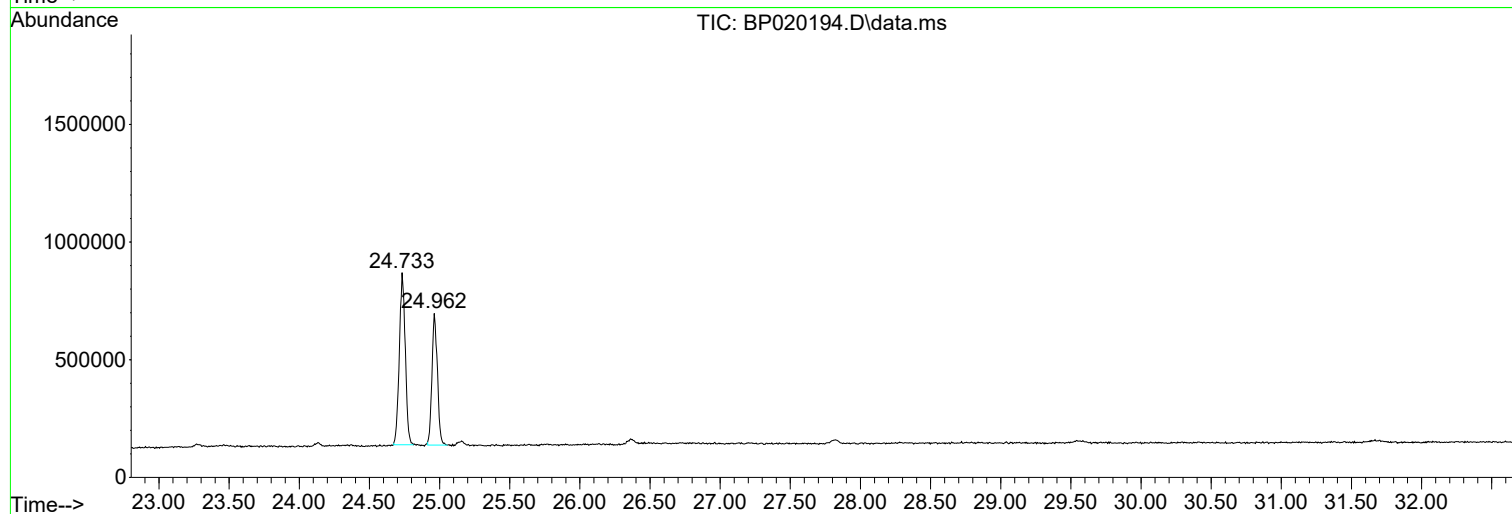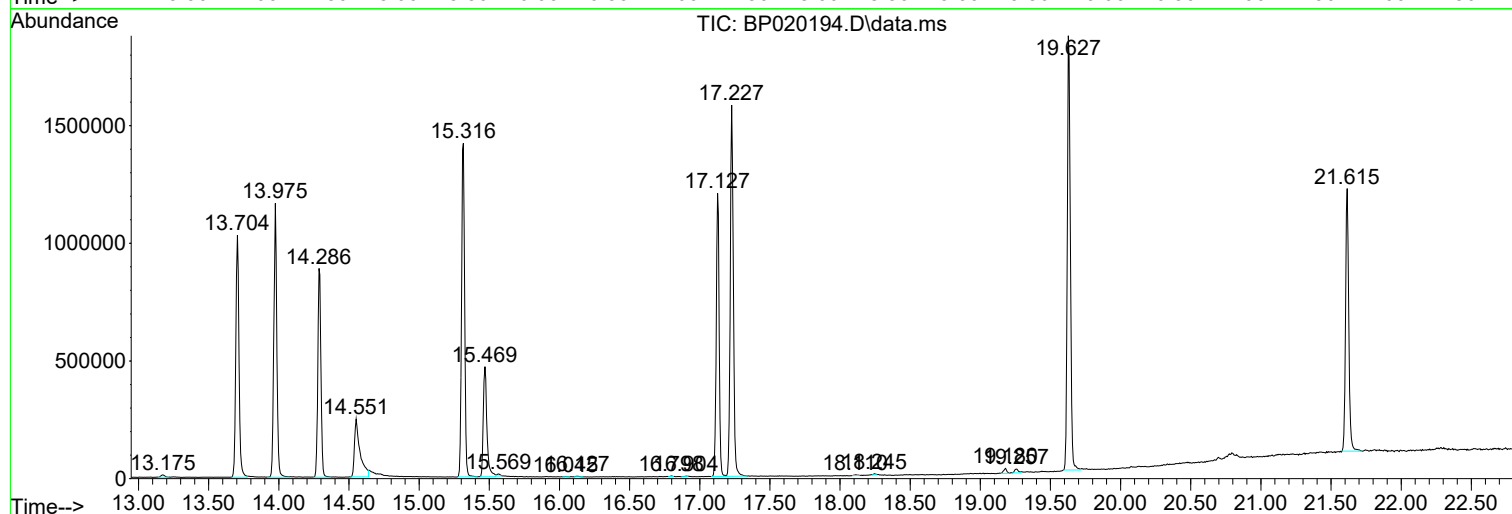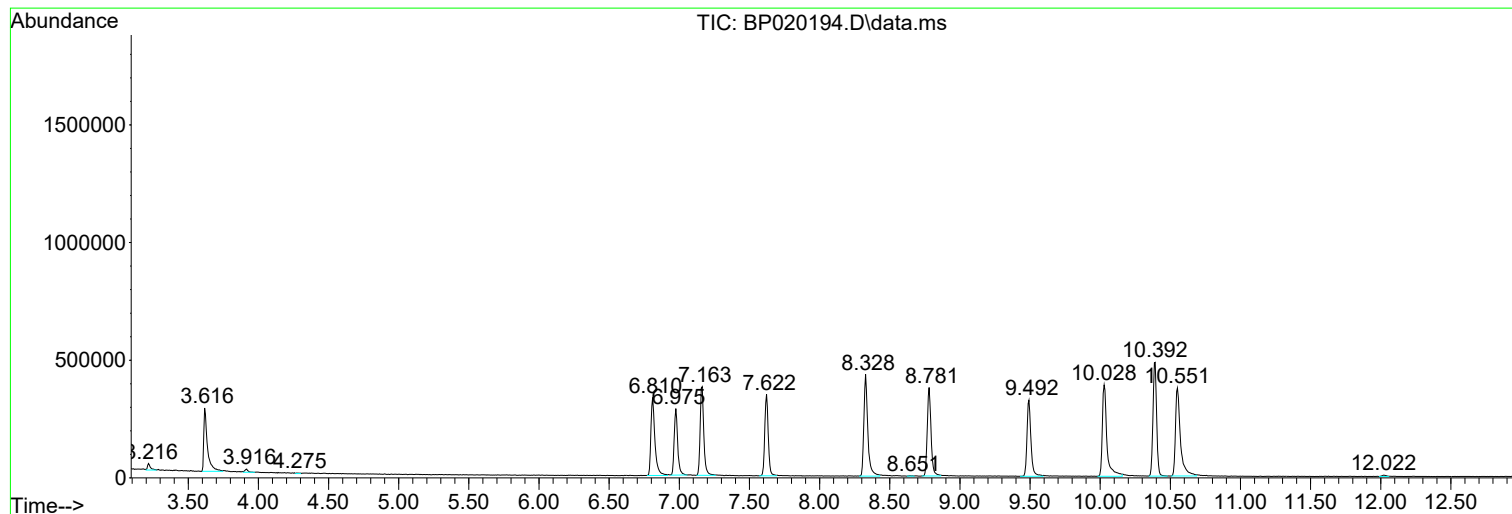

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020194.D
Acq On : 04 May 2024 04:49
Operator : MA/JU
Sample : PB160586BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020194.D
Acq On : 04 May 2024 04:49
Operator : MA/JU
Sample : PB160586BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK586

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------