


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050224\
Data File : BP020139.D
Acq On : 02 May 2024 07:36
Operator : MA/JU
Sample : DFTPP719
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP719

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Title : SVOA CALIBRATION
Last Update : Wed May 01 17:34:36 2024

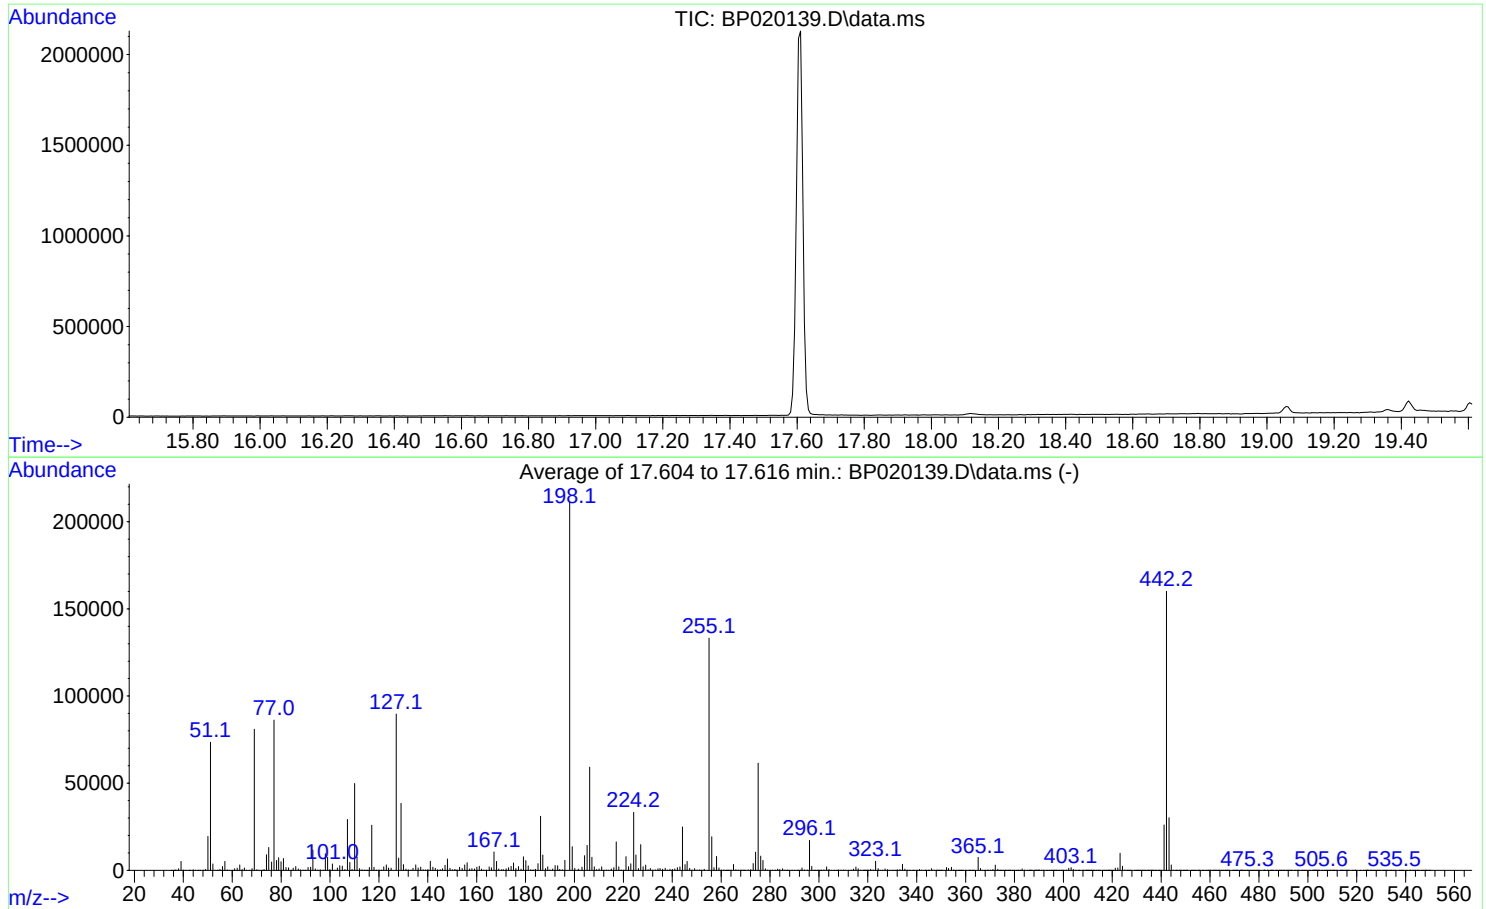

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	73538	PASS
68	69	0.00	2	1.2	1011	PASS
69	198	0.00	100	38.4	80997	PASS
70	69	0.00	2	0.5	414	PASS
127	198	10	80	42.5	89706	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	211005	PASS
199	198	5	9	6.4	13544	PASS
275	198	10	60	29.1	61456	PASS
365	198	1	100	3.5	7439	PASS
441	198	0.01	100	12.3	26056	PASS
442	198	50	100	75.9	160084	PASS
443	442	15	24	18.9	30240	PASS

m/z	Abundance
35.30	19.0
36.00	10.0
36.80	28.0
38.10	12.0
39.00	90.0
40.00	286.0
41.00	158.0
41.90	15.0
43.20	71.0
44.00	924.0
45.00	75.0
45.80	2.0
46.70	20.0
47.20	16.0
47.90	18.0
49.00	144.0
50.00	64.0
51.10	62.0
51.80	16.0
53.00	25.0
54.00	15.0
54.70	21.0
55.20	17.0
56.20	1.0
57.00	53.0
57.80	13.0
59.00	21.0
59.60	3.0
60.30	6.0
60.90	14.0
61.60	10.0
62.70	15.0
63.90	51.0
65.00	82.0
65.90	106.0
67.00	98.0
68.00	20.0
68.80	7.0
69.30	4.0
70.10	11.0
71.10	19.0
71.90	13.0
73.00	558.0
74.00	29.0
74.90	27.0
75.80	4.0
76.90	57.0
78.10	48.0
79.00	13.0
79.80	17.0
80.80	18.0
81.30	8.0
81.70	9.0
82.30	6.0
82.80	12.0
83.10	9.0
84.00	204.0
84.90	15.0
85.90	51.0
86.60	24.0
87.10	18.0
88.00	18.0
88.60	41.0
89.30	1.0
89.60	1.0
90.20	8.0
91.00	30.0
92.30	23.0
93.40	2.0
94.00	5.0
95.00	29.0
95.90	204.0
96.60	35.0
97.60	17.0
98.40	2.0
98.70	3.0
99.30	1.0
99.70	1.0
100.30	15.0
101.00	1.0
101.90	10.0
103.00	19.0
104.00	15.0
104.70	21.0
105.20	10.0
106.10	13.0
106.60	3.0
107.70	14.0
108.10	17.0
108.80	15.0
109.80	2.0
110.80	9.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

111.60	3.0
113.10	3.0
113.60	2.0
114.60	2.0
115.20	28.0
116.20	17.0
116.90	6.0
117.90	7.0
118.80	20.0
119.40	14.0
120.10	12.0
121.00	14.0
122.30	10.0
123.30	8.0
123.90	3.0
124.70	11.0
125.60	2.0
126.20	1.0
127.20	17.0
127.70	7.0
128.90	11.0
130.30	4.0
130.80	12.0
131.70	2.0
132.10	3.0
132.80	85.0
134.20	16.0
134.90	72.0
136.50	4.0
138.10	2.0
139.00	8.0
139.60	2.0
140.30	1.0
140.80	7.0
141.40	1.0
142.00	9.0
143.00	11.0
143.70	16.0
144.30	3.0
145.10	9.0
146.00	2.0
146.50	17.0
147.00	80.0
148.00	8.0
149.00	11.0
150.20	17.0
151.30	9.0
151.80	3.0
152.30	11.0
152.90	4.0
153.80	4.0
155.10	3.0
155.70	3.0
157.10	9.0
157.90	0.0
158.70	3.0
160.10	18.0
161.00	13.0
162.00	6.0
162.90	66.0
163.90	8.0
165.20	84.0
165.90	5.0
166.40	3.0
167.20	18.0
167.80	3.0
169.00	24.0
169.90	18.0
170.70	23.0
172.40	2.0
173.00	2.0
173.70	1.0
174.20	2.0
175.00	9.0
175.70	2.0
176.30	13.0
177.10	35.0
178.20	43.0
178.80	50.0
179.70	15.0
180.60	3.0
181.20	12.0
182.30	3.0
183.10	0.0
183.90	1.0
184.40	2.0
185.10	2.0
185.60	3.0
186.10	5.0
187.00	5.0
188.70	9.0
189.30	0.0
190.00	19.0
191.10	287.0
191.80	2.0
193.10	176.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

193.90	10.0
194.10	12.0
194.80	12.0
195.40	1.0
196.20	2.0
197.00	1.0
197.90	3.0
198.50	1.0
199.00	3.0
199.60	4.0
200.50	7.0
201.20	22.0
202.50	2.0
203.30	14.0
204.20	4.0
204.80	22.0
205.90	4.0
207.10	1501.0
208.10	234.0
209.00	294.0
210.30	24.0
211.10	23.0
211.80	2.0
212.40	3.0
213.40	13.0
214.70	0.0
215.20	3.0
216.10	2.0
217.00	2.0
217.60	0.0
218.30	4.0
219.00	19.0
219.90	4.0
221.20	94.0
222.30	5.0
222.90	15.0
223.50	1.0
224.30	22.0
225.50	1.0
226.70	4.0
227.80	3.0
228.20	2.0
229.10	6.0
230.20	9.0
231.00	11.0
232.00	9.0
232.70	4.0
233.10	5.0
234.20	6.0
235.00	4.0
236.00	2.0
237.30	6.0
237.80	1.0
238.50	19.0
240.20	8.0
240.90	1.0
242.10	3.0
242.80	1.0
243.90	12.0
245.20	3.0
246.20	11.0
246.80	4.0
247.50	1.0
248.40	12.0
249.70	14.0
250.20	14.0
250.80	0.0
251.50	11.0
252.10	1.0
253.00	8.0
253.80	11.0
255.00	22.0
256.50	4.0
257.10	7.0
257.80	3.0
259.30	2.0
260.60	3.0
261.40	2.0
262.80	3.0
263.50	3.0
264.10	3.0
265.00	62.0
266.00	21.0
267.10	56.0
268.10	12.0
268.90	8.0
270.10	16.0
271.20	14.0
272.00	4.0
272.80	9.0
273.50	3.0
274.10	1.0
275.00	3.0
275.80	0.0
276.70	2.0
277.70	0.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

278.30	2.0
279.80	3.0
280.30	1.0
281.10	316.0
282.10	91.0
282.90	74.0
283.90	15.0
284.40	25.0
285.30	18.0
286.10	4.0
287.10	1.0
287.60	3.0
288.40	1.0
289.20	3.0
289.60	2.0
290.70	3.0
292.30	1.0
292.90	1.0
293.40	1.0
294.20	3.0
295.60	4.0
297.00	3.0
297.40	2.0
298.00	14.0
298.70	2.0
299.30	10.0
300.10	2.0
300.90	1.0
302.10	9.0
303.00	1.0
303.50	11.0
304.40	1.0
305.00	4.0
306.50	2.0
307.30	19.0
308.00	3.0
308.90	9.0
309.70	2.0
310.60	12.0
311.30	5.0
312.80	4.0
313.40	0.0
314.40	2.0
315.10	17.0
316.00	3.0
317.50	3.0
318.10	1.0
319.20	3.0
319.90	0.0
320.40	2.0
320.80	2.0
321.30	1.0
322.20	1.0
322.70	1.0
323.70	2.0
324.20	10.0
325.00	7.0
325.90	4.0
327.00	67.0
328.20	17.0
329.20	1.0
330.40	4.0
331.00	1.0
331.60	2.0
332.10	1.0
332.90	1.0
333.50	2.0
334.10	0.0
334.80	4.0
336.30	1.0
336.90	2.0
338.00	4.0
338.60	2.0
339.40	7.0
339.90	3.0
340.60	2.0
341.10	12.0
342.10	20.0
342.90	11.0
343.30	3.0
344.20	16.0
345.40	13.0
346.30	1.0
347.40	3.0
347.80	2.0
349.00	2.0
349.60	2.0
350.60	2.0
351.00	2.0
352.30	2.0
352.90	1.0
353.80	3.0
355.10	43.0
355.80	13.0
357.30	2.0
358.00	1.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

358.40	2.0
359.10	20.0
359.90	2.0
360.70	2.0
361.60	3.0
362.30	2.0
363.20	4.0
363.70	1.0
364.30	18.0
364.80	2.0
365.10	2.0
366.00	1.0
366.40	4.0
368.20	12.0
368.90	1.0
369.40	2.0
370.20	5.0
371.00	3.0
371.50	1.0
372.60	2.0
373.30	5.0
374.00	2.0
375.00	1.0
375.60	2.0
376.20	2.0
376.90	7.0
378.30	1.0
379.30	4.0
380.30	2.0
380.80	2.0
381.90	2.0
382.30	3.0
382.80	0.0
383.50	2.0
384.50	1.0
385.20	3.0
385.90	1.0
386.80	3.0
388.30	3.0
388.90	2.0
390.00	5.0
391.50	3.0
392.10	1.0
393.10	2.0
393.60	1.0
394.10	1.0
394.80	2.0
396.20	4.0
397.80	3.0
398.30	2.0
399.40	2.0
400.80	15.0
401.50	1.0
402.50	3.0
404.00	3.0
404.60	2.0
405.00	8.0
405.70	2.0
407.20	3.0
408.10	1.0
408.60	2.0
408.90	3.0
410.50	3.0
412.00	3.0
413.10	16.0
413.70	2.0
415.20	14.0
416.20	15.0
417.00	2.0
418.30	3.0
419.20	3.0
419.90	3.0
420.70	0.0
421.60	15.0
422.70	11.0
423.30	1.0
423.70	1.0
424.70	2.0
426.20	3.0
426.60	3.0
427.70	3.0
428.20	1.0
429.00	4.0
429.40	7.0
430.10	10.0
430.80	3.0
431.60	1.0
432.50	2.0
432.90	2.0
434.00	2.0
434.60	1.0
435.50	2.0
436.40	1.0
437.20	3.0
438.70	3.0
440.60	3.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

441.20	0.0
441.70	2.0
442.40	1.0
442.90	1.0
443.50	3.0
444.10	1.0
444.90	2.0
445.70	0.0
446.50	1.0
447.00	3.0
448.30	6.0
449.80	2.0
451.60	4.0
453.10	16.0
454.40	4.0
454.80	2.0
455.60	1.0
456.10	3.0
456.70	1.0
457.60	2.0
458.60	2.0
459.30	3.0
460.60	3.0
461.20	2.0
462.20	1.0
462.80	2.0
464.00	5.0
464.40	1.0
465.70	3.0
466.10	1.0
467.10	3.0
467.90	1.0
468.40	2.0
469.00	5.0
470.10	3.0
470.60	1.0
471.60	2.0
472.30	1.0
473.50	2.0
474.10	1.0
474.70	1.0
475.50	6.0
476.40	2.0
476.80	3.0
477.90	3.0
478.40	1.0
479.80	6.0
480.30	16.0
481.00	3.0
481.60	1.0
482.70	3.0
483.10	3.0
483.70	4.0
484.20	4.0
484.80	1.0
486.10	2.0
487.50	3.0
488.60	1.0
489.40	5.0
490.60	3.0
491.20	1.0
491.60	1.0
492.40	3.0
493.00	0.0
493.70	3.0
494.20	1.0
495.30	3.0
496.70	2.0
497.80	3.0
498.40	2.0
499.50	2.0
499.90	1.0
500.30	2.0
501.10	1.0
501.90	3.0
503.20	2.0
504.80	3.0
505.40	2.0
506.40	5.0
507.40	1.0
508.10	4.0
509.50	3.0
510.40	0.0
511.10	2.0
511.90	3.0
512.70	4.0
513.30	1.0
514.60	3.0
515.30	16.0
515.90	3.0
517.20	5.0
517.70	3.0
518.90	15.0
519.60	2.0
520.30	3.0
520.70	4.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

521.10	2.0
522.10	2.0
523.10	2.0
523.60	3.0
524.60	1.0
525.20	2.0
526.30	2.0
527.00	3.0
527.80	11.0
528.50	4.0
529.90	3.0
530.30	2.0
531.70	3.0
533.10	2.0
533.50	1.0
534.50	2.0
535.10	1.0
535.80	2.0
536.30	4.0
536.80	1.0
537.50	1.0
538.00	3.0
539.30	3.0
539.80	1.0
540.20	1.0
541.10	3.0
542.10	2.0
542.60	17.0
543.20	2.0
544.30	3.0
545.50	3.0
546.90	1.0
547.40	3.0
548.80	16.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

m/z	Abundance
35.00	21.0
36.00	25.0
37.00	436.0
38.10	1105.0
39.10	6179.0
40.00	538.0
41.10	253.0
41.80	4.0
43.00	137.0
44.00	1186.0
45.10	176.0
46.00	13.0
46.80	76.0
47.40	13.0
48.10	66.0
49.20	956.0
50.10	23352.0
51.10	91512.0
52.00	4535.0
53.00	171.0
53.80	10.0
55.00	666.0
56.00	2872.0
57.00	6794.0
58.00	308.0
59.10	64.0
60.00	114.0
61.10	1268.0
62.10	1560.0
63.00	4151.0
64.10	611.0
65.00	1818.0
65.90	211.0
66.90	122.0
68.20	2119.0
69.00	101544.0
70.10	480.0
70.90	90.0
72.20	44.0
73.10	1302.0
74.10	10849.0
75.00	16230.0
76.10	5748.0
77.10	107432.0
78.10	6793.0
79.00	9188.0
80.00	5601.0
81.00	8513.0
82.00	2012.0
83.10	1991.0
84.00	238.0
85.00	1439.0
86.00	2857.0
87.00	1053.0
88.00	365.0
89.00	294.0
91.00	2224.0
92.10	2454.0
93.00	13836.0
94.00	1038.0
95.00	279.0
96.10	707.0
98.10	11911.0
99.00	8850.0
100.00	537.0
101.10	4475.0
102.10	171.0
103.00	1620.0
104.00	3030.0
105.10	2809.0
106.20	877.0
107.10	35584.0
108.10	5955.0
110.10	59584.0
111.00	8826.0
112.10	1434.0
113.10	471.0
114.20	131.0
114.90	152.0
116.10	1954.0
117.10	30280.0
118.00	2018.0
119.10	268.0
120.00	337.0
121.10	209.0
122.00	2370.0
123.10	4023.0
124.00	1696.0
125.00	1579.0
127.10	104584.0
128.10	8281.0
129.10	46424.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

130.10	3541.0
131.10	790.0
132.10	361.0
133.10	304.0
134.00	1286.0
135.10	3744.0
136.10	1459.0
137.10	2036.0
138.10	446.0
139.10	404.0
140.00	676.0
141.10	6215.0
142.10	2092.0
143.10	1413.0
144.10	503.0
145.20	520.0
146.00	1197.0
147.10	3803.0
148.10	7578.0
149.10	1579.0
150.10	440.0
151.10	646.0
151.70	359.0
153.00	1875.0
154.10	1144.0
155.10	3560.0
156.10	5383.0
157.20	843.0
158.00	1092.0
159.10	740.0
160.10	2247.0
161.10	2745.0
162.00	985.0
163.00	221.0
164.10	285.0
165.10	2542.0
166.10	1710.0
167.10	12008.0
168.10	5924.0
169.10	902.0
170.10	467.0
170.90	519.0
172.00	917.0
173.10	1587.0
174.10	2370.0
175.10	4796.0
176.10	1284.0
177.10	2636.0
178.20	734.0
179.10	8768.0
180.10	6306.0
181.10	3048.0
182.00	389.0
183.20	182.0
184.10	740.0
185.10	4488.0
186.10	35968.0
187.10	9986.0
188.20	1111.0
189.10	2104.0
190.10	385.0
191.10	1125.0
192.10	2954.0
193.10	3192.0
194.10	571.0
195.10	261.0
196.10	6949.0
198.10	230272.0
199.10	14662.0
200.10	1681.0
201.60	825.0
203.10	2014.0
204.10	9044.0
205.20	15793.0
206.20	64784.0
207.20	9762.0
208.10	2272.0
209.00	715.0
210.20	880.0
211.20	2407.0
213.20	179.0
214.10	77.0
215.00	743.0
216.10	1762.0
217.10	17808.0
218.10	2045.0
218.90	210.0
220.00	260.0
221.10	8937.0
222.10	2234.0
223.10	3961.0
224.20	36520.0
225.20	9229.0
226.20	1120.0
227.10	15982.0
228.10	2575.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

229.10	2974.0
230.10	405.0
231.00	1213.0
232.10	236.0
233.00	189.0
234.20	1088.0
235.00	1175.0
236.10	743.0
237.10	1410.0
238.10	196.0
239.10	673.0
240.00	566.0
241.10	712.0
242.10	1719.0
243.20	2518.0
244.20	28232.0
245.20	3548.0
246.10	5238.0
247.20	1447.0
248.10	173.0
249.20	937.0
250.10	185.0
251.20	243.0
252.10	185.0
253.20	809.0
255.10	146496.0
256.10	21472.0
257.20	2129.0
258.10	8653.0
259.10	1664.0
260.10	203.0
261.10	265.0
262.30	11.0
263.10	96.0
264.10	319.0
265.10	3802.0
266.10	529.0
267.00	260.0
267.80	74.0
268.10	91.0
269.30	15.0
270.30	136.0
271.10	402.0
272.20	607.0
273.10	4313.0
274.20	11165.0
275.20	66680.0
276.20	9227.0
277.10	5336.0
278.10	1222.0
279.10	251.0
280.00	18.0
281.00	434.0
282.10	258.0
283.10	719.0
284.10	466.0
285.20	1039.0
286.10	177.0
287.10	16.0
288.10	67.0
289.10	256.0
290.00	105.0
291.10	129.0
292.50	214.0
293.10	1578.0
294.00	354.0
295.20	523.0
296.10	18592.0
297.10	2434.0
298.10	300.0
299.30	25.0
299.90	21.0
300.30	26.0
301.10	139.0
302.00	337.0
303.20	2210.0
304.10	551.0
305.30	77.0
306.00	15.0
306.50	2.0
307.20	2.0
308.10	242.0
309.10	288.0
310.10	317.0
311.00	49.0
312.20	87.0
313.20	222.0
314.20	759.0
315.10	1881.0
316.20	968.0
317.10	255.0
318.10	16.0
318.90	14.0
319.50	0.0
320.20	159.0
321.20	455.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

323.20	5126.0
324.20	1123.0
325.10	195.0
326.10	161.0
327.10	1166.0
328.10	457.0
329.20	86.0
330.10	16.0
331.20	35.0
332.00	307.0
333.10	339.0
334.20	3289.0
335.10	864.0
336.30	112.0
337.10	11.0
338.10	1.0
339.10	134.0
340.20	44.0
341.20	411.0
342.10	173.0
343.00	9.0
343.60	3.0
344.20	20.0
344.60	14.0
346.10	1018.0
347.10	172.0
347.90	15.0
348.80	2.0
350.10	29.0
351.20	60.0
352.10	1602.0
353.10	1239.0
354.20	1714.0
355.10	267.0
356.20	8.0
357.10	85.0
358.00	12.0
359.30	99.0
361.20	20.0
361.80	12.0
362.50	2.0
363.10	16.0
365.10	7066.0
366.10	1190.0
367.00	106.0
367.70	7.0
368.80	24.0
370.10	300.0
371.30	497.0
372.20	2909.0
373.10	751.0
374.20	19.0
375.10	2.0
376.00	1.0
376.80	7.0
377.30	15.0
378.20	6.0
379.30	1.0
380.20	2.0
380.80	14.0
381.40	3.0
382.20	11.0
383.20	692.0
384.20	231.0
385.30	28.0
385.90	5.0
386.60	2.0
387.00	1.0
388.20	17.0
388.70	18.0
389.40	15.0
390.10	380.0
391.20	191.0
392.00	126.0
393.10	21.0
394.10	3.0
394.70	2.0
395.30	21.0
395.90	9.0
396.40	9.0
397.20	54.0
398.10	9.0
398.90	10.0
399.90	1.0
401.20	209.0
402.20	1082.0
403.10	1671.0
404.20	528.0
405.00	150.0
406.30	24.0
407.20	1.0
408.20	3.0
409.10	10.0
410.00	14.0
411.20	21.0
411.90	0.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

413.00	2.0
413.30	2.0
414.30	1.0
415.30	61.0
416.40	9.0
416.70	7.0
417.30	6.0
418.10	9.0
418.80	5.0
419.50	10.0
420.20	18.0
421.20	1213.0
422.20	1384.0
423.20	8916.0
424.20	2564.0
425.20	268.0
426.00	19.0
427.00	11.0
427.50	15.0
428.30	0.0
429.20	13.0
430.40	7.0
431.40	1.0
431.90	1.0
432.40	11.0
433.50	18.0
434.50	13.0
435.20	3.0
436.00	3.0
436.80	10.0
437.50	27.0
438.10	74.0
439.20	198.0
440.10	327.0
441.20	23528.0
442.20	143488.0
443.20	28112.0
444.20	3281.0
445.10	119.0
445.90	2.0
446.30	2.0
447.60	3.0
449.00	3.0
449.50	2.0
450.60	3.0
451.40	1.0
452.20	2.0
453.00	0.0
454.00	2.0
454.60	1.0
455.30	2.0
455.60	4.0
456.90	3.0
457.90	0.0
458.50	2.0
459.40	15.0
460.10	3.0
461.40	7.0
462.00	2.0
463.50	3.0
464.60	10.0
466.30	2.0
467.00	0.0
467.90	2.0
468.30	2.0
469.50	2.0
470.00	1.0
471.10	4.0
472.50	4.0
473.10	1.0
474.10	3.0
474.30	3.0
475.30	12.0
476.10	6.0
477.40	2.0
478.10	1.0
478.90	3.0
479.90	1.0
480.50	3.0
481.10	0.0
481.90	3.0
482.20	2.0
483.70	3.0
484.20	3.0
484.90	1.0
485.50	2.0
486.70	2.0
487.20	1.0
487.70	0.0
488.40	3.0
488.80	3.0
489.80	4.0
490.30	1.0
491.60	2.0
492.80	2.0
493.30	3.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

494.50	2.0
495.30	1.0
496.20	2.0
496.80	2.0
497.90	5.0
499.10	1.0
499.50	2.0
500.00	0.0
501.20	2.0
502.20	2.0
502.50	2.0
503.10	17.0
504.20	4.0
504.80	1.0
505.60	19.0
506.30	1.0
507.20	4.0
507.80	0.0
508.40	1.0
508.90	4.0
509.70	1.0
510.30	2.0
510.70	2.0
512.10	3.0
513.10	2.0
513.60	3.0
515.00	2.0
515.70	1.0
516.50	2.0
517.40	1.0
518.10	5.0
519.00	1.0
519.80	3.0
520.20	2.0
521.30	10.0
522.10	2.0
522.90	2.0
523.40	1.0
524.70	4.0
526.00	3.0
526.30	4.0
527.60	3.0
528.20	1.0
528.90	7.0
529.50	3.0
531.10	2.0
531.50	1.0
532.50	3.0
533.10	2.0
534.00	2.0
535.00	0.0
535.60	3.0
537.20	3.0
538.50	2.0
539.00	2.0
540.60	2.0
541.10	0.0
542.00	3.0
542.60	1.0
543.60	3.0
544.30	2.0
545.20	3.0
546.80	3.0
547.80	2.0
548.50	2.0
549.90	4.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

m/z	Abundance
36.00	21.0
37.00	405.0
38.10	860.0
39.10	6095.0
40.00	570.0
41.10	255.0
42.10	33.0
43.00	111.0
44.00	1485.0
45.10	149.0
45.80	11.0
46.10	15.0
46.80	62.0
49.10	795.0
50.10	23256.0
51.10	83336.0
52.10	4217.0
53.00	107.0
53.90	12.0
54.90	571.0
56.00	2425.0
57.00	5651.0
57.90	278.0
59.00	63.0
60.00	125.0
61.00	1035.0
62.00	1481.0
63.10	3430.0
64.10	516.0
65.10	1613.0
66.00	93.0
67.10	262.0
69.00	91352.0
70.00	364.0
71.00	90.0
73.00	1063.0
74.00	10661.0
75.00	14609.0
76.10	5608.0
77.10	98152.0
78.10	6504.0
79.00	7907.0
80.00	5981.0
81.00	7874.0
82.00	1833.0
83.00	1585.0
84.00	292.0
85.00	1473.0
86.00	2386.0
87.10	1011.0
87.90	361.0
89.00	262.0
89.70	6.0
91.00	1673.0
92.00	2099.0
93.00	13092.0
94.00	867.0
95.10	221.0
96.10	803.0
97.20	372.0
98.10	10315.0
99.00	8236.0
100.00	532.0
101.00	4444.0
102.10	282.0
103.00	1309.0
104.00	3220.0
105.00	3041.0
106.00	613.0
107.10	32728.0
108.10	5011.0
109.10	1153.0
110.00	55568.0
111.10	8701.0
112.10	1003.0
113.10	387.0
114.20	49.0
115.20	172.0
116.10	1980.0
117.10	29328.0
118.10	1904.0
119.00	234.0
120.20	329.0
121.10	233.0
122.00	2165.0
123.00	3254.0
124.00	1636.0
125.00	1355.0
127.10	102096.0
128.10	7697.0
129.10	42032.0
130.00	3982.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

131.00	822.0
132.10	297.0
133.10	257.0
133.90	1257.0
135.10	3545.0
136.00	1608.0
137.10	1764.0
138.10	413.0
139.10	261.0
140.10	506.0
141.00	5834.0
142.10	2074.0
143.10	1512.0
144.00	367.0
145.20	376.0
146.10	1061.0
147.10	3342.0
148.10	7494.0
149.10	1364.0
150.10	299.0
151.20	947.0
152.10	449.0
153.10	2084.0
154.00	1187.0
155.10	3487.0
156.10	4804.0
157.00	927.0
158.10	1148.0
159.10	1181.0
160.10	1813.0
161.10	2601.0
162.10	700.0
163.10	289.0
163.90	262.0
165.10	2453.0
166.10	1571.0
167.10	11350.0
168.10	5535.0
169.10	1181.0
170.10	299.0
170.90	516.0
172.00	1158.0
173.10	1769.0
174.10	2715.0
175.10	4662.0
176.00	1389.0
177.10	2380.0
178.10	908.0
179.10	8818.0
180.10	6667.0
181.10	3071.0
182.20	385.0
183.20	244.0
184.10	736.0
185.20	3990.0
186.10	33224.0
187.10	10055.0
188.10	980.0
189.10	2216.0
190.00	386.0
191.10	1295.0
192.10	3170.0
193.20	3466.0
194.10	628.0
195.00	468.0
196.10	5918.0
198.10	240512.0
199.10	16080.0
200.10	1127.0
201.70	514.0
203.10	2025.0
204.10	10072.0
205.20	16792.0
206.20	68096.0
207.10	9890.0
208.10	2543.0
209.10	965.0
210.00	871.0
211.00	2299.0
213.10	258.0
214.00	77.0
215.10	942.0
216.20	1285.0
217.10	18072.0
218.10	2525.0
219.30	243.0
220.20	429.0
221.10	9318.0
222.10	2374.0
223.10	4540.0
224.20	38832.0
225.20	10169.0
226.20	1349.0
227.10	17584.0
228.10	2248.0
229.10	3808.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

230.10	428.0
231.10	1284.0
232.10	354.0
233.10	362.0
234.10	965.0
235.10	1197.0
236.10	616.0
237.10	1441.0
238.10	132.0
239.10	707.0
240.10	562.0
241.20	1157.0
242.10	1914.0
243.10	2296.0
244.20	28216.0
245.20	3979.0
246.10	6205.0
247.10	1091.0
248.20	242.0
249.10	1171.0
250.10	215.0
251.10	411.0
252.20	275.0
253.10	741.0
255.10	151616.0
256.20	21944.0
257.10	1490.0
258.10	8931.0
259.10	1618.0
260.10	249.0
261.10	252.0
262.00	2.0
262.40	8.0
263.20	93.0
264.00	162.0
265.10	3737.0
266.10	375.0
267.10	165.0
268.20	50.0
269.00	30.0
270.10	173.0
271.00	210.0
272.20	437.0
273.10	4217.0
274.10	12027.0
275.20	70304.0
276.20	9323.0
277.10	6942.0
278.10	972.0
279.00	127.0
279.90	7.0
281.20	527.0
282.30	181.0
283.20	839.0
284.00	561.0
285.10	1066.0
286.00	205.0
286.90	9.0
287.20	9.0
288.10	100.0
289.00	179.0
290.00	155.0
291.00	209.0
292.20	253.0
293.10	1465.0
294.10	395.0
296.10	19224.0
297.10	2832.0
298.30	124.0
299.30	2.0
301.10	333.0
302.10	430.0
303.20	2098.0
304.10	694.0
305.10	90.0
306.10	6.0
306.60	4.0
307.20	23.0
308.10	329.0
309.00	136.0
310.20	371.0
311.00	39.0
312.20	107.0
313.20	172.0
314.20	859.0
315.10	2445.0
316.10	1062.0
317.00	127.0
318.30	18.0
319.00	14.0
319.50	8.0
320.30	79.0
321.10	736.0
322.20	555.0
323.20	5989.0
324.20	1188.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

325.10	92.0
326.10	188.0
327.10	1022.0
328.10	527.0
329.10	140.0
330.00	16.0
331.20	50.0
332.10	395.0
333.20	661.0
334.20	3864.0
335.20	833.0
336.20	164.0
337.00	1.0
337.30	0.0
337.90	3.0
339.10	117.0
340.10	79.0
341.10	870.0
342.20	202.0
343.00	21.0
344.20	9.0
345.30	15.0
346.10	1126.0
347.10	344.0
348.20	25.0
348.70	5.0
349.60	10.0
350.20	24.0
351.10	136.0
352.20	1879.0
353.10	1437.0
354.20	2196.0
355.30	332.0
356.10	18.0
357.00	15.0
357.50	22.0
358.30	20.0
359.10	64.0
360.10	64.0
361.10	14.0
363.20	26.0
365.10	8533.0
366.20	1230.0
367.00	74.0
367.80	4.0
368.60	1.0
370.20	202.0
371.20	575.0
372.20	3503.0
373.20	595.0
373.80	67.0
375.10	2.0
375.70	4.0
377.00	127.0
377.90	14.0
379.10	9.0
380.80	3.0
381.90	3.0
383.10	1026.0
384.30	182.0
385.20	66.0
386.10	14.0
387.00	25.0
388.20	2.0
388.90	9.0
390.20	567.0
391.10	260.0
392.10	162.0
393.00	22.0
394.00	1.0
394.90	22.0
395.90	5.0
396.30	3.0
397.20	57.0
398.10	2.0
399.20	24.0
399.90	1.0
402.20	1332.0
403.20	1951.0
404.10	520.0
405.30	242.0
406.10	16.0
407.20	3.0
408.00	8.0
409.00	13.0
409.70	4.0
410.30	16.0
411.30	21.0
412.10	2.0
412.80	0.0
413.40	3.0
414.10	1.0
415.30	82.0
416.20	8.0
417.40	7.0
418.10	9.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

418.50	8.0
419.20	13.0
419.60	19.0
421.20	1755.0
422.20	1532.0
423.20	11365.0
424.20	2504.0
425.20	345.0
426.20	17.0
426.80	15.0
427.90	5.0
429.40	2.0
430.80	7.0
432.00	16.0
432.90	2.0
433.80	2.0
434.20	2.0
435.20	1.0
435.70	15.0
436.20	17.0
436.90	11.0
437.40	7.0
438.00	148.0
439.00	89.0
439.50	120.0
441.20	30872.0
442.20	186944.0
443.20	35008.0
444.20	3466.0
445.00	226.0
446.20	24.0
447.10	1.0
447.40	1.0
448.10	3.0
448.80	1.0
449.70	1.0
450.20	5.0
451.40	5.0
452.30	2.0
452.70	2.0
453.30	1.0
454.30	2.0
455.30	1.0
455.70	3.0
456.80	12.0
457.60	4.0
458.20	1.0
459.20	16.0
459.90	1.0
460.70	4.0
461.10	8.0
462.20	3.0
463.70	2.0
464.20	2.0
465.10	2.0
465.60	2.0
466.20	1.0
467.10	16.0
467.60	0.0
468.30	2.0
468.80	1.0
469.50	1.0
470.20	3.0
471.70	3.0
473.40	2.0
474.20	2.0
475.00	4.0
475.60	0.0
476.70	3.0
477.80	2.0
478.20	2.0
479.40	2.0
479.80	2.0
481.00	3.0
482.10	1.0
482.60	3.0
482.90	2.0
483.40	1.0
484.00	2.0
484.60	2.0
485.60	1.0
486.50	0.0
487.50	2.0
489.10	3.0
490.10	1.0
490.50	1.0
491.10	2.0
492.10	3.0
492.60	1.0
493.70	3.0
494.20	1.0
495.50	3.0
496.80	3.0
497.60	0.0
498.50	3.0
499.30	1.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

500.00	2.0
500.60	2.0
501.70	2.0
503.30	3.0
503.80	5.0
504.50	1.0
504.90	2.0
506.30	3.0
507.10	1.0
507.70	3.0
509.20	7.0
509.70	2.0
510.80	2.0
511.20	2.0
512.70	3.0
514.20	2.0
515.20	1.0
515.90	3.0
517.30	2.0
518.40	0.0
519.10	4.0
520.50	2.0
522.00	3.0
523.60	3.0
523.90	2.0
525.00	2.0
525.50	1.0
526.60	2.0
527.60	0.0
528.30	2.0
530.00	3.0
530.70	0.0
531.60	3.0
532.90	2.0
533.40	1.0
534.80	3.0
536.20	4.0
537.50	2.0
538.00	11.0
539.40	2.0
540.30	0.0
540.90	5.0
541.80	8.0
542.40	4.0
542.90	2.0
543.40	0.0
544.40	3.0
545.60	2.0
547.40	3.0
548.70	3.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

m/z	Abundance
35.60	0.0
36.30	18.0
37.10	225.0
38.10	721.0
39.10	3311.0
39.90	412.0
41.20	182.0
42.10	64.0
42.90	139.0
44.00	1160.0
45.00	121.0
45.80	9.0
46.70	59.0
49.10	474.0
50.10	12011.0
51.10	45952.0
52.00	2396.0
53.10	163.0
54.10	15.0
55.00	393.0
55.90	1408.0
57.00	3226.0
58.10	229.0
59.00	152.0
60.00	58.0
60.90	562.0
62.00	823.0
63.00	1709.0
64.00	335.0
65.00	915.0
65.90	209.0
68.00	973.0
69.00	50096.0
70.10	431.0
71.00	49.0
73.00	842.0
74.10	5557.0
75.00	8526.0
76.10	2942.0
77.10	53256.0
78.10	3867.0
79.00	4834.0
80.00	3250.0
81.00	4193.0
82.00	1258.0
83.10	806.0
84.10	194.0
85.00	893.0
86.00	1403.0
87.10	591.0
87.80	195.0
89.00	144.0
89.80	3.0
91.00	1179.0
92.00	1043.0
93.00	8066.0
94.10	478.0
95.10	126.0
96.00	280.0
97.00	149.0
98.00	6347.0
99.10	5150.0
99.90	438.0
101.10	2163.0
102.00	219.0
103.00	1171.0
104.10	1853.0
105.10	1553.0
107.00	19328.0
108.10	2969.0
109.00	629.0
110.00	34448.0
111.10	5222.0
112.10	677.0
113.10	308.0
113.90	12.0
114.90	263.0
116.00	1075.0
117.10	18192.0
118.00	1456.0
118.90	133.0
120.10	215.0
121.00	123.0
122.00	1657.0
123.10	2144.0
124.00	919.0
125.10	913.0
127.10	62488.0
128.10	5205.0
129.10	26824.0
130.10	2282.0
131.10	531.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

132.10	269.0
133.00	156.0
134.00	1009.0
135.00	2355.0
136.00	1061.0
137.10	1694.0
138.10	221.0
139.10	238.0
140.00	247.0
141.10	3808.0
142.10	1464.0
143.00	829.0
144.10	249.0
145.00	172.0
146.10	628.0
147.10	1997.0
148.10	4584.0
149.00	756.0
150.00	325.0
151.00	415.0
151.90	171.0
153.10	1179.0
154.00	960.0
155.10	2271.0
156.10	2925.0
157.10	627.0
158.00	800.0
159.10	567.0
160.00	1397.0
161.10	1756.0
162.00	649.0
162.90	143.0
163.90	168.0
165.10	1426.0
166.10	1233.0
167.10	8324.0
168.10	4024.0
169.10	594.0
170.20	314.0
170.90	283.0
172.10	759.0
173.00	1211.0
174.10	1905.0
175.10	3187.0
176.10	754.0
177.10	1579.0
178.10	594.0
179.10	5756.0
180.10	3906.0
181.10	1659.0
182.00	364.0
182.60	90.0
182.90	114.0
184.10	395.0
185.10	3157.0
186.10	23960.0
187.10	6555.0
188.10	843.0
189.10	1846.0
190.00	240.0
191.10	845.0
192.10	2143.0
193.20	1882.0
194.00	477.0
195.10	405.0
196.10	4590.0
198.10	162240.0
199.10	9900.0
200.10	892.0
201.50	921.0
202.20	204.0
203.10	1486.0
204.10	6358.0
205.10	10456.0
206.20	44824.0
207.10	7510.0
208.10	2074.0
209.00	479.0
210.10	861.0
211.20	1478.0
212.10	267.0
213.00	154.0
213.90	73.0
215.10	705.0
216.10	1577.0
217.10	13027.0
218.10	1461.0
219.10	163.0
221.20	5762.0
222.10	1792.0
223.20	2731.0
224.10	24680.0
225.10	7083.0
226.10	695.0
227.10	10737.0
228.10	1600.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

229.10	2275.0
230.10	336.0
231.10	977.0
231.90	59.0
233.10	257.0
234.10	625.0
235.10	861.0
236.10	554.0
237.20	823.0
238.10	124.0
239.10	421.0
240.10	457.0
241.00	695.0
242.10	1020.0
243.20	1222.0
244.20	18176.0
245.20	2522.0
246.10	4027.0
247.20	680.0
248.00	206.0
249.10	909.0
250.20	140.0
251.10	155.0
252.10	165.0
253.00	438.0
255.10	101616.0
256.20	14450.0
257.10	1090.0
258.10	6431.0
259.20	851.0
260.10	168.0
261.10	202.0
262.20	15.0
262.80	10.0
263.30	46.0
264.10	170.0
265.10	2854.0
266.00	279.0
267.10	175.0
268.00	41.0
269.00	95.0
270.00	133.0
271.10	271.0
272.30	330.0
273.10	3210.0
274.10	8323.0
275.20	47392.0
276.20	5962.0
277.10	4911.0
278.00	557.0
279.00	180.0
279.90	14.0
281.10	360.0
282.10	261.0
283.10	654.0
284.10	427.0
285.10	707.0
286.10	230.0
286.80	16.0
287.40	8.0
288.10	17.0
288.90	209.0
290.00	118.0
291.30	135.0
292.20	166.0
293.10	1068.0
294.10	138.0
296.20	13811.0
297.10	1745.0
298.00	148.0
299.20	12.0
300.00	0.0
301.20	144.0
302.10	209.0
303.20	1657.0
304.20	358.0
305.20	83.0
306.10	23.0
307.20	49.0
308.10	299.0
309.20	221.0
310.20	243.0
311.00	88.0
312.10	27.0
313.00	171.0
314.10	547.0
315.10	1434.0
316.00	827.0
317.10	149.0
318.00	8.0
318.60	6.0
319.80	4.0
320.40	51.0
321.20	367.0
322.20	229.0
323.10	4462.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

324.10	647.0
325.20	51.0
326.00	85.0
327.10	603.0
328.10	361.0
329.00	46.0
330.00	21.0
331.00	9.0
332.10	397.0
333.10	471.0
334.20	3223.0
335.10	603.0
336.10	169.0
336.90	2.0
338.30	13.0
339.20	61.0
340.20	57.0
341.10	519.0
342.20	212.0
343.20	21.0
344.10	8.0
344.90	3.0
346.10	894.0
347.10	167.0
348.00	19.0
349.00	18.0
350.00	31.0
351.10	101.0
352.20	1413.0
353.10	714.0
354.20	1342.0
355.10	302.0
356.90	14.0
357.20	11.0
358.00	18.0
359.10	101.0
360.10	41.0
360.70	4.0
361.30	18.0
362.20	3.0
363.10	45.0
365.10	6725.0
366.20	828.0
367.00	57.0
367.90	7.0
369.00	10.0
370.10	179.0
371.10	300.0
372.10	2635.0
373.20	611.0
373.80	47.0
374.20	52.0
374.90	1.0
376.30	14.0
377.00	71.0
378.10	7.0
379.40	2.0
379.80	2.0
380.90	3.0
381.70	3.0
383.20	793.0
384.10	277.0
385.20	88.0
385.90	4.0
386.80	8.0
388.20	1.0
388.80	10.0
390.00	244.0
391.10	246.0
392.10	175.0
393.20	18.0
393.80	2.0
395.30	22.0
396.30	2.0
396.80	8.0
397.30	14.0
398.30	4.0
399.90	2.0
401.20	240.0
402.20	1305.0
403.20	1143.0
404.20	737.0
405.00	120.0
406.40	8.0
406.90	0.0
407.80	3.0
408.60	1.0
409.30	8.0
410.00	11.0
410.90	3.0
411.50	4.0
412.50	3.0
414.00	2.0
414.50	13.0
415.20	103.0
415.90	20.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

417.10	5.0
418.40	11.0
419.20	2.0
420.00	9.0
421.20	995.0
422.30	1322.0
423.20	9320.0
424.20	2127.0
425.10	224.0
426.20	18.0
426.80	2.0
427.30	18.0
428.20	3.0
429.20	13.0
429.70	11.0
430.60	6.0
431.30	4.0
432.00	0.0
433.00	20.0
434.30	14.0
435.20	0.0
435.80	14.0
436.30	18.0
436.80	24.0
438.10	95.0
438.90	56.0
439.60	196.0
441.20	23768.0
442.20	149824.0
443.20	27600.0
444.20	2498.0
445.10	125.0
446.20	1.0
447.30	3.0
447.90	1.0
448.50	2.0
448.90	2.0
449.80	1.0
450.40	3.0
451.40	1.0
452.30	1.0
453.30	3.0
453.80	1.0
454.40	1.0
455.00	3.0
456.60	3.0
457.20	7.0
458.20	4.0
458.90	6.0
459.80	3.0
461.10	13.0
462.40	12.0
463.10	2.0
464.10	2.0
464.70	1.0
466.00	4.0
466.70	1.0
467.60	2.0
468.20	1.0
469.20	3.0
470.20	5.0
470.70	5.0
471.50	1.0
472.20	4.0
472.80	1.0
473.70	4.0
474.50	1.0
475.50	2.0
476.30	0.0
476.90	2.0
477.60	1.0
478.60	3.0
479.70	2.0
480.10	3.0
480.40	2.0
481.10	1.0
481.60	3.0
482.00	1.0
483.30	3.0
485.10	2.0
486.20	4.0
486.80	2.0
487.50	1.0
488.10	3.0
489.30	3.0
490.40	2.0
491.00	5.0
491.40	3.0
492.00	0.0
492.90	2.0
493.70	1.0
494.60	3.0
495.10	1.0
496.00	9.0
496.70	0.0
497.40	3.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719

498.20	1.0
498.90	6.0
499.60	2.0
500.70	10.0
501.80	10.0
502.70	1.0
503.70	2.0
504.30	3.0
505.30	3.0
506.60	2.0
507.20	9.0
507.60	1.0
508.40	3.0
510.00	4.0
511.50	4.0
512.60	0.0
513.30	3.0
513.80	2.0
515.20	12.0
516.10	2.0
516.50	3.0
518.00	3.0
519.30	3.0
520.10	3.0
521.00	3.0
521.40	2.0
522.60	2.0
524.10	2.0
524.40	2.0
525.80	2.0
526.30	2.0
527.30	4.0
528.90	3.0
529.40	1.0
530.60	3.0
531.90	5.0
532.80	0.0
533.50	4.0
534.70	1.0
535.40	18.0
536.30	7.0
536.70	3.0
538.30	3.0
539.30	0.0
540.50	8.0
541.50	3.0
542.80	2.0
543.60	3.0
544.60	2.0
545.20	2.0
546.30	6.0
547.10	1.0
548.10	12.0
549.40	4.0

Instrument :
BNA_P
ClientSampleId :
DFTPP719