

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050225\
 Data File : BP024512.D
 Acq On : 02 May 2025 17:00
 Operator : RC/JU
 Sample : Q1928-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MH-Q

Quant Time: May 02 17:48:24 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 18 12:04:48 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	116610	20.000	ng	-0.02
21) Naphthalene-d8	10.481	136	441564	20.000	ng	#-0.02
39) Acenaphthene-d10	14.340	164	271829	20.000	ng	-0.01
64) Phenanthrene-d10	17.151	188	549619	20.000	ng	# 0.00
76) Chrysene-d12	21.592	240	679402	20.000	ng	0.00
86) Perylene-d12	24.951	264	816732	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.328	112	548011	77.704	ng	-0.02
7) Phenol-d6	6.893	99	690637	71.518	ng	-0.02
23) Nitrobenzene-d5	8.857	82	400086	51.665	ng	-0.01
42) 2,4,6-Tribromophenol	15.863	330	372684	99.094	ng	0.00
45) 2-Fluorobiphenyl	12.951	172	827960	46.636	ng	-0.01
79) Terphenyl-d14	19.875	244	1617694	47.993	ng	0.00
Target Compounds						
63) Azobenzene	15.728	77	77772	4.154	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050225\
Data File : BP024512.D
Acq On : 02 May 2025 17:00
Operator : RC/JU
Sample : Q1928-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MH-Q

Quant Time: May 02 17:48:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration




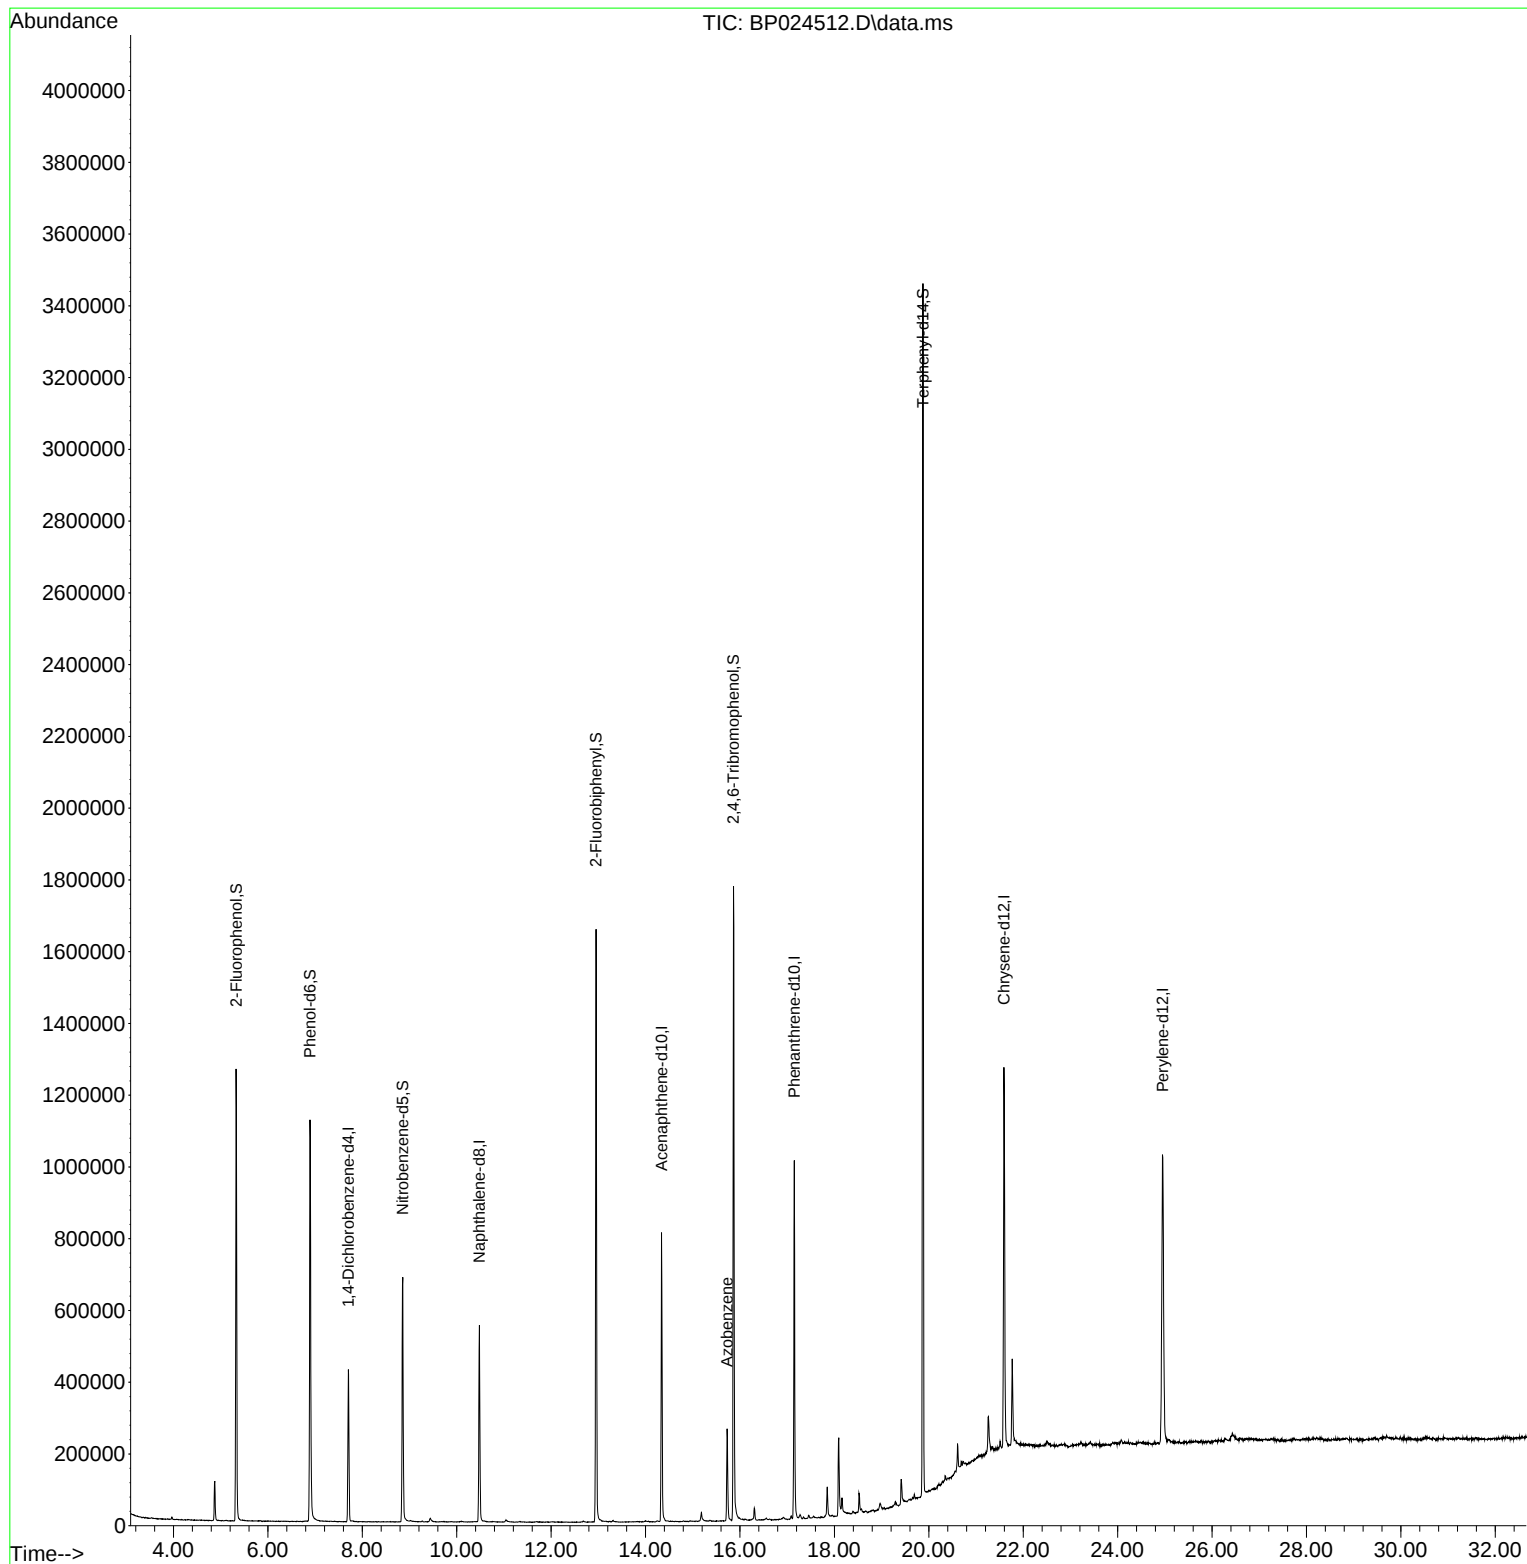




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.705 min Scan# 71
Delta R.T. -0.017 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00




Instrument :
BNA_P
ClientSampleId :
MH-Q


Tgt Ion:152 Resp: 116610
Ion Ratio Lower Upper
152 100
150 153.5 124.9 187.3
115 62.4 47.7 71.5

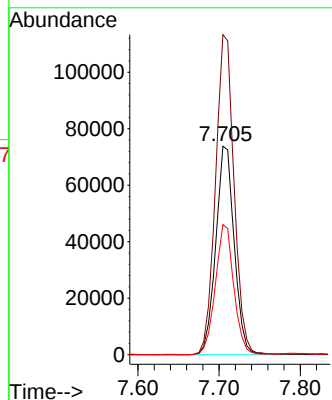

#5
2-Fluorophenol
Concen: 77.704 ng
RT: 5.328 min Scan# 381
Delta R.T. -0.018 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Tgt Ion:112 Resp: 548011
Ion Ratio Lower Upper
112 100
64 54.4 41.1 61.7
63 29.2 20.6 30.8


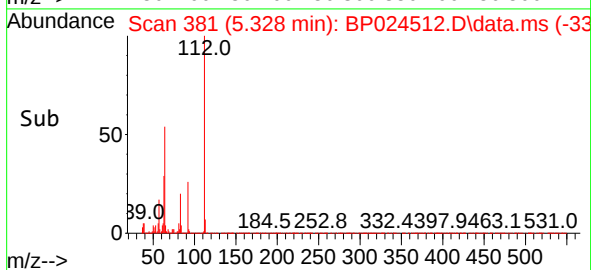
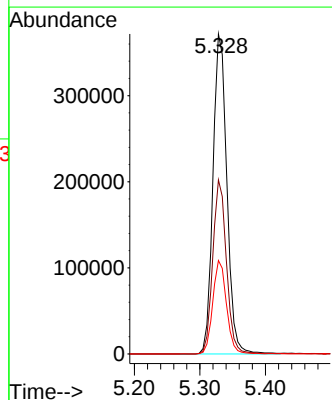





#7
Phenol-d6
Concen: 71.518 ng
RT: 6.893 min Scan# 64
Delta R.T. -0.018 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00




Instrument :
BNA_P
ClientSampleId :
MH-Q


Tgt Ion: 99 Resp: 690637
Ion Ratio Lower Upper
99 100
42 16.6 10.6 16.0#
71 35.6 23.7 35.5#

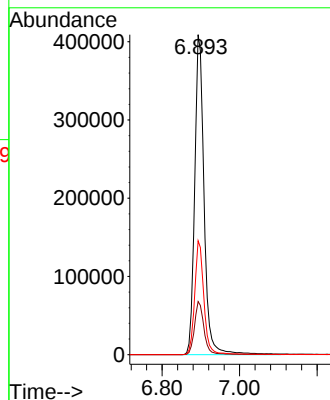

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.481 min Scan# 1257
Delta R.T. -0.018 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Tgt Ion: 136 Resp: 441564
Ion Ratio Lower Upper
136 100
137 10.7 9.2 13.8
54 6.8 6.0 9.0
68 4.9 5.5 8.3#


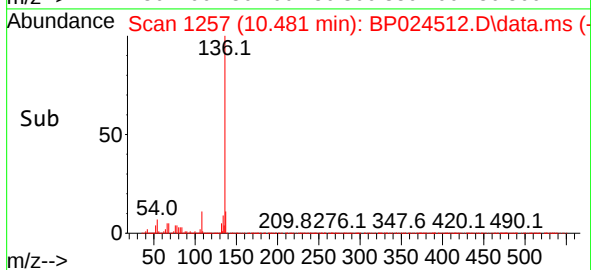
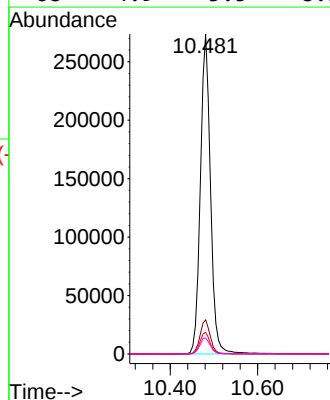





#23
Nitrobenzene-d5
Concen: 51.665 ng
RT: 8.857 min Scan# 91
Delta R.T. -0.012 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00




Instrument :
BNA_P
ClientSampleId :
MH-Q


Tgt Ion: 82 Resp: 400086
Ion Ratio Lower Upper
82 100
128 47.1 36.5 54.7
54 45.7 33.4 50.2

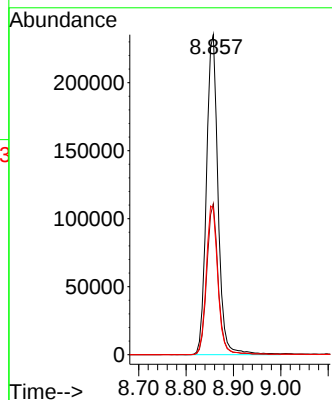

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.340 min Scan# 1913
Delta R.T. -0.012 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Tgt Ion: 164 Resp: 271829
Ion Ratio Lower Upper
164 100
162 101.3 80.6 120.8
160 45.5 35.3 52.9


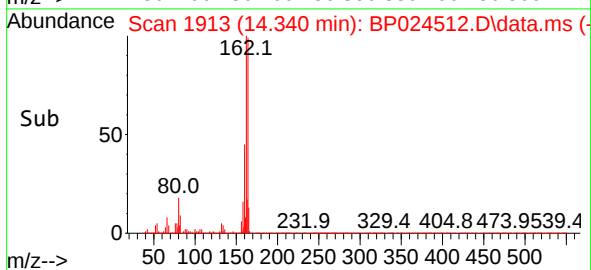
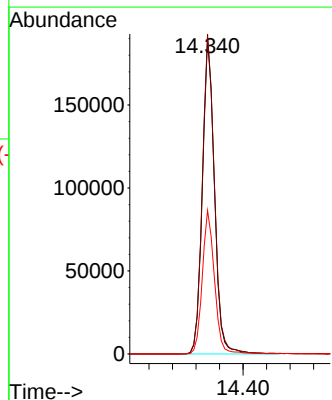





#42
2,4,6-Tribromophenol
Concen: 99.094 ng
RT: 15.863 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00




Instrument :
BNA_P
ClientSampleId :
MH-Q


Tgt Ion: 330 Resp: 372684
Ion Ratio Lower Upper
330 100
332 96.9 77.1 115.7
141 29.9 24.7 37.1

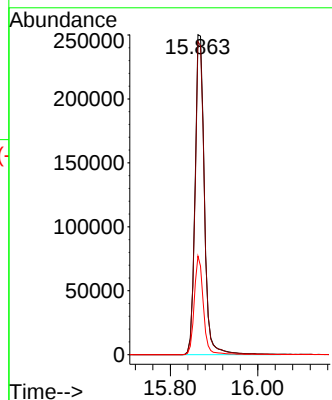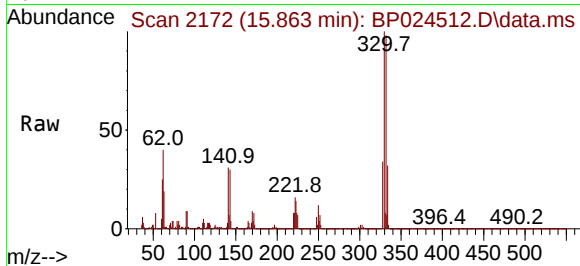

#45
2-Fluorobiphenyl
Concen: 46.636 ng
RT: 12.951 min Scan# 1677
Delta R.T. -0.012 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Tgt Ion: 172 Resp: 827960
Ion Ratio Lower Upper
172 100
171 35.1 28.2 42.2
170 23.3 18.6 27.8


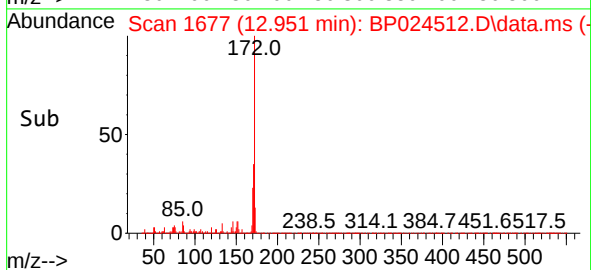
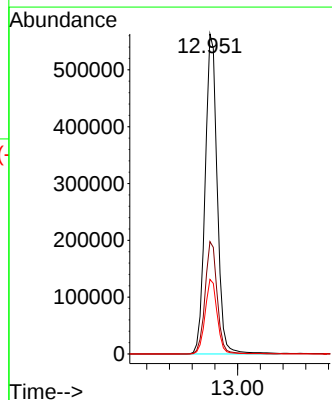
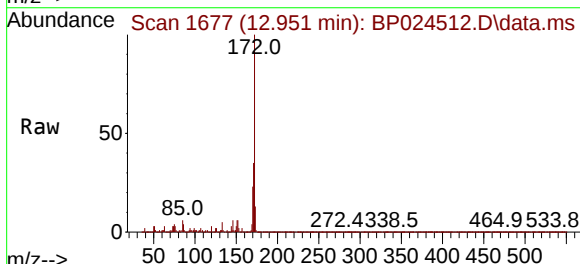




#63
Azobenzene
Concen: 4.154 ng
RT: 15.728 min Scan# 2149
Delta R.T. 0.018 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00




Instrument :
BNA_P
ClientSampleId :
MH-Q


Tgt Ion: 77	Resp: 77772
Ion Ratio	Lower Upper
77 100	
182 78.7	7.3 47.3#
105 155.0	2.3 42.3#
51 37.5	3.4 43.4

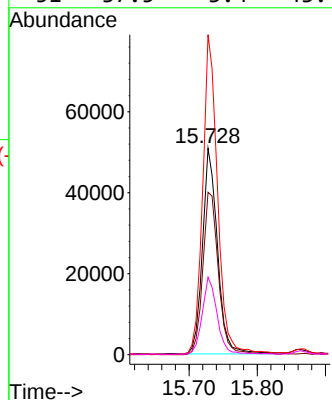

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.151 min Scan# 2391
Delta R.T. 0.006 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Tgt Ion:188	Resp: 549619
Ion Ratio	Lower Upper
188 100	
94 8.5	8.6 13.0#
80 9.5	9.8 14.6#


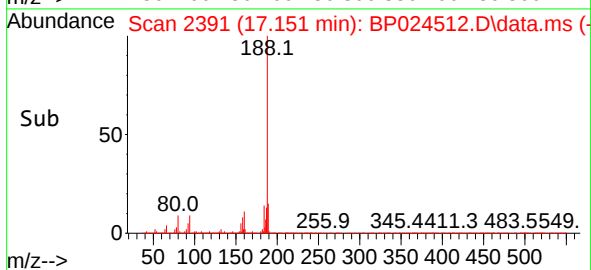
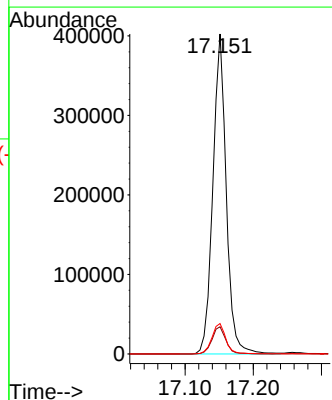





#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.592 min Scan# 3151
Delta R.T. 0.000 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00




Instrument :
BNA_P
ClientSampleId :
MH-Q


Tgt Ion:240 Resp: 679402
Ion Ratio Lower Upper
240 100
120 10.2 9.8 14.8
236 26.1 20.9 31.3

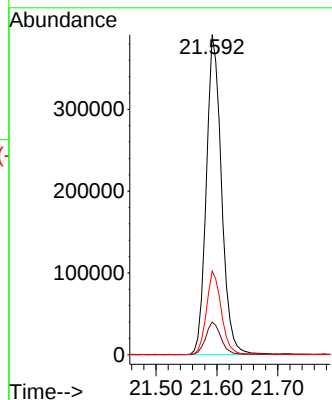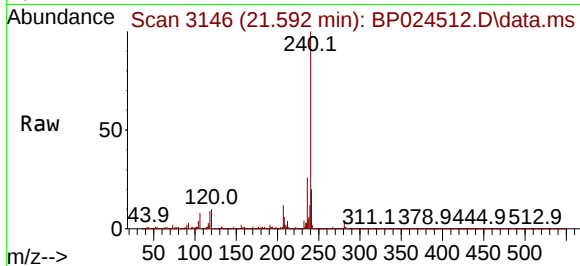

#79
Terphenyl-d14
Concen: 47.993 ng
RT: 19.875 min Scan# 2854
Delta R.T. 0.000 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Tgt Ion:244 Resp: 1617694
Ion Ratio Lower Upper
244 100
212 6.8 5.6 8.4
122 9.4 9.4 14.0

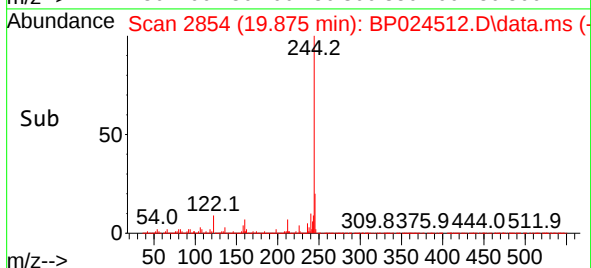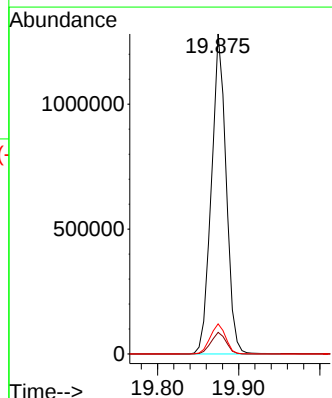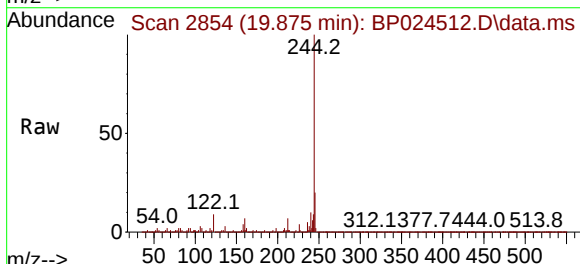

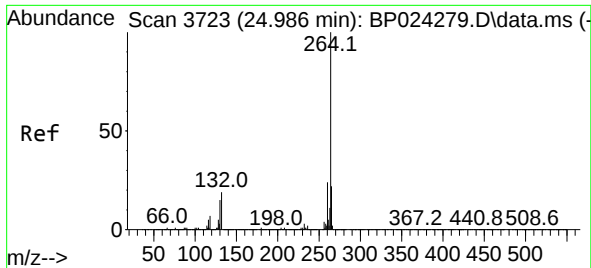

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.951 min Scan# 31
Delta R.T. 0.018 min
Lab File: BP024512.D
Acq: 02 May 2025 17:00

Instrument :
BNA_P
ClientSampleId :
MH-Q

Tgt Ion:264 Resp: 816732

Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.9	28.3
265	22.1	17.8	26.6

