




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP050423\  
 Data File : BP014944.D  
 Acq On : 04 May 2023 10:32  
 Operator : CG/JU  
 Sample : 02447-23  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 EW941

## Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/05/2023  
 Supervised By :Jagrut Upadhyay 05/05/2023

Quant Time: May 04 22:58:47 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP050323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu May 04 11:40:49 2023  
 Response via : Initial Calibration

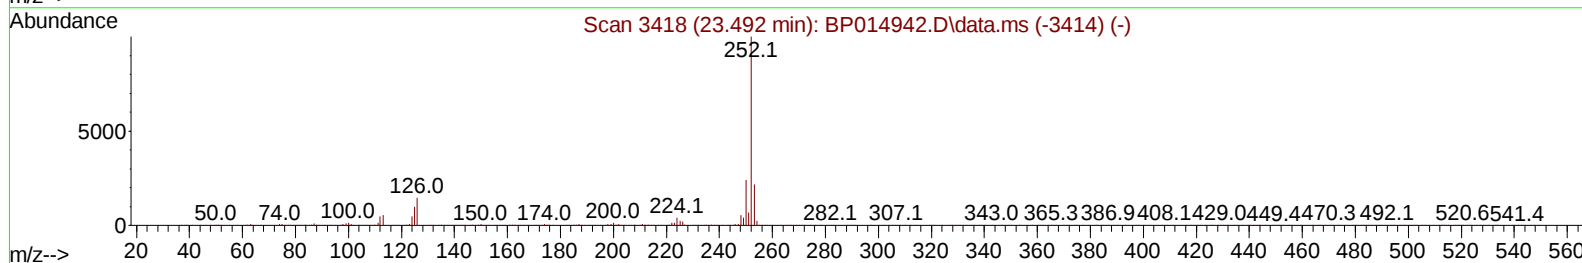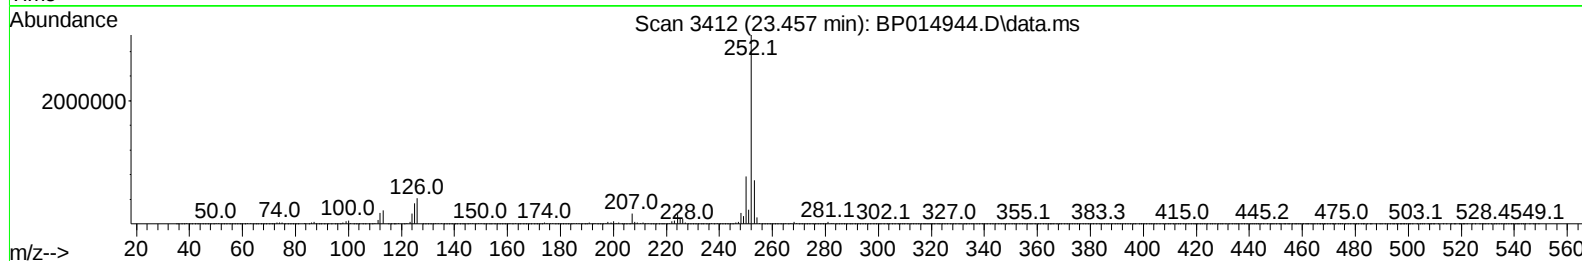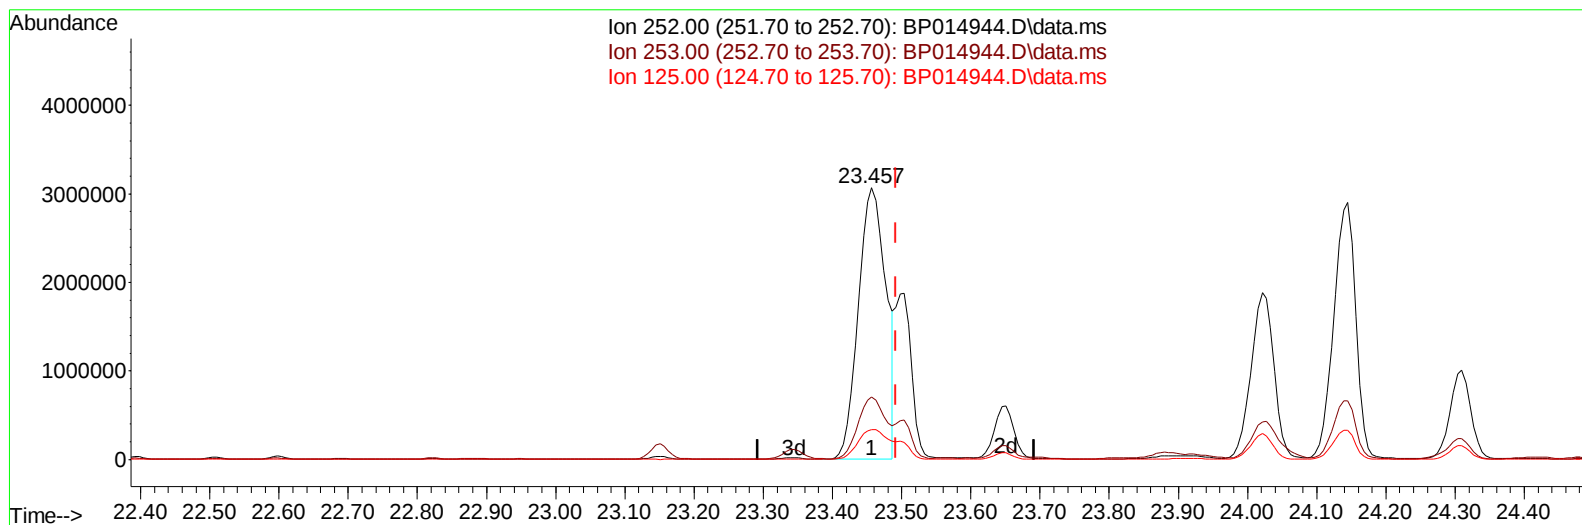

TIC: BP014944.D\data.ms

## (91) Benzo(k)fluoranthene

23.457min (-0.035) 95.65 ng/u1

response 8510959

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 22.20  | 23.09  |
| 125.00 | 11.10  | 10.95  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP050423\  
 Data File : BP014944.D  
 Acq On : 04 May 2023 10:32  
 Operator : CG/JU  
 Sample : 02447-23  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 EW941

Manual IntegrationsAPPROVED

Quant Time: May 04 22:58:47 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP050323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu May 04 11:40:49 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/05/2023  
 Supervised By :Jagrut Upadhyay 05/05/2023

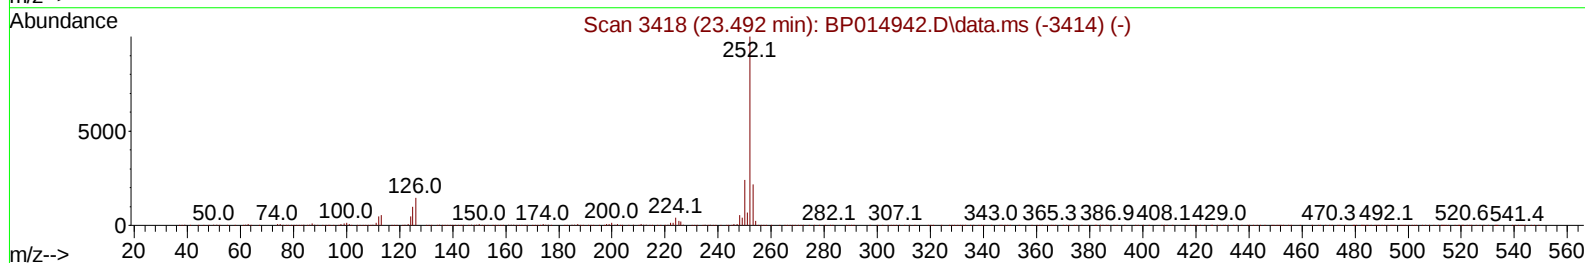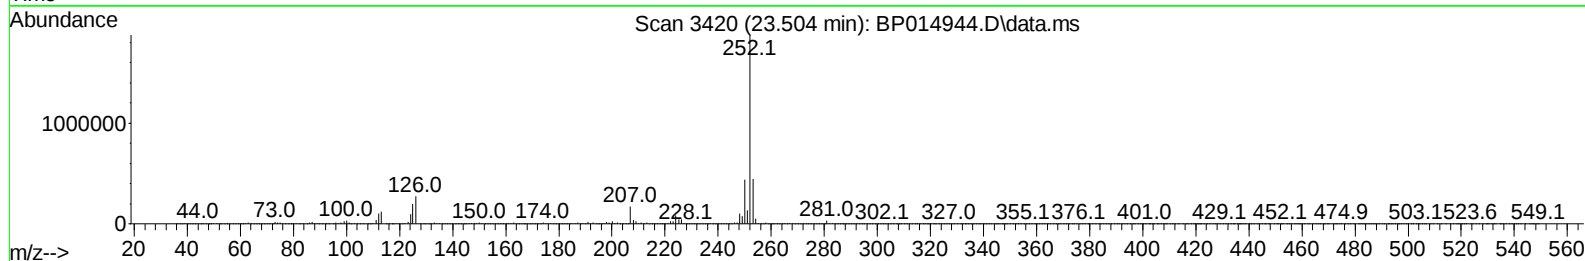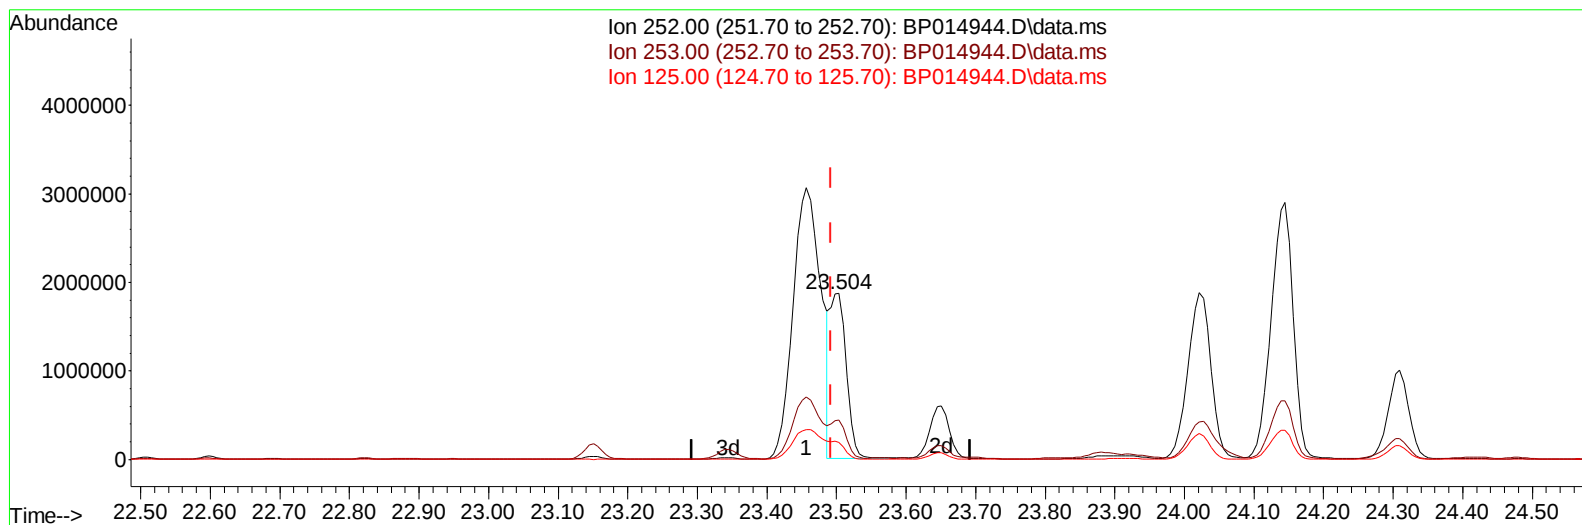

TIC: BP014944.D\data.ms

**(91) Benzo(k)fluoranthene**

**23.504min (+ 0.012) 33.60 ng/ul m**

**response 2989410**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 22.20  | 23.60  |
| 125.00 | 11.10  | 10.42  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP050423\  
 Data File : BP014944.D  
 Acq On : 04 May 2023 10:32  
 Operator : CG/JU  
 Sample : 02447-23  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 EW941

Manual IntegrationsAPPROVED

Quant Time: May 04 22:59:26 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP050323.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu May 04 11:40:49 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/05/2023  
 Supervised By :Jagrut Upadhyay 05/05/2023

| Compound                      | R.T.   | QIon | Response | Conc    | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|---------|--------|----------|
| -----                         |        |      |          |         |        |          |
| Internal Standards            |        |      |          |         |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.163  | 152  | 276748   | 20.000  | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.998 | 136  | 1052108  | 20.000  | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.810 | 164  | 568690   | 20.000  | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.569 | 188  | 1185514  | 20.000  | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.651 | 240  | 1081664  | 20.000  | ng/ul  | 0.00     |
| 88) Perylene-d12              | 24.251 | 264  | 1352810  | 20.000  | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |         |        |          |
| 3) 1,4-Dioxane-d8             | 3.458  | 96   | 22268    | 2.992   | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.899  | 84   | 233770   | 11.491  | ng/ul  | 0.00     |
| 7) Phenol-d5                  | 7.305  | 99   | 343688   | 14.324  | ng/ul  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.481  | 67   | 226645   | 15.283  | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.687  | 132  | 284513   | 16.127  | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.869  | 113  | 237058   | 12.821  | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.340  | 128  | 126711   | 16.934  | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 10.069 | 143  | 132825   | 17.287  | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.610 | 165  | 238784   | 15.827  | ng/ul  | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.134 | 131  | 221831   | 10.166  | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 14.210 | 166  | 697768   | 17.336  | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.504 | 160  | 834737   | 17.293  | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.987 | 143  | 46355    | 6.620   | ng/ul  | 0.00     |
| 60) Fluorene-d10              | 15.798 | 176  | 613111   | 17.706  | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.916 | 200  | 43863    | 6.573   | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.663 | 188  | 931090   | 17.480  | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.880 | 212  | 1133566  | 15.538  | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 24.080 | 264  | 1229569  | 18.654  | ng/ul  | 0.01     |
| Target Compounds              |        |      |          |         |        |          |
|                               |        |      |          |         | Qvalue |          |
| 52) Acenaphthene              | 14.875 | 153  | 602541   | 15.911  | ng/ul  | 98       |
| 56) Dibenzofuran              | 15.204 | 168  | 382688   | 7.489   | ng/ul  | 99       |
| 61) Fluorene                  | 15.857 | 166  | 689206   | 17.098  | ng/ul  | 99       |
| 72) Phenanthrene              | 17.616 | 178  | 9738326  | 148.689 | ng/ul  | 98       |
| 74) Anthracene                | 17.698 | 178  | 3041207  | 46.640  | ng/ul  | 100      |
| 77) Carbazole                 | 17.963 | 167  | 928856   | 16.936  | ng/ul  | 99       |
| 80) Fluoranthene              | 19.569 | 202  | 13487602 | 150.668 | ng/ul# | 93       |
| 82) Pyrene                    | 19.922 | 202  | 11784907 | 124.258 | ng/ul  | 94       |
| 85) Benzo(a)anthracene        | 21.633 | 228  | 6491715  | 89.916  | ng/ul  | 98       |
| 87) Chrysene                  | 21.692 | 228  | 5856647  | 80.564  | ng/ul  | 97       |
| 90) Benzo(b)fluoranthene      | 23.457 | 252  | 8510959  | 97.346  | ng/ul  | 98       |
| 91) Benzo(k)fluoranthene      | 23.504 | 252  | 2989410m | 33.596  | ng/ul  |          |
| 93) Benzo(a)pyrene            | 24.145 | 252  | 6342265  | 82.715  | ng/ul  | 98       |
| 94) Indeno(1,2,3-cd)pyrene    | 27.015 | 276  | 4610219  | 49.291  | ng/ul  | 97       |
| 95) Dibenzo(a,h)anthracene    | 27.021 | 278  | 1071262  | 13.974  | ng/ul# | 84       |
| 96) Benzo(g,h,i)perylene      | 27.868 | 276  | 4032141  | 50.653  | ng/ul  | 98       |
| -----                         |        |      |          |         |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP050423\  
Data File : BP014944.D  
Acq On : 04 May 2023 10:32  
Operator : CG/JU  
Sample : 02447-23  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
EW941

## Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/05/2023  
Supervised By :Jagrut Upadhyay 05/05/2023

Quant Time: May 04 22:59:26 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP050323.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu May 04 11:40:49 2023  
Response via : Initial Calibration

