

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050423\
 Data File : BP014958.D
 Acq On : 04 May 2023 18:20
 Operator : CG/JU
 Sample : PB152461BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK461

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.464	9	13	21	rVB	98598	130961	2.15%	0.208%
2	3.899	84	87	101	rBV	974328	1352094	22.23%	2.147%
3	4.246	143	146	153	rVB	24489	32314	0.53%	0.051%
4	7.311	659	667	686	rBV	1122442	1799092	29.57%	2.857%
5	7.481	689	696	708	rVB	989615	1520527	24.99%	2.415%
6	7.687	724	731	742	rBV	1225522	1935721	31.82%	3.074%
7	8.163	805	812	822	rBV	1129358	1809456	29.74%	2.874%
8	8.875	925	933	947	rBV	1311931	2172695	35.71%	3.450%
9	9.340	1003	1012	1025	rBV	1034884	1691084	27.80%	2.686%
10	10.069	1129	1136	1148	rBV	814762	1363251	22.41%	2.165%
11	10.610	1220	1228	1242	rBV	1228545	2093178	34.41%	3.324%
12	10.999	1286	1294	1304	rBV	1395034	2343110	38.52%	3.721%
13	11.134	1309	1317	1337	rBV	1086649	1887589	31.03%	2.998%
14	12.575	1556	1562	1568	rBV3	18904	33886	0.56%	0.054%
15	14.210	1833	1840	1853	rBV	1928134	2675505	43.98%	4.249%
16	14.504	1882	1890	1906	rBV	2436272	3544814	58.27%	5.629%
17	14.810	1934	1942	1953	rBV	1928428	2784726	45.78%	4.422%
18	14.987	1964	1972	1989	rBV	754145	1251960	20.58%	1.988%
19	15.798	2104	2110	2123	rBV	2796975	4095167	67.32%	6.503%
20	15.916	2123	2130	2141	rVV	797616	1110633	18.26%	1.764%
21	16.040	2147	2151	2156	rVB4	13939	22578	0.37%	0.036%
22	17.351	2370	2374	2378	rBV3	6421	9902	0.16%	0.016%
23	17.563	2403	2410	2420	rBV	2225460	3243691	53.32%	5.151%
24	17.663	2420	2427	2439	rVV2	3118774	4485657	73.74%	7.124%
25	17.810	2449	2452	2462	rBV2	8866	21557	0.35%	0.034%
26	19.457	2729	2732	2736	rVB3	41124	52968	0.87%	0.084%
27	19.528	2740	2744	2750	rVV	37850	56625	0.93%	0.090%
28	19.881	2798	2804	2811	rBV	4309099	5580833	91.74%	8.863%
29	21.645	3099	3104	3111	rBV	2659828	3669289	60.32%	5.827%
30	24.074	3509	3517	3530	rBV2	2861344	6083428	100.00%	9.661%
31	24.245	3539	3546	3559	rVB2	1897193	4115441	67.65%	6.536%




Sum of corrected areas: 62969732

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050423\
Data File : BP014958.D
Acq On : 04 May 2023 18:20
Operator : CG/JU
Sample : PB152461BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

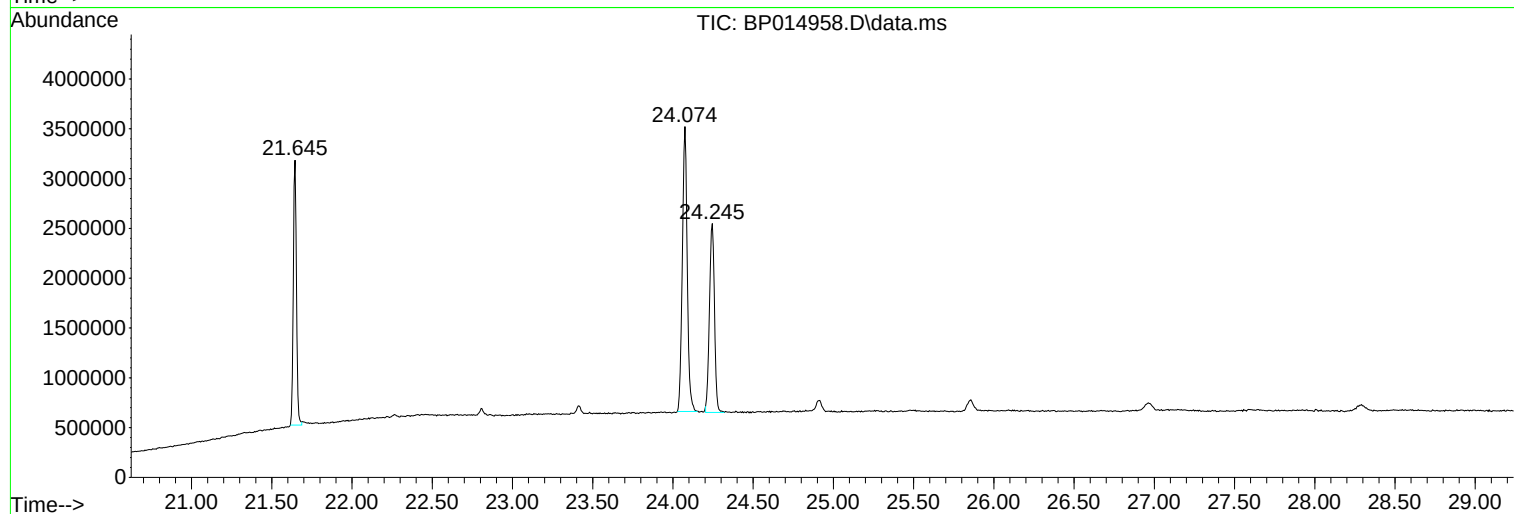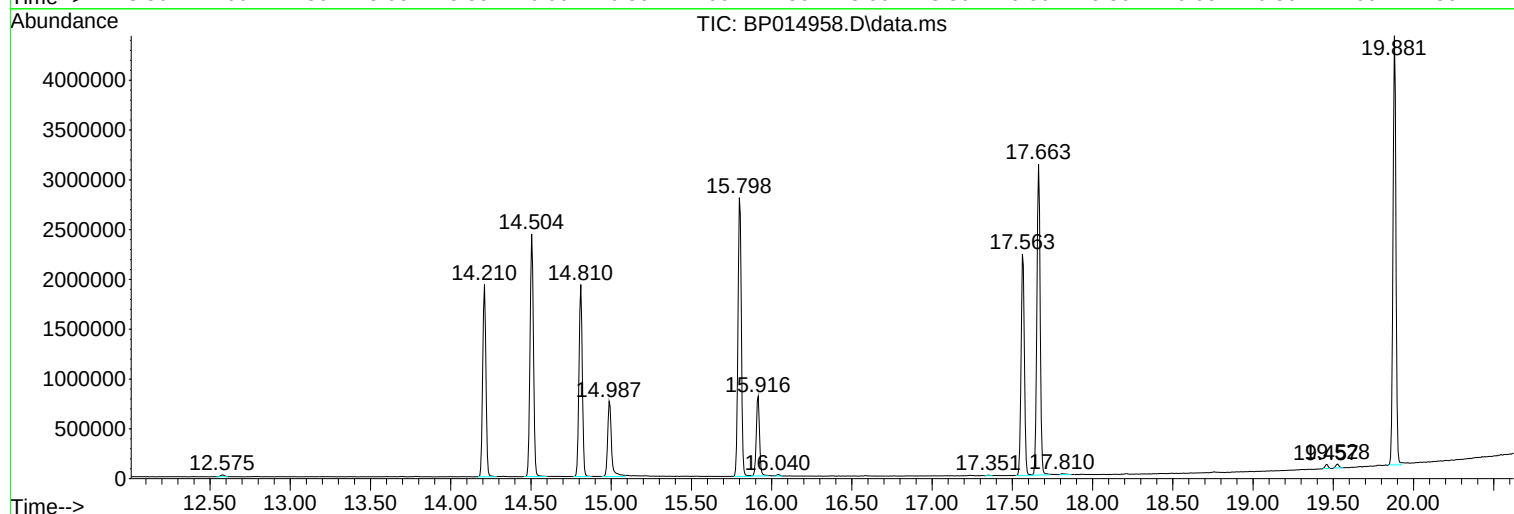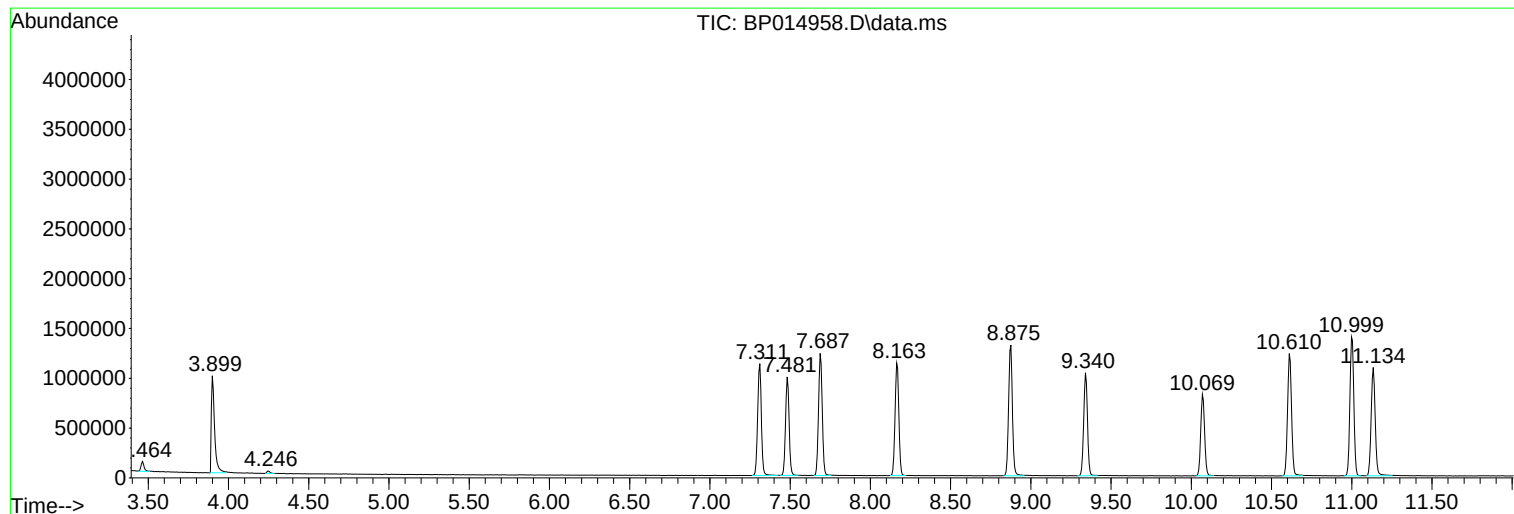

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050423\
Data File : BP014958.D
Acq On : 04 May 2023 18:20
Operator : CG/JU
Sample : PB152461BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050423\
Data File : BP014958.D
Acq On : 04 May 2023 18:20
Operator : CG/JU
Sample : PB152461BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc