
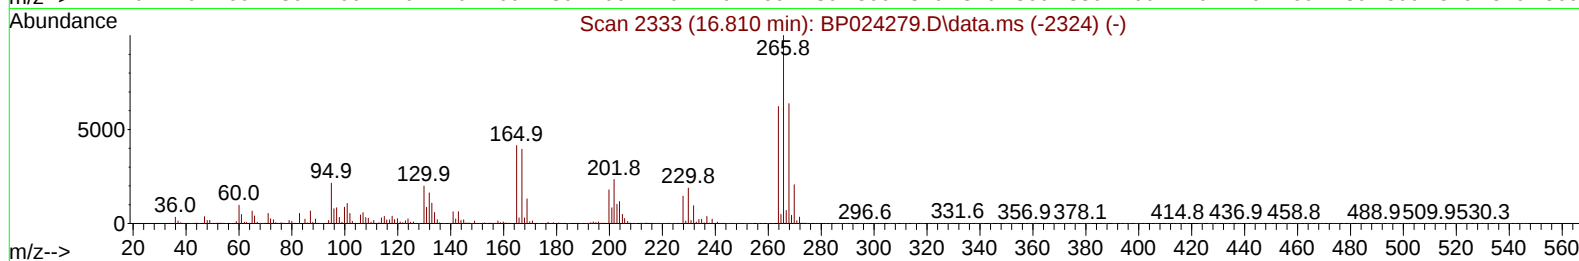
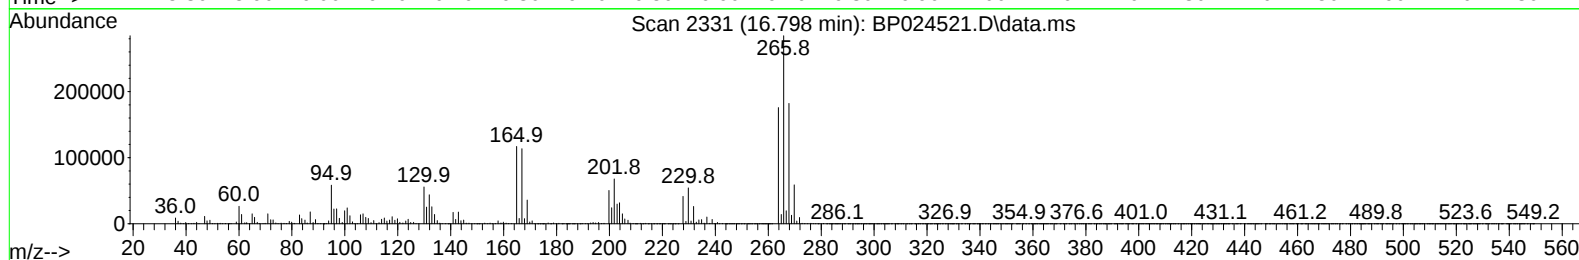


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050525\
Data File : BP024521.D
Acq On : 05 May 2025 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 13:04:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

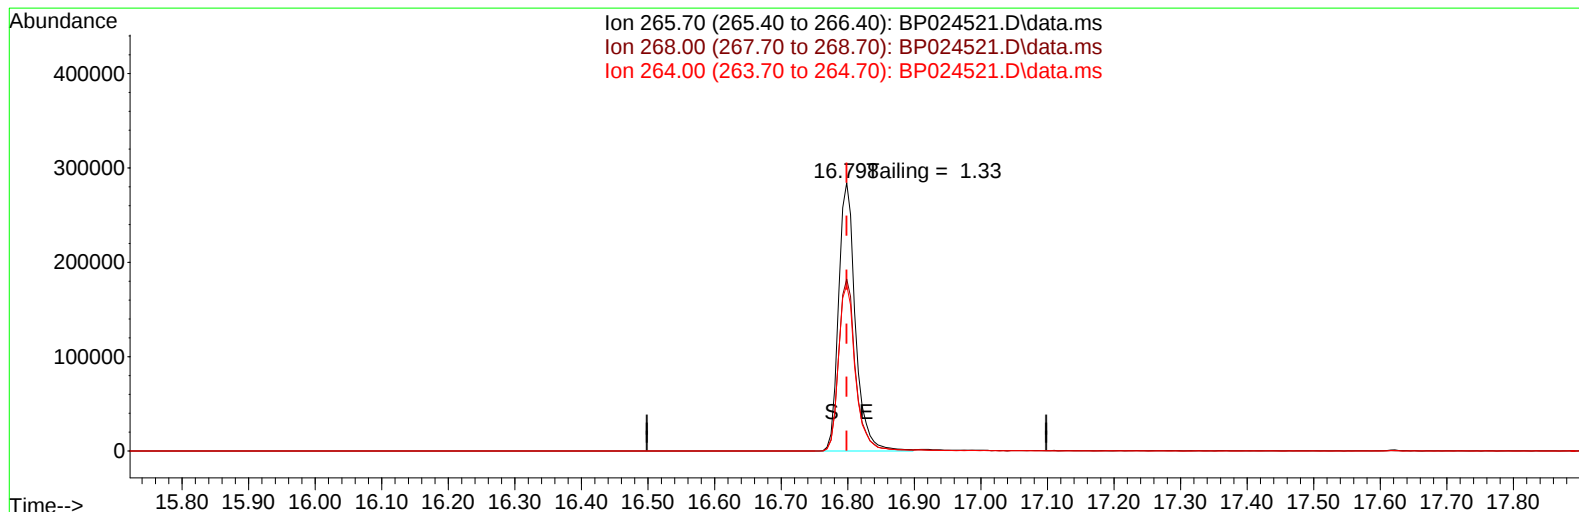

TIC: BP024521.D\data.ms

(70) Pentachlorophenol (C)




16.798min (+ 0.000) 40429.31 ng

response **499235**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.03
264.00	62.20	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050525\
Data File : BP024521.D
Acq On : 05 May 2025 11:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 13:04:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

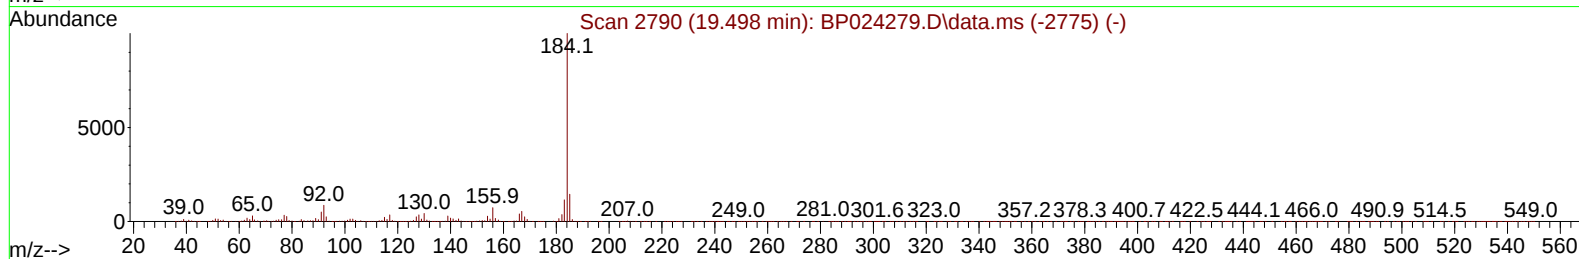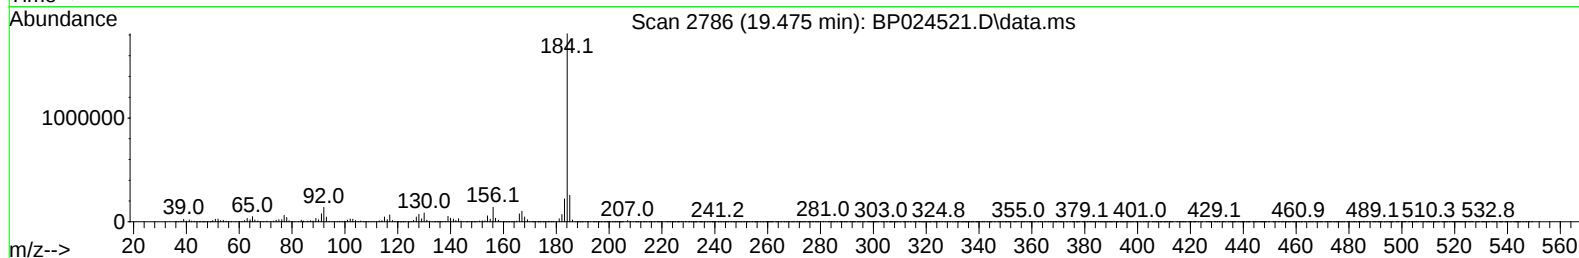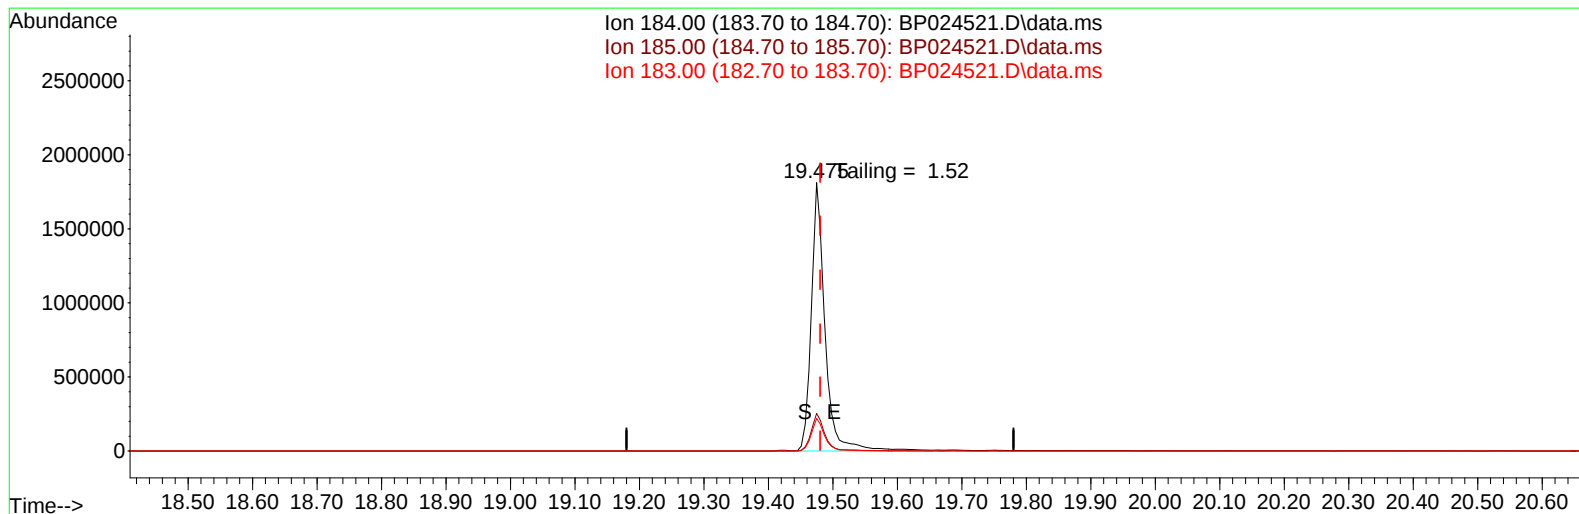

TIC: BP024521.D\data.ms

(77) Benzidine**19.475min (-0.006) 48141.36 ng****response 2700279**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.03
183.00	11.50	12.14
0.00	0.00	0.00