
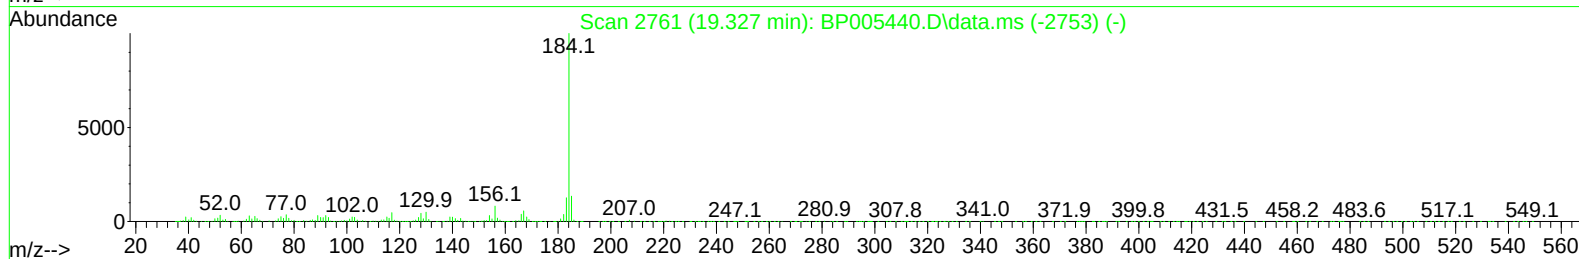
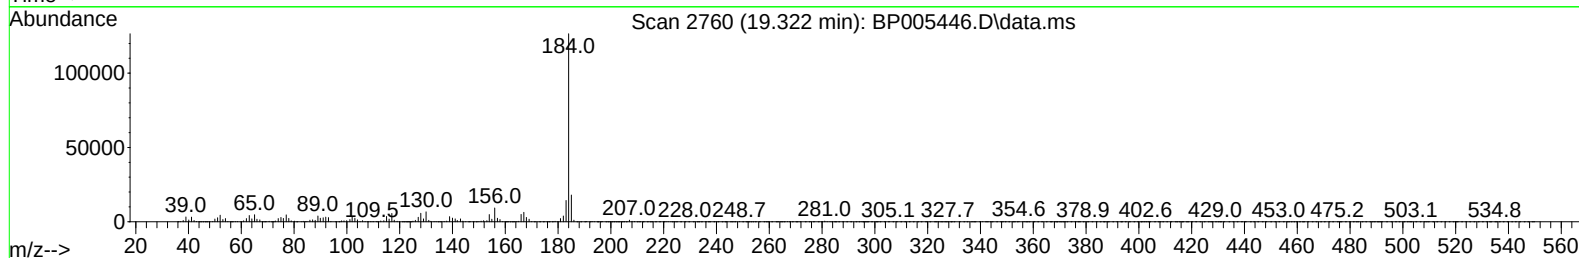


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
 Data File : BP005446.D
 Acq On : 06 May 2021 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 12:09:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 19:00:25 2021
 Response via : Initial Calibration

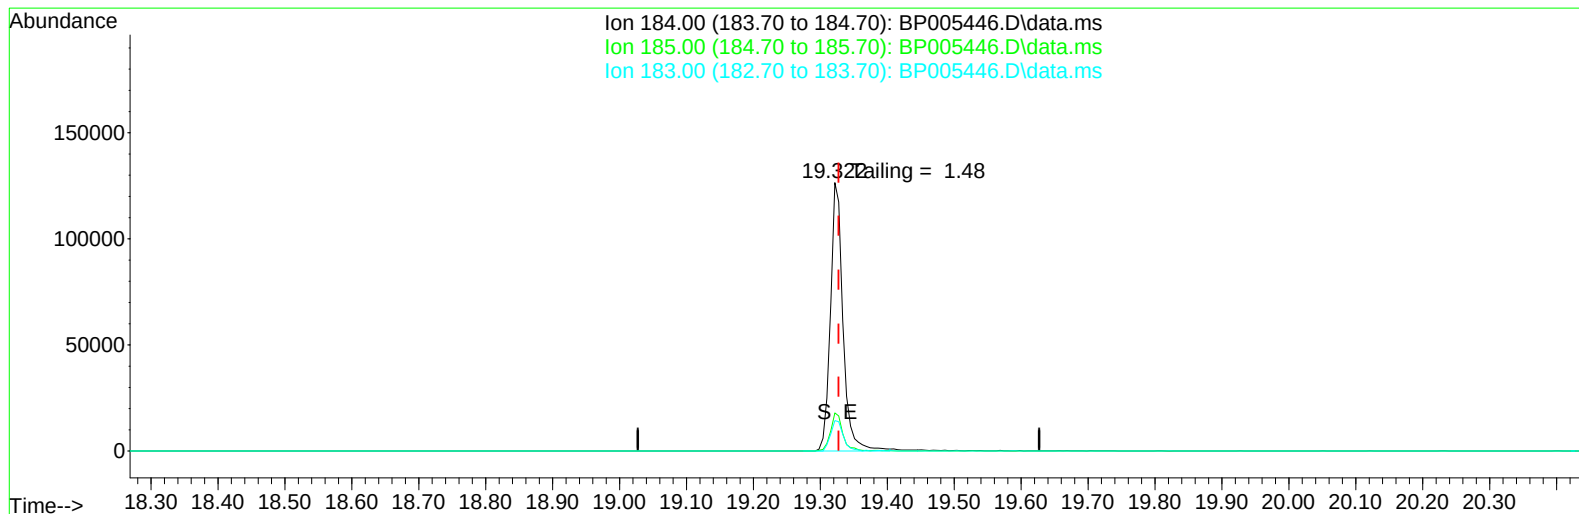




TIC: BP005446.D\data.ms

(77) Benzidine**19.322min (-0.006) 564997.33 ng****response 166164**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.19
183.00	12.30	11.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
Data File : BP005446.D
Acq On : 06 May 2021 11:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 12:09:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 19:00:25 2021
Response via : Initial Calibration

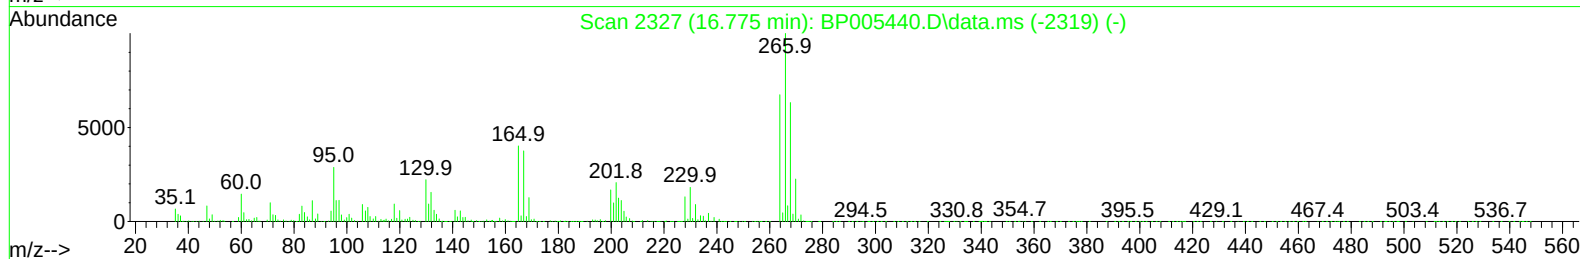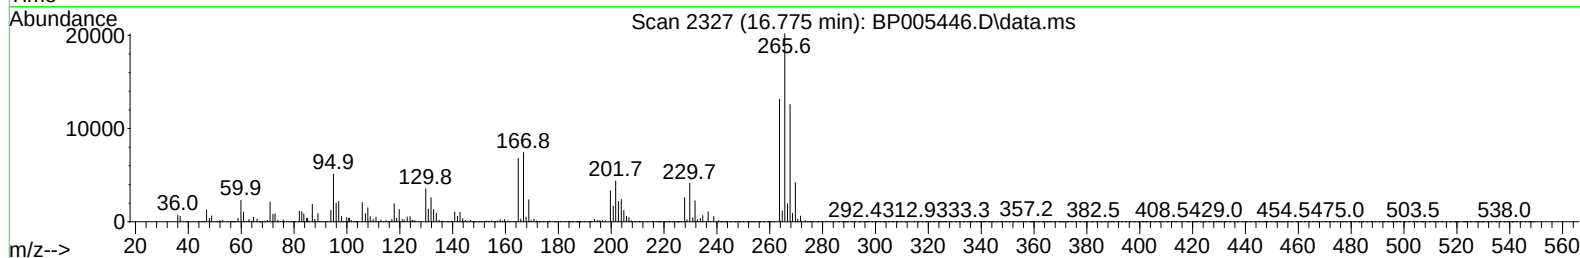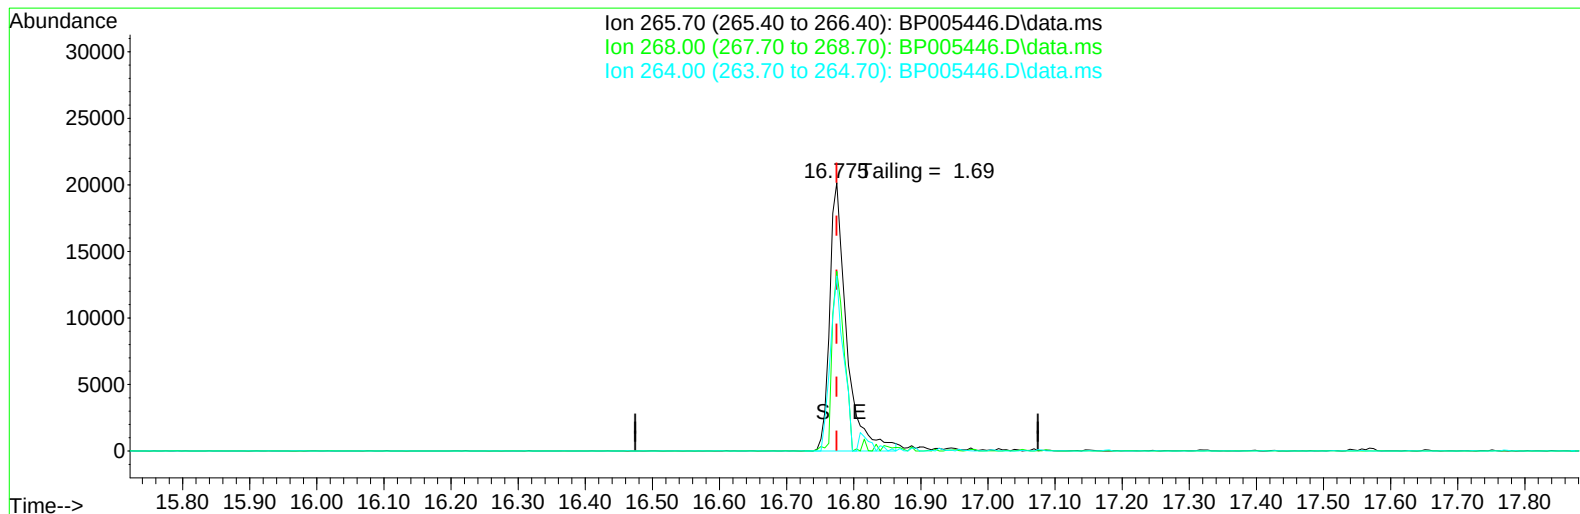

TIC: BP005446.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 566300.65 ng

response 35689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.93
264.00	67.10	71.00
0.00	0.00	0.00