

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
 Data File : BP005448.D
 Acq On : 06 May 2021 12:36
 Operator : CG/JU
 Sample : PB136120BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136120BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.305	371	377	393	rBV	304801	428278	30.03%	8.638%
2	6.905	641	649	664	rBV	251206	401898	28.18%	8.106%
3	7.716	780	787	795	rBV	58278	92070	6.46%	1.857%
4	8.881	978	985	997	rBV	156087	268064	18.80%	5.407%
5	10.510	1255	1262	1277	rBV	53437	99567	6.98%	2.008%
6	12.981	1674	1682	1692	rBV	457190	689998	48.38%	13.917%
7	14.363	1909	1917	1926	rBV	88199	136176	9.55%	2.747%
8	15.857	2161	2171	2192	rBV	456505	695993	48.81%	14.038%
9	17.116	2376	2385	2399	rBV	108282	175516	12.31%	3.540%
10	19.686	2816	2822	2829	rBV	1293594	1426062	100.00%	28.763%
11	21.210	3077	3081	3093	rBV	186393	254595	17.85%	5.135%
12	23.527	3469	3475	3485	rBV	142179	289672	20.31%	5.843%




Sum of corrected areas: 4957889

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
Data File : BP005448.D
Acq On : 06 May 2021 12:36
Operator : CG/JU
Sample : PB136120BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136120BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

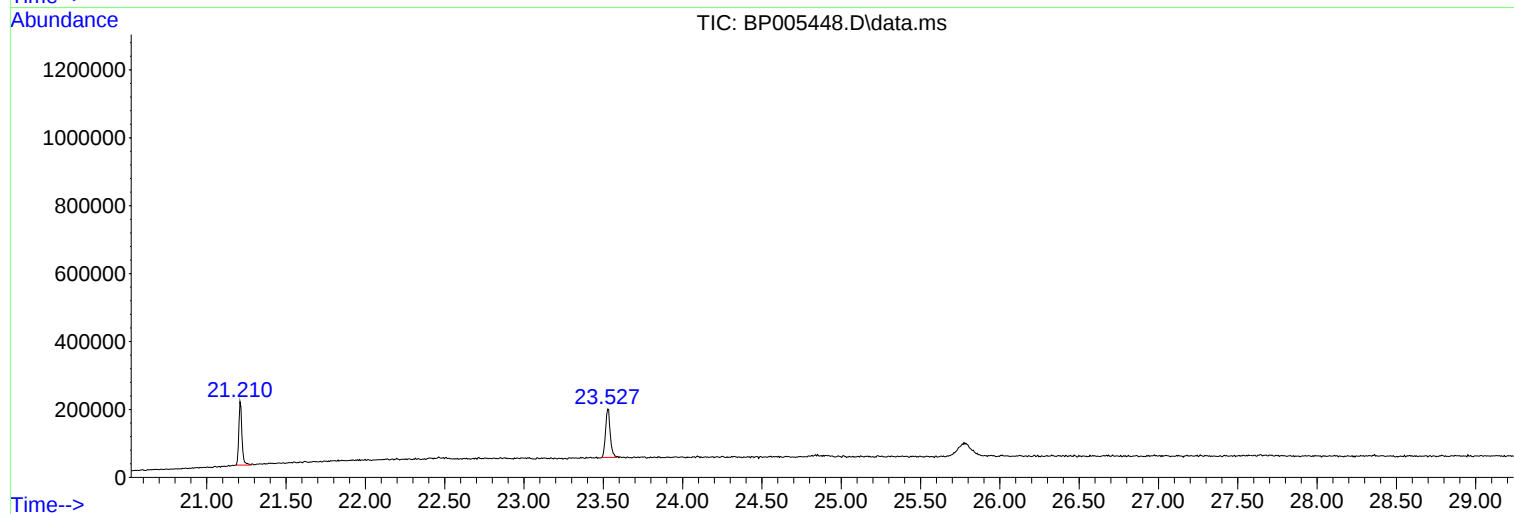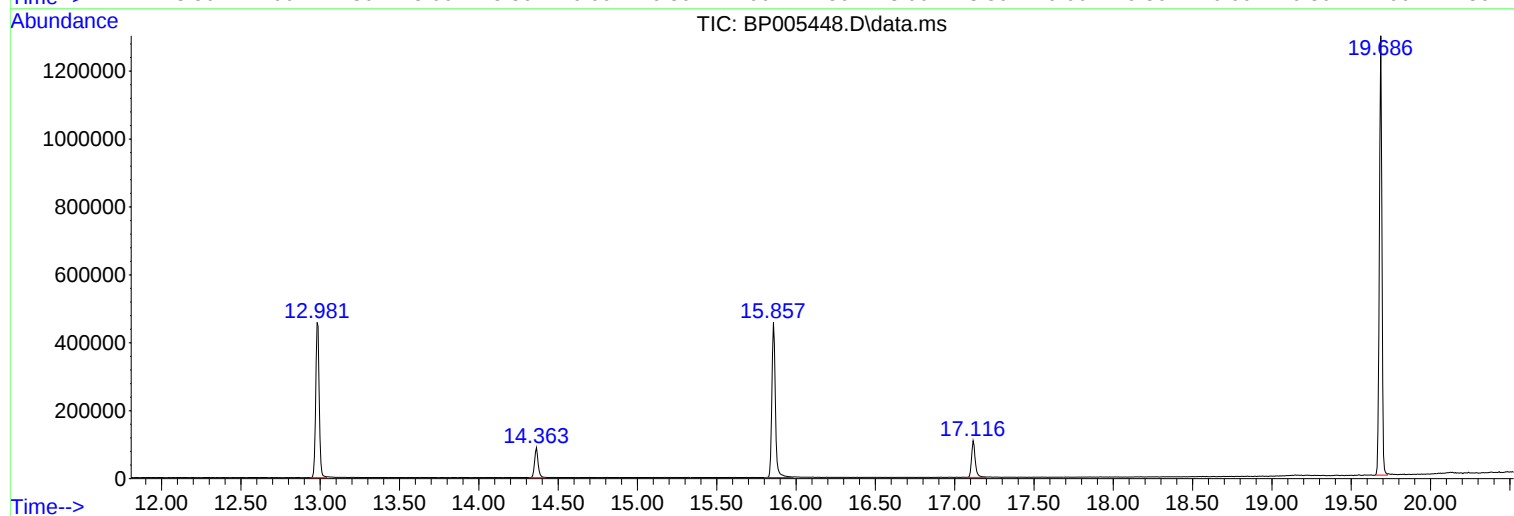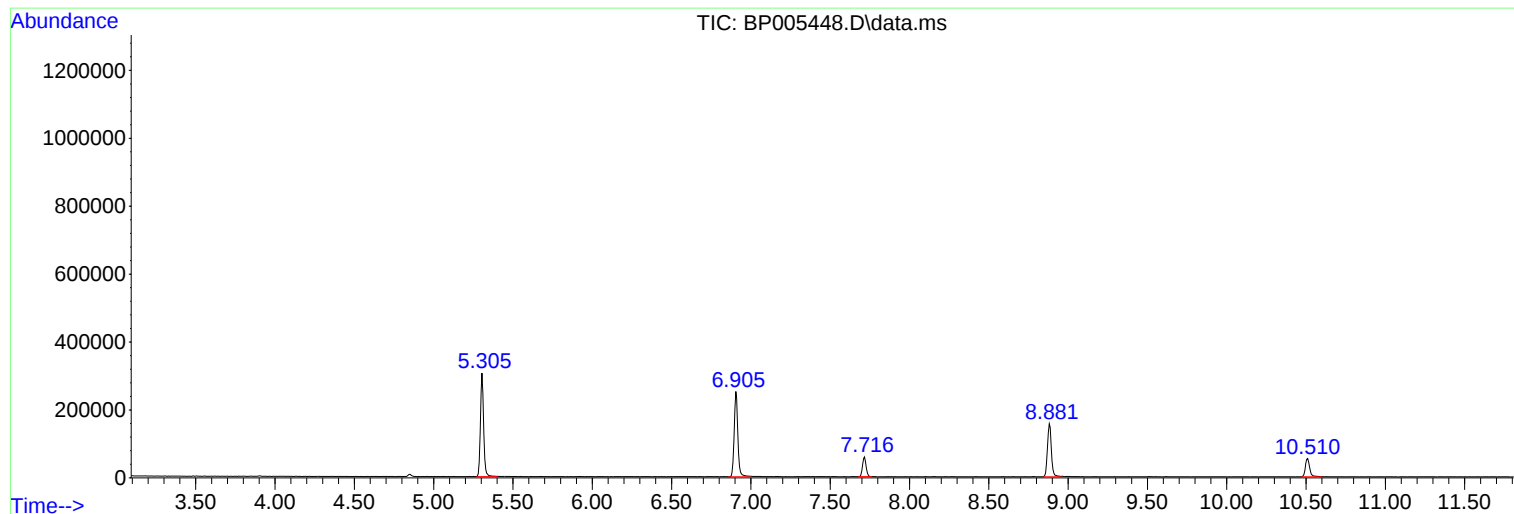

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
Data File : BP005448.D
Acq On : 06 May 2021 12:36
Operator : CG/JU
Sample : PB136120BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136120BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
Data File : BP005448.D
Acq On : 06 May 2021 12:36
Operator : CG/JU
Sample : PB136120BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136120BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------