
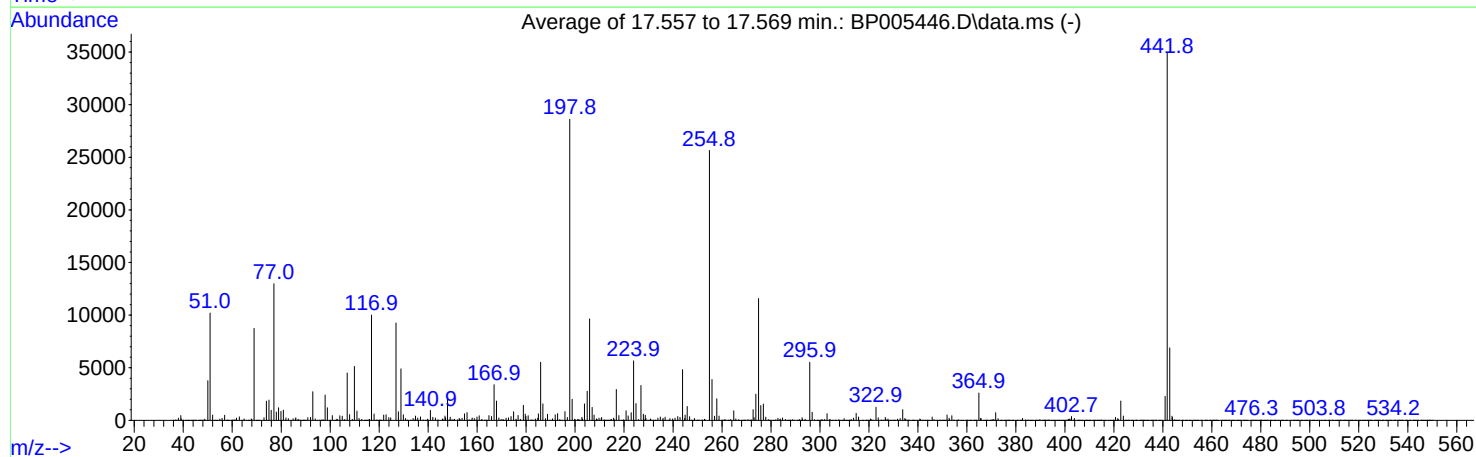


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
 Data File : BP005446.D
 Acq On : 06 May 2021 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 07 12:37:06 2021

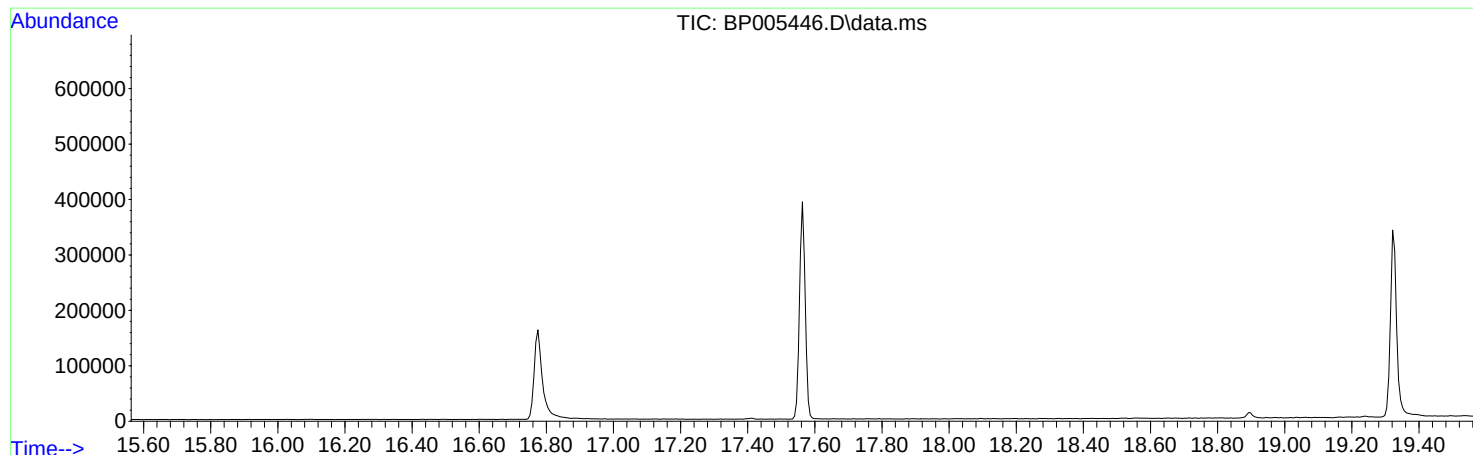




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	10207	PASS
68	69	0.00	2	1.5	134	PASS
69	198	0.00	100	30.5	8739	PASS
70	69	0.00	2	0.1	10	PASS
127	198	10	80	32.3	9254	PASS
197	198	0.00	2	1.0	281	PASS
198	198	100	100	100.0	28616	PASS
199	198	5	9	7.0	2009	PASS
275	198	10	60	40.4	11566	PASS
365	198	1	100	9.1	2596	PASS
441	198	0.01	100	8.0	2276	PASS
442	442	100	100	100.0	34955	PASS
443	442	15	24	19.7	6895	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
 Data File : BP005446.D
 Acq On : 06 May 2021 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 06 12:09:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 19:00:25 2021
 Response via : Initial Calibration

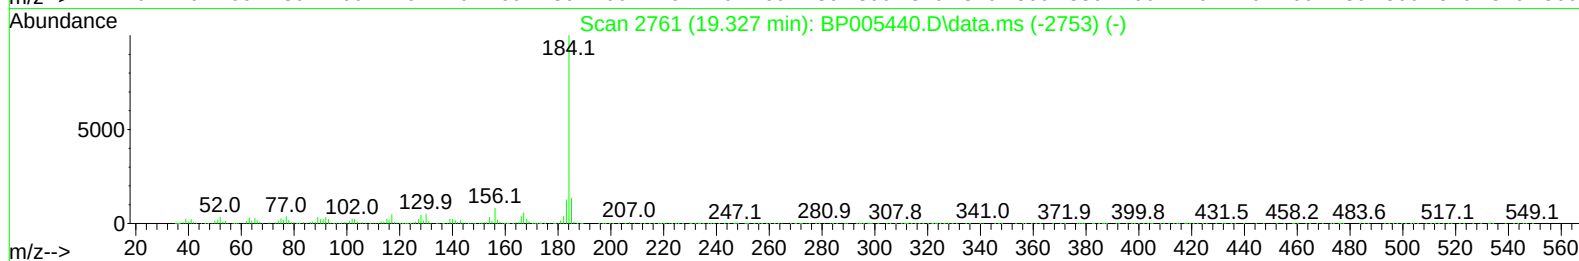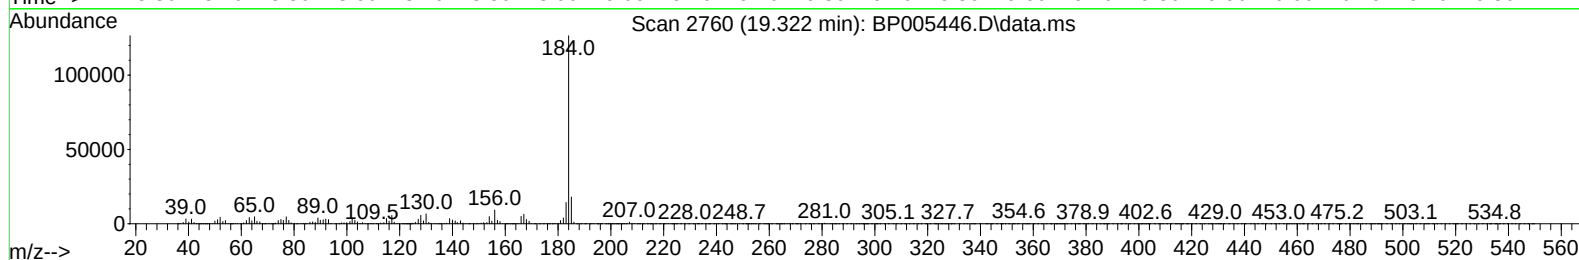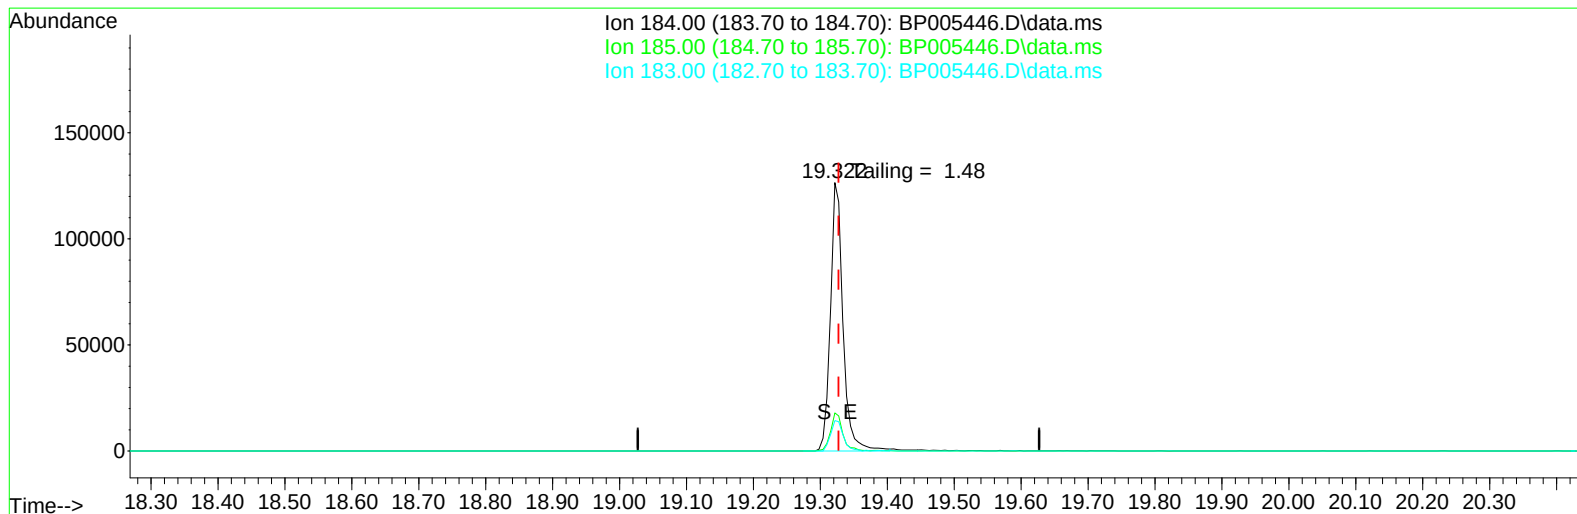

TIC: BP005446.D\data.ms

(77) Benzidine

19.322min (-0.006) 564997.33 ng




response 166164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.19
183.00	12.30	11.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050621\
 Data File : BP005446.D
 Acq On : 06 May 2021 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 06 12:09:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 19:00:25 2021
 Response via : Initial Calibration

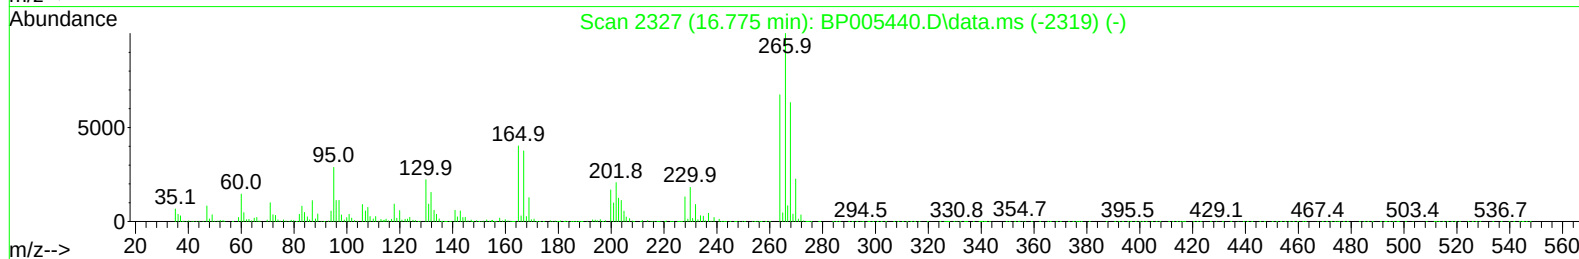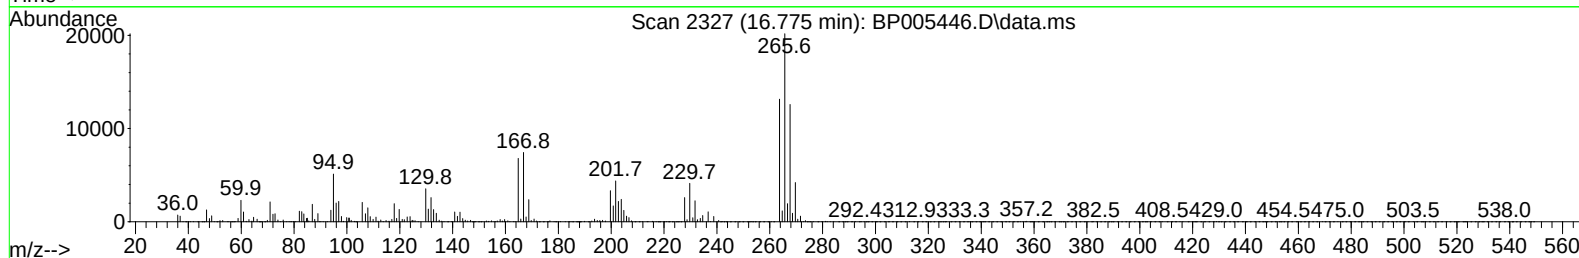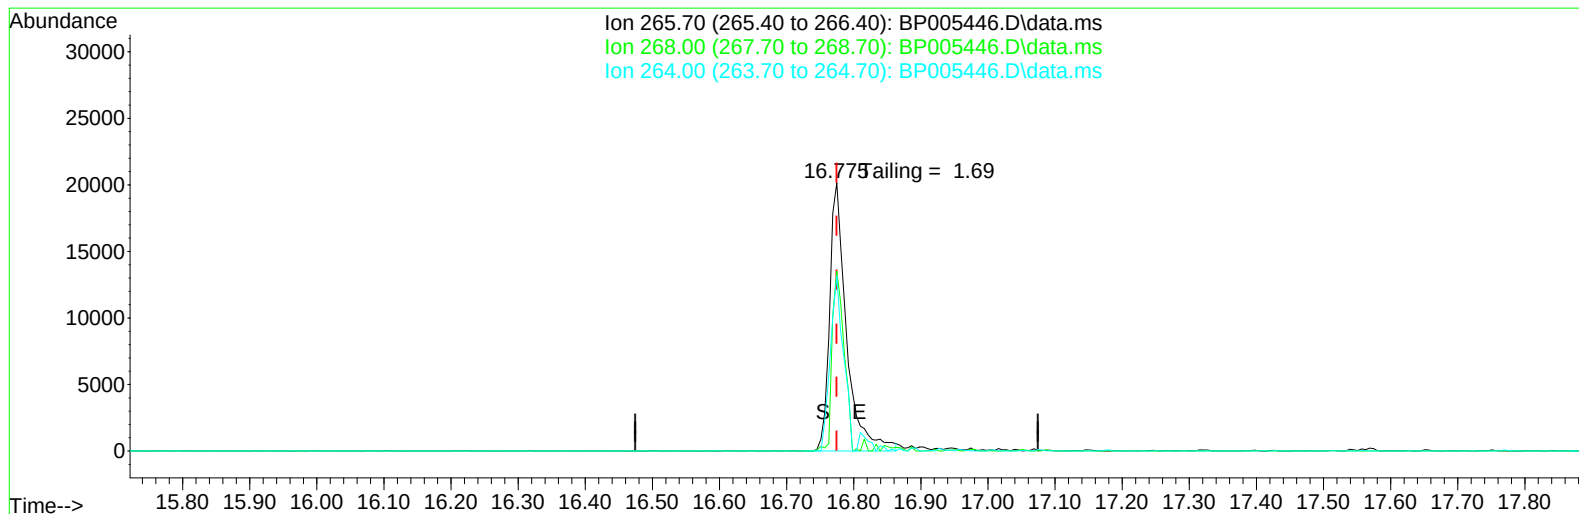

TIC: BP005446.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 566300.65 ng

response 35689

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	66.93
264.00	67.10	71.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2021	BNA_P	BP005446.D
Compound Name	Response	Retention Time
DDT	124933	20.51
DDD	732	20.09
DDE	393	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1125	126058	0.89