

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020212.D
 Acq On : 06 May 2024 18:48
 Operator : MA/JU
 Sample : P2373-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y1

Quant Time: May 06 22:44:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	73105	20.000	ng/ul	0.02
20) Naphthalene-d8	10.393	136	304676	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.304	164	211602	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	441230	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	320555	20.000	ng/ul	0.00
88) Perylene-d12	24.998	264	352716	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	8773	5.068	ng/uL	0.00
4) Pyridine-d5	3.634	84	30989	6.161	ng/ul	0.03
7) Phenol-d5	6.822	99	41721	6.645	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	6.981	67	134933	35.380	ng/ul	0.03
11) 2-Chlorophenol-d4	7.164	132	124829	27.813	ng/ul	0.02
15) 4-Methylphenol-d8	8.334	113	83921	16.534	ng/ul	0.02
21) Nitrobenzene-d5	8.787	128	83504	36.601	ng/ul	0.03
24) 2-Nitrophenol-d4	9.493	143	91041	34.846	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.034	165	148243	31.093	ng/ul	0.02
31) 4-Chloroaniline-d4	10.557	131	200945	30.114	ng/ul	0.02
46) Dimethylphthalate-d6	13.710	166	611157	39.551	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160	633016	37.084	ng/ul	0.00
54) 4-Nitrophenol-d4	14.563	143	11	0.005	ng/ul	0.02
60) Fluorene-d10	15.322	176	501794	38.933	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	88845	31.731	ng/ul	0.00
73) Anthracene-d10	17.245	188	843328	44.181	ng/ul	0.00
81) Pyrene-d10	19.645	212	904054	48.247	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.763	264	773747	45.370	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.746	107	6921	1.199	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020212.D
Acq On : 06 May 2024 18:48
Operator : MA/JU
Sample : P2373-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43Y1

Quant Time: May 06 22:44:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

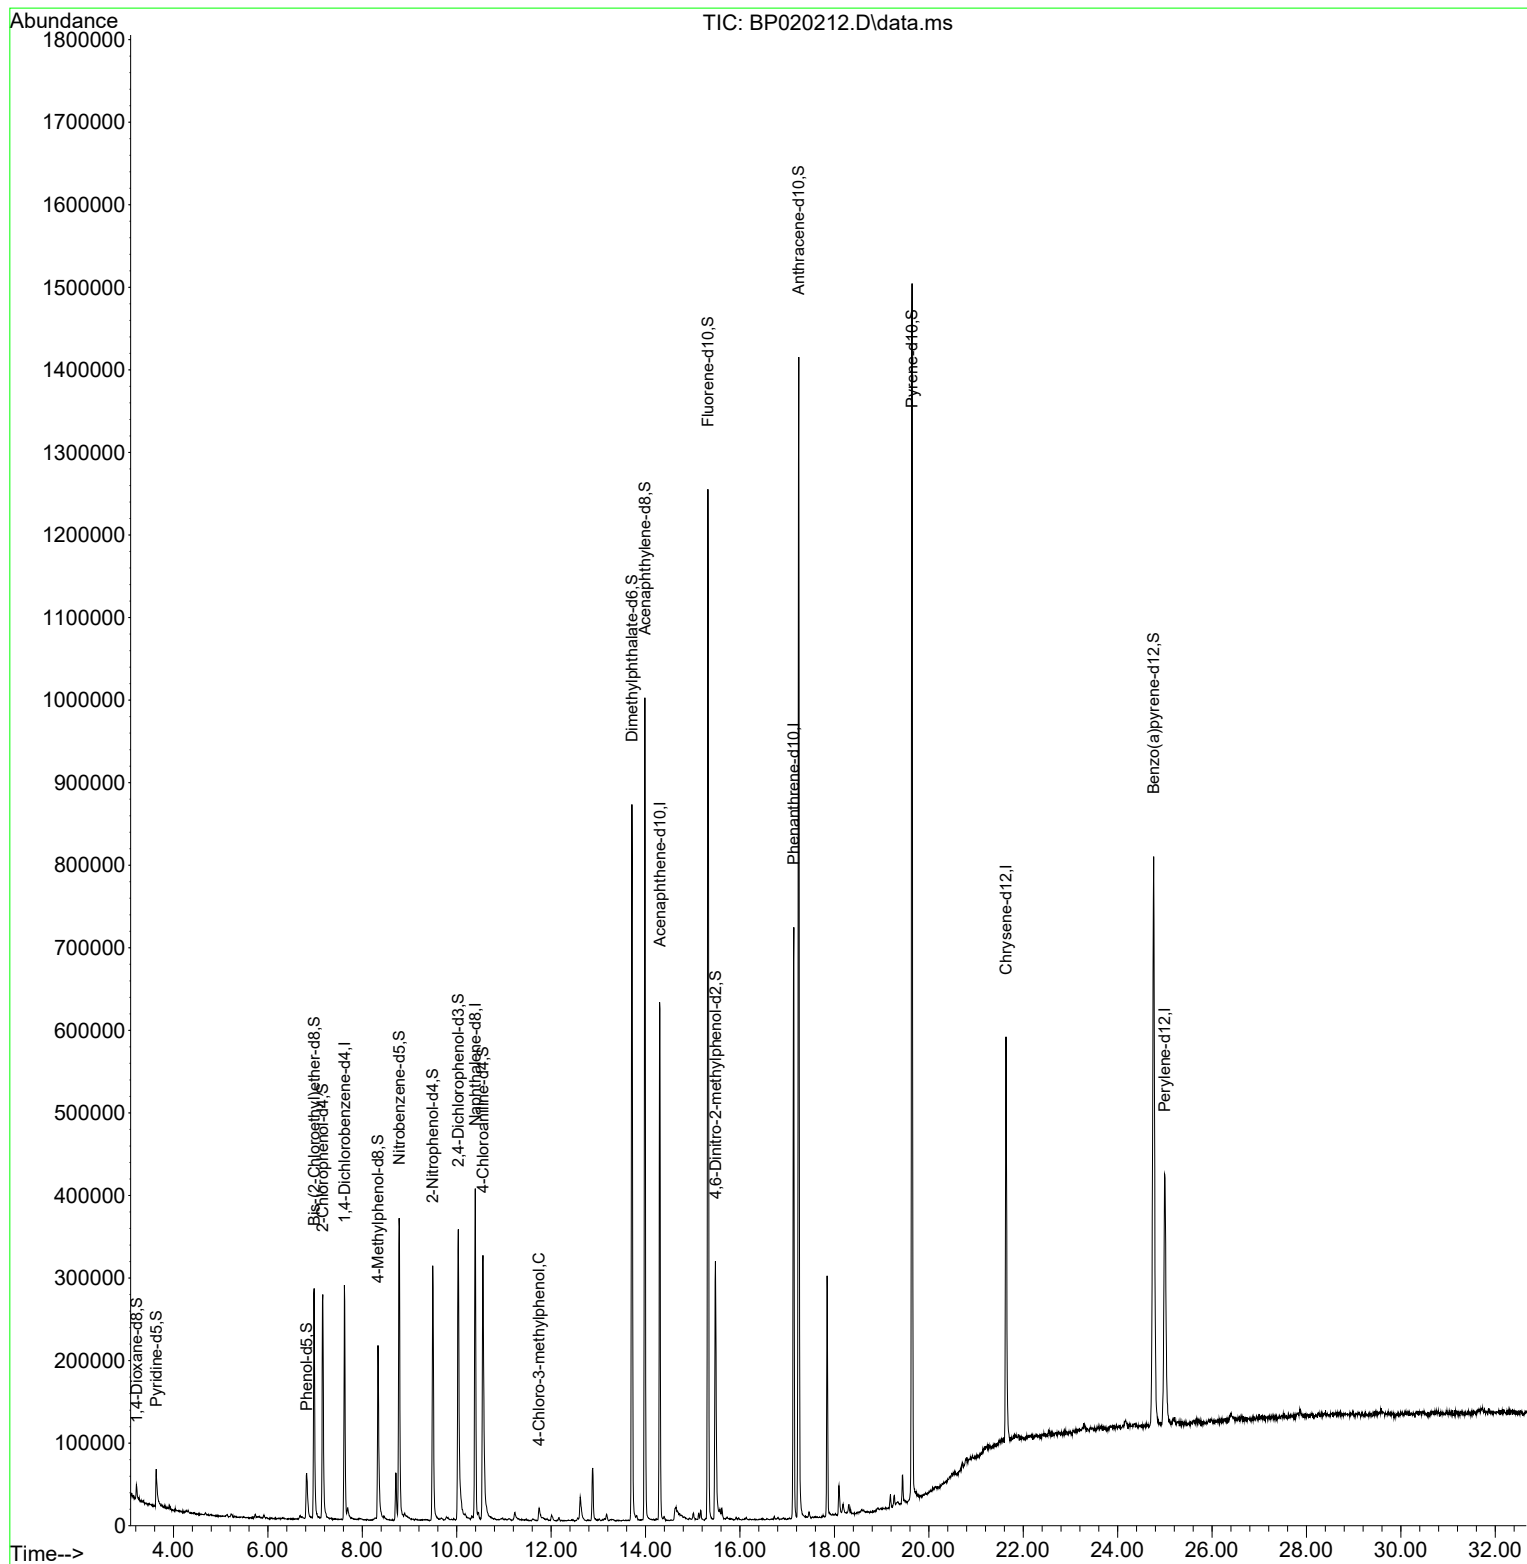

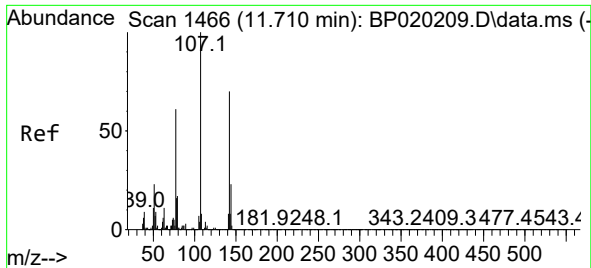

#35
 4-Chloro-3-methylphenol
 Concen: 1.199 ng/ul
 RT: 11.746 min Scan# 14
 Delta R.T. 0.053 min
 Lab File: BP020212.D
 Acq: 06 May 2024 18:48

Instrument :
 BNA_P
 ClientSampleId :
 A43Y1

Tgt Ion:107 Resp: 6921
 Ion Ratio Lower Upper
 107 100
 144 22.2 18.3 27.5
 142 65.7 56.6 84.8

