




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020212.D
 Acq On : 06 May 2024 18:48
 Operator : MA/JU
 Sample : P2373-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y1

Manual IntegrationsAPPROVED

Quant Time: May 06 22:48:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

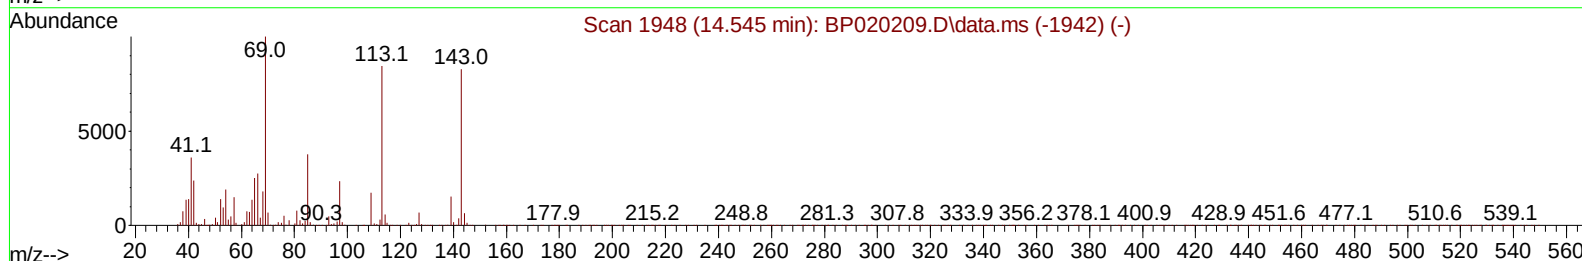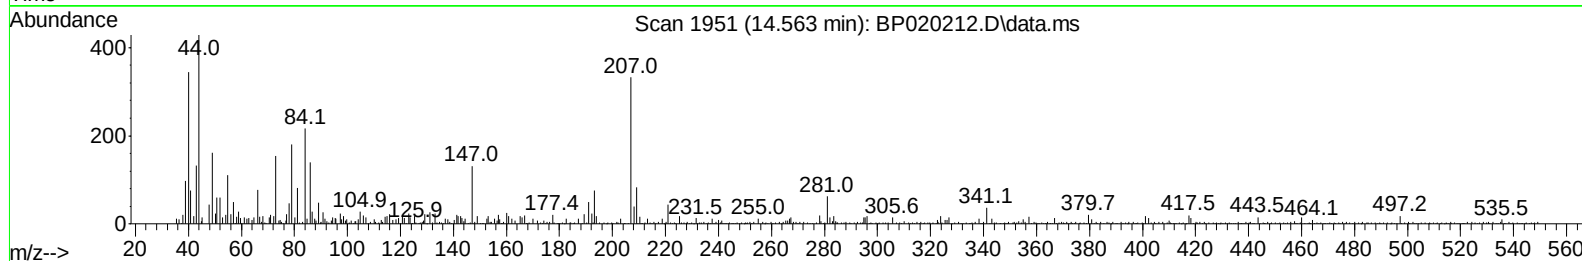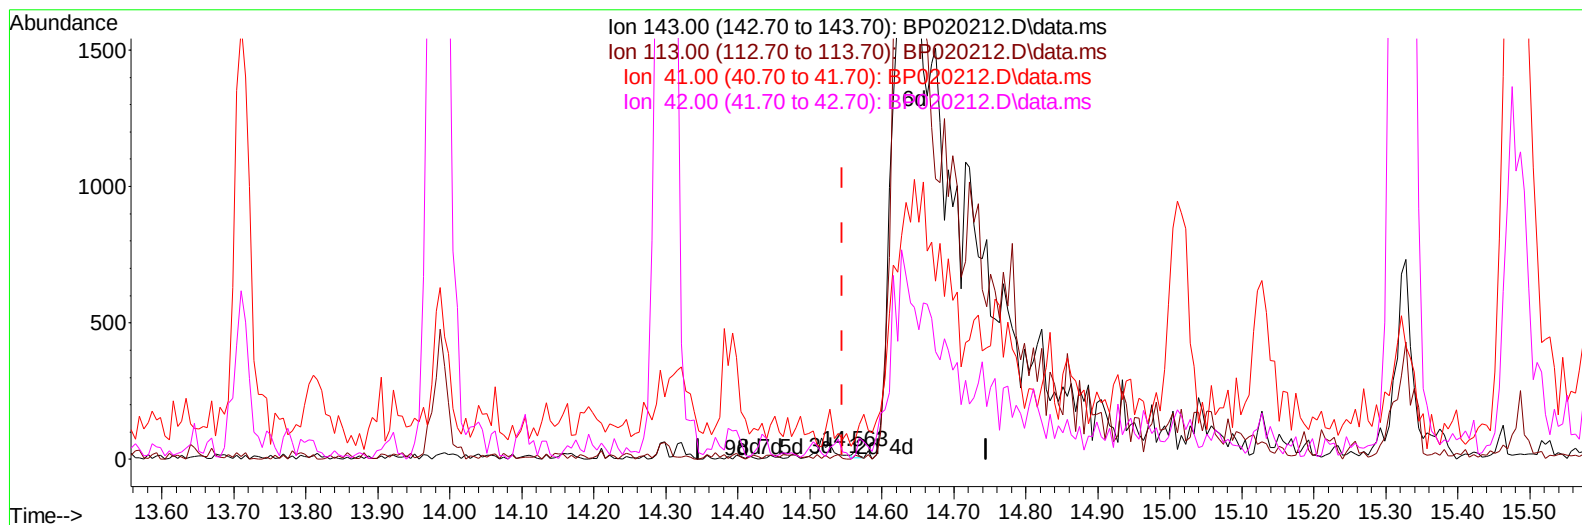

TIC: BP020212.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.563min (+ 0.018) 0.00 ng/ul

response 11

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	45.16#
41.00	50.30	241.94#
42.00	32.50	54.84#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020212.D
 Acq On : 06 May 2024 18:48
 Operator : MA/JU
 Sample : P2373-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y1

Manual IntegrationsAPPROVED

Quant Time: May 07 05:44:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

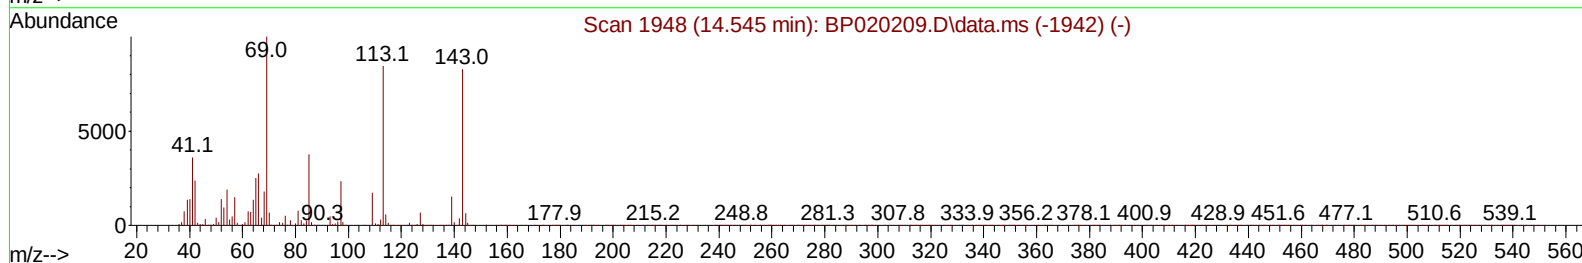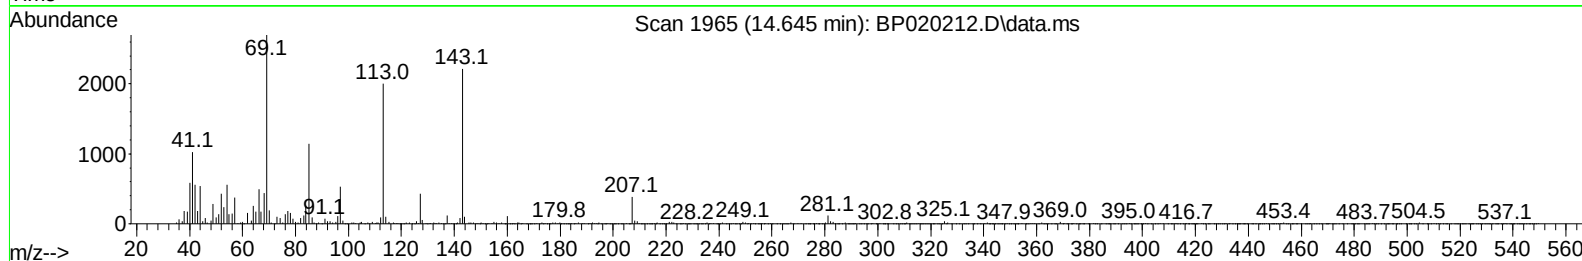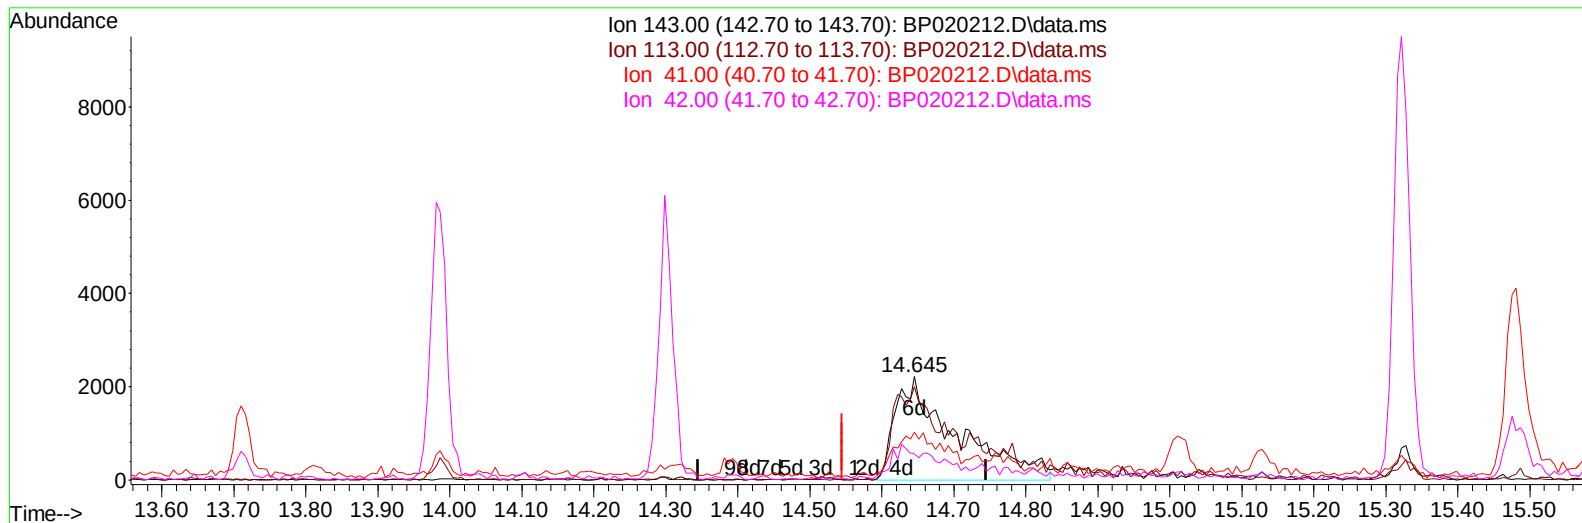

TIC: BP020212.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.645min (+ 0.100) 5.49 ng/ul m

response 13036

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	90.17
41.00	50.30	46.28
42.00	32.50	25.17#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020212.D
 Acq On : 06 May 2024 18:48
 Operator : MA/JU
 Sample : P2373-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 05:48:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	73105	20.000	ng/ul	0.02
20) Naphthalene-d8	10.393	136	304676	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.304	164	211602	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	441230	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	320555	20.000	ng/ul	0.00
88) Perylene-d12	24.998	264	352716	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	8773	5.068	ng/uL	0.00
4) Pyridine-d5	3.634	84	30989	6.161	ng/ul	0.03
7) Phenol-d5	6.822	99	41721	6.645	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	6.981	67	134933	35.380	ng/ul	0.03
11) 2-Chlorophenol-d4	7.164	132	124829	27.813	ng/ul	0.02
15) 4-Methylphenol-d8	8.334	113	83921	16.534	ng/ul	0.02
21) Nitrobenzene-d5	8.787	128	83504	36.601	ng/ul	0.03
24) 2-Nitrophenol-d4	9.493	143	91041	34.846	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.034	165	148243	31.093	ng/ul	0.02
31) 4-Chloroaniline-d4	10.557	131	200945	30.114	ng/ul	0.02
46) Dimethylphthalate-d6	13.710	166	611157	39.551	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160	633016	37.084	ng/ul	0.00
54) 4-Nitrophenol-d4	14.645	143	13036m	5.489	ng/ul	0.10
60) Fluorene-d10	15.322	176	501794	38.933	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	88845	31.731	ng/ul	0.00
73) Anthracene-d10	17.245	188	843328	44.181	ng/ul	0.00
81) Pyrene-d10	19.645	212	904054	48.247	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.763	264	773747	45.370	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020212.D
Acq On : 06 May 2024 18:48
Operator : MA/JU
Sample : P2373-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43Y1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 05:48:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

