




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020218.D
 Acq On : 06 May 2024 23:16
 Operator : MA/JU
 Sample : P2368-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43L4

Manual IntegrationsAPPROVED

Quant Time: May 06 23:44:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

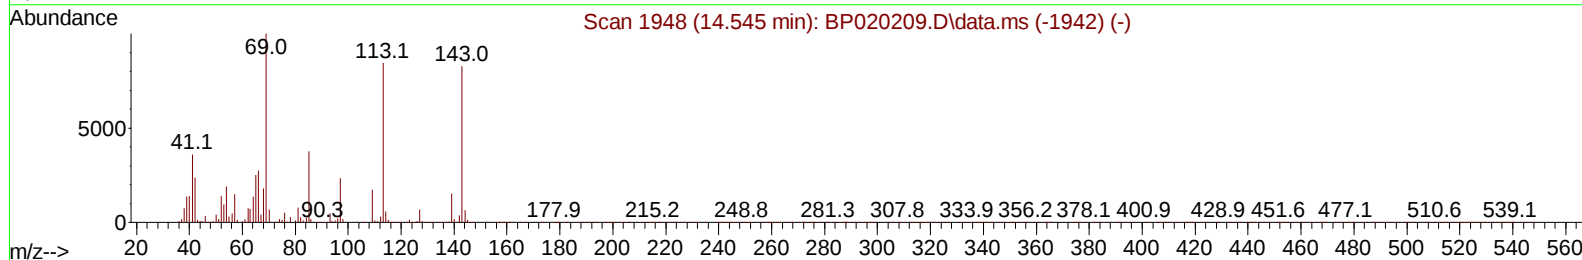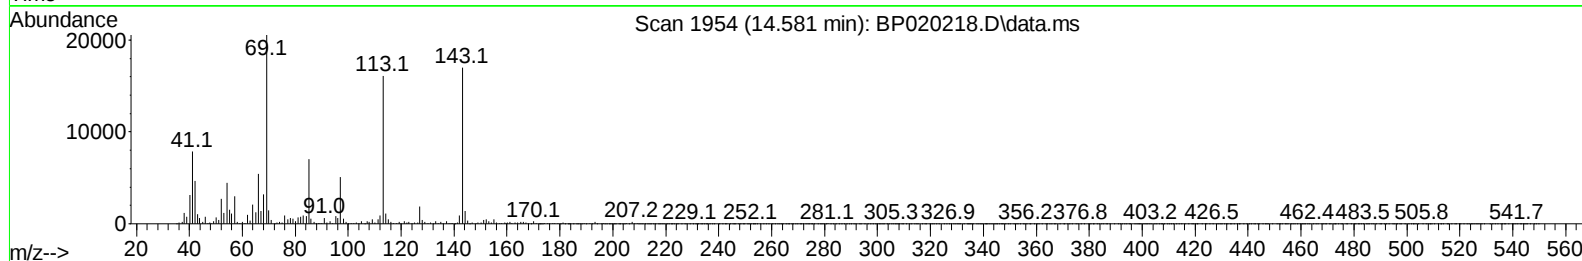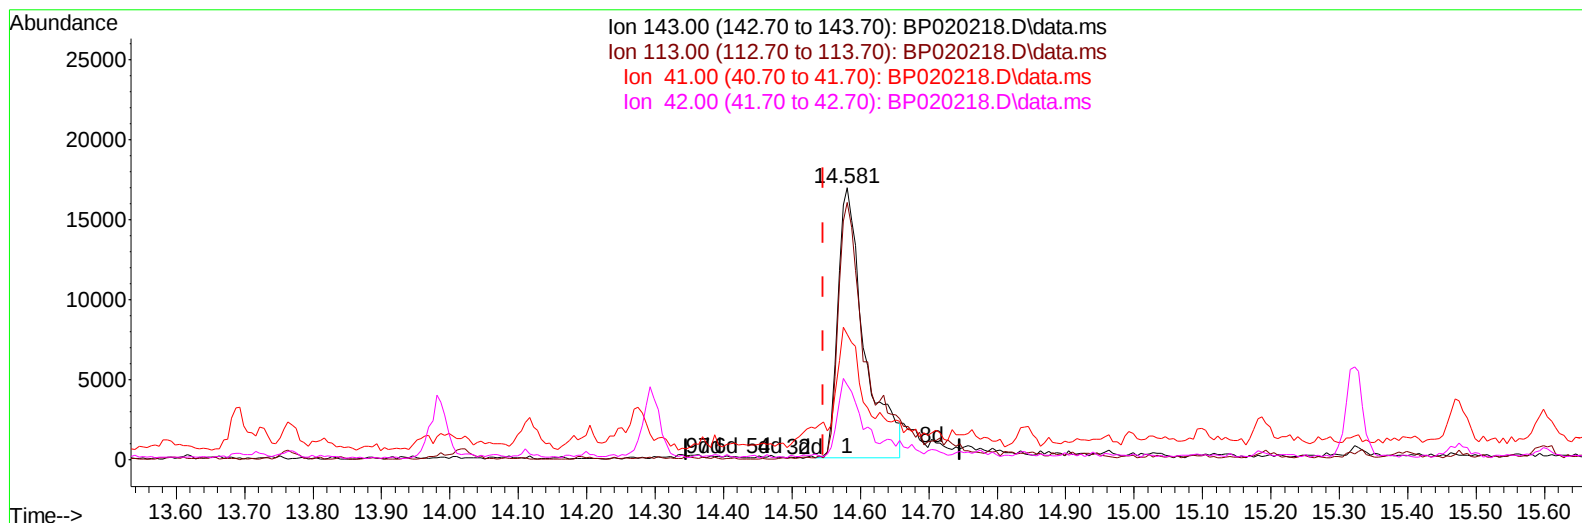

TIC: BP020218.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 19.41 ng/u1

response 45048

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	94.69
41.00	50.30	46.20
42.00	32.50	27.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020218.D
 Acq On : 06 May 2024 23:16
 Operator : MA/JU
 Sample : P2368-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43L4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 03:44:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	90245	20.000	ng/ul	0.02
20) Naphthalene-d8	10.399	136	339216	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.293	164	206827	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.134	188	405816	20.000	ng/ul	0.00
79) Chrysene-d12	21.622	240	444204	20.000	ng/ul	-0.01
88) Perylene-d12	24.980	264	535881	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	8943	4.185	ng/uL	0.00
4) Pyridine-d5	3.623	84	63220	10.182	ng/ul	0.02
7) Phenol-d5	6.805	99	179113	23.111	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.981	67	113330	24.072	ng/ul	0.03
11) 2-Chlorophenol-d4	7.158	132	139403	25.161	ng/ul	0.02
15) 4-Methylphenol-d8	8.334	113	129571	20.679	ng/ul	0.02
21) Nitrobenzene-d5	8.781	128	69205	27.245	ng/ul	0.02
24) 2-Nitrophenol-d4	9.499	143	77052	26.489	ng/ul	0.03
28) 2,4-Dichlorophenol-d3	10.040	165	136324	25.682	ng/ul	0.03
31) 4-Chloroaniline-d4	10.563	131	111189	14.966	ng/ul	0.03
46) Dimethylphthalate-d6	13.722	166	405255	26.831	ng/ul	0.02
49) Acenaphthylene-d8	13.981	160	461030	27.632	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	49564m	21.352	ng/ul	0.04
60) Fluorene-d10	15.322	176	346052	27.469	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	47846	18.580	ng/ul	0.00
73) Anthracene-d10	17.234	188	528221	30.088	ng/ul	0.00
81) Pyrene-d10	19.634	212	683292	26.315	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.751	264	769258	29.689	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020218.D
Acq On : 06 May 2024 23:16
Operator : MA/JU
Sample : P2368-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43L4

Manual IntegrationsAPPROVED

Quant Time: May 07 03:44:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

