




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020219.D
Acq On : 07 May 2024 00:01
Operator : MA/JU
Sample : P2368-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43L6

Manual IntegrationsAPPROVED

Quant Time: May 07 01:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

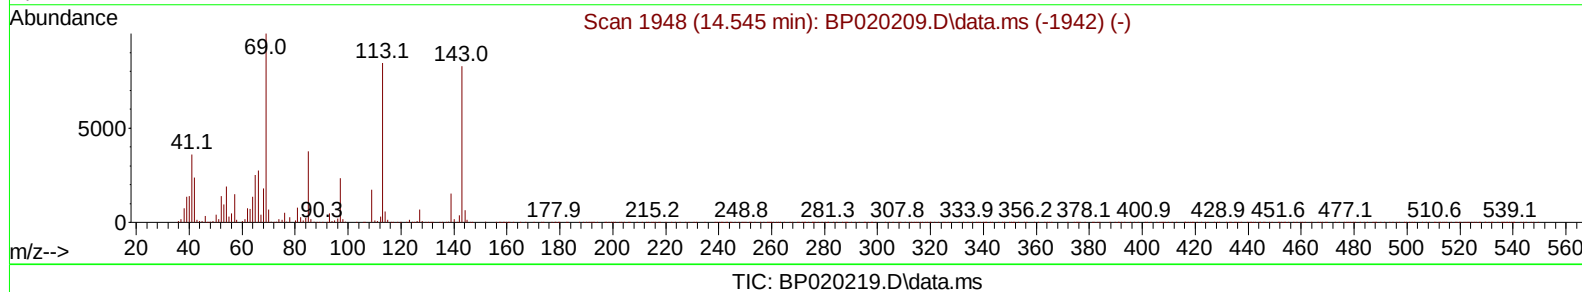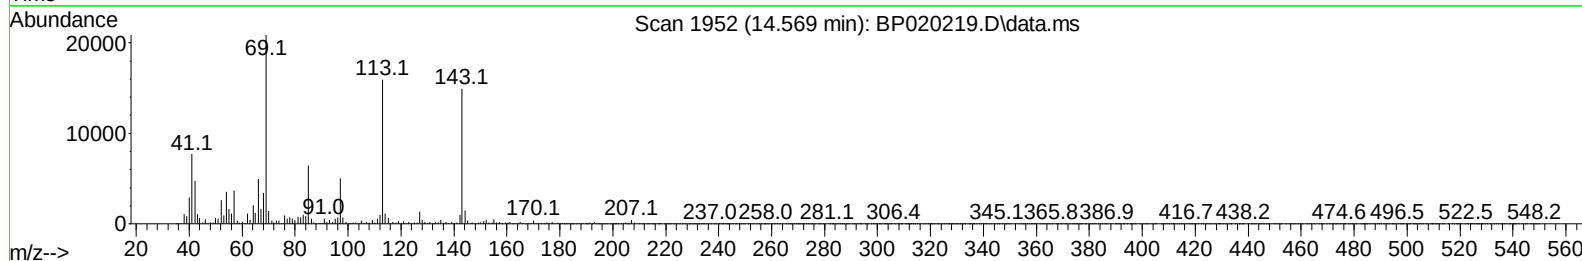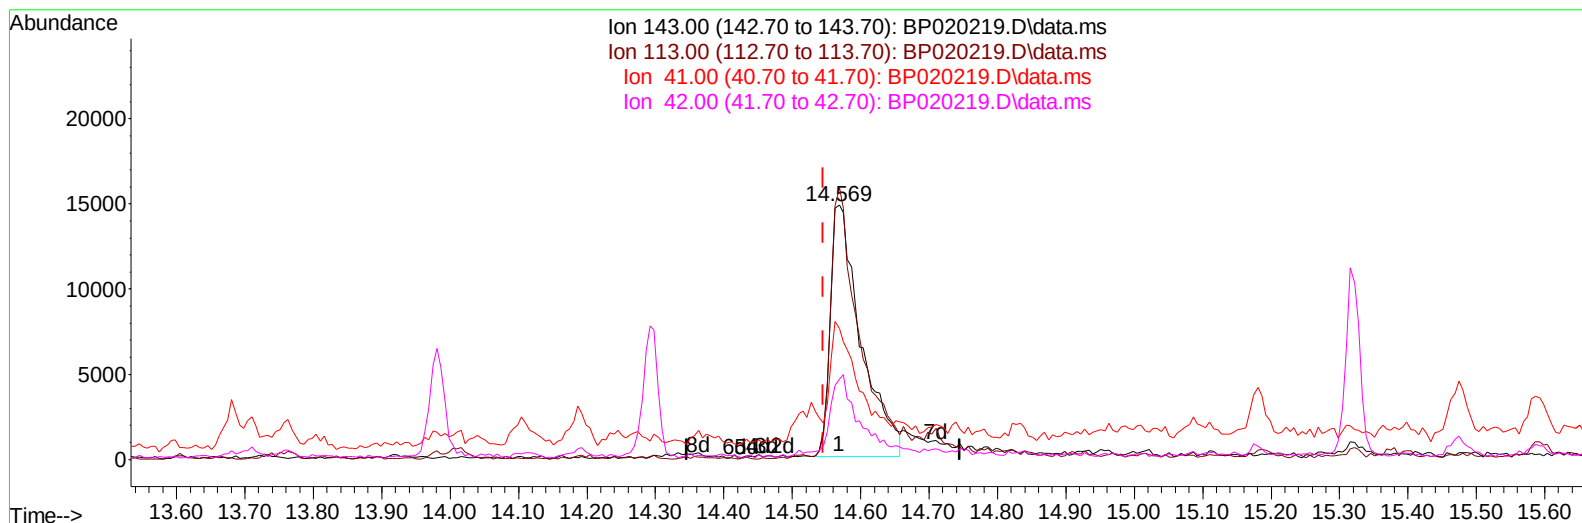

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.023) 12.62 ng/ul

response 45870

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	106.74
41.00	50.30	51.60
42.00	32.50	31.73




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020219.D
Acq On : 07 May 2024 00:01
Operator : MA/JU
Sample : P2368-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43L6

Manual IntegrationsAPPROVED

Quant Time: May 07 01:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

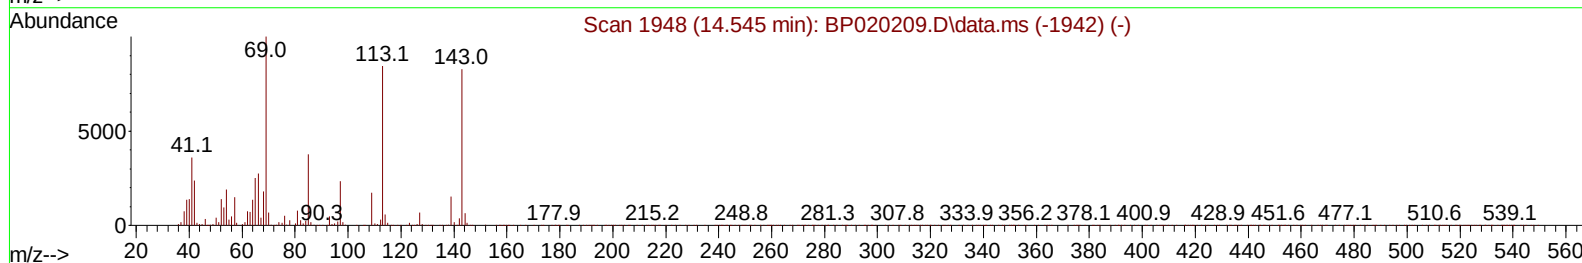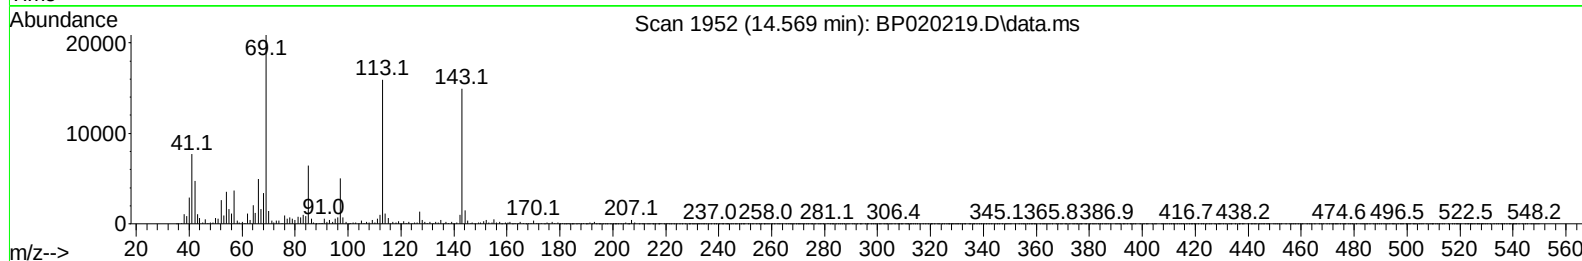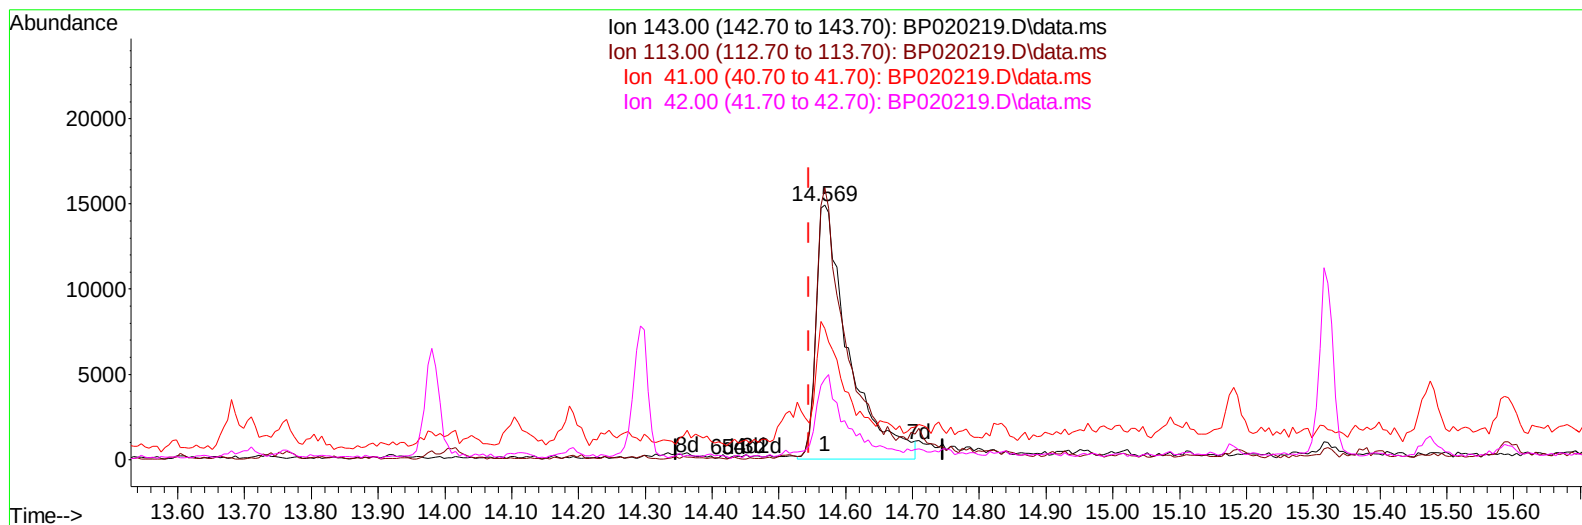

TIC: BP020219.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.023) 13.98 ng/ul m

response 50781

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	106.74
41.00	50.30	51.60
42.00	32.50	31.73

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020219.D
 Acq On : 07 May 2024 00:01
 Operator : MA/JU
 Sample : P2368-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43L6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 03:51:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	107902	20.000	ng/ul	0.02
20) Naphthalene-d8	10.393	136	463339	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.292	164	323729	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.127	188	684256	20.000	ng/ul	-0.01
79) Chrysene-d12	21.627	240	495021	20.000	ng/ul	0.00
88) Perylene-d12	24.986	264	504385	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	10785	4.221	ng/uL	0.01
4) Pyridine-d5	3.634	84	34355	4.628	ng/ul	0.03
7) Phenol-d5	6.804	99	206842	22.321	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.975	67	135236	24.024	ng/ul	0.02
11) 2-Chlorophenol-d4	7.163	132	163123	24.625	ng/ul	0.02
15) 4-Methylphenol-d8	8.328	113	151294	20.195	ng/ul	0.02
21) Nitrobenzene-d5	8.787	128	88061	25.381	ng/ul	0.03
24) 2-Nitrophenol-d4	9.493	143	93832	23.616	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.034	165	167133	23.051	ng/ul	0.02
31) 4-Chloroaniline-d4	10.557	131	150663	14.847	ng/ul	0.02
46) Dimethylphthalate-d6	13.710	166	648175	27.418	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	694372	26.589	ng/ul	0.00
54) 4-Nitrophenol-d4	14.569	143	50781m	13.976	ng/ul	0.02
60) Fluorene-d10	15.322	176	551275	27.958	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	62163	14.316	ng/ul	0.00
73) Anthracene-d10	17.233	188	869160	29.362	ng/ul	0.00
81) Pyrene-d10	19.633	212	995678	34.409	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.751	264	713448	29.255	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020219.D
Acq On : 07 May 2024 00:01
Operator : MA/JU
Sample : P2368-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43L6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 03:51:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

