




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020222.D
 Acq On : 07 May 2024 02:13
 Operator : MA/JU
 Sample : P2368-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43L5

Manual IntegrationsAPPROVED

Quant Time: May 07 02:46:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

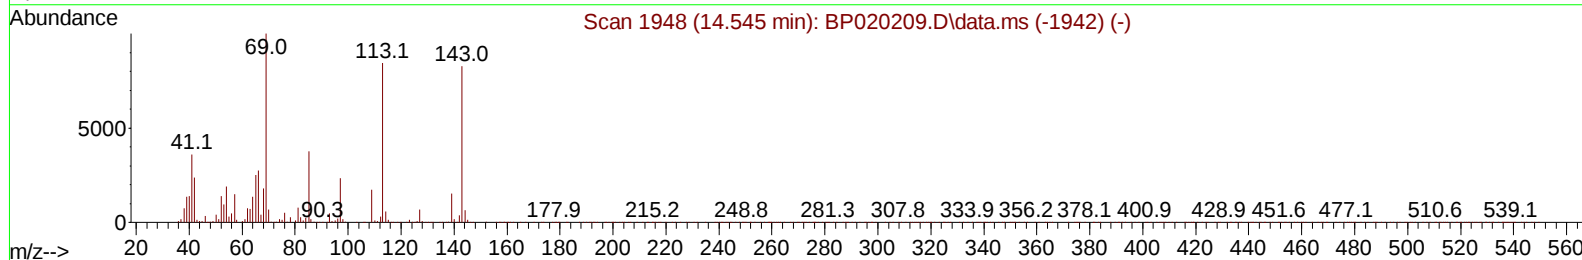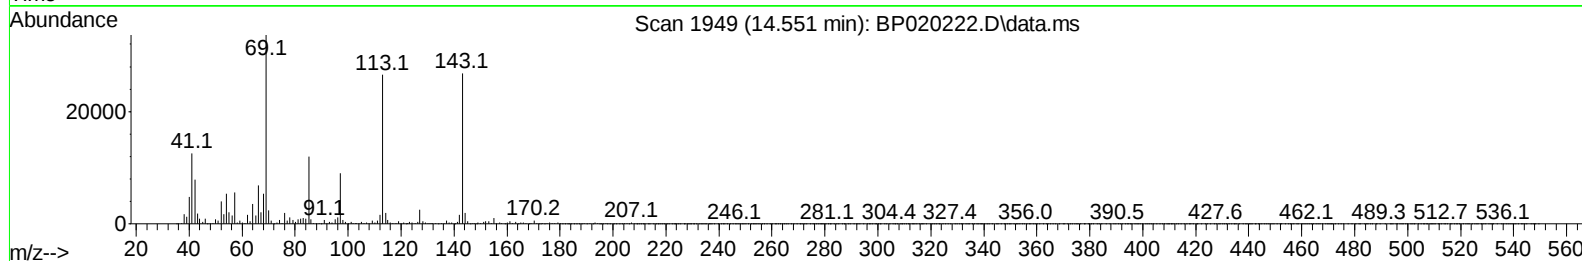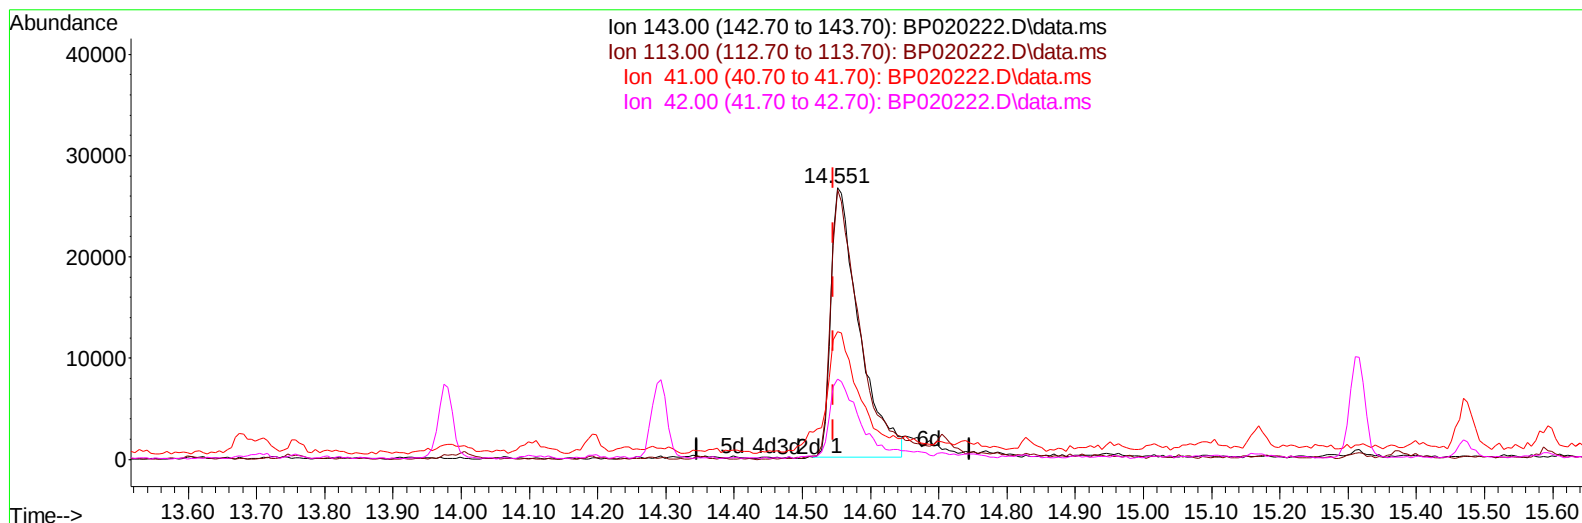

TIC: BP020222.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.006) 19.87 ng/u1

response 76985

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	99.31
41.00	50.30	46.98
42.00	32.50	29.53




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020222.D
 Acq On : 07 May 2024 02:13
 Operator : MA/JU
 Sample : P2368-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43L5

Manual IntegrationsAPPROVED

Quant Time: May 07 02:46:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

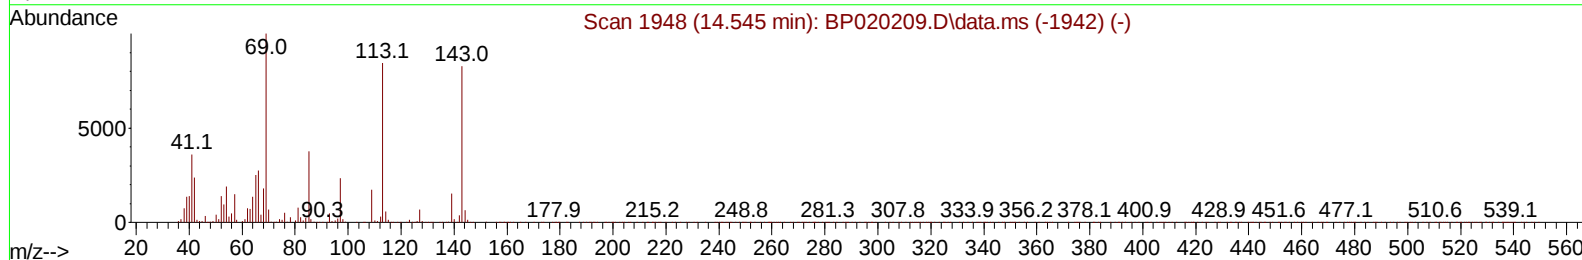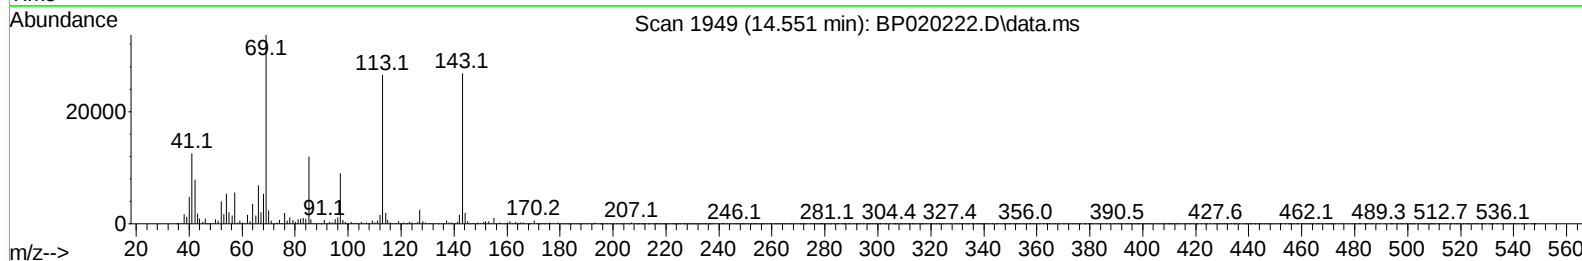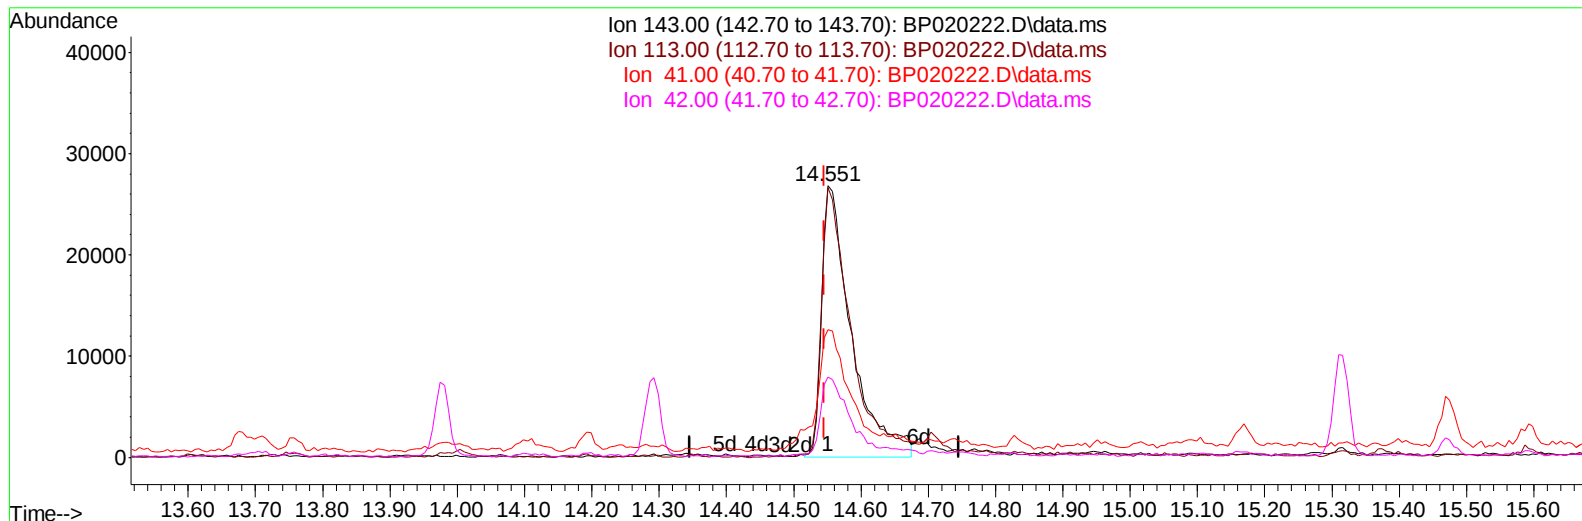

TIC: BP020222.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.006) 21.17 ng/ul m

response 82007

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	99.31
41.00	50.30	46.98
42.00	32.50	29.53

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020222.D
 Acq On : 07 May 2024 02:13
 Operator : MA/JU
 Sample : P2368-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43L5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 04:20:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	114265	20.000	ng/ul	0.02
20) Naphthalene-d8	10.393	136	497673	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.293	164	345127	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	729677	20.000	ng/ul	-0.01
79) Chrysene-d12	21.622	240	522603	20.000	ng/ul	-0.01
88) Perylene-d12	24.986	264	555108	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	10721	3.963	ng/uL	0.00
4) Pyridine-d5	3.623	84	85012	10.814	ng/ul	0.02
7) Phenol-d5	6.805	99	225696	23.000	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.975	67	144449	24.232	ng/ul	0.02
11) 2-Chlorophenol-d4	7.158	132	179770	25.626	ng/ul	0.02
15) 4-Methylphenol-d8	8.328	113	173951	21.926	ng/ul	0.02
21) Nitrobenzene-d5	8.781	128	95603	25.653	ng/ul	0.02
24) 2-Nitrophenol-d4	9.493	143	111967	26.236	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.028	165	198031	25.428	ng/ul	0.02
31) 4-Chloroaniline-d4	10.552	131	185912	17.057	ng/ul	0.02
46) Dimethylphthalate-d6	13.710	166	687681	27.285	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	745545	26.779	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	82007m	21.171	ng/ul	0.00
60) Fluorene-d10	15.316	176	569052	27.070	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	88589	19.132	ng/ul	0.00
73) Anthracene-d10	17.234	188	887694	28.122	ng/ul	0.00
81) Pyrene-d10	19.633	212	942045	30.837	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.757	264	727867	27.119	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020222.D
Acq On : 07 May 2024 02:13
Operator : MA/JU
Sample : P2368-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43L5

Manual IntegrationsAPPROVED

Quant Time: May 07 04:20:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

