




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020225.D
 Acq On : 07 May 2024 08:22
 Operator : MA/JU
 Sample : PB160715BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK715

Manual IntegrationsAPPROVED

Quant Time: May 07 10:47:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

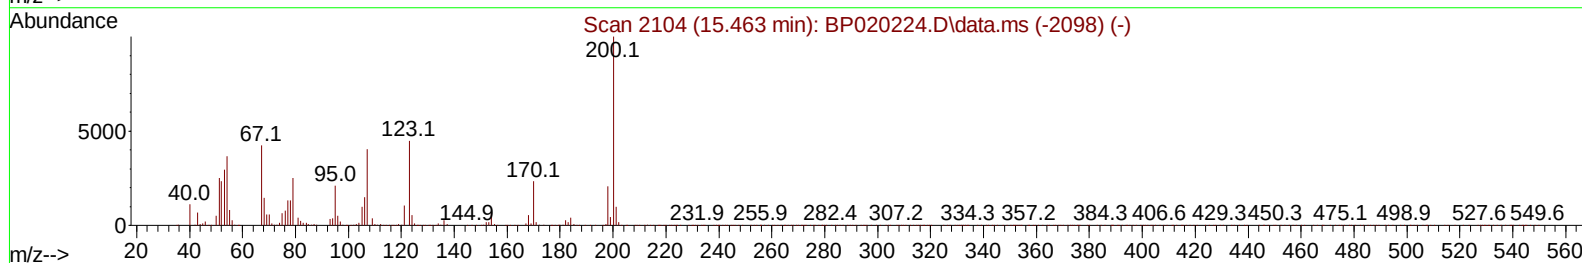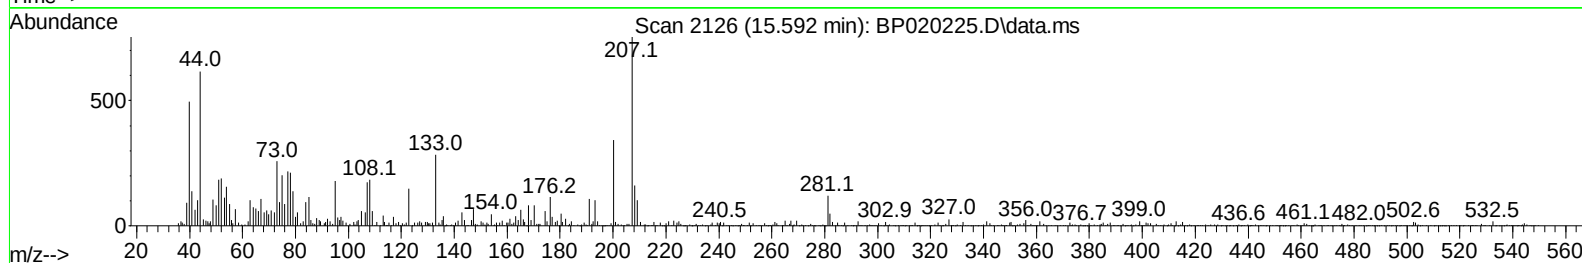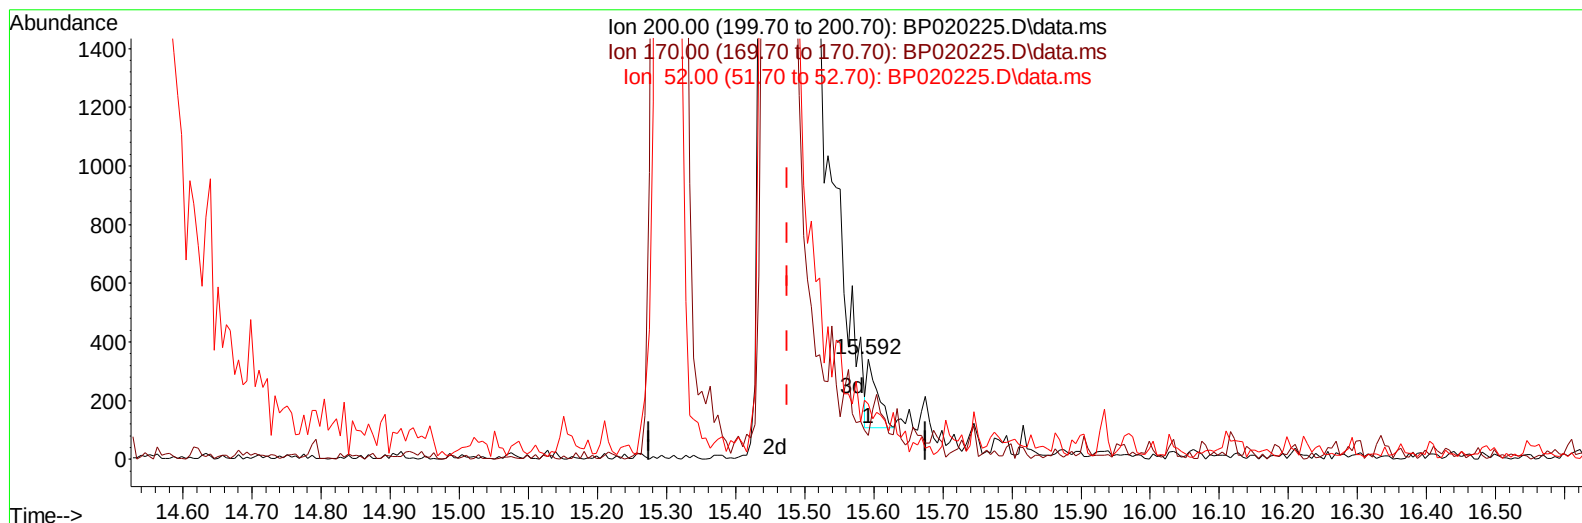

TIC: BP020225.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.592min (+ 0.118) 0.05 ng/ul

response 247

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.00	23.98
52.00	48.40	54.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020225.D
 Acq On : 07 May 2024 08:22
 Operator : MA/JU
 Sample : PB160715BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK715

Manual IntegrationsAPPROVED

Quant Time: May 07 10:47:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

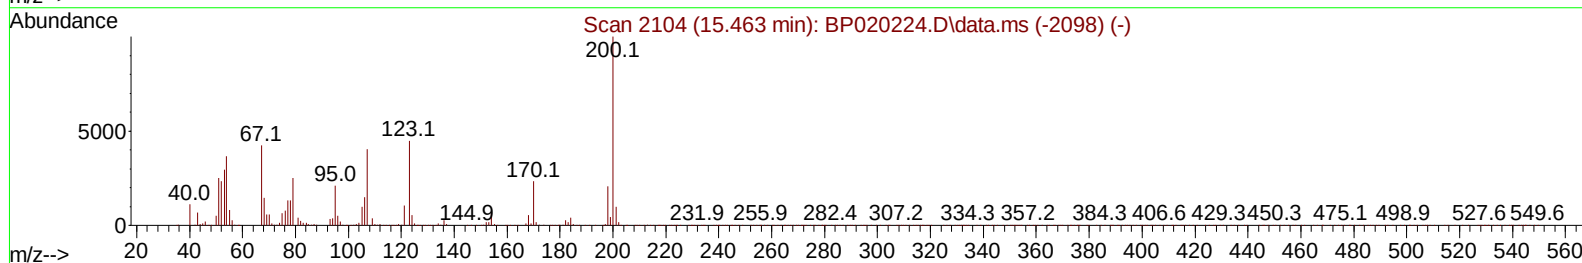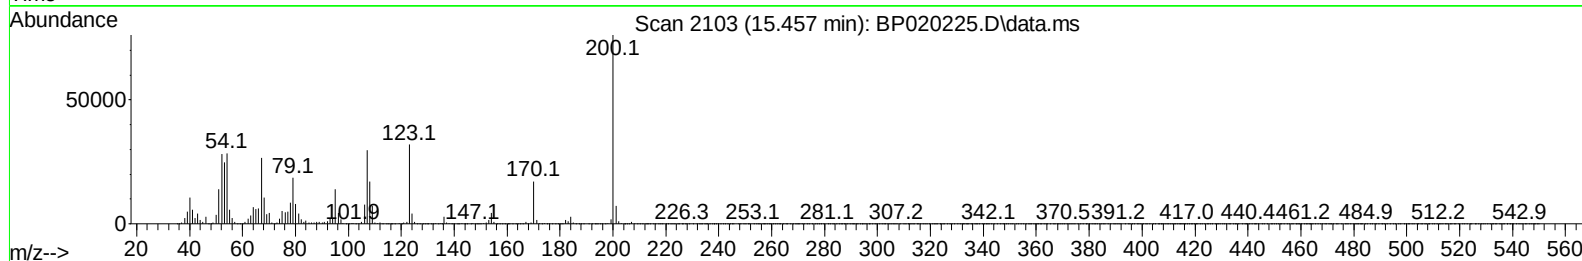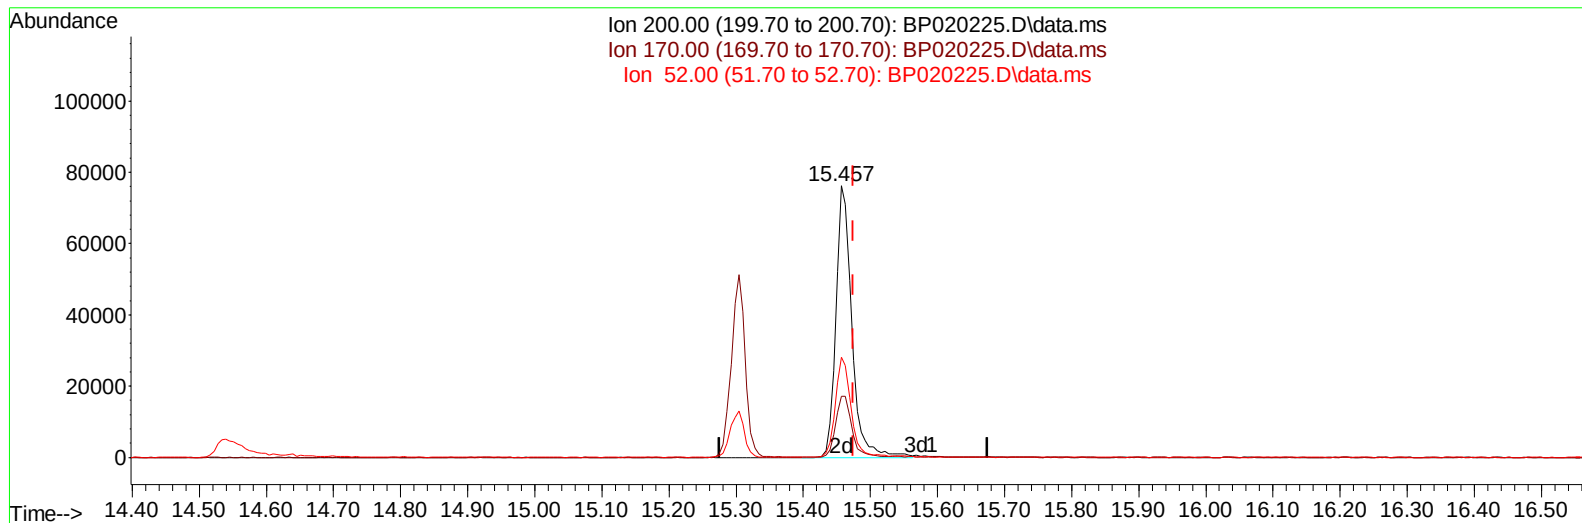

TIC: BP020225.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.457min (-0.018) 24.63 ng/ul m

response 124791

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.00	22.51
52.00	48.40	36.81#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020225.D
 Acq On : 07 May 2024 08:22
 Operator : MA/JU
 Sample : PB160715BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK715

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/07/2024
 Supervised By :mohammad ahmed 05/08/2024

Quant Time: May 07 10:48:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	114408	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	491582	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	357931	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.122	188	798546	20.000	ng/ul	-0.02
79) Chrysene-d12	21.633	240	749723	20.000	ng/ul	0.00
88) Perylene-d12	24.998	264	753133	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	14439	5.330	ng/uL	0.00
4) Pyridine-d5	3.605	84	202435	25.718	ng/ul	0.00
7) Phenol-d5	6.781	99	249746	25.419	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.952	67	156560	26.231	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	190780	27.162	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	205673	25.892	ng/ul	0.00
21) Nitrobenzene-d5	8.757	128	98678	26.807	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	115941	27.504	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.004	165	182591	23.736	ng/ul	0.00
31) 4-Chloroaniline-d4	10.534	131	331132	30.756	ng/ul	0.00
46) Dimethylphthalate-d6	13.698	166	721933	27.620	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	762280	26.400	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.539	143	106024	26.392	ng/ul	0.00
60) Fluorene-d10	15.304	176	599375	27.492	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.457	200	124791m	24.626	ng/ul	-0.02
73) Anthracene-d10	17.222	188	995510	28.817	ng/ul	-0.02
81) Pyrene-d10	19.633	212	1188332	27.115	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.768	264	996981	27.378	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020225.D
Acq On : 07 May 2024 08:22
Operator : MA/JU
Sample : PB160715BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK715

Manual IntegrationsAPPROVED

Quant Time: May 07 10:48:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/07/2024
Supervised By :mohammad ahmed 05/08/2024

